

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
 Data File : PD068176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 15:44
 Operator : AR\AJ
 Sample : PB142895BS
 Misc : CHLOR BS
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB142895BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 01:04:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:16:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.176	34365067	201.7E6	23.606	21.811
28)	SA Decachlor...	8.223	9.375	30613389	113.4E6	21.363	22.784
Target Compounds							
23)	Chlordane-1	4.329	5.198	12218497	93503363	201.354	223.353
24)	Chlordane-2	4.833	5.672	15426731	91274953	219.269	221.350
25)	Chlordane-3	5.401	6.328	42389432	314.8E6	203.429	216.908
26)	Chlordane-4	5.460	6.406	35628142	366.3E6	202.593	219.769
27)	Chlordane-5	6.298	7.217	13768637	62718410	208.549	233.291



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
Data File : PD068176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 15:44
Operator : AR\AJ
Sample : PB142895BS
Misc : CHLOR BS
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB142895BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 01:04:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:16:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

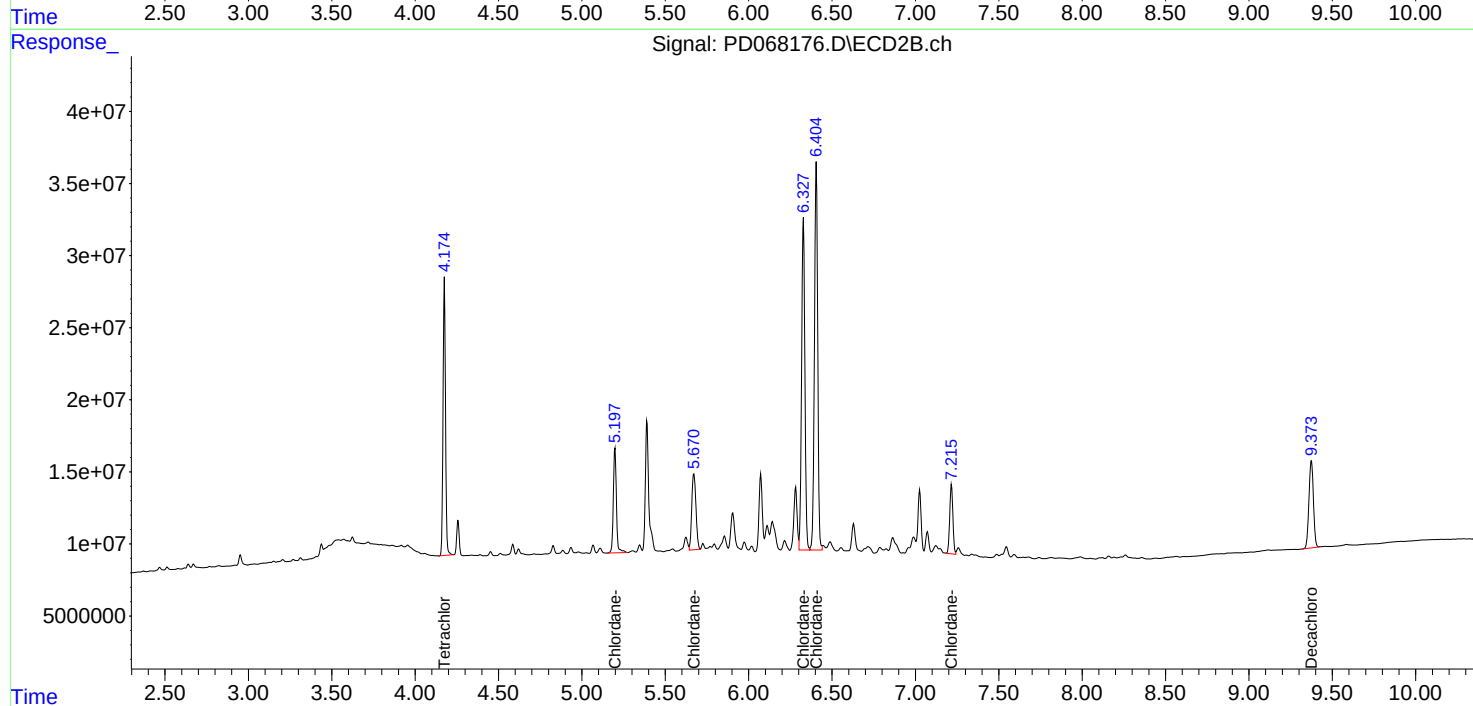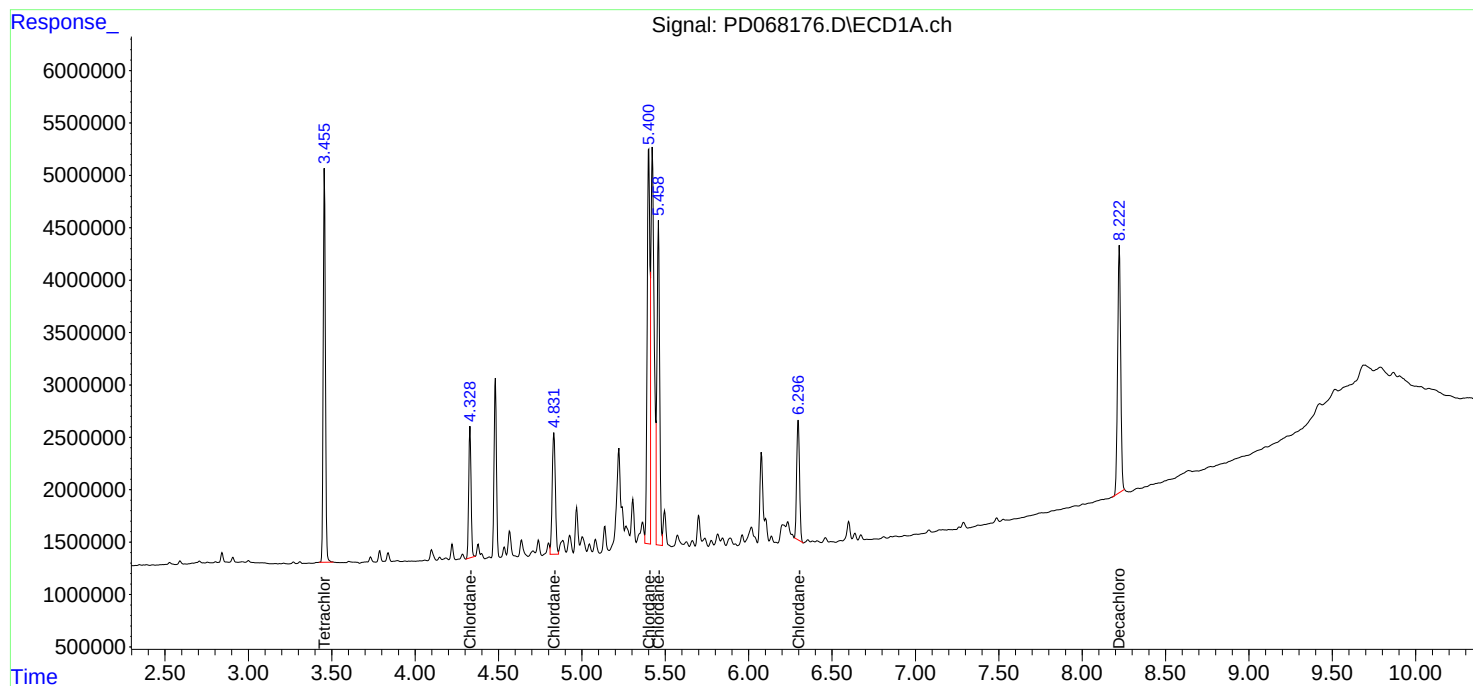


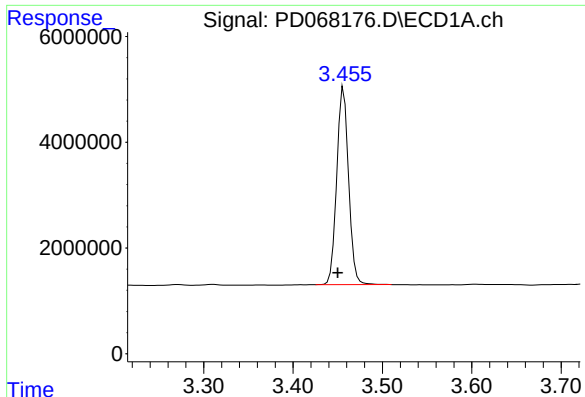

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.007 min
Response: 34365067
Conc: 23.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB142895BS

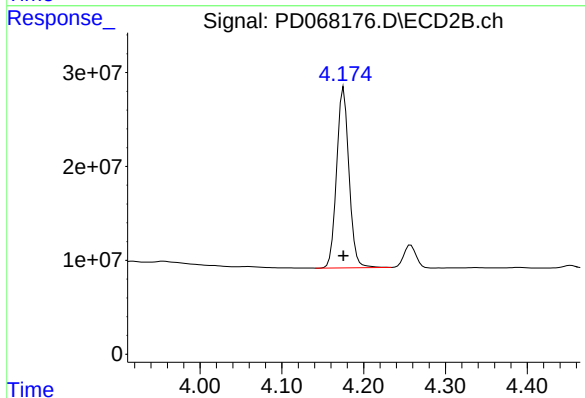


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 201696069
Conc: 21.81 ng/ml

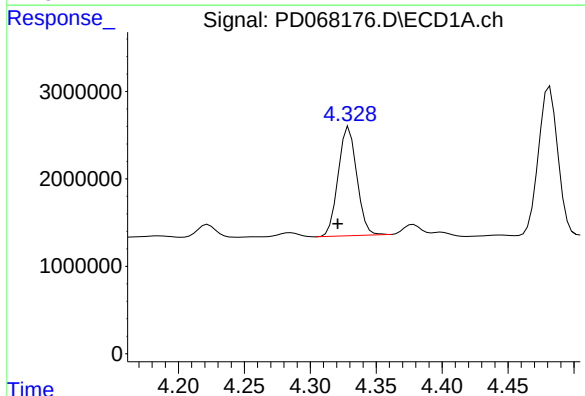


#23 Chlordane-1

R.T.: 4.329 min
Delta R.T.: 0.009 min
Response: 12218497
Conc: 201.35 ng/ml

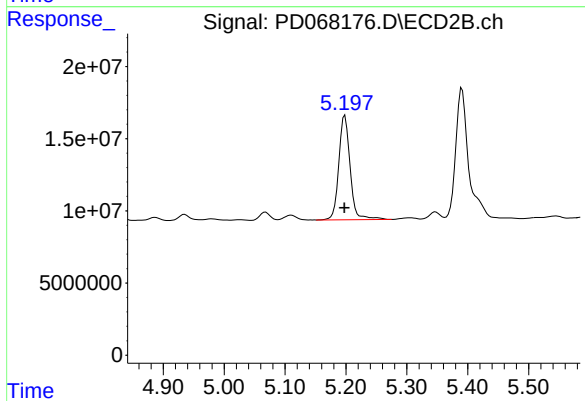

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.001 min
Response: 93503363
Conc: 223.35 ng/ml

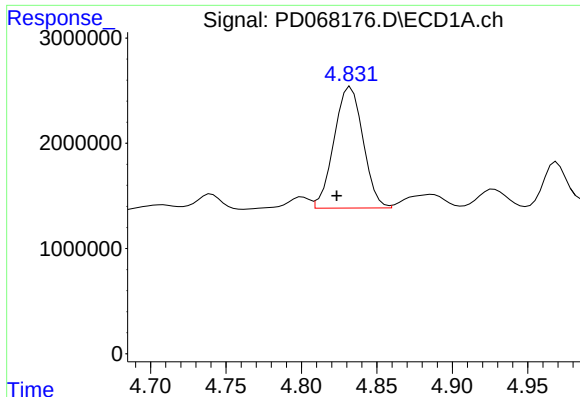

#24 Chlordane-2


R.T.: 4.833 min
Delta R.T.: 0.009 min
Response: 15426731
Conc: 219.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB142895BS

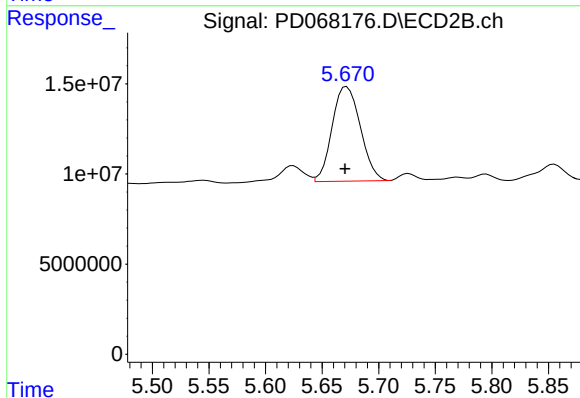


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.001 min
Response: 91274953
Conc: 221.35 ng/ml

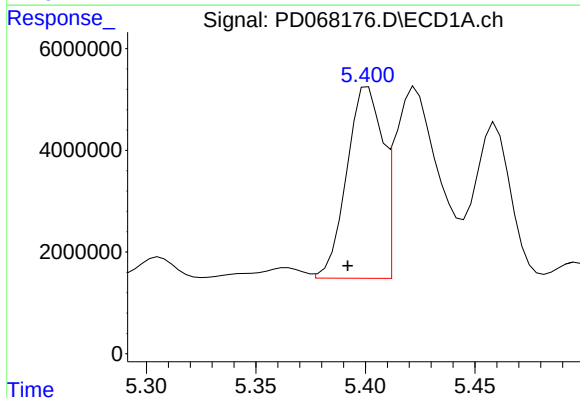


#25 Chlordane-3

R.T.: 5.401 min
Delta R.T.: 0.009 min
Response: 42389432
Conc: 203.43 ng/ml

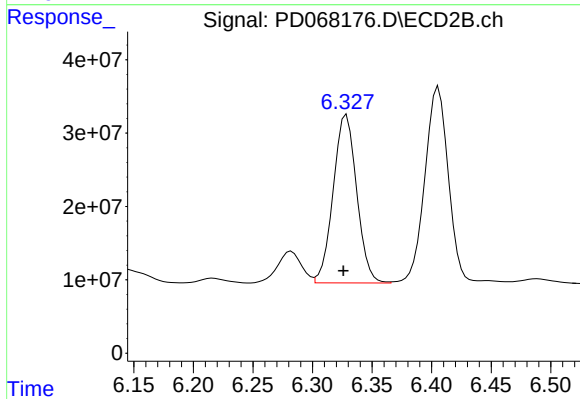

#25 Chlordane-3


R.T.: 6.328 min
Delta R.T.: 0.002 min
Response: 314848588
Conc: 216.91 ng/ml

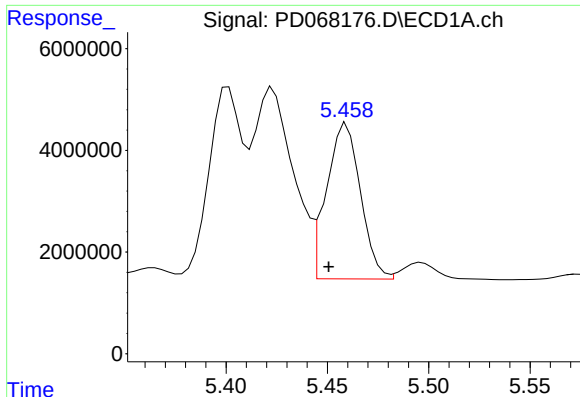

#26 Chlordane-4


R.T.: 5.460 min
Delta R.T.: 0.009 min
Response: 35628142
Conc: 202.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB142895BS

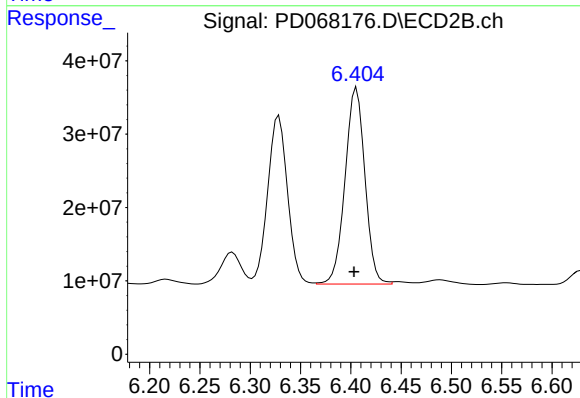


#26 Chlordane-4

R.T.: 6.406 min
Delta R.T.: 0.002 min
Response: 366333022
Conc: 219.77 ng/ml

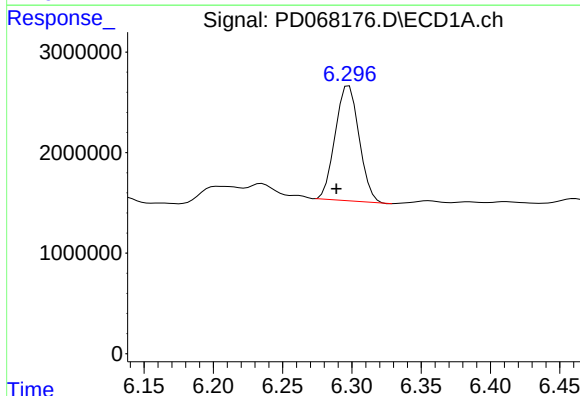


#27 Chlordane-5

R.T.: 6.298 min
Delta R.T.: 0.009 min
Response: 13768637
Conc: 208.55 ng/ml

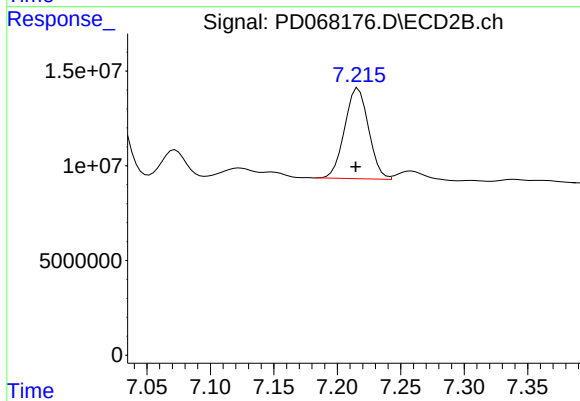

#27 Chlordane-5


R.T.: 7.217 min
Delta R.T.: 0.002 min
Response: 62718410
Conc: 233.29 ng/ml

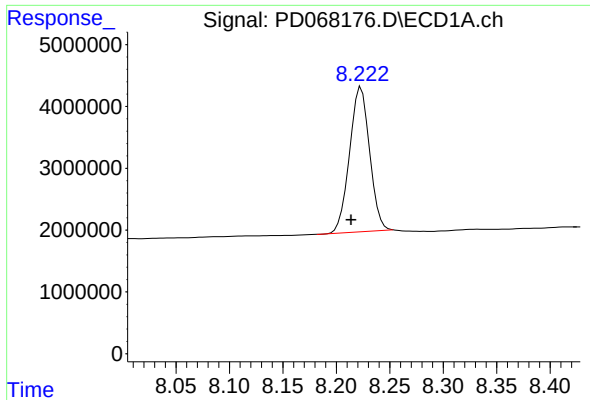

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: 0.010 min
Response: 30613389
Conc: 21.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB142895BS

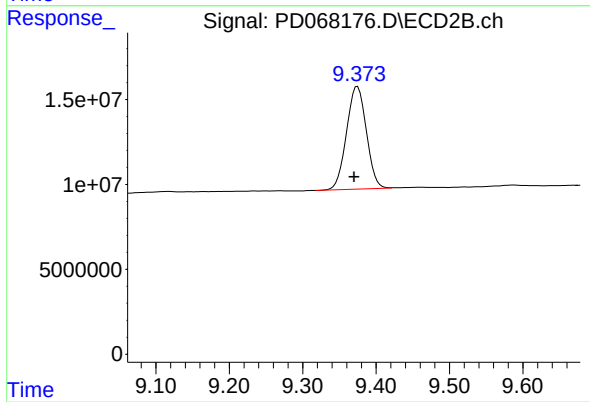

#28 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: 0.005 min
Response: 113426380
Conc: 22.78 ng/ml