

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
 Data File : PD068188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2022 18:38
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 06:20:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 13:16:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	84387775	455.4E6	57.967	49.246
28)	SA Decachlor...	8.212	9.369	74545470	262.1E6	52.020	52.657
Target Compounds							
23)	Chlordane-1	4.320	5.198	29649743	204.2E6	488.612	487.716
24)	Chlordane-2	4.822	5.671	34284989	200.4E6	487.311	485.896
25)	Chlordane-3	5.391	6.326	104.4E6	722.0E6	501.116	497.376
26)	Chlordane-4	5.449	6.403	87853299	841.1E6	499.561	504.573
27)	Chlordane-5	6.287	7.215	33970018	144.7E6	514.533	538.294



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022422\
Data File : PD068188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2022 18:38
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 06:20:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 13:16:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

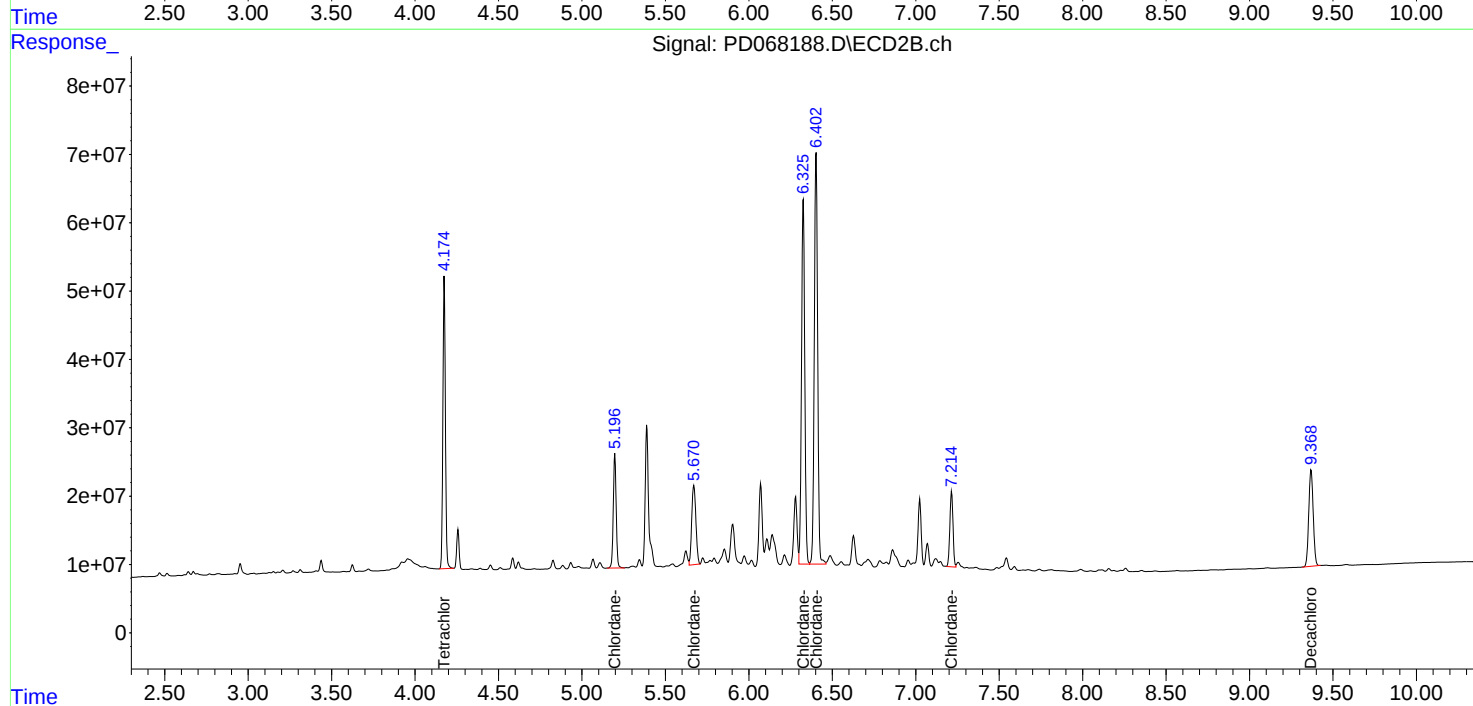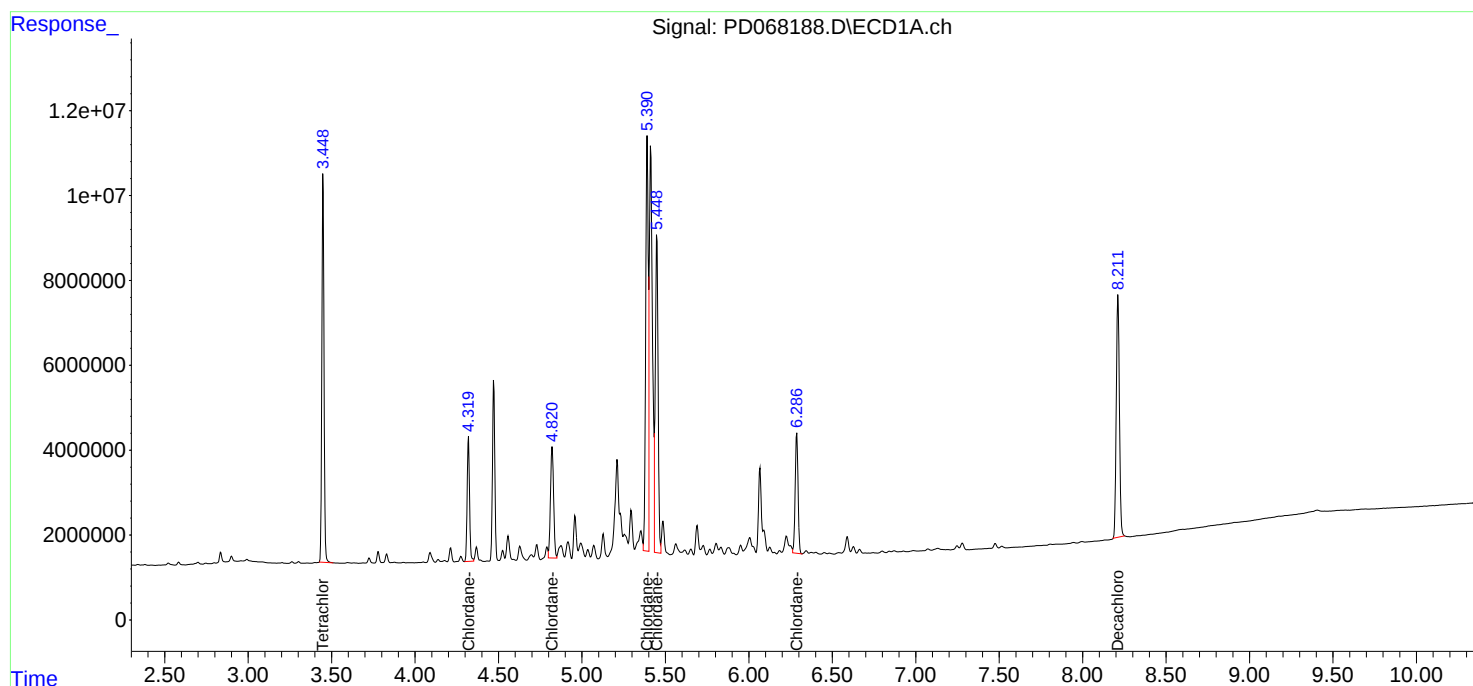


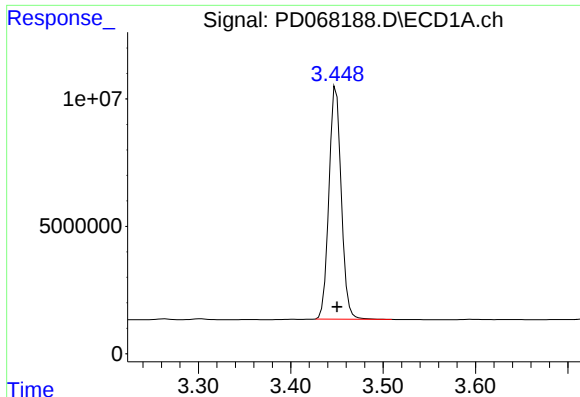

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 84387775
Conc: 57.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

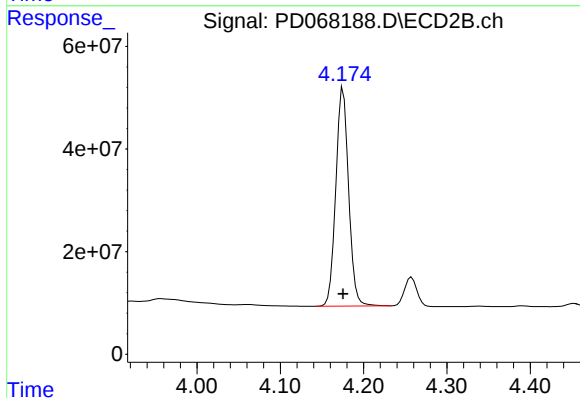


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 455407865
Conc: 49.25 ng/ml

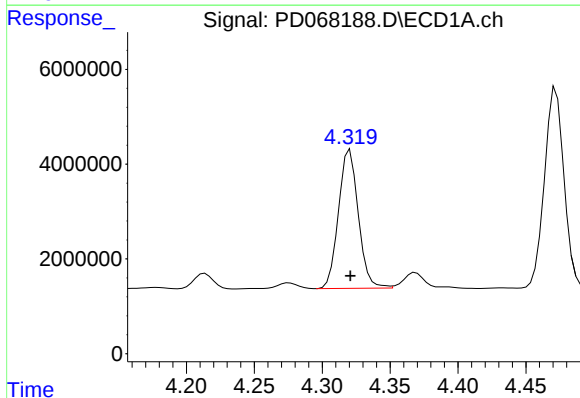


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 29649743
Conc: 488.61 ng/ml

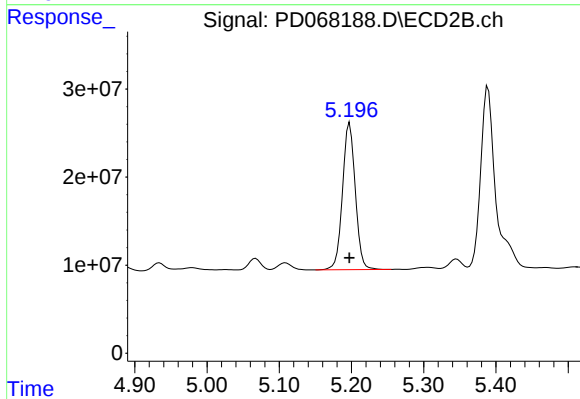

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 204174409
Conc: 487.72 ng/ml

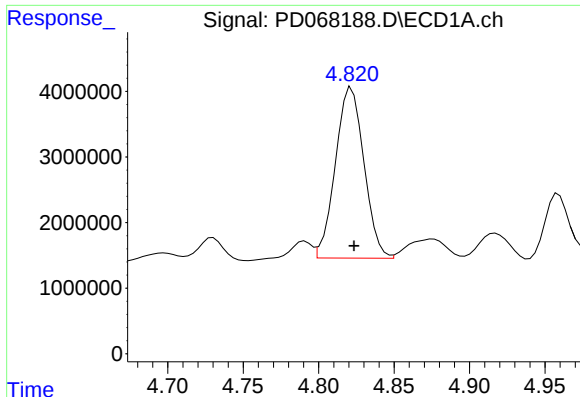

#24 Chlordane-2


R.T.: 4.822 min
Delta R.T.: -0.002 min
Response: 34284989
Conc: 487.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

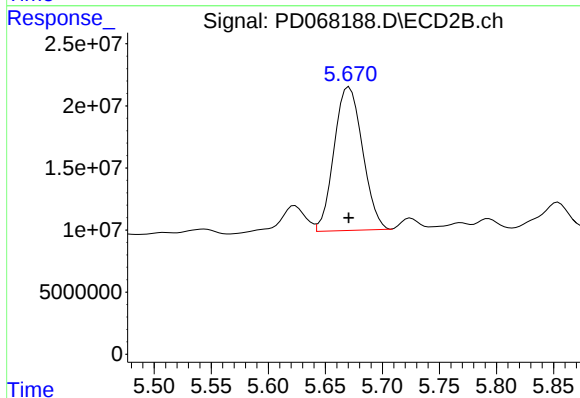


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 200362065
Conc: 485.90 ng/ml

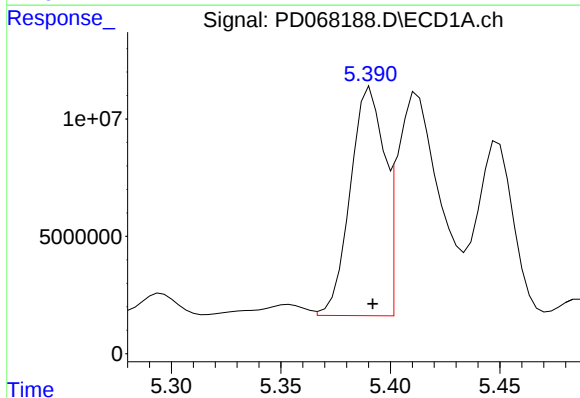


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 104419926
Conc: 501.12 ng/ml

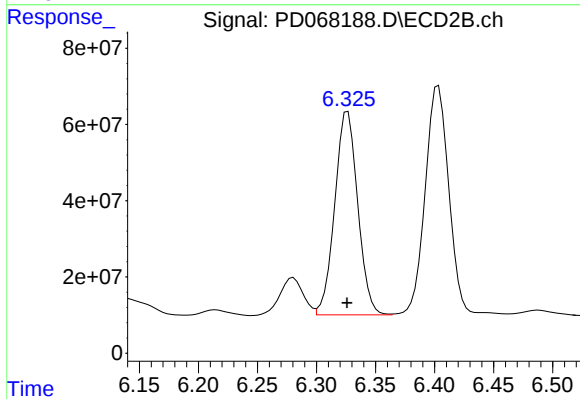

#25 Chlordane-3


R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 721956632
Conc: 497.38 ng/ml

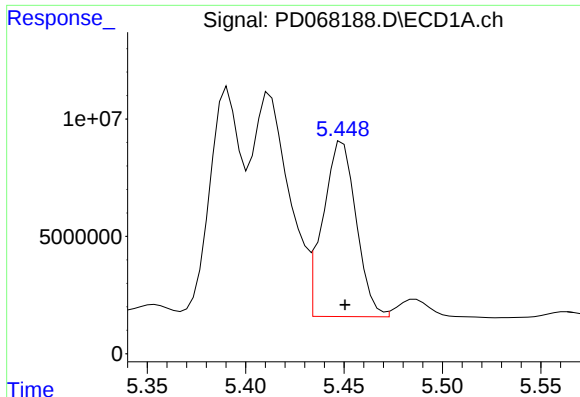

#26 Chlordane-4


R.T.: 5.449 min
Delta R.T.: -0.001 min
Response: 87853299
Conc: 499.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

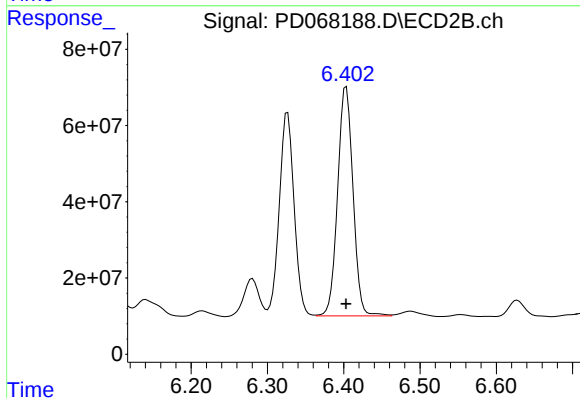


#26 Chlordane-4

R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 841071222
Conc: 504.57 ng/ml

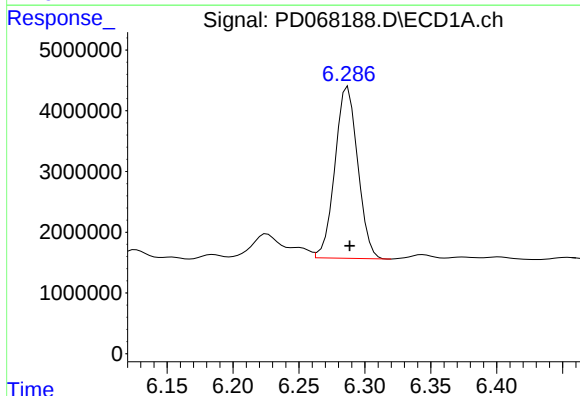


#27 Chlordane-5

R.T.: 6.287 min
Delta R.T.: -0.001 min
Response: 33970018
Conc: 514.53 ng/ml

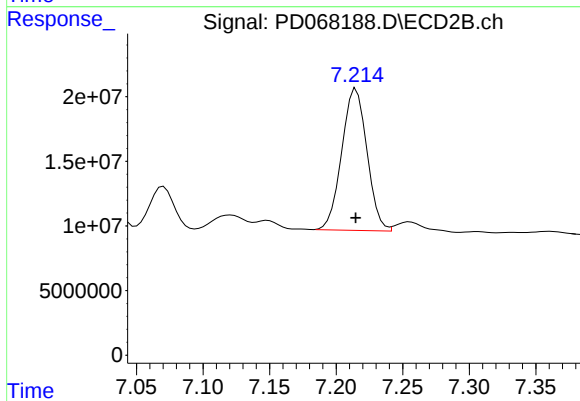

#27 Chlordane-5


R.T.: 7.215 min
Delta R.T.: 0.000 min
Response: 144715900
Conc: 538.29 ng/ml

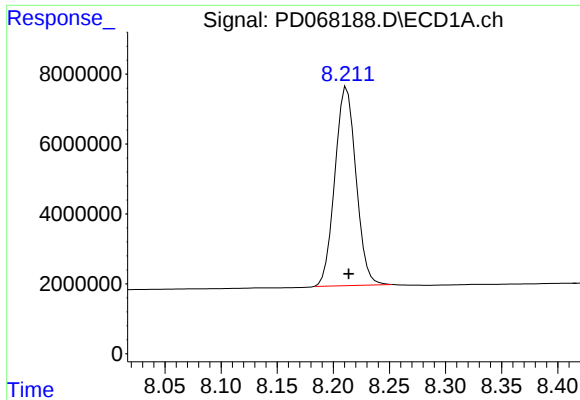

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.002 min
Response: 74545470
Conc: 52.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

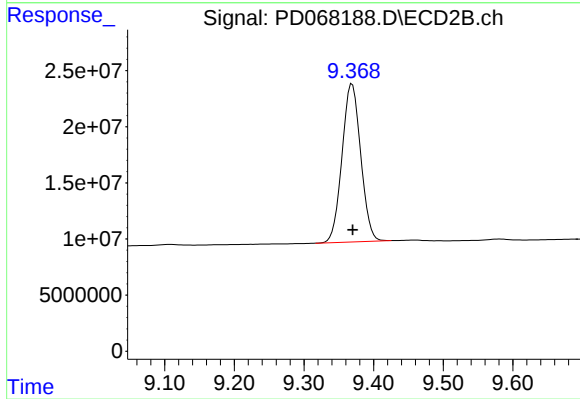

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 262137350
Conc: 52.66 ng/ml