

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022619\
 Data File : PD051393.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Feb 2019 14:33
 Operator : AJ\SJ
 Sample : PIBLK02
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:52:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.224	4.044	29623408	630.7E6	20.614	20.413
2) SA Decachlor...	7.825	9.156	43150670	614.7E6	35.880	32.424
Target Compounds						
6) B beta-BHC	0.000	4.937f	0 57333442	N.D.		2.890
20) A Methoxychlor	0.000	7.640	0 50667112	N.D.		4.786


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022619\
Data File : PD051393.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2019 14:33
Operator : AJ\SJ
Sample : PIBLK02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:52:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

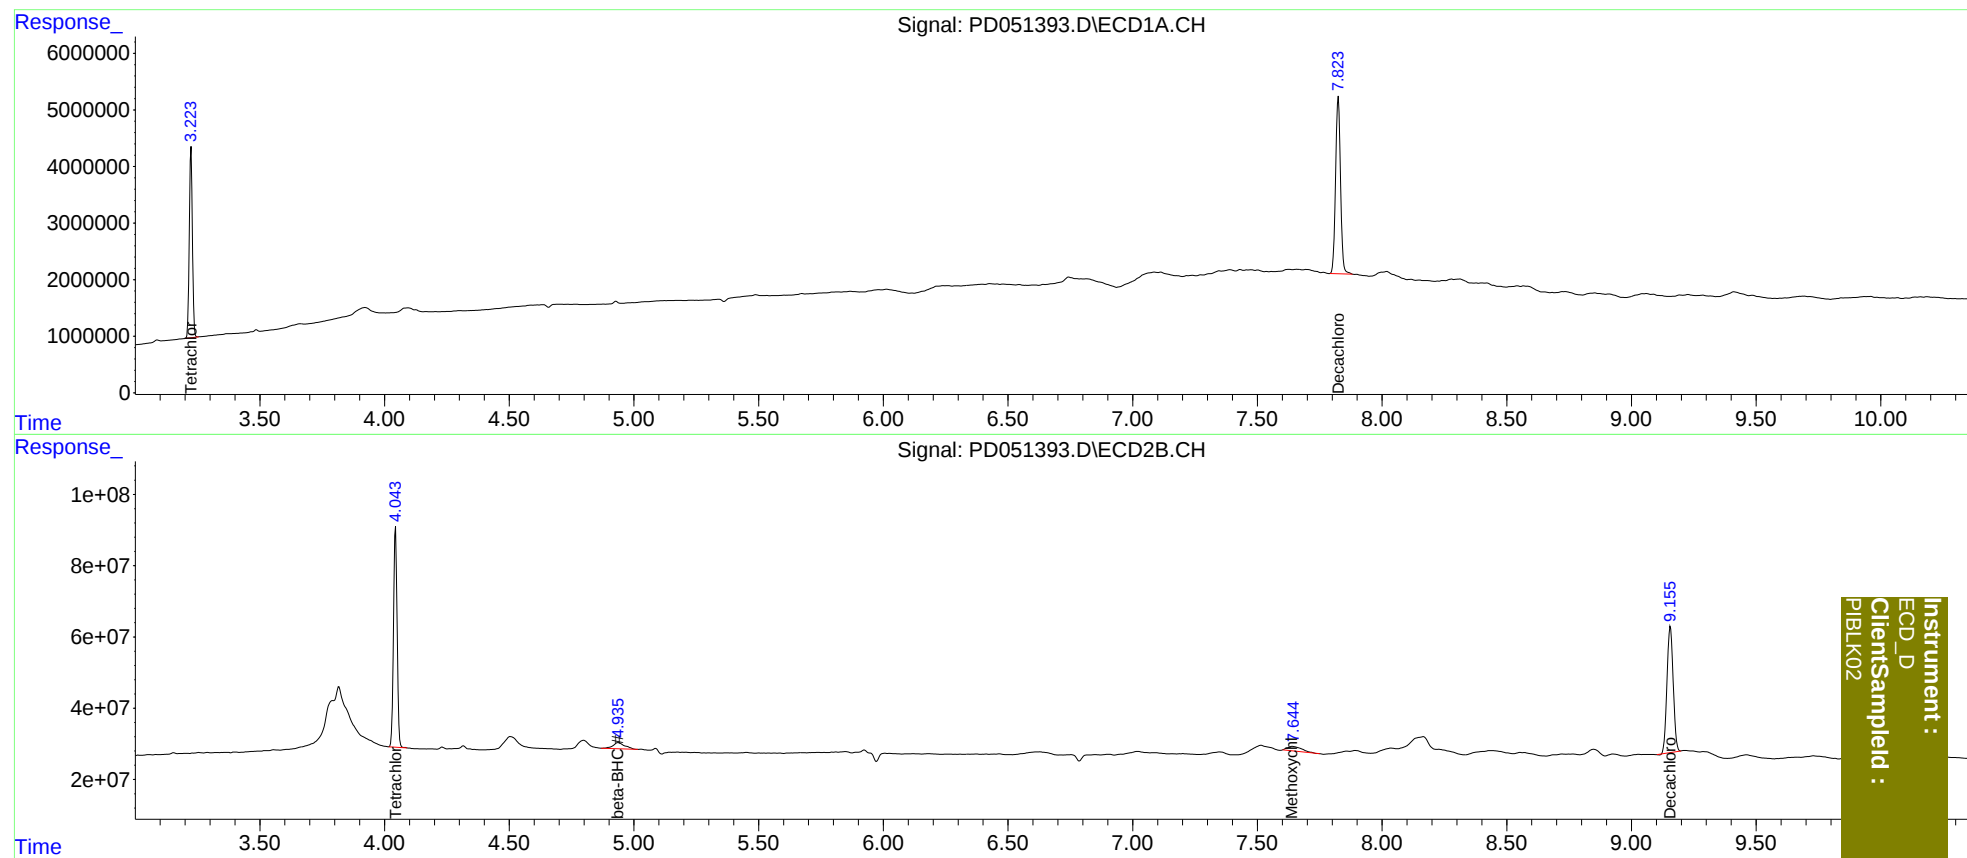


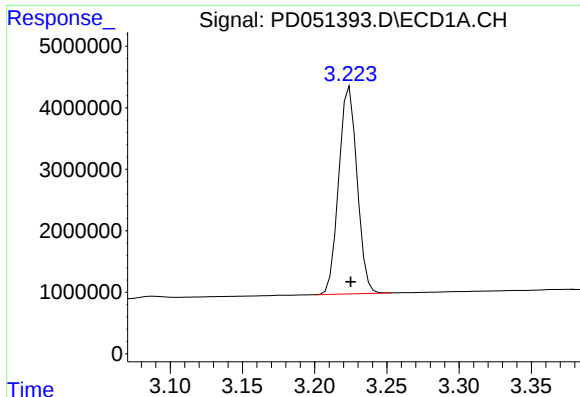

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 29623408
Conc: 20.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK02

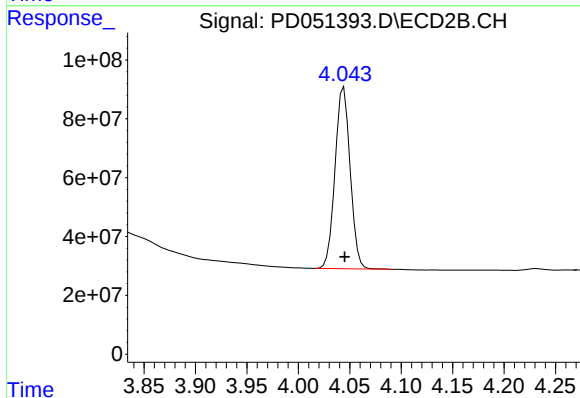


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 630679768
Conc: 20.41 ng/ml

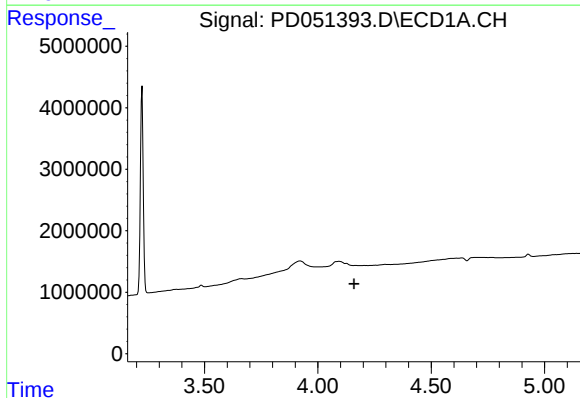


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

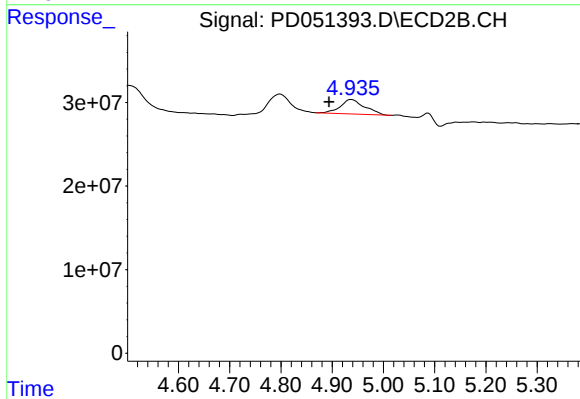

#6 beta-BHC


R.T.: 4.937 min
Delta R.T.: 0.043 min
Response: 57333442
Conc: 2.89 ng/ml

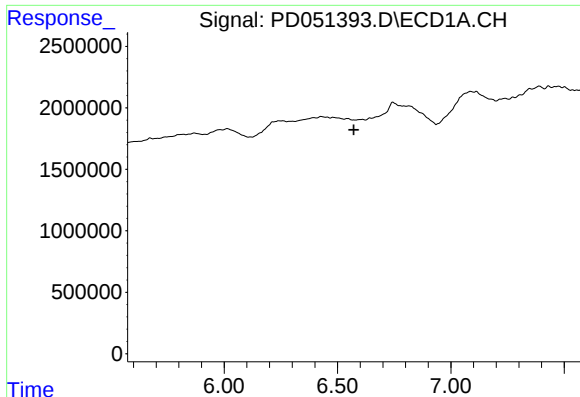

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK02

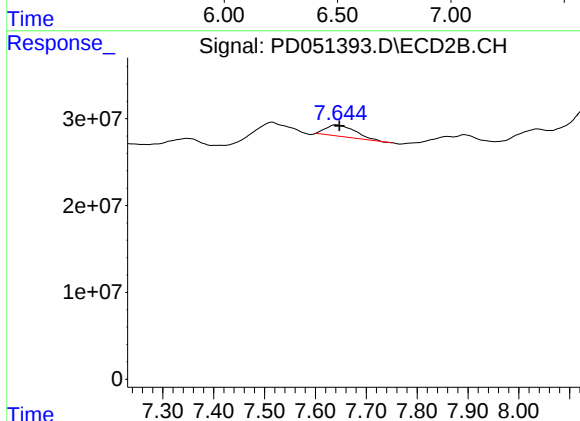


#20 Methoxychlor

R.T.: 7.640 min
Delta R.T.: -0.007 min
Response: 50667112
Conc: 4.79 ng/ml

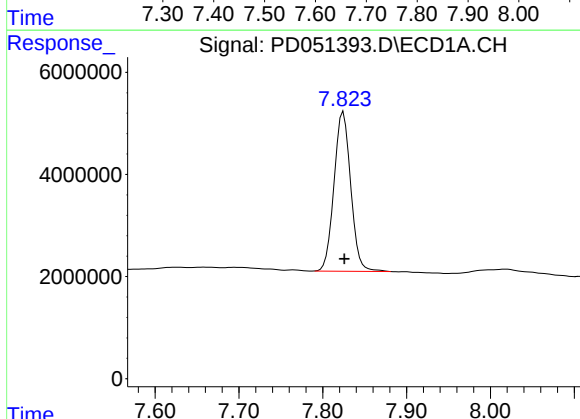

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.001 min
Response: 43150670
Conc: 35.88 ng/ml

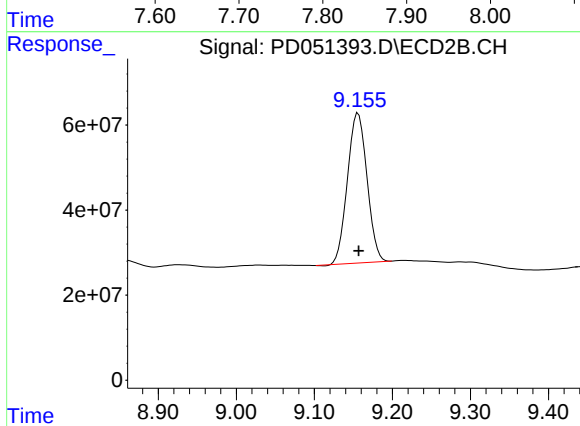

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 614675895
Conc: 32.42 ng/ml