

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022620\
 Data File : PD057454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2020 09:35
 Operator : AJ\MA
 Sample : L1645-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:45:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 24 16:58:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.885	0	26947	N.D.	<MDL
27)	SA Decachlor...	0.000	8.886	0	61807	N.D.	<MDL
Target Compounds							
2)	A alpha-BHC	0.000	4.261	0	172354	N.D.	<MDL
3)	MA gamma-BHC...	0.000	4.579	0	125027	N.D.	<MDL
4)	MA Heptachlor	0.000	5.072	0	187141	N.D.	<MDL
6)	B beta-BHC	0.000	4.699f	0	1827	N.D.	<MDL
7)	B delta-BHC	0.000	4.915f	0	564943	N.D.	0.187
8)	B Heptachlo...	0.000	5.736	0	1117324	N.D.	0.363
9)	A Endosulfan I	0.000	6.101	0	480950	N.D.	0.170
10)	B trans-Chl...	0.000	5.966	0	252537	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.062	0	109004	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.232	0	37921	N.D.	<MDL
13)	MA Dieldrin	0.000	6.383	0	75795	N.D.	<MDL
14)	MA Endrin	0.000	6.549	0	81108	N.D.	<MDL
15)	B Endosulfa...	0.000	6.800	0	323786	N.D.	0.124
17)	MA 4,4'-DDT	0.000	7.009	0	472120	N.D.	0.208
18)	B Endrin al...	0.000	6.905	0	39056	N.D.	<MDL
19)	B Endosulfa...	6.282f	7.131	-100777	394059	N.D.	0.146
20)	A Methoxychlor	0.000	7.451	0	30539	N.D.	<MDL
21)	B Endrin ke...	0.000	7.588	0	73994	N.D.	<MDL
22)	Toxaphene-1	0.000	6.232	0	37921	N.D.	2.471
23)	Toxaphene-2	0.000	6.549	0	81108	N.D.	4.150
24)	Toxaphene-3	0.000	6.928	0	86535	N.D.	3.566
25)	Toxaphene-4	0.000	7.009	0	472120	N.D.	6.688
26)	Toxaphene-5	0.000	7.513	0	8121	N.D.	0.249


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022620\
Data File : PD057454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2020 09:35
Operator : AJ\MA
Sample : L1645-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:45:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 24 16:58:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

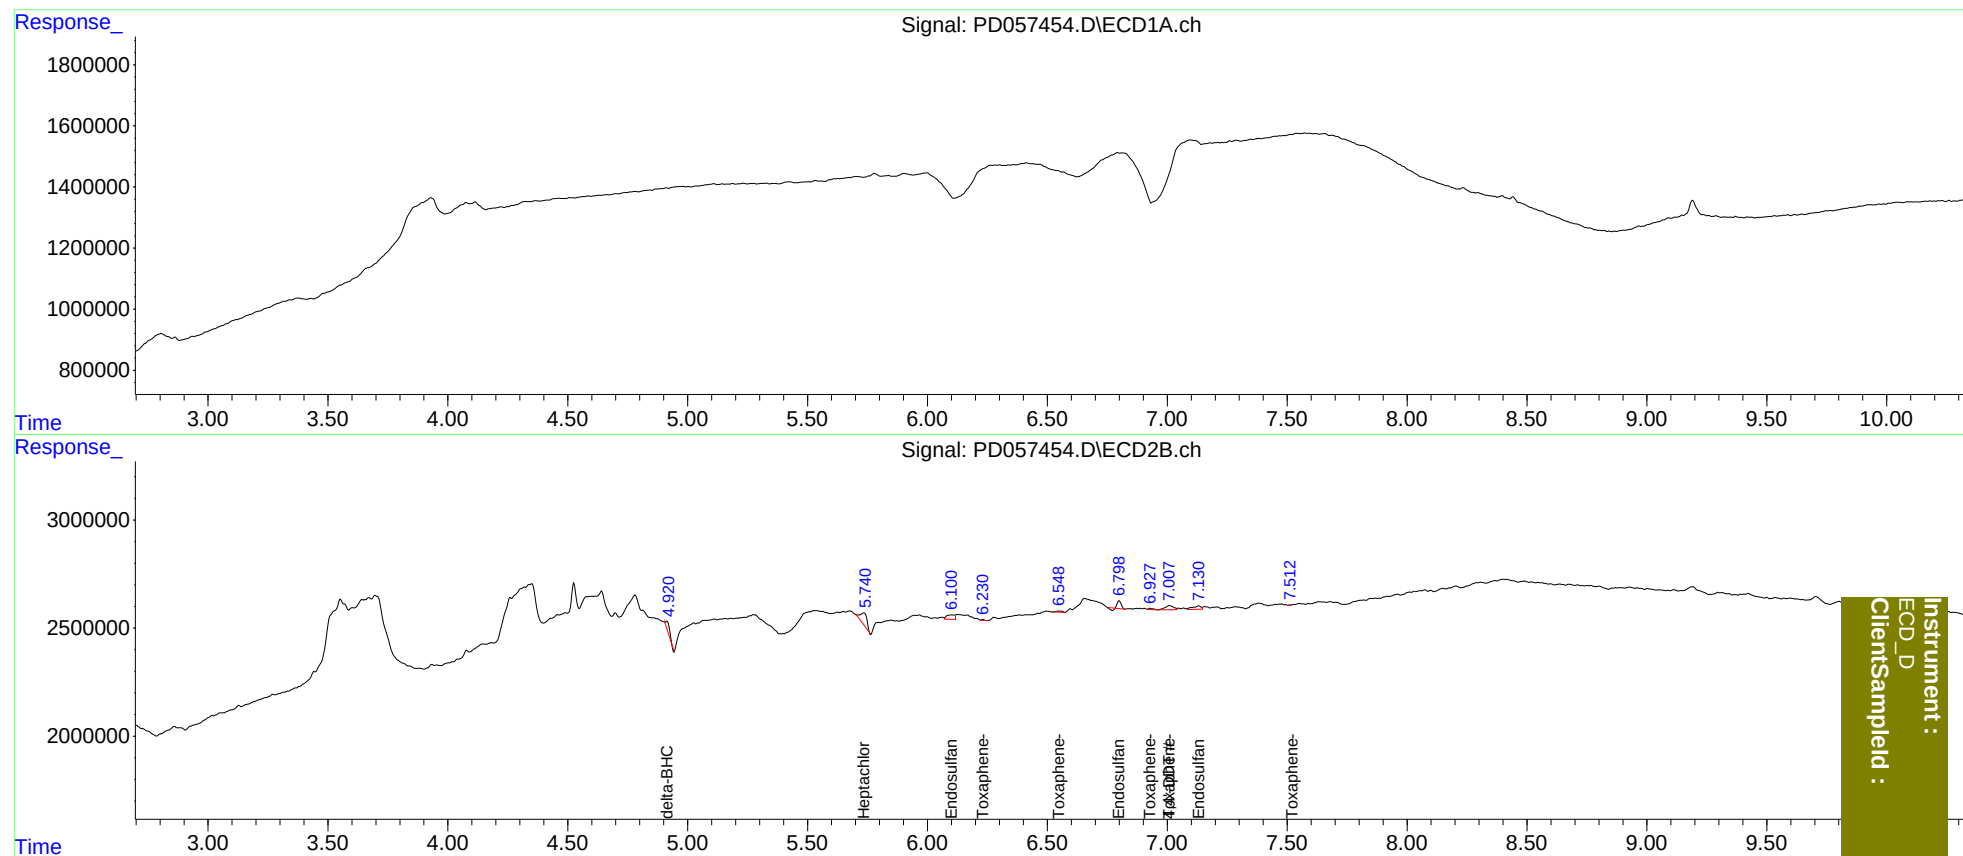


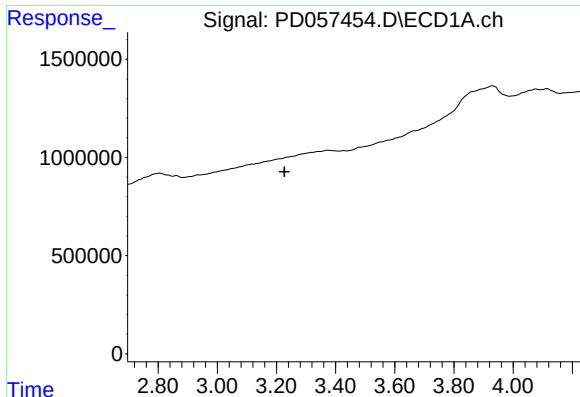

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

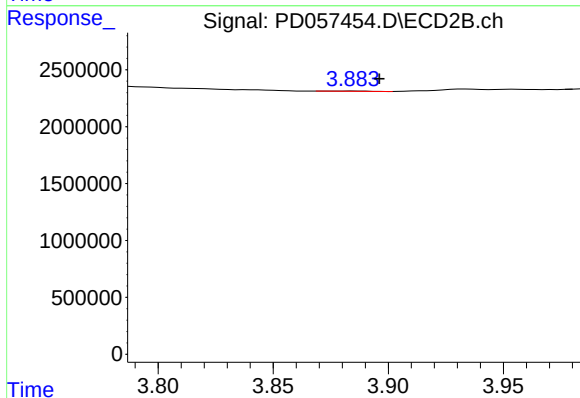


#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: -0.011 min
Response: 26947
Conc: N.D.

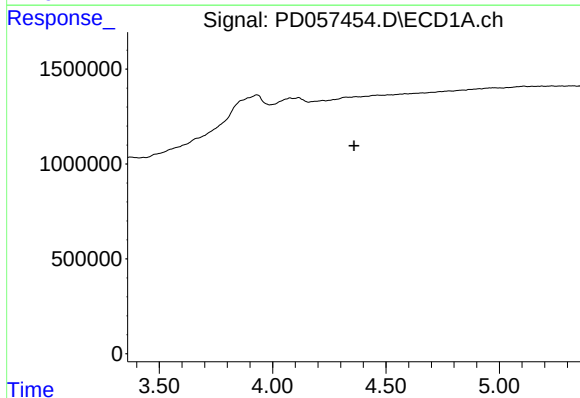


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.360 min
Response: 0
Conc: N.D.

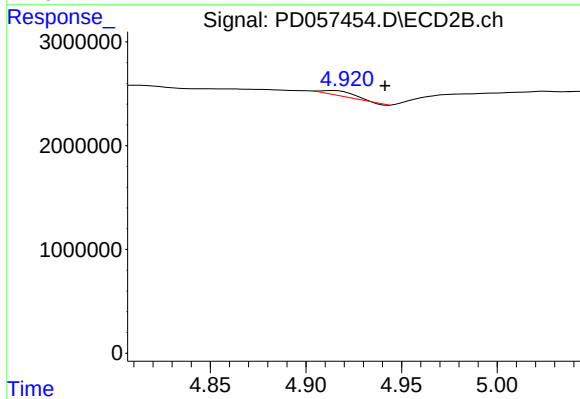

#7 delta-BHC


R.T.: 4.915 min
Delta R.T.: -0.027 min
Response: 564943
Conc: 0.19 ng/ml

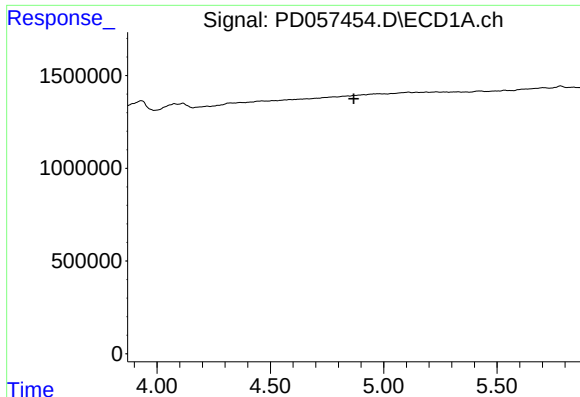

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.869 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

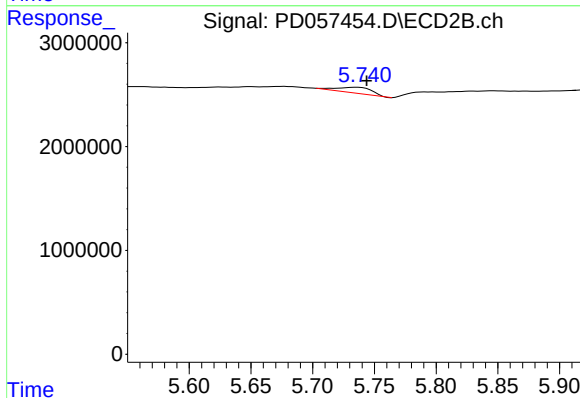


#8 Heptachlor epoxide

R.T.: 5.736 min
Delta R.T.: -0.008 min
Response: 1117324
Conc: 0.36 ng/ml

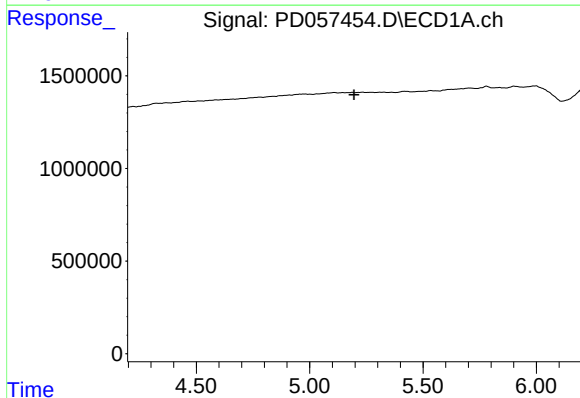


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.196 min
Response: 0
Conc: N.D.

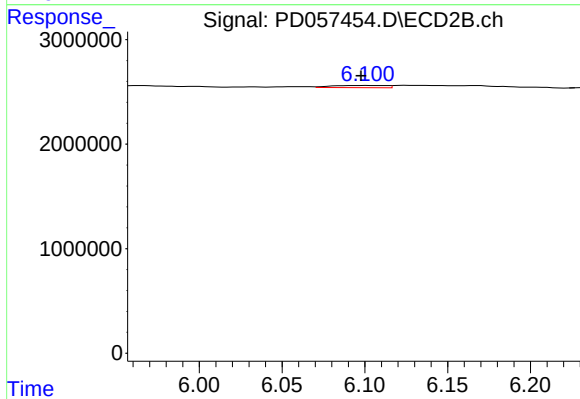

#9 Endosulfan I


R.T.: 6.101 min
Delta R.T.: 0.004 min
Response: 480950
Conc: 0.17 ng/ml

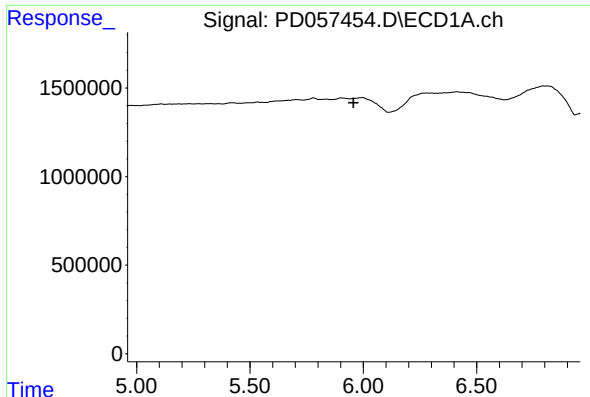

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

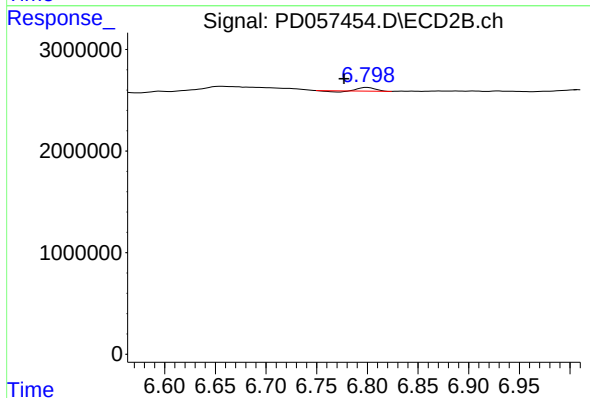


#15 Endosulfan II

R.T.: 6.800 min
Delta R.T.: 0.023 min
Response: 323786
Conc: 0.12 ng/ml

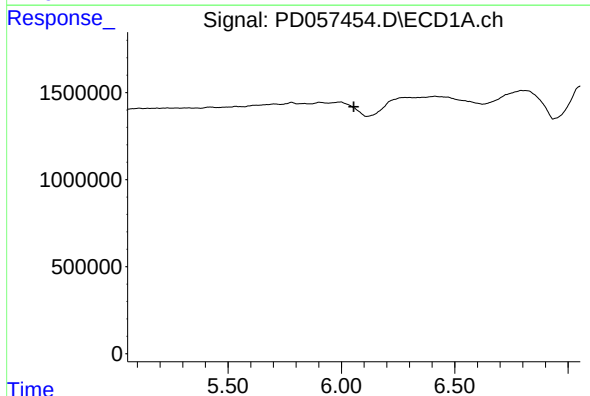


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.055 min
Response: 0
Conc: N.D.

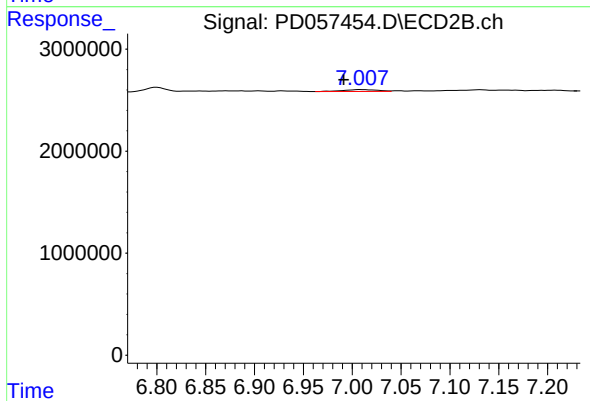

#17 4,4'-DDT


R.T.: 7.009 min
Delta R.T.: 0.017 min
Response: 472120
Conc: 0.21 ng/ml

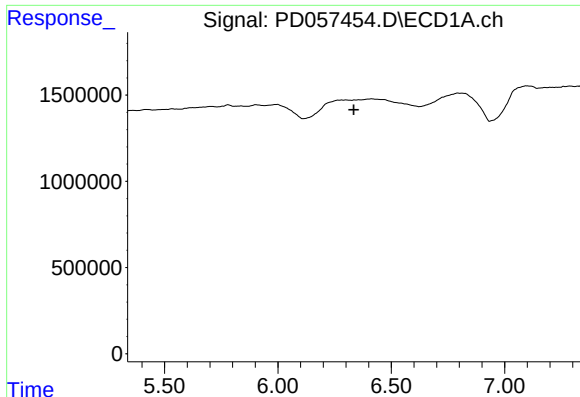

#19 Endosulfan Sulfate


R.T.: 6.282 min
Delta R.T.: -0.053 min
Response: -100777
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

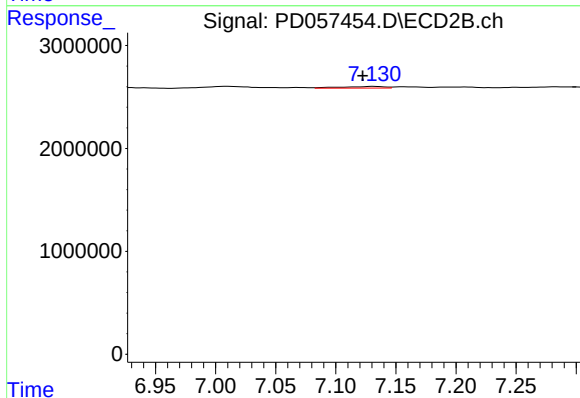


#19 Endosulfan Sulfate

R.T.: 7.131 min
Delta R.T.: 0.009 min
Response: 394059
Conc: 0.15 ng/ml

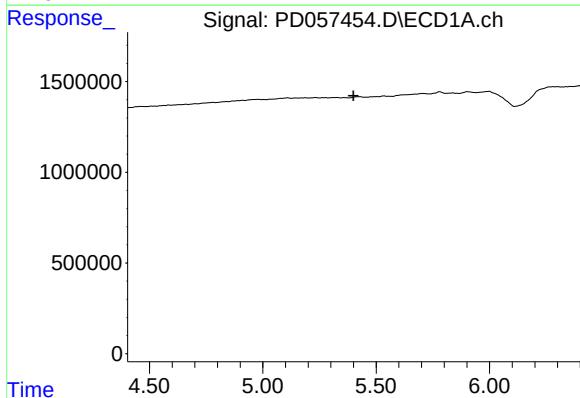


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.400 min
Response: 0
Conc: N.D.

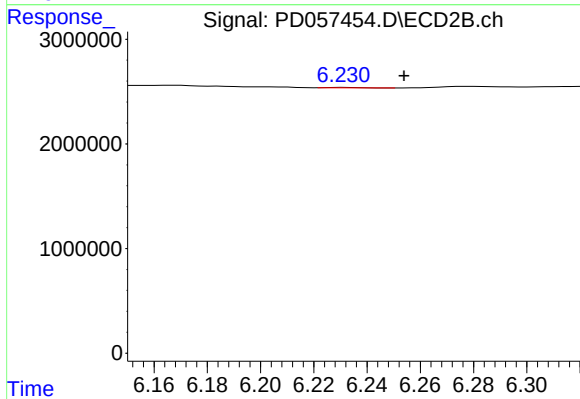

#22 Toxaphene-1


R.T.: 6.232 min
Delta R.T.: -0.022 min
Response: 37921
Conc: 2.47 ng/ml

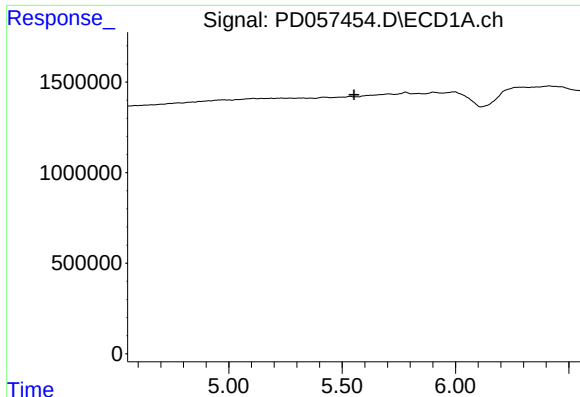

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 5.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

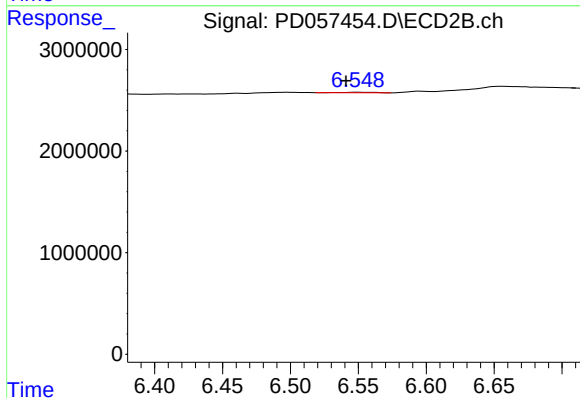


#23 Toxaphene-2

R.T.: 6.549 min
Delta R.T.: 0.008 min
Response: 81108
Conc: 4.15 ng/ml

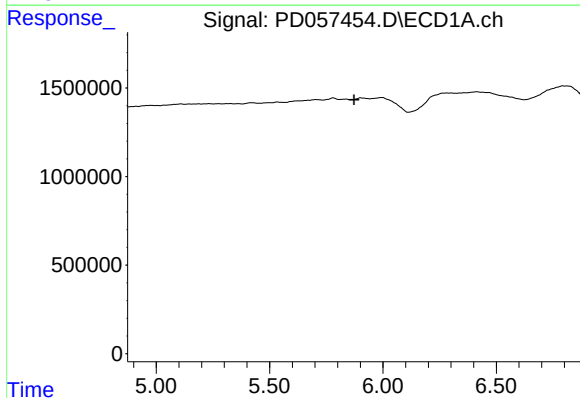


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 5.872 min
Response: 0
Conc: N.D.

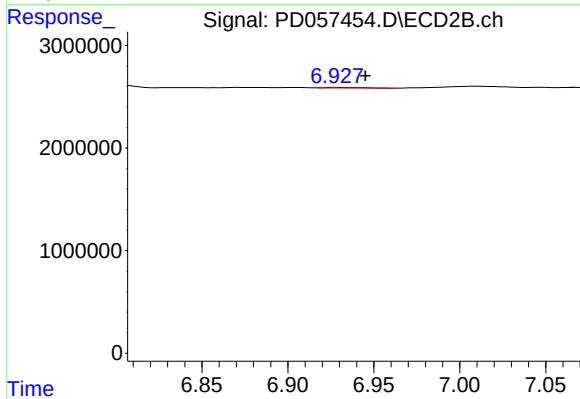

#24 Toxaphene-3


R.T.: 6.928 min
Delta R.T.: -0.017 min
Response: 86535
Conc: 3.57 ng/ml

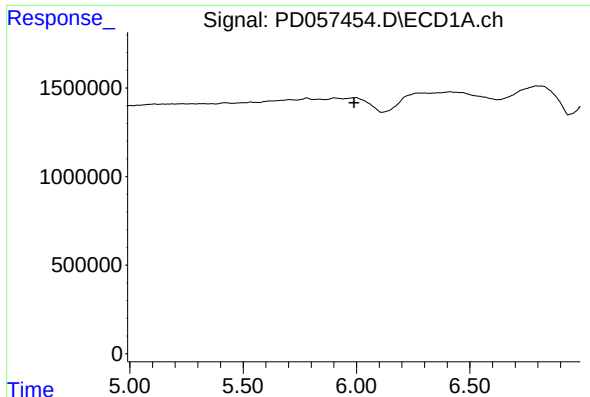

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 5.990 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

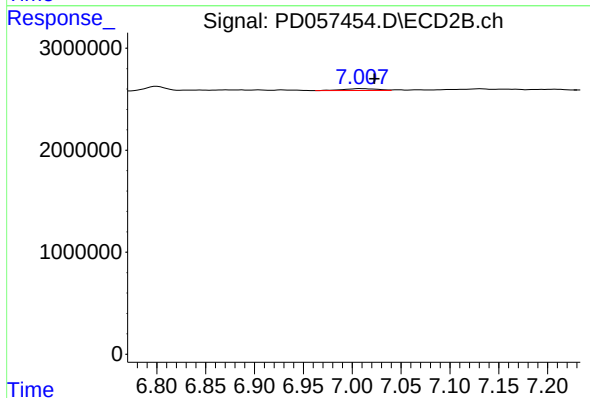


#25 Toxaphene-4

R.T.: 7.009 min
Delta R.T.: -0.014 min
Response: 472120
Conc: 6.69 ng/ml

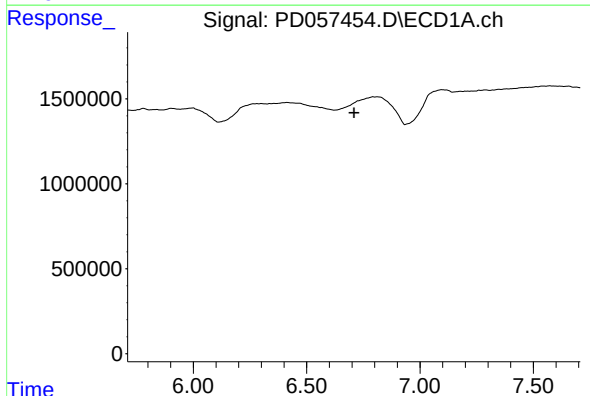


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 6.709 min
Response: 0
Conc: N.D.

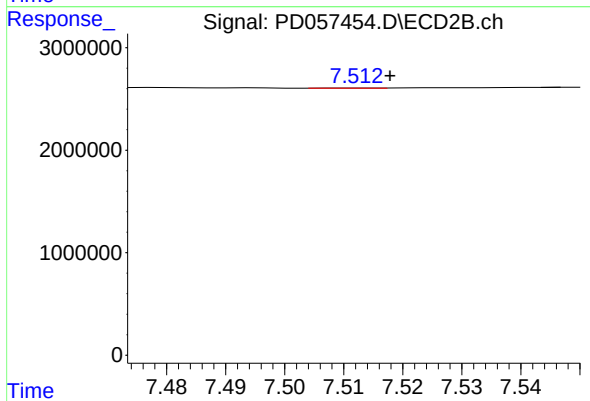

#26 Toxaphene-5


R.T.: 7.513 min
Delta R.T.: -0.005 min
Response: 8121
Conc: 0.25 ng/ml

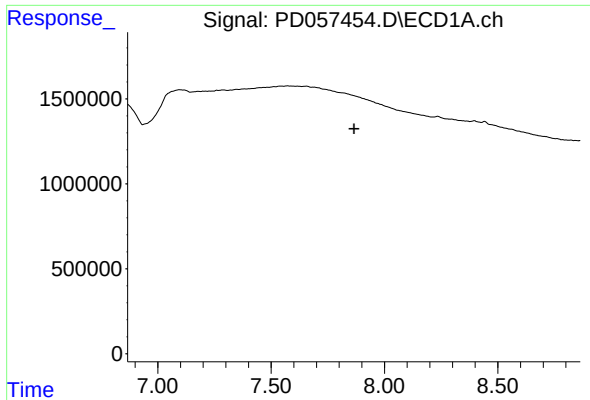

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

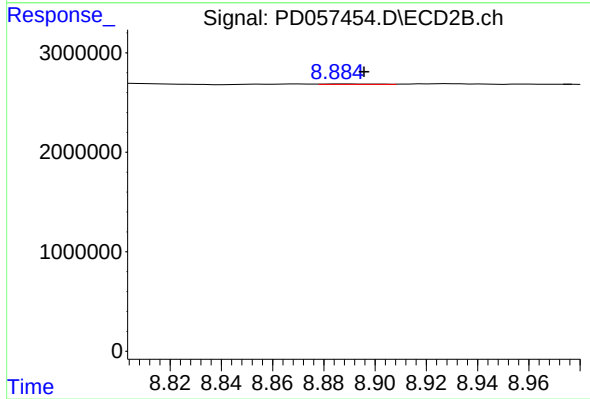

#27 Decachlorobiphenyl

R.T.: 8.886 min
Delta R.T.: -0.010 min
Response: 61807
Conc: N.D.