

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022624\
 Data File : PD081652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2024 15:03
 Operator : AR\AJ
 Sample : P1526-04MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E10A5MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 21:27:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	28496267	50324147	20.844	20.527
27)	SA Decachlor...	9.112	7.929	45734549	60025083	23.705	24.197
Target Compounds							
2)	A alpha-BHC	4.022	3.295	130.2E6	207.7E6	55.747	54.015
3)	MA gamma-BHC...	4.356	3.624	121.7E6	183.9E6	52.688	50.781
4)	MA Heptachlor	4.948	3.965	126.1E6	172.2E6	51.403	48.532
5)	MB Aldrin	5.291	4.245	123.0E6	172.8E6	52.030	51.017
6)	B beta-BHC	4.550	3.919	51349700	76797853	49.412	45.451
7)	B delta-BHC	4.799	4.150	127.8E6	189.5E6	53.962	50.593
8)	B Heptachlo...	5.718	4.746	115.3E6	162.3E6	50.912	50.592
9)	A Endosulfan I	6.105	5.116	109.7E6	152.4E6	52.102	50.914
10)	B trans-Chl...	5.974	4.996	112.5E6	159.8E6	51.380	51.205
11)	B cis-Chlor...	6.054	5.060	113.7E6	160.2E6	50.470	50.021
12)	B 4,4'-DDE	6.225	5.248	226.7E6	313.3E6	105.603	105.958
13)	MA Dieldrin	6.380	5.380	236.0E6	340.2E6	106.276	103.583
14)	MA Endrin	6.610	5.655	198.6E6	303.9E6	105.811	105.768
15)	B Endosulfa...	6.829	5.948	199.0E6	294.7E6	103.092	104.416
16)	A 4,4'-DDD	6.742	5.802	172.2E6	261.1E6	103.671	103.621
17)	MA 4,4'-DDT	7.057	6.053	191.7E6	276.4E6	110.336	107.045
18)	B Endrin al...	6.959	6.128	147.1E6	214.6E6	98.505	99.025
19)	B Endosulfa...	7.193	6.349	183.9E6	276.4E6	100.469	103.017
20)	A Methoxychlor	7.532	6.627	484.7E6	651.3E6	528.431	487.513
21)	B Endrin ke...	7.680	6.856	208.7E6	313.6E6	107.918	104.577

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022624\
Data File : PD081652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2024 15:03
Operator : AR\AJ
Sample : P1526-04MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 21:27:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

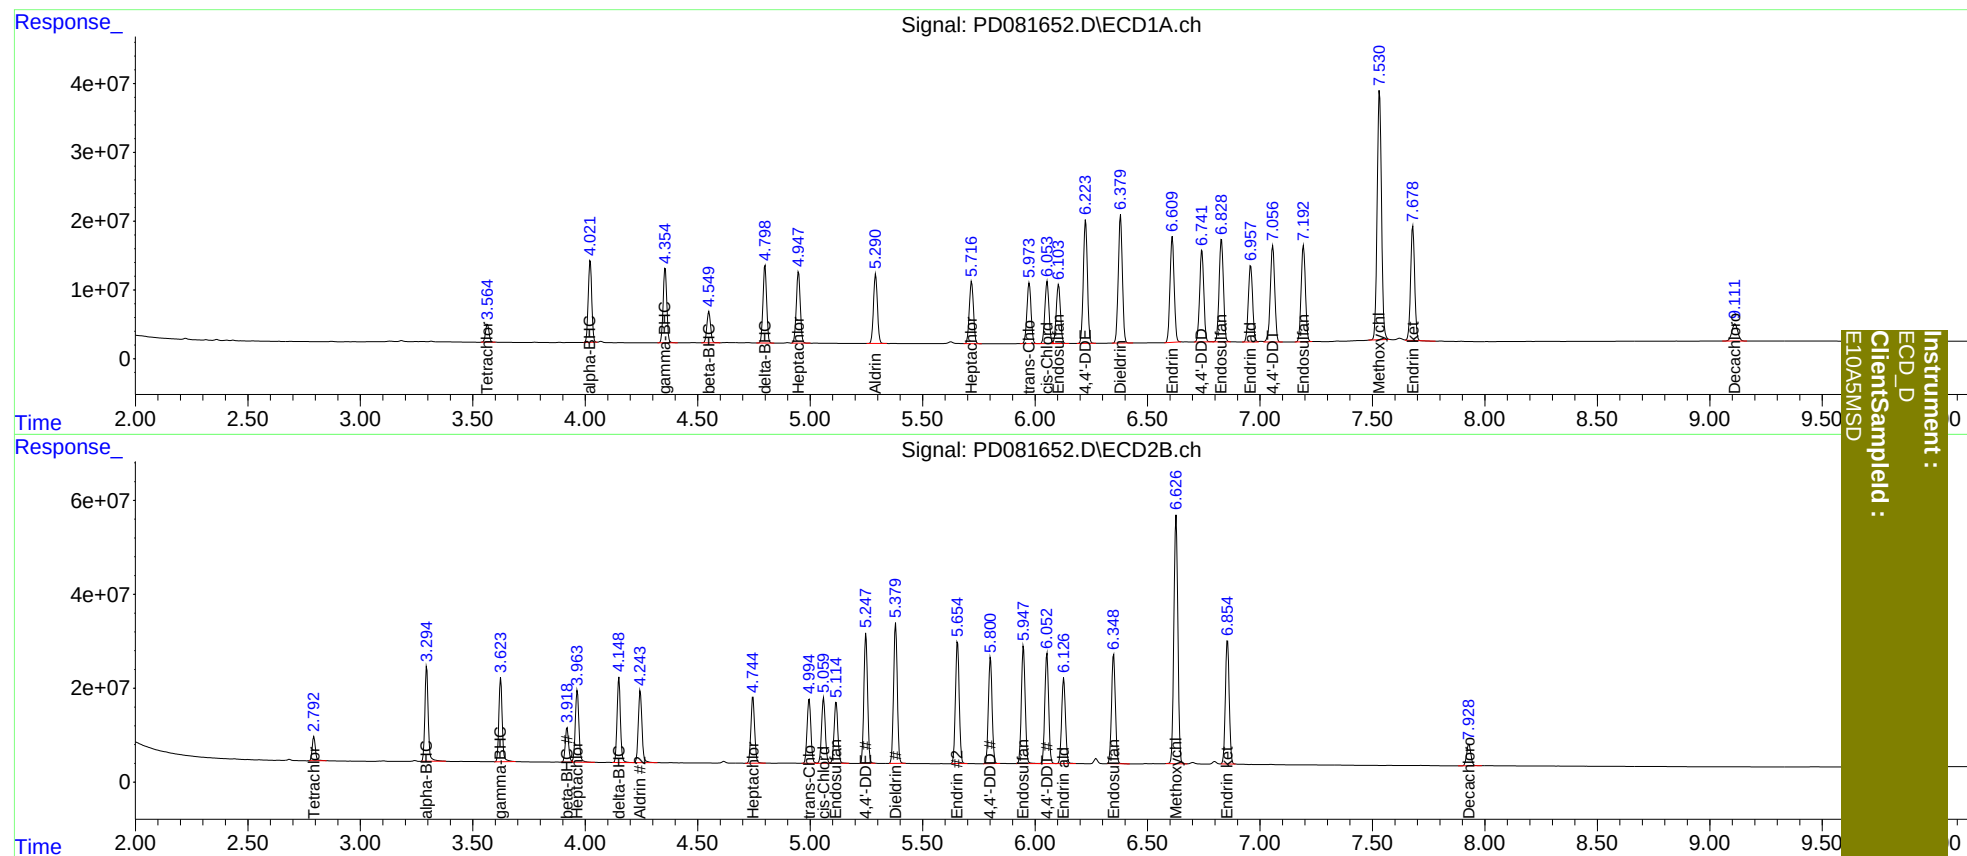

Instrument :
ECD_D
ClientSampled :
E10A5MSD