

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022624\
 Data File : PD081651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2024 14:49
 Operator : AR\AJ
 Sample : P1526-03MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E10A5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 21:27:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.794	28936957	51295961	21.166	20.924
27)	SA Decachlor...	9.112	7.930	45736081	61365467	23.705	24.737
Target Compounds							
2)	A alpha-BHC	4.022	3.295	130.2E6	212.8E6	55.757	55.334
3)	MA gamma-BHC...	4.356	3.624	121.2E6	187.8E6	52.455	51.849
4)	MA Heptachlor	4.948	3.965	126.4E6	176.1E6	51.550	49.651
5)	MB Aldrin	5.292	4.245	123.1E6	176.7E6	52.075	52.156
6)	B beta-BHC	4.550	3.919	51433563	78392153	49.492	46.394
7)	B delta-BHC	4.799	4.150	128.1E6	193.0E6	54.089	51.552
8)	B Heptachlo...	5.718	4.746	115.6E6	166.1E6	51.035	51.756
9)	A Endosulfan I	6.105	5.116	109.8E6	156.3E6	52.157	52.186
10)	B trans-Chl...	5.974	4.996	112.1E6	163.8E6	51.186	52.492
11)	B cis-Chlor...	6.054	5.060	113.9E6	164.2E6	50.558	51.248
12)	B 4,4'-DDE	6.225	5.249	222.1E6	321.8E6	103.454	108.817
13)	MA Dieldrin	6.381	5.380	238.1E6	347.8E6	107.232	105.884
14)	MA Endrin	6.611	5.656	218.5E6	312.1E6	116.416	108.639
15)	B Endosulfa...	6.830	5.948	220.6E6	301.4E6	114.265	106.794
16)	A 4,4'-DDD	6.743	5.802	191.6E6	267.2E6	115.346	106.032
17)	MA 4,4'-DDT	7.057	6.053	215.4E6	282.7E6	123.993	109.493
18)	B Endrin al...	6.959	6.128	162.1E6	218.7E6	108.512	100.927
19)	B Endosulfa...	7.194	6.350	206.7E6	282.8E6	112.903	105.405
20)	A Methoxychlor	7.532	6.628	507.4E6	662.1E6	553.164	495.558
21)	B Endrin ke...	7.680	6.856	216.8E6	319.4E6	112.101	106.522

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022624\
Data File : PD081651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2024 14:49
Operator : AR\AJ
Sample : P1526-03MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 21:27:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

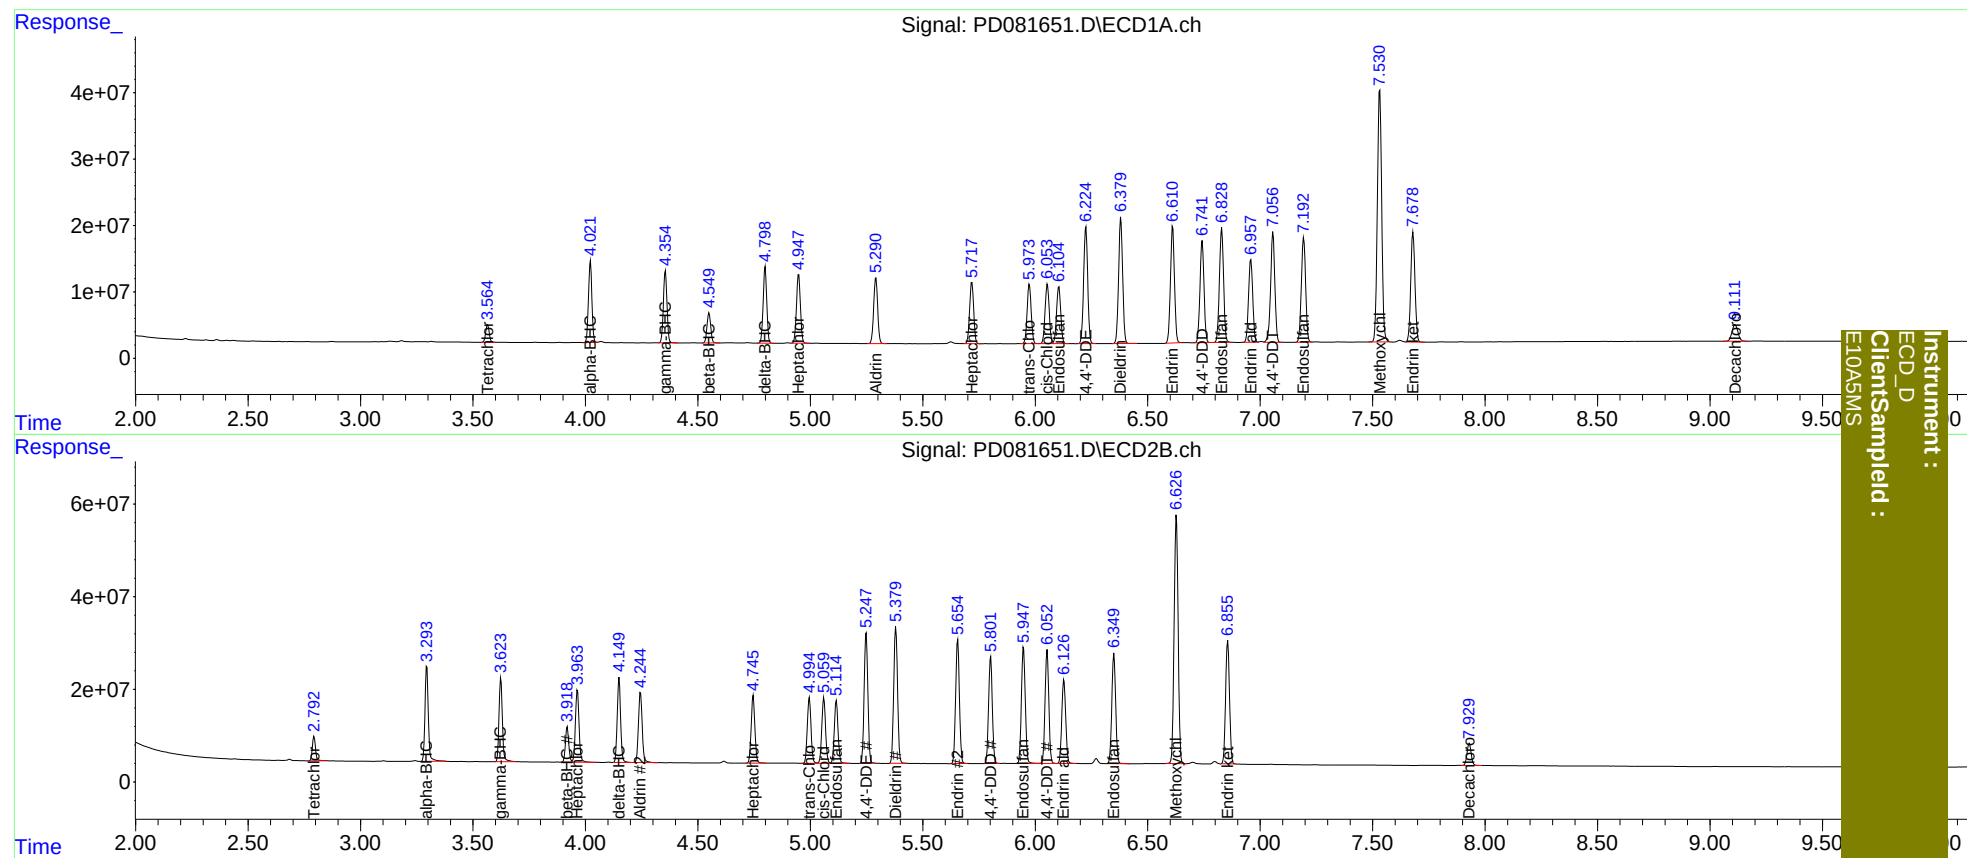

Instrument :
ECD_D
ClientSampled :
E10A5MS