

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022719\
 Data File : PD051423.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Feb 2019 21:43
 Operator : AJ\SJ
 Sample : K1600-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF7Y4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:01:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	25656609	566.1E6	17.854	18.324
27)	SA Decachlor...	7.825	9.158	36409850	574.5E6	30.275	30.303
Target Compounds							
6)	B beta-BHC	0.000	4.938f	0 60442012	N.D.	3.046	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022719\
Data File : PD051423.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2019 21:43
Operator : AJ\SJ
Sample : K1600-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF7Y4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:01:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

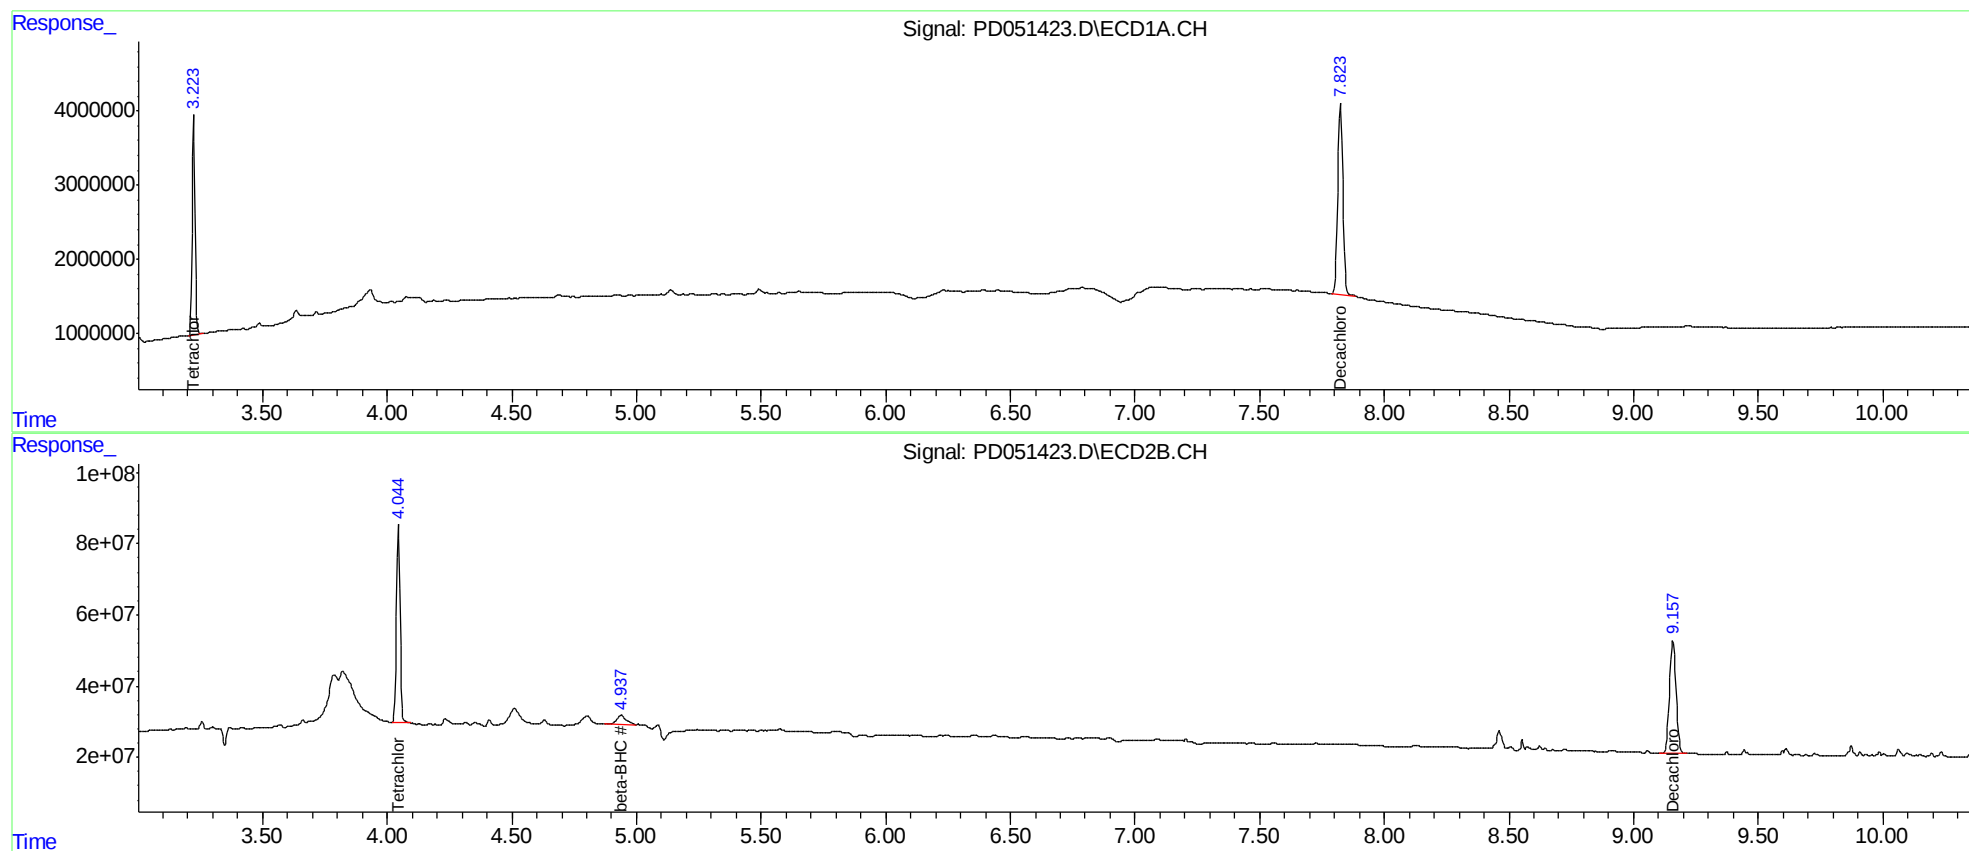


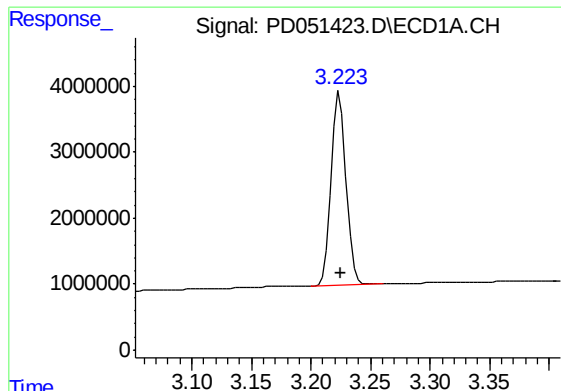

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 25656609
Conc: 17.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF7Y4

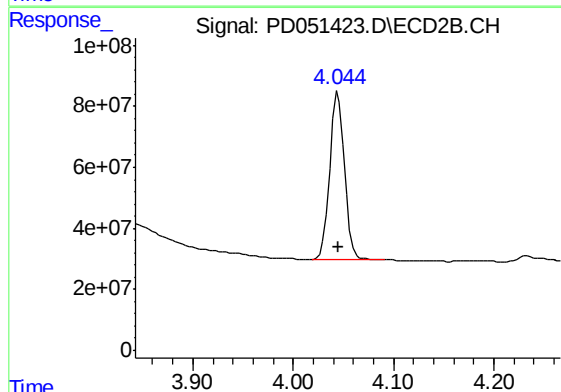


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 566143466
Conc: 18.32 ng/ml

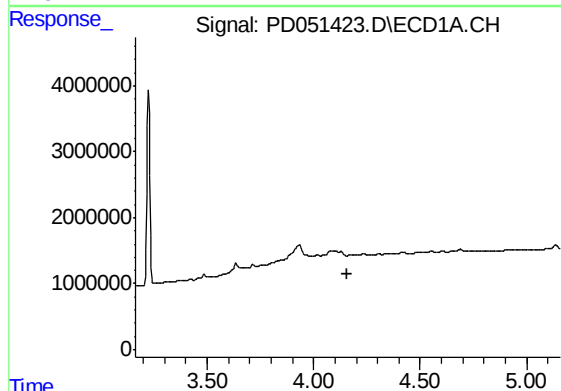


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

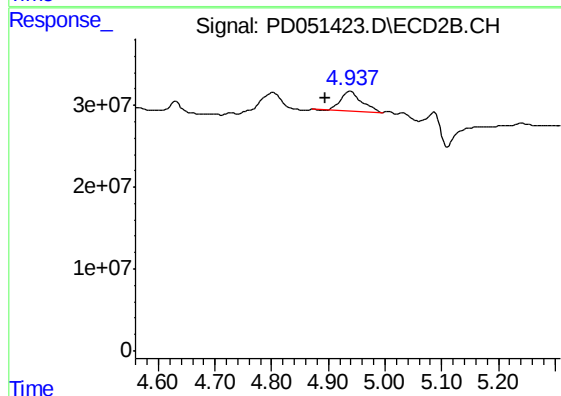

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.045 min
Response: 60442012
Conc: 3.05 ng/ml

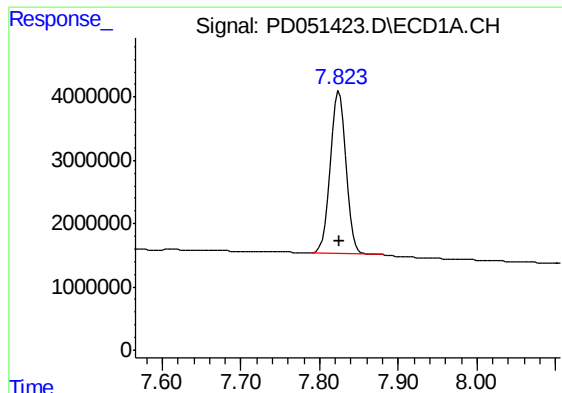

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.001 min
Response: 36409850
Conc: 30.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF7Y4

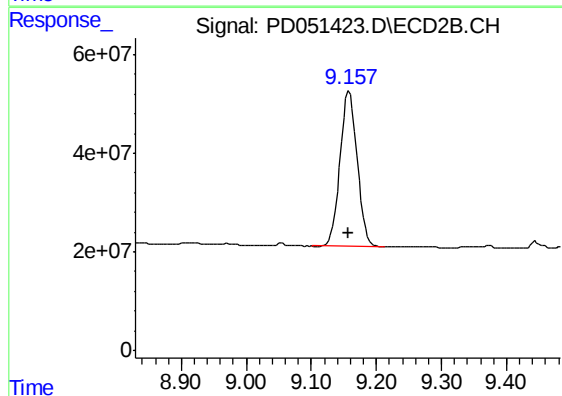

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.001 min
Response: 574473771
Conc: 30.30 ng/ml