

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022724\
 Data File : PD081675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 14:48
 Operator : AR\AJ
 Sample : P1553-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGS91

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/29/2024
 Supervised By : Ankita Jodhani 02/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 21:55:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.793	35851590	63050599	26.224	25.719
27)	SA Decachlor...	9.112	7.929	58432398	77560573	30.286	31.266
Target Compounds							
10)	B trans-Chl...	5.973	4.996	3073794	4218238	1.404	1.352
11)	B cis-Chlor...	6.054	5.059	3701546	1371769	1.643m	0.428m#
13)	MA Dieldrin	6.380	5.378	7842707	11008830	3.532	3.352m
19)	B Endosulfa...	7.186	6.372	2098888	1457453	1.146m	0.543m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022724\
Data File : PD081675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 14:48
Operator : AR\AJ
Sample : P1553-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 21:55:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

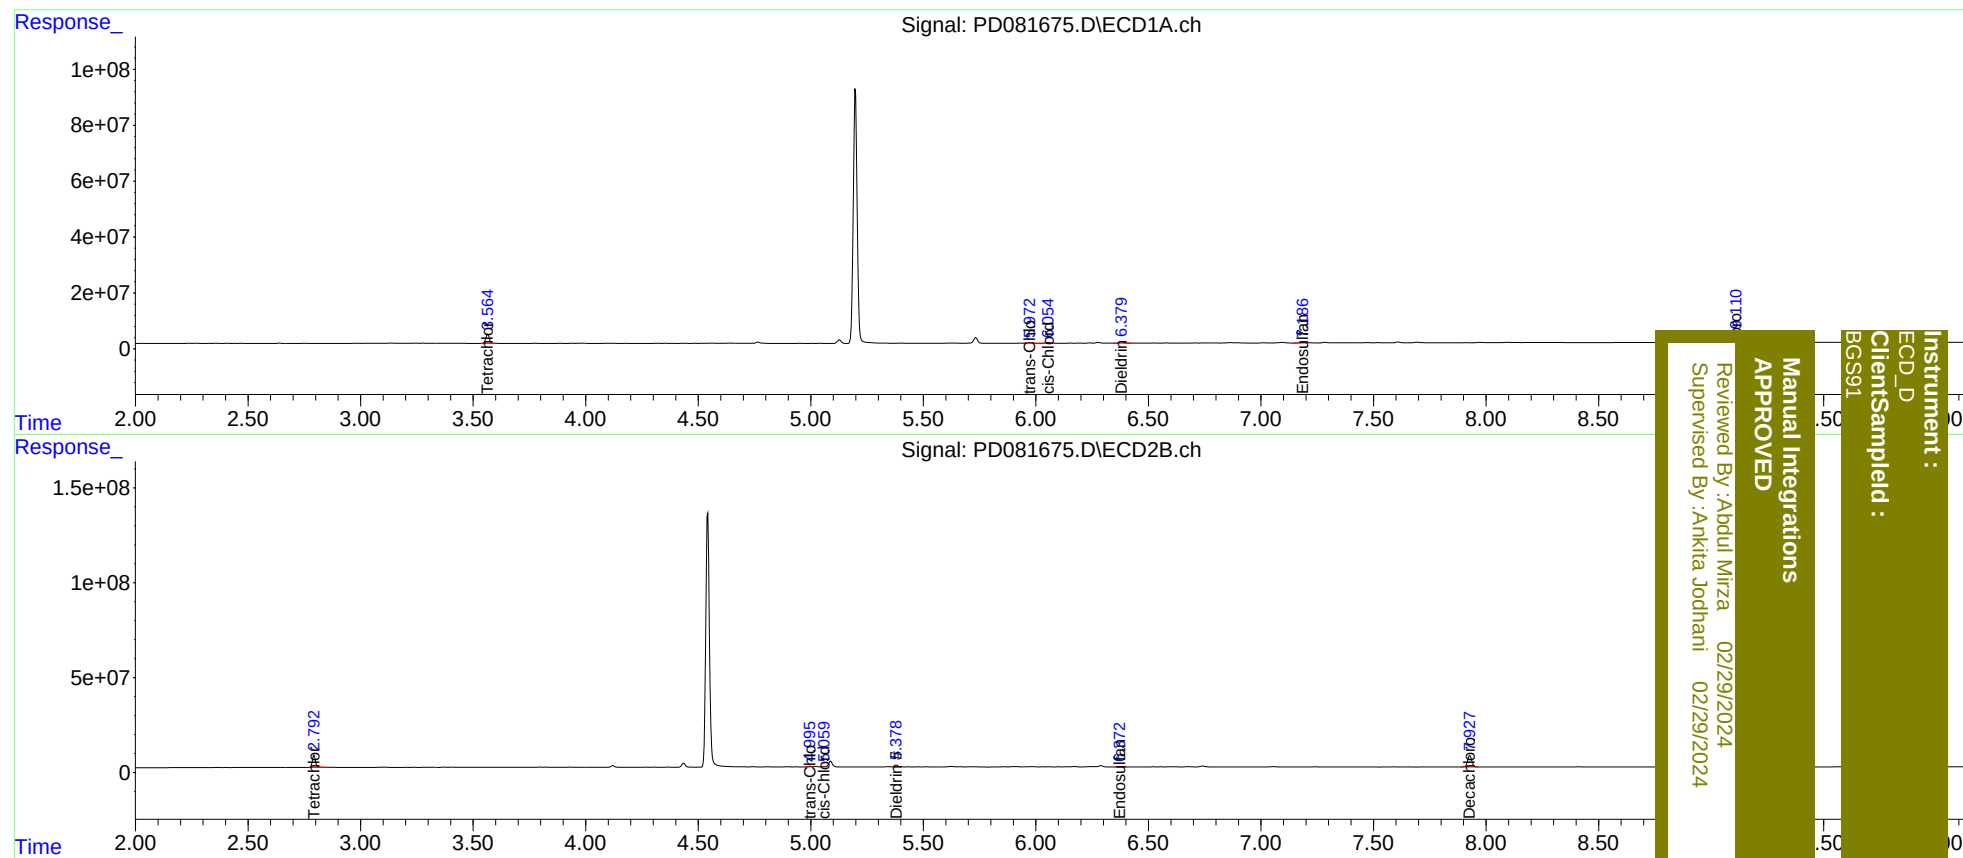

Instrument :
ECD_D
ClientSampled :
BGS91

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/29/2024
Supervised By :Ankita Jodhani 02/29/2024