

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022724\
 Data File : PD081714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 23:55
 Operator : AR\AJ
 Sample : P1554-12MSD
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGS8MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/28/2024
 Supervised By :Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:10:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.793	29430606	52209322	21.527	21.296
27)	SA Decachlor...	9.111	7.929	42891974	59402530	22.231	23.946
Target Compounds							
2)	A alpha-BHC	4.020	3.293	133.7E6	218.3E6	57.250m	56.766m
3)	MA gamma-BHC...	4.355	3.623	123.2E6	196.3E6	53.325	54.208
4)	MA Heptachlor	4.947	3.964	132.1E6	195.5E6	53.851	55.119
5)	MB Aldrin	5.290	4.244	127.3E6	181.0E6	53.831	53.438
6)	B beta-BHC	4.550	3.919	55559070	84542056	53.462	50.034
7)	B delta-BHC	4.799	4.150	129.7E6	201.1E6	54.745	53.713
8)	B Heptachlo...	5.718	4.746	114.9E6	172.6E6	50.743	53.802
9)	A Endosulfan I	6.105	5.115	109.0E6	162.7E6	51.746	54.345
10)	B trans-Chl...	5.974	4.995	113.7E6	176.2E6	51.933	56.457
11)	B cis-Chlor...	6.054	5.059	115.1E6	173.4E6	51.097	54.133
12)	B 4,4'-DDE	6.225	5.248	224.8E6	330.2E6	104.731	111.652
13)	MA Dieldrin	6.380	5.380	266.4E6	393.2E6	119.964	119.702
14)	MA Endrin	6.610	5.653	200.2E6	328.2E6	106.694	114.224m
15)	B Endosulfa...	6.828	5.946	190.9E6	287.7E6	98.906	101.913m
16)	A 4,4'-DDD	6.742	5.801	177.3E6	266.7E6	106.772	105.825
17)	MA 4,4'-DDT	7.057	6.052	184.1E6	299.3E6	105.990	115.910
18)	B Endrin al...	6.959	6.127	137.9E6	213.5E6	92.334	98.533
19)	B Endosulfa...	7.193	6.349	213.6E6	297.1E6	116.666	110.764
20)	A Methoxychlor	7.531	6.627	491.7E6	697.2E6	536.074	521.855
21)	B Endrin ke...	7.679	6.855	214.7E6	321.8E6	111.031	107.324

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022724\
Data File : PD081714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 23:55
Operator : AR\AJ
Sample : P1554-12MSD
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:10:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

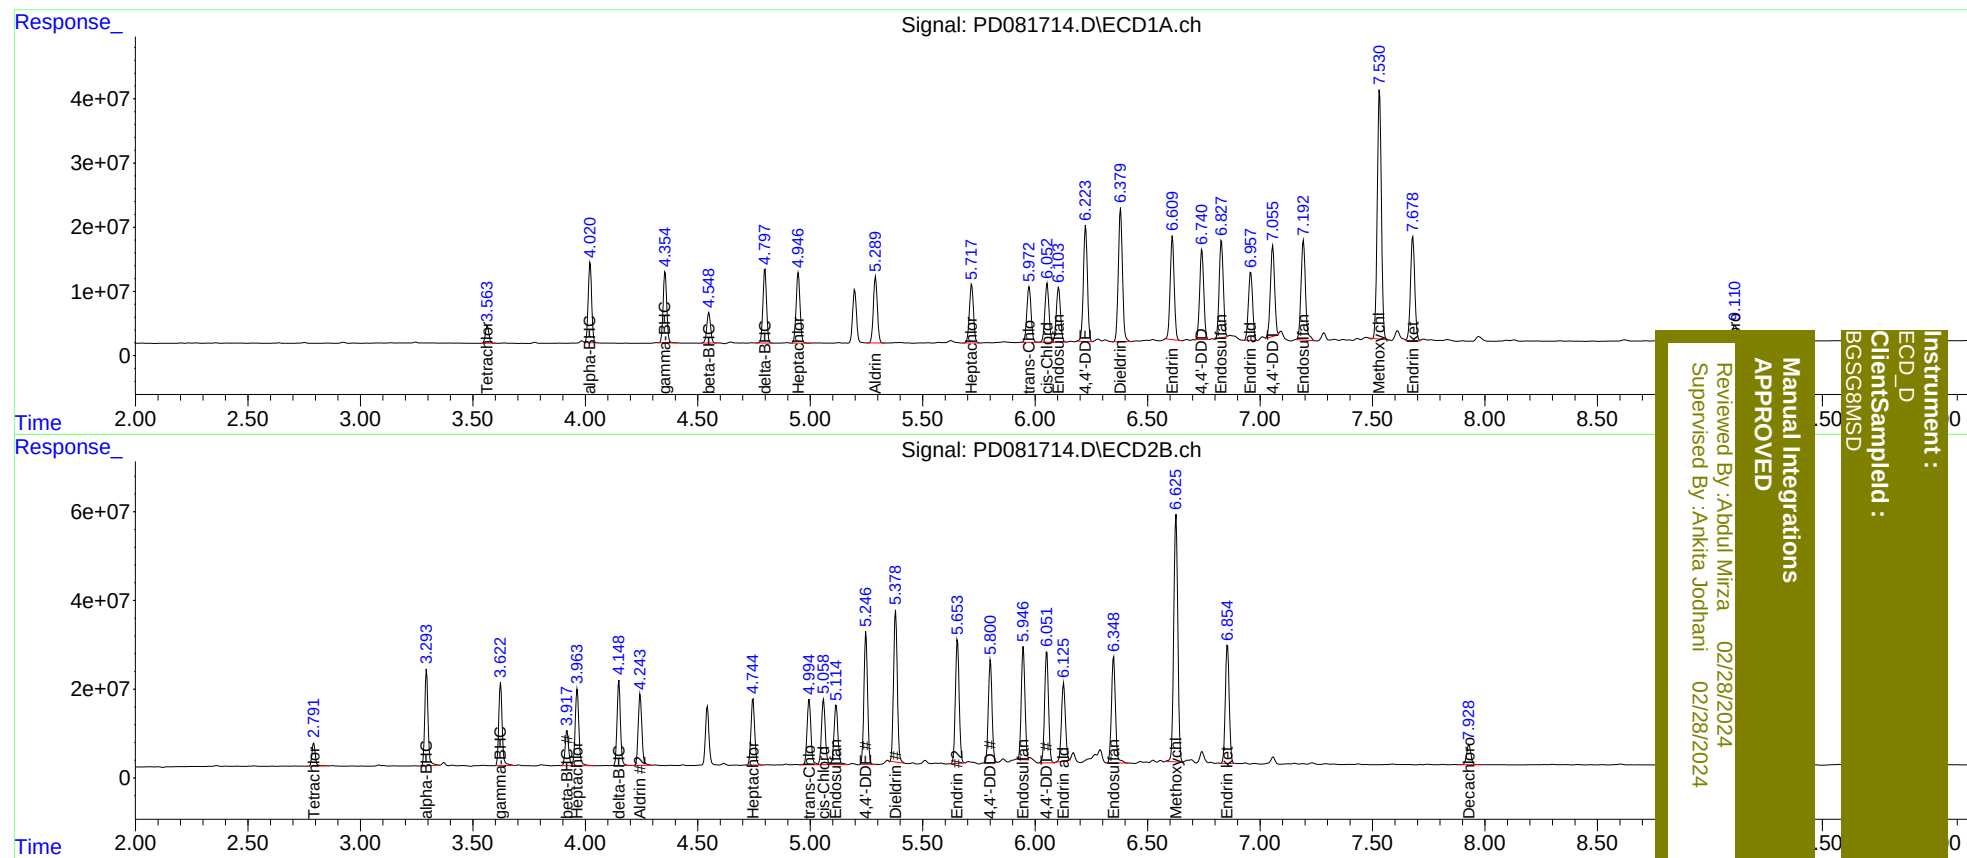

Instrument :
ECD_D
ClientSampled :
BGSG8MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/28/2024
Supervised By :Ankita Jodhani 02/28/2024