

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022819\
 Data File : PD051445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Feb 2019 19:05
 Operator : AJ\SJ
 Sample : K1625-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:31:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	28833954	599.9E6	20.065	19.418
27)	SA Decachlor...	7.823	9.156	48046096	695.3E6	39.950	36.676
Target Compounds							
6)	B beta-BHC	0.000	4.939f	0	31265506	N.D.	1.576
8)	B Heptachlo...	0.000	5.950	0	217.4E6	N.D.	6.072
9)	A Endosulfan I	5.151	0.000	8391696	0	4.107	N.D. #
11)	B cis-Chlor...	5.151	0.000	8391696	0	3.926	N.D. #
16)	A 4,4'-DDD	0.000	6.868	0	32094668	N.D.	1.226

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022819\
Data File : PD051445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Feb 2019 19:05
Operator : AJ\SJ
Sample : K1625-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:31:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

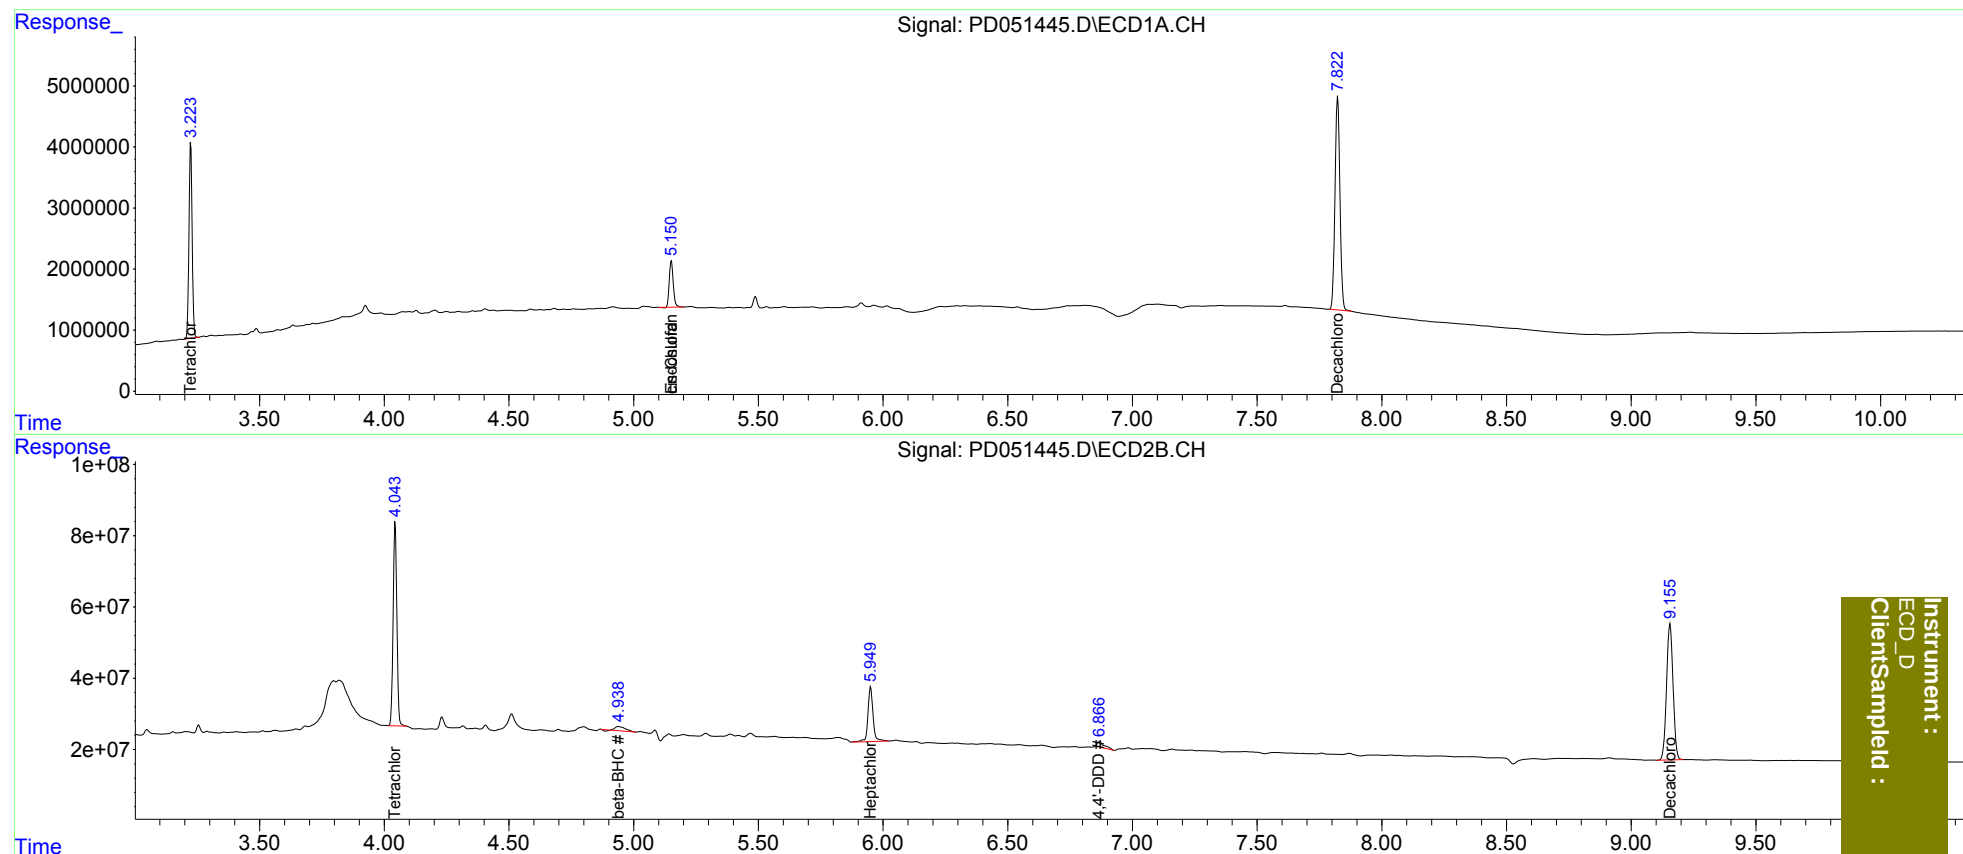


Instrument :
ECD_D
ClientSampleId :

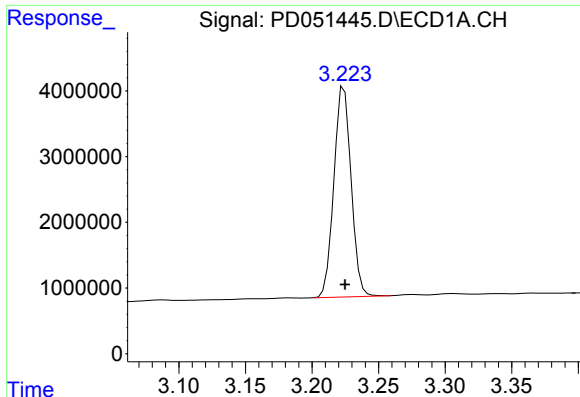

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 28833954
Conc: 20.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

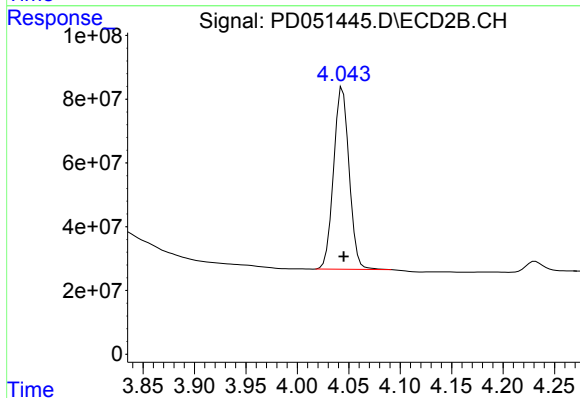


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 599932375
Conc: 19.42 ng/ml

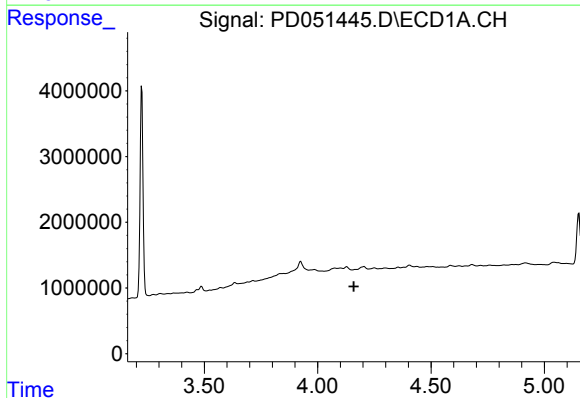


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

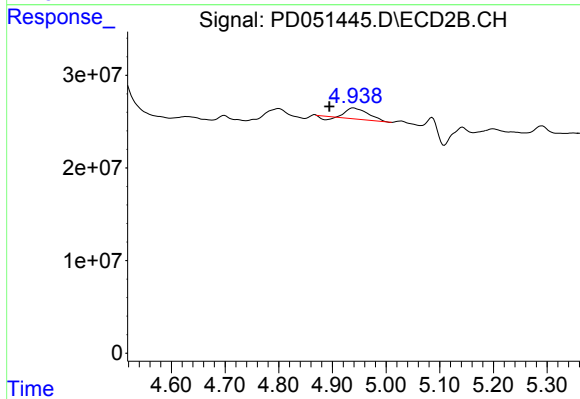

#6 beta-BHC


R.T.: 4.939 min
Delta R.T.: 0.045 min
Response: 31265506
Conc: 1.58 ng/ml

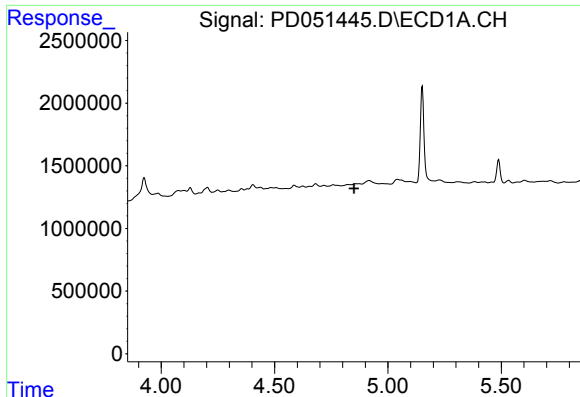

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

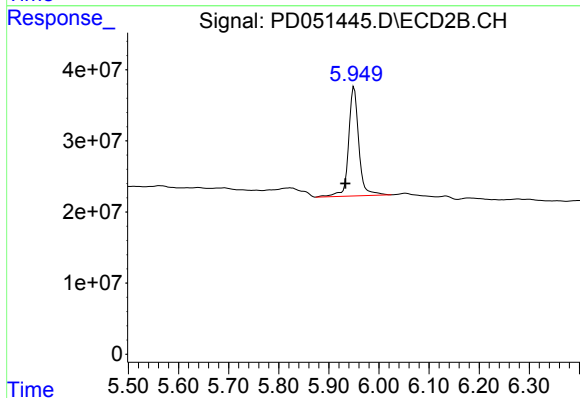


#8 Heptachlor epoxide

R.T.: 5.950 min
Delta R.T.: 0.017 min
Response: 217417138
Conc: 6.07 ng/ml

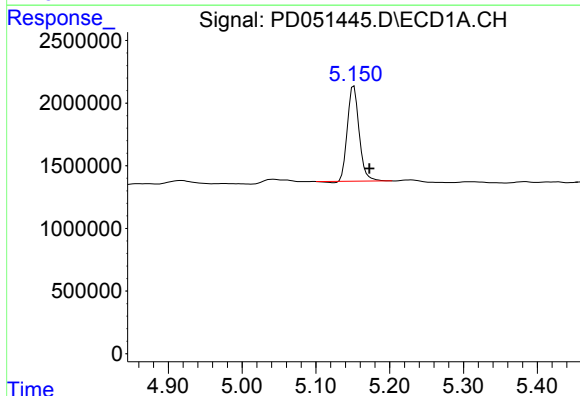


#9 Endosulfan I

R.T.: 5.151 min
Delta R.T.: -0.021 min
Response: 8391696
Conc: 4.11 ng/ml

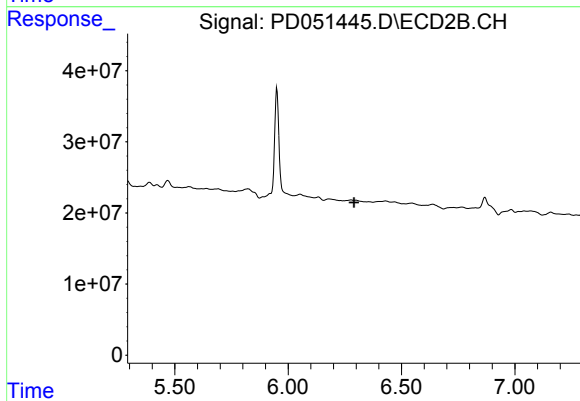

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.292 min
Response: 0
Conc: N.D.

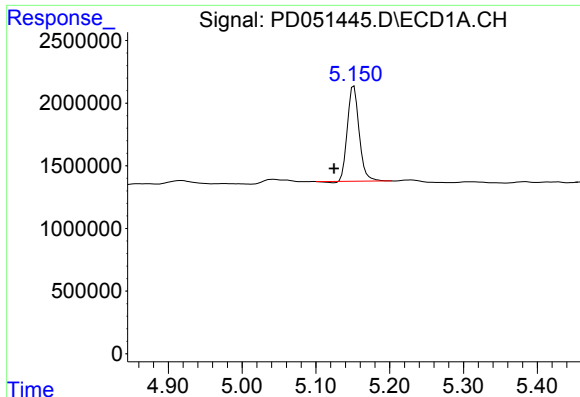

#11 cis-Chlordane


R.T.: 5.151 min
Delta R.T.: 0.027 min
Response: 8391696
Conc: 3.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

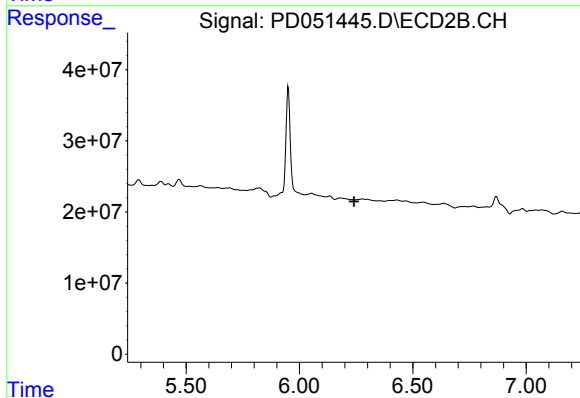


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

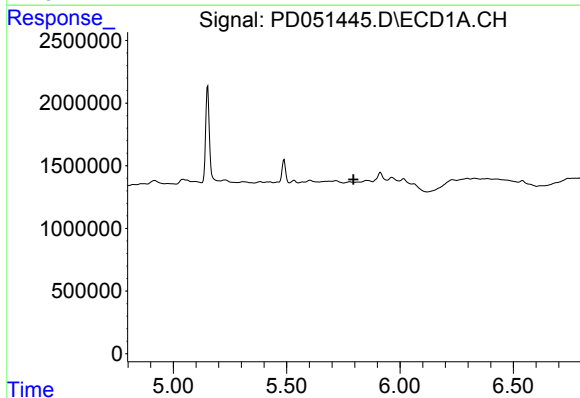


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.795 min
Response: 0
Conc: N.D.

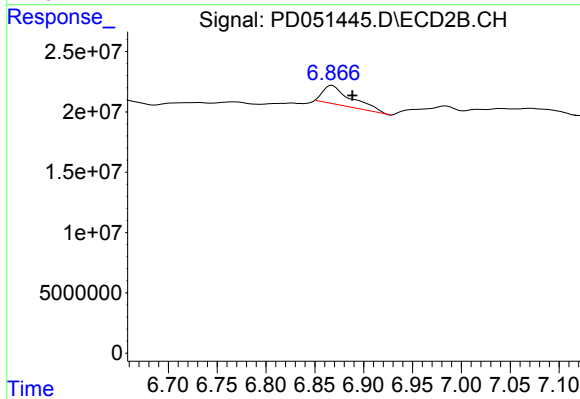

#16 4,4'-DDD


R.T.: 6.868 min
Delta R.T.: -0.021 min
Response: 32094668
Conc: 1.23 ng/ml

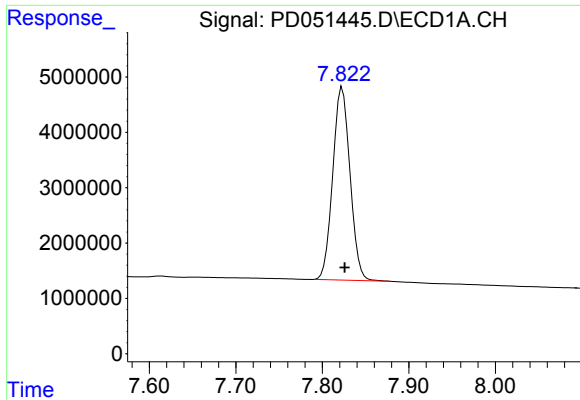

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 48046096
Conc: 39.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

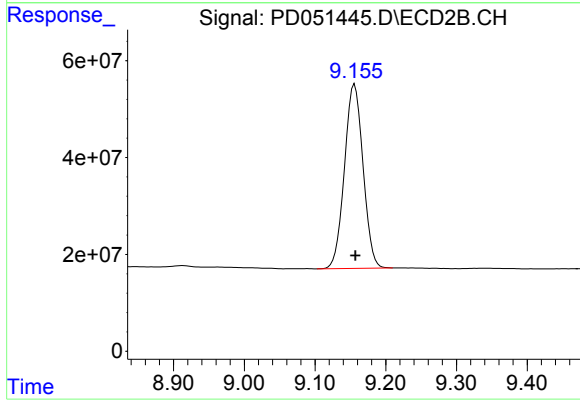

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.001 min
Response: 695276519
Conc: 36.68 ng/ml