

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022820\
 Data File : PD057469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 15:59
 Operator : AJ\MA
 Sample : L1708-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 05:51:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 24 16:58:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.897	17339557	42575874	20.184	20.998
2)	SA Decachlor...	7.870	8.902	25533991	56387188	28.096	25.731
Target Compounds							
3)	MA gamma-BHC...	3.934	4.526f	3636859	6404286	3.068	1.949 #
19)	B Endosulfa...	6.284f	0.000	955804	0	1.027	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022820\
Data File : PD057469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 15:59
Operator : AJ\MA
Sample : L1708-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 05:51:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022120CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 24 16:58:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

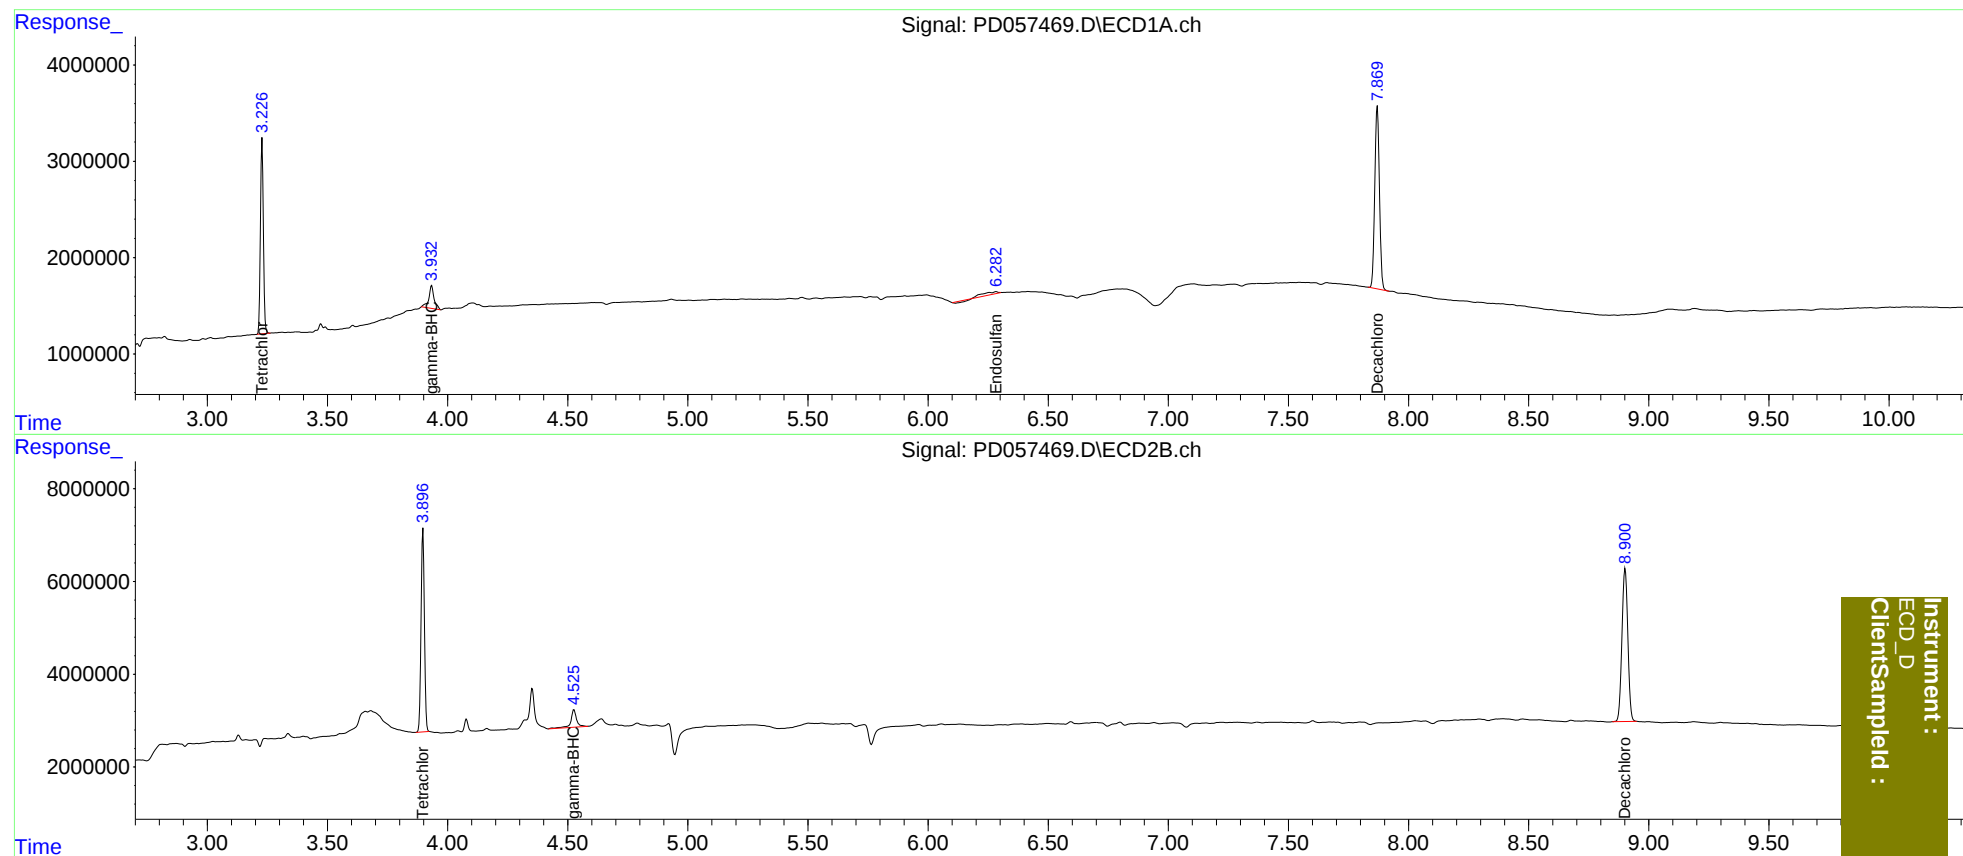


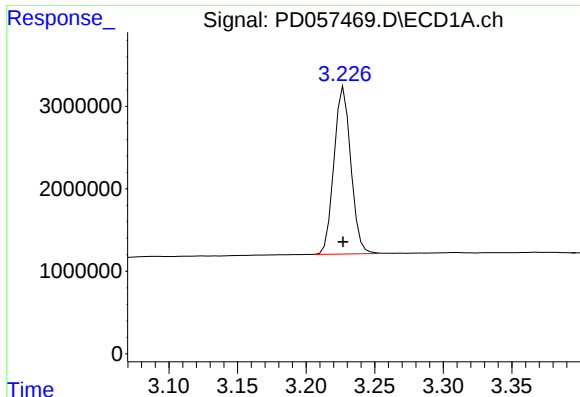

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 17339557
Conc: 20.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

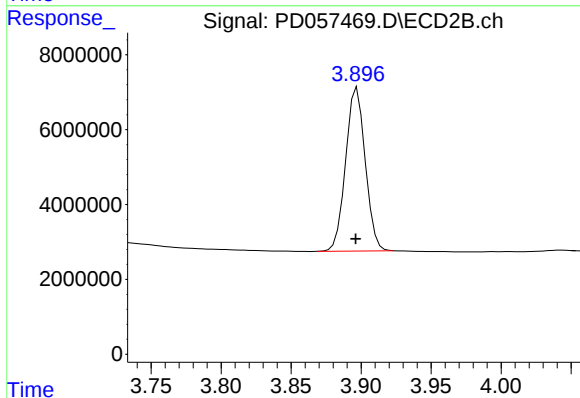


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.001 min
Response: 42575874
Conc: 21.00 ng/ml

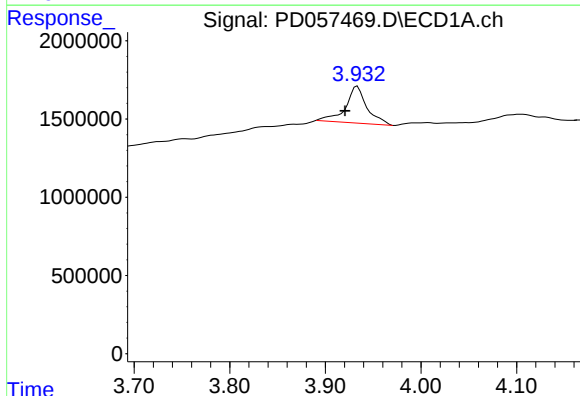


#3 gamma-BHC (Lindane)

R.T.: 3.934 min
Delta R.T.: 0.013 min
Response: 3636859
Conc: 3.07 ng/ml

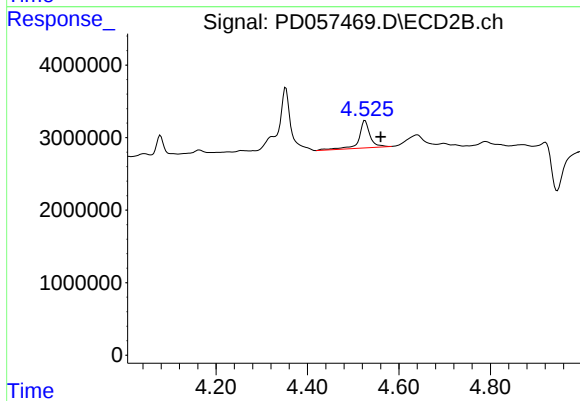

#3 gamma-BHC (Lindane)


R.T.: 4.526 min
Delta R.T.: -0.034 min
Response: 6404286
Conc: 1.95 ng/ml

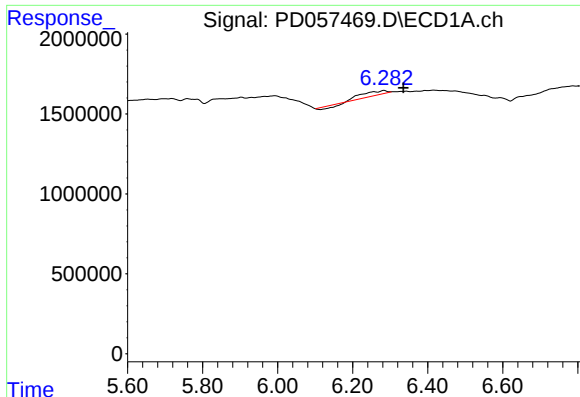

#19 Endosulfan Sulfate


R.T.: 6.284 min
Delta R.T.: -0.051 min
Response: 955804
Conc: 1.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

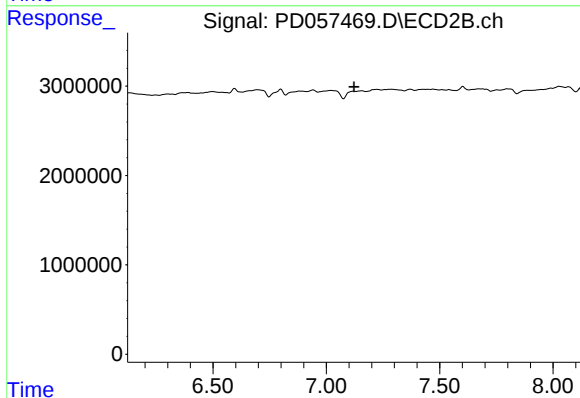


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.122 min
Response: 0
Conc: N.D.

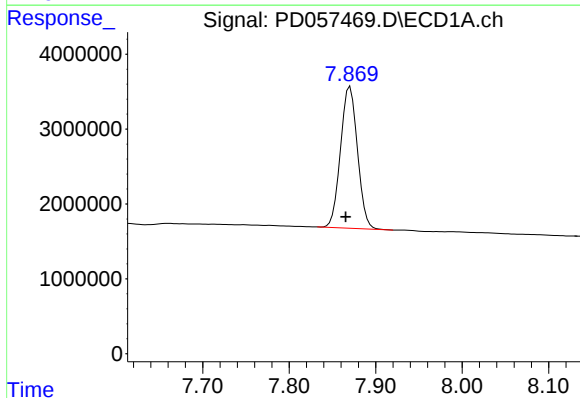

#27 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.005 min
Response: 25533991
Conc: 28.10 ng/ml

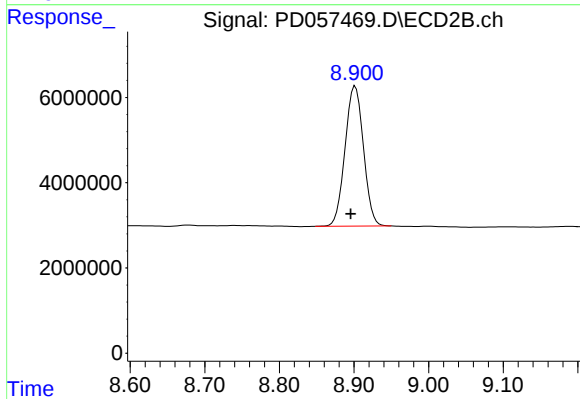

#27 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.006 min
Response: 56387188
Conc: 25.73 ng/ml