

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022824\
 Data File : PD081761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2024 21:49
 Operator : AR\AJ
 Sample : P1556-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRK0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/01/2024
 Supervised By : Ankita Jodhani 03/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 05:07:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.792	20581593	39137063	15.054	15.964
27)	SA Decachlor...	9.114	7.929	31784103	45127870	16.474	18.192
Target Compounds							
5)	MB Aldrin	5.291	4.242	1325936	1965674	0.561m	0.580m
10)	B trans-Chl...	5.972	4.994	1508803	3197713	0.689m	1.025m#
13)	MA Dieldrin	6.379	5.377	5862311	10001542	2.640m	3.045m
19)	B Endosulfa...	7.187	6.383	6848802	3906742	3.741m	1.456m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022824\
Data File : PD081761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2024 21:49
Operator : AR\AJ
Sample : P1556-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 05:07:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

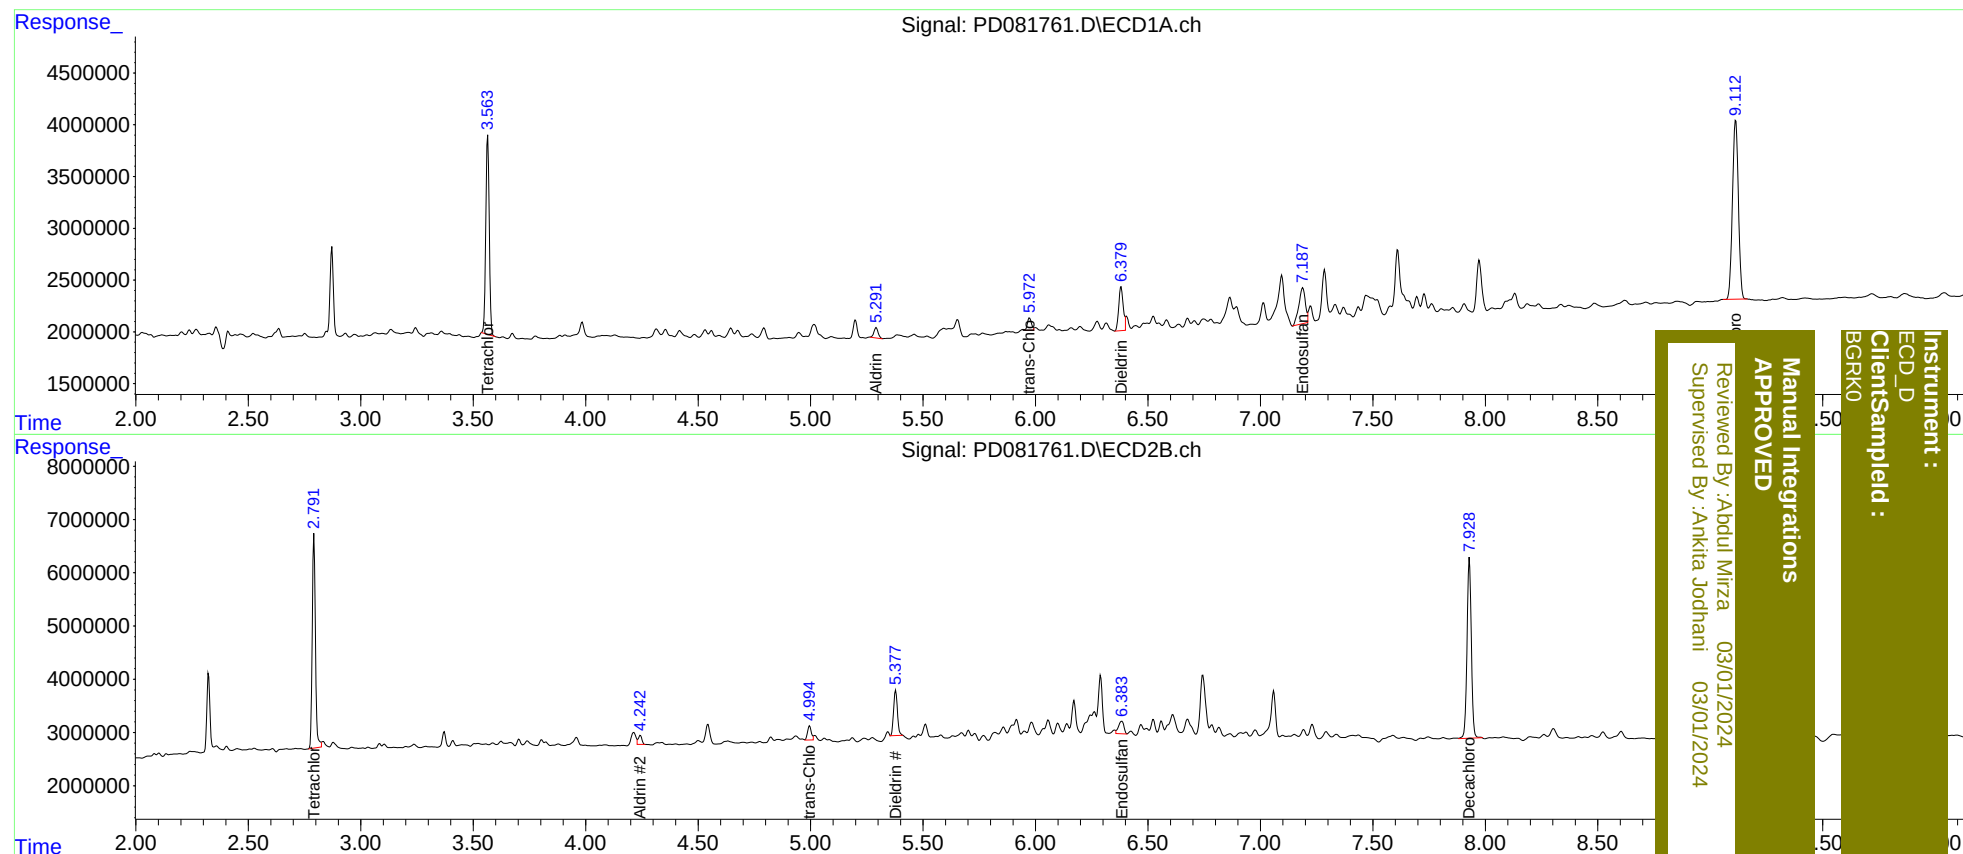

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/01/2024
Supervised By: Ankita Jodhani 03/01/2024

Instrument :
ECD_D
ClientSampled :
BGRKO