

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022924\
 Data File : PD081817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Feb 2024 17:34
 Operator : AR\AJ
 Sample : P1597-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGST7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/01/2024
 Supervised By :Ankita Jodhani 03/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 22:10:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.792	15917309	33035602	11.643	13.475
27)	SA Decachlor...	9.107	7.925	27196766	39501387	14.096	15.924m
Target Compounds							
10)	B trans-Chl...	5.971	4.993	751816	1990344	0.343m	0.638m#
11)	B cis-Chlor...	6.057	5.058	1874763	960885	0.832m	0.300m#
13)	MA Dieldrin	6.377	5.376	5247509	9681721	2.363m	2.948m
19)	B Endosulfa...	7.187	6.374	3774323	1886907	2.062m	0.703m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022924\
Data File : PD081817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Feb 2024 17:34
Operator : AR\AJ
Sample : P1597-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 22:10:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

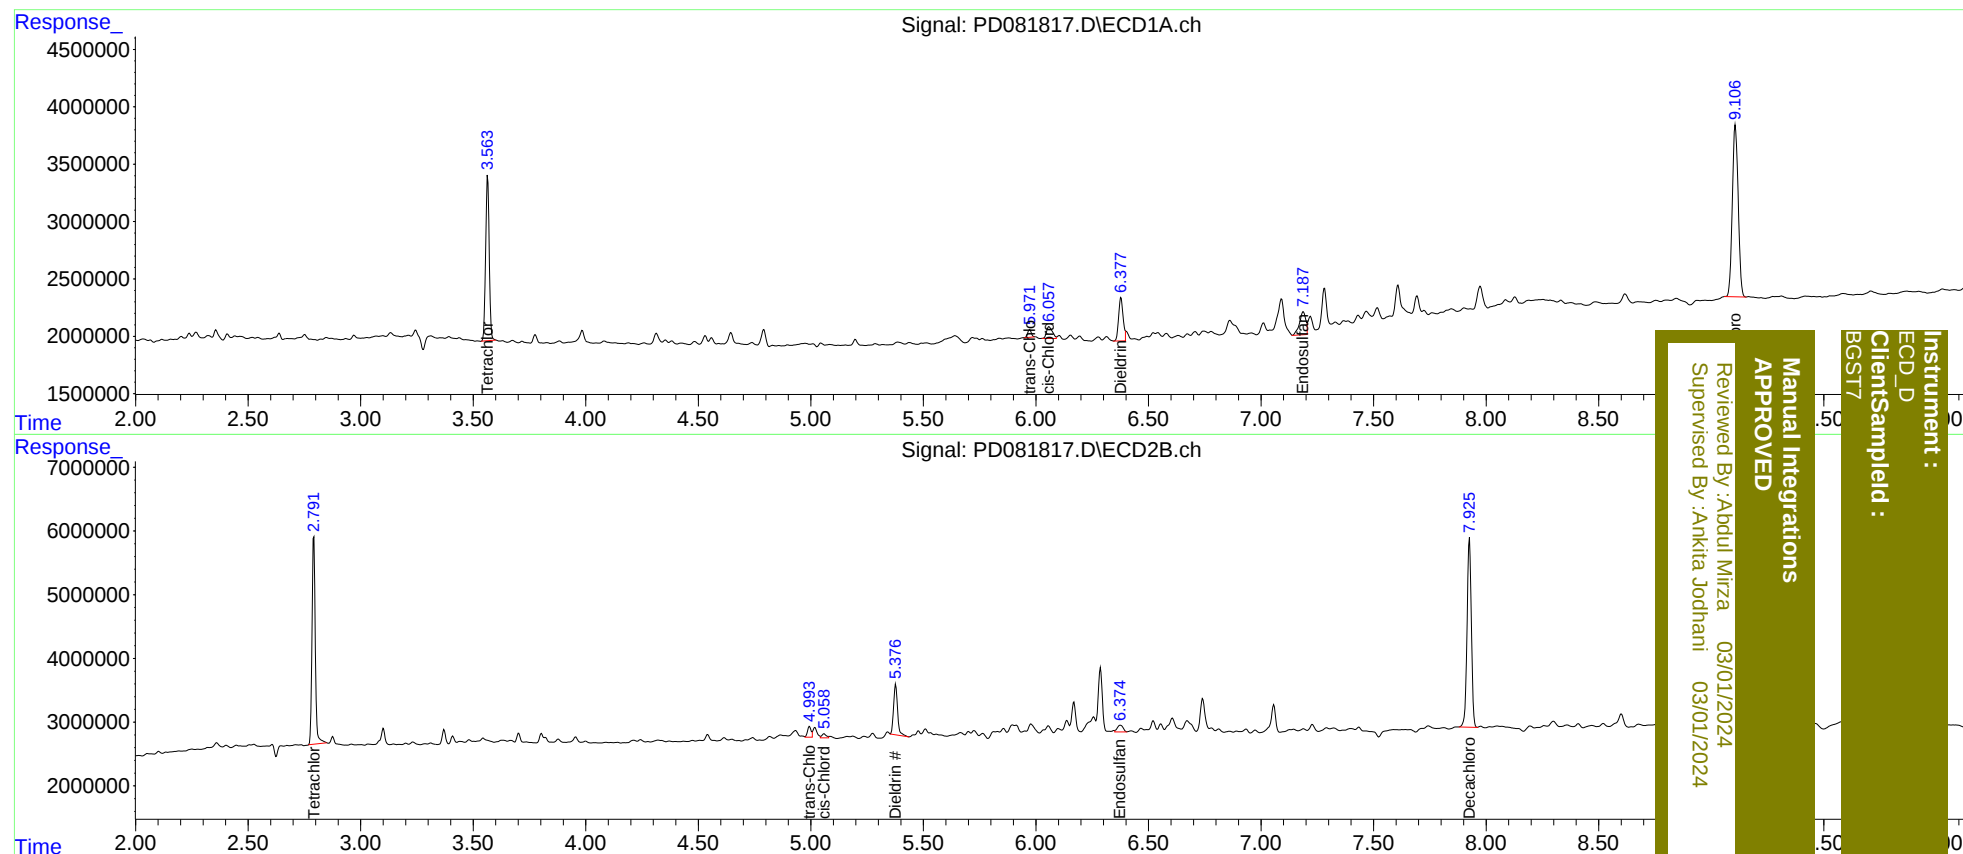

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 03/01/2024
Supervised By: Ankita Jodhani 03/01/2024

Instrument :
ECD_D
Client Sampled :
BGST7