

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022924\
 Data File : PD081829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Feb 2024 20:43
 Operator : AR\AJ
 Sample : P1597-14MS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGR68MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/01/2024
 Supervised By :Ankita Jodhani 03/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 22:13:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.793	12258586	23173266	8.967	9.452
27)	SA Decachlor...	9.107	7.924	19260425	32806155	9.983m	13.225m#
Target Compounds							
2)	A alpha-BHC	4.021	3.294	79716843	140.9E6	34.136	36.640
3)	MA gamma-BHC...	4.353	3.623	74671144	125.6E6	32.321m	34.667
4)	MA Heptachlor	4.947	3.963	80025063	125.7E6	32.630	35.429
5)	MB Aldrin	5.290	4.243	77816093	123.1E6	32.910	36.333
6)	B beta-BHC	4.549	3.918	32440450	52980058	31.216	31.355
7)	B delta-BHC	4.798	4.149	82404381	128.5E6	34.793	34.310
8)	B Heptachlo...	5.716	4.744	70388310	111.1E6	31.079	34.622
9)	A Endosulfan I	6.103	5.114	67751248	104.0E6	32.176	34.724
10)	B trans-Chl...	5.973	4.994	67883023	113.6E6	31.006	36.403
11)	B cis-Chlor...	6.052	5.058	70614218	112.2E6	31.352	35.038
12)	B 4,4'-DDE	6.223	5.246	141.7E6	214.0E6	66.014	72.353
13)	MA Dieldrin	6.378	5.378	165.2E6	249.8E6	74.384	76.045
14)	MA Endrin	6.609	5.652	133.7E6	204.2E6	71.218	71.078m
15)	B Endosulfa...	6.828	5.946	137.3E6	209.3E6	71.100	74.156
16)	A 4,4'-DDD	6.741	5.800	121.1E6	178.3E6	72.925	70.742
17)	MA 4,4'-DDT	7.056	6.051	125.3E6	187.6E6	72.115	72.637
18)	B Endrin al...	6.957	6.125	96015162	138.8E6	64.275	64.041
19)	B Endosulfa...	7.192	6.347	130.5E6	181.1E6	71.259	67.489
20)	A Methoxychlor	7.530	6.625	297.3E6	424.1E6	324.141	317.444
21)	B Endrin ke...	7.678	6.853	137.1E6	217.9E6	70.887	72.669

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022924\
Data File : PD081829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Feb 2024 20:43
Operator : AR\AJ
Sample : P1597-14MS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 22:13:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

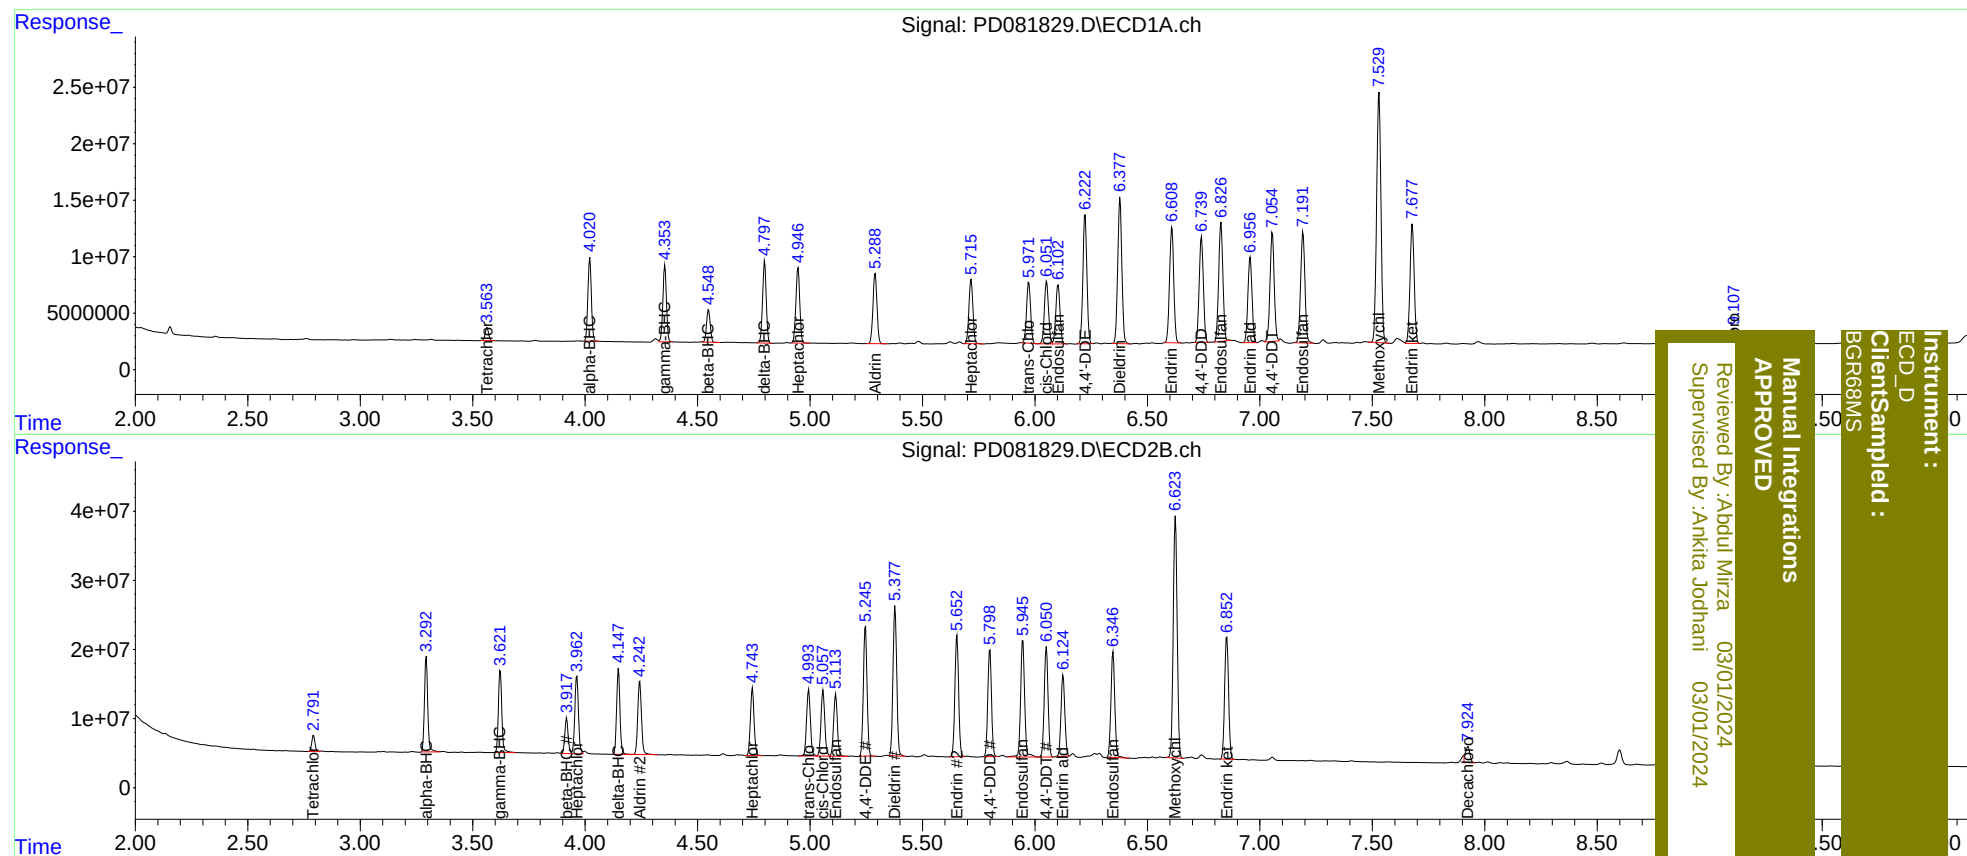

Instrument :
ECD_D
ClientSampled :
BGR68MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 03/01/2024
Supervised By: Ankita Jodhani 03/01/2024