

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022924\
 Data File : PD081830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Feb 2024 20:56
 Operator : AR\AJ
 Sample : P1597-15MSD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGR68MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/01/2024
 Supervised By : Ankita Jodhani 03/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 22:14:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.792	12967339	22757941	9.485	9.283
27)	SA Decachlor...	9.106	7.925	19764560	33597202	10.244m	13.543m#
Target Compounds							
2)	A alpha-BHC	4.021	3.293	84752605	139.9E6	36.292	36.389
3)	MA gamma-BHC...	4.353	3.623	79036600	124.6E6	34.210m	34.410
4)	MA Heptachlor	4.946	3.962	84531812	124.3E6	34.467	35.037
5)	MB Aldrin	5.290	4.242	82307165	122.1E6	34.809	36.034
6)	B beta-BHC	4.549	3.918	33901146	52383646	32.622	31.002
7)	B delta-BHC	4.797	4.148	86302652	127.4E6	36.438	34.014
8)	B Heptachlo...	5.716	4.744	74382067	110.4E6	32.842	34.418
9)	A Endosulfan I	6.103	5.114	71239338	103.5E6	33.833	34.557
10)	B trans-Chl...	5.972	4.994	71605834	112.8E6	32.706	36.150
11)	B cis-Chlor...	6.052	5.058	73801192	111.4E6	32.767	34.778
12)	B 4,4'-DDE	6.223	5.246	144.9E6	210.7E6	67.518	71.256
13)	MA Dieldrin	6.378	5.378	163.0E6	247.7E6	73.412	75.422
14)	MA Endrin	6.608	5.652	124.9E6	202.4E6	66.558	70.453m
15)	B Endosulfa...	6.827	5.946	129.2E6	207.3E6	66.905	73.456
16)	A 4,4'-DDD	6.740	5.800	113.2E6	177.0E6	68.136	70.237
17)	MA 4,4'-DDT	7.055	6.051	118.4E6	186.0E6	68.142	72.024
18)	B Endrin al...	6.957	6.125	91083199	138.7E6	60.974	63.994
19)	B Endosulfa...	7.191	6.347	124.8E6	181.2E6	68.146	67.530
20)	A Methoxychlor	7.530	6.625	288.7E6	420.2E6	314.708	314.508
21)	B Endrin ke...	7.678	6.853	141.0E6	216.6E6	72.944	72.239

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD022924\
Data File : PD081830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Feb 2024 20:56
Operator : AR\AJ
Sample : P1597-15MSD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 22:14:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

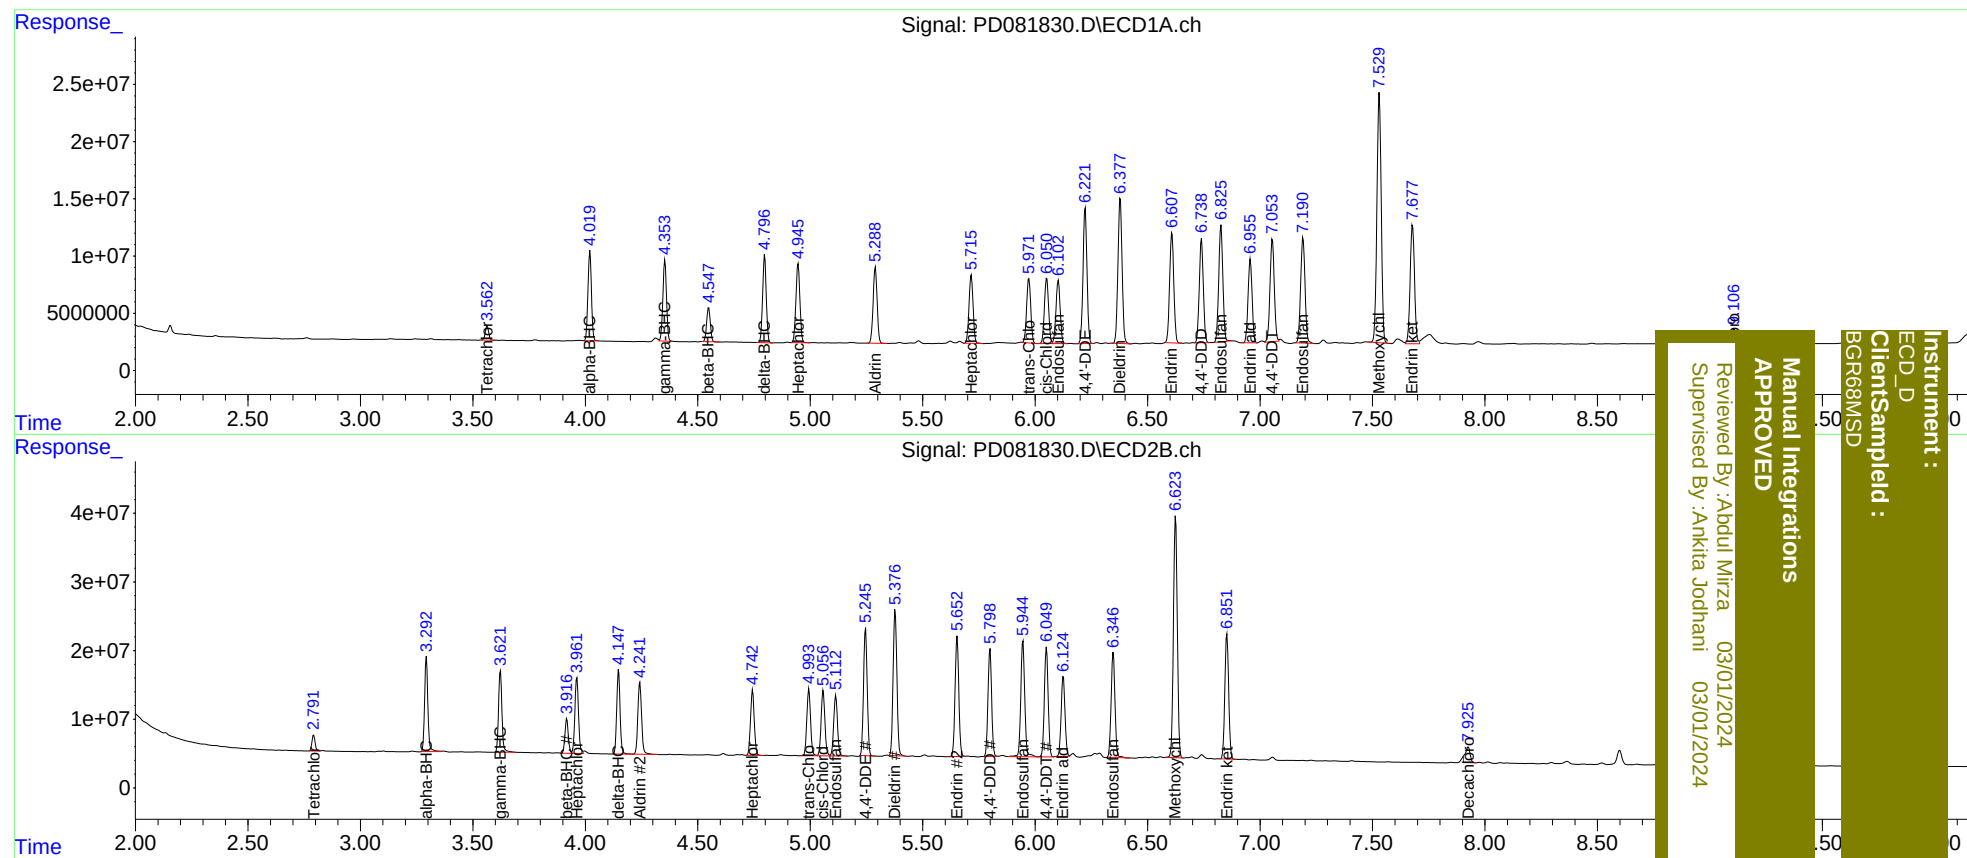

Instrument :
ECD_D
ClientSampled :
BGR68MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 03/01/2024
Supervised By: Ankita Jodhani 03/01/2024