

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030119\
 Data File : PD051463.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 11:33
 Operator : AJ\SJ
 Sample : PB117472BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:02:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	4.045	27828300	609.0E6	19.365	19.712
27)	SA Decachlor...	7.826	9.158	52741966	729.2E6	43.855	38.466
Target Compounds							
15)	B Endosulfa...	0.000	6.977	0	23887873	N.D.	0.870

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030119\
Data File : PD051463.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 11:33
Operator : AJ\SJ
Sample : PB117472BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:02:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

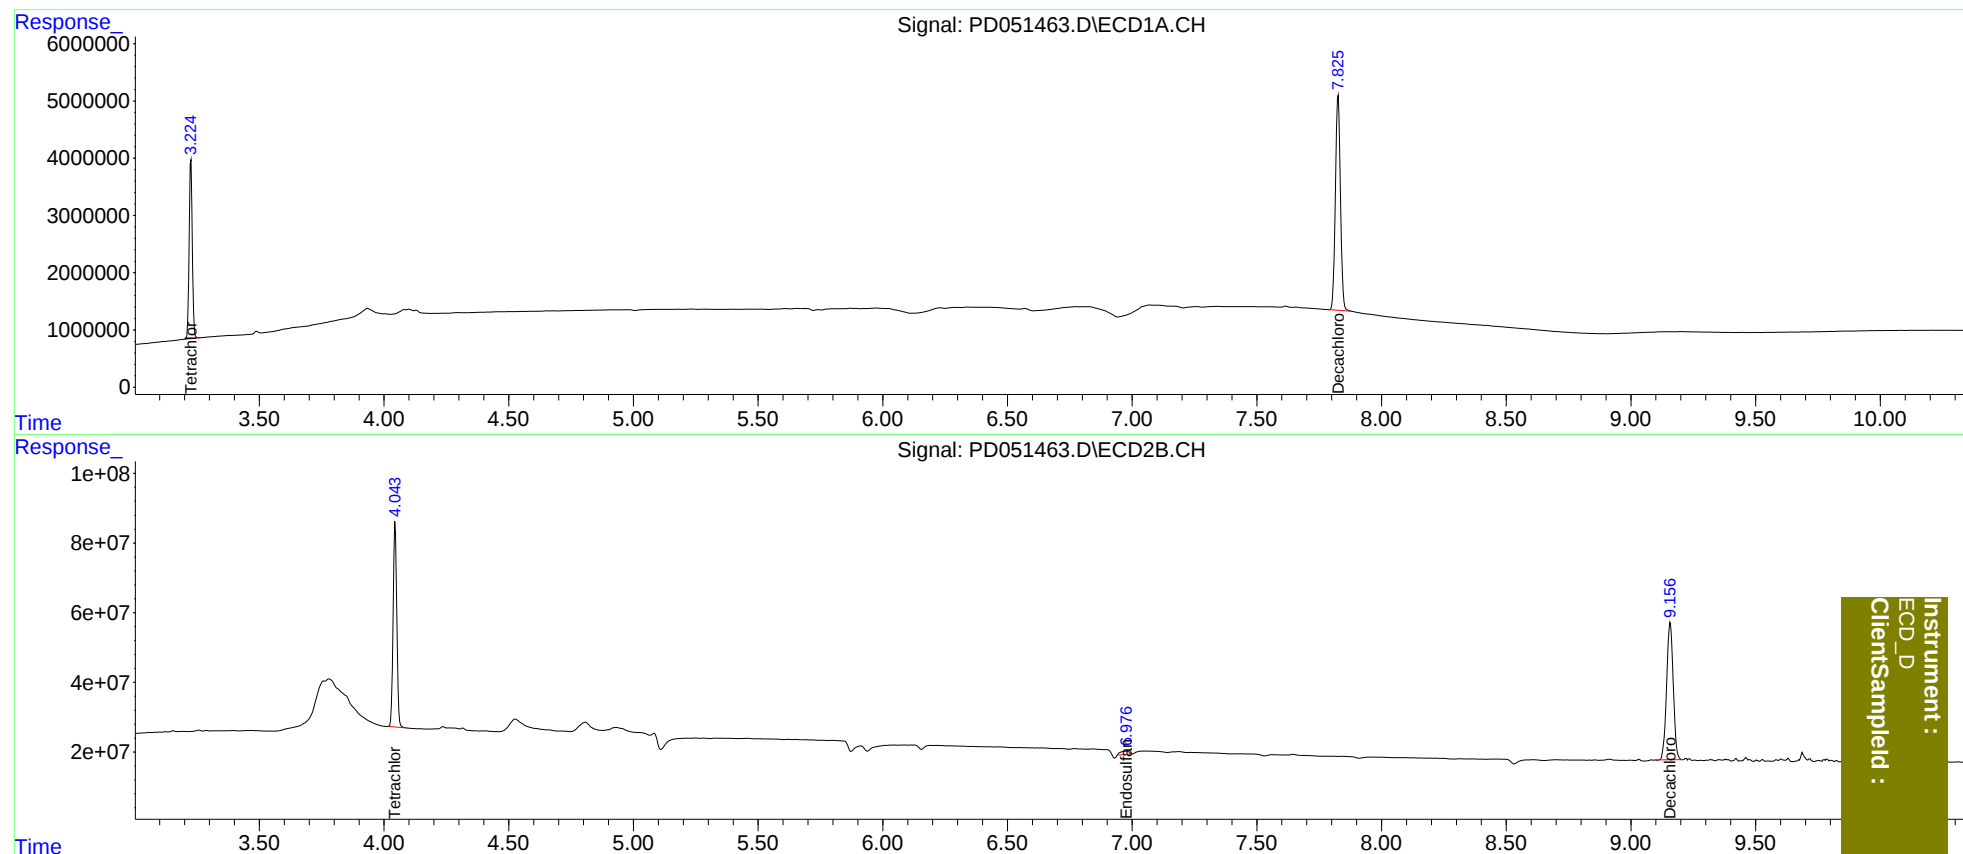


Instrument :
ECD_D
ClientSampleId :

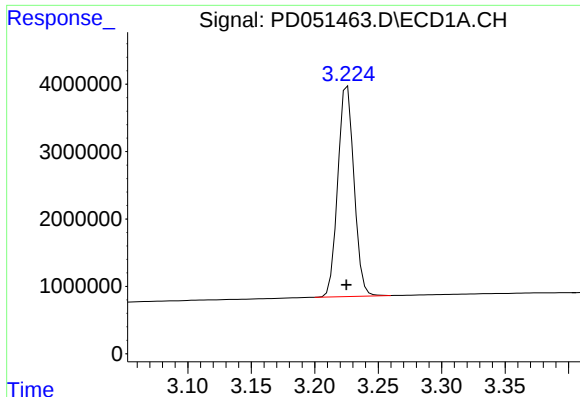

#1 Tetrachloro-m-xylene


R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 27828300
Conc: 19.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

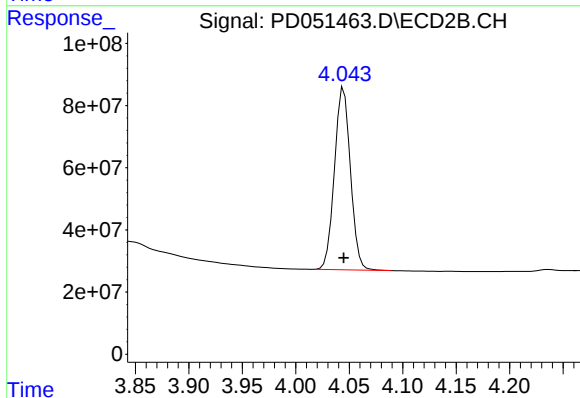


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 609008891
Conc: 19.71 ng/ml

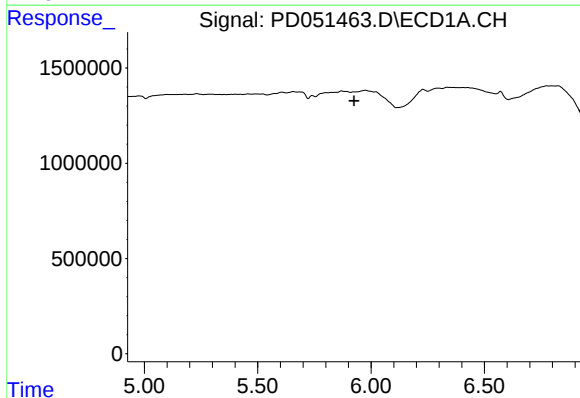


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

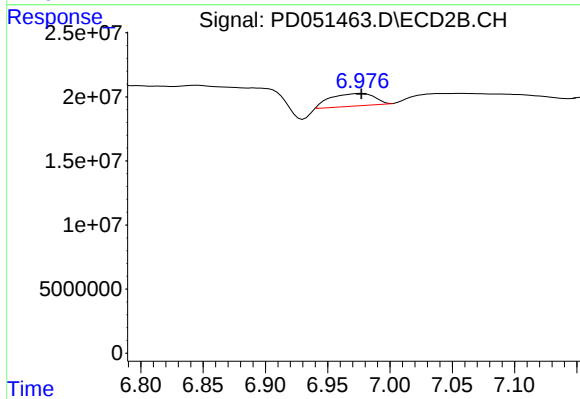

#15 Endosulfan II


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 23887873
Conc: 0.87 ng/ml

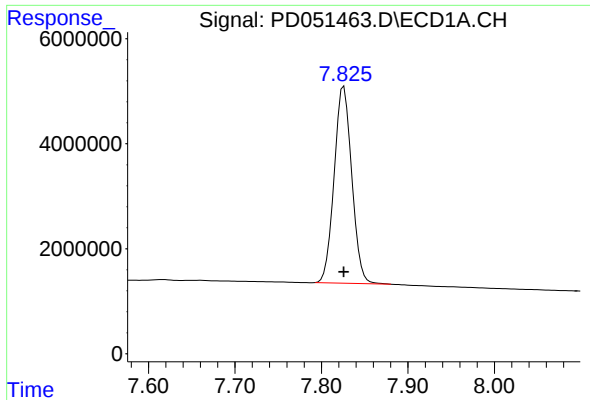

#27 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 52741966
Conc: 43.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

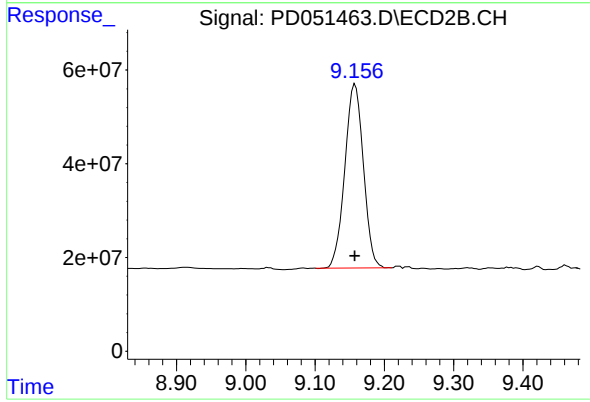

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.000 min
Response: 729219489
Conc: 38.47 ng/ml