

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030119\
 Data File : PD051464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 11:47
 Operator : AJ\SJ
 Sample : PB117481BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:02:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.044	27561038	596.5E6	19.179	19.308
27)	SA Decachlor...	7.824	9.155	52822419	737.4E6	43.922	38.898
Target Compounds							
6)	B beta-BHC	0.000	4.937f	0 49749584	N.D.	2.507	
10)	B trans-Chl...	0.000	6.113f	0 35366278	N.D.	0.979	
15)	B Endosulfa...	0.000	6.977	0 20381304	N.D.	0.743	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030119\
Data File : PD051464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 11:47
Operator : AJ\SJ
Sample : PB117481BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:02:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

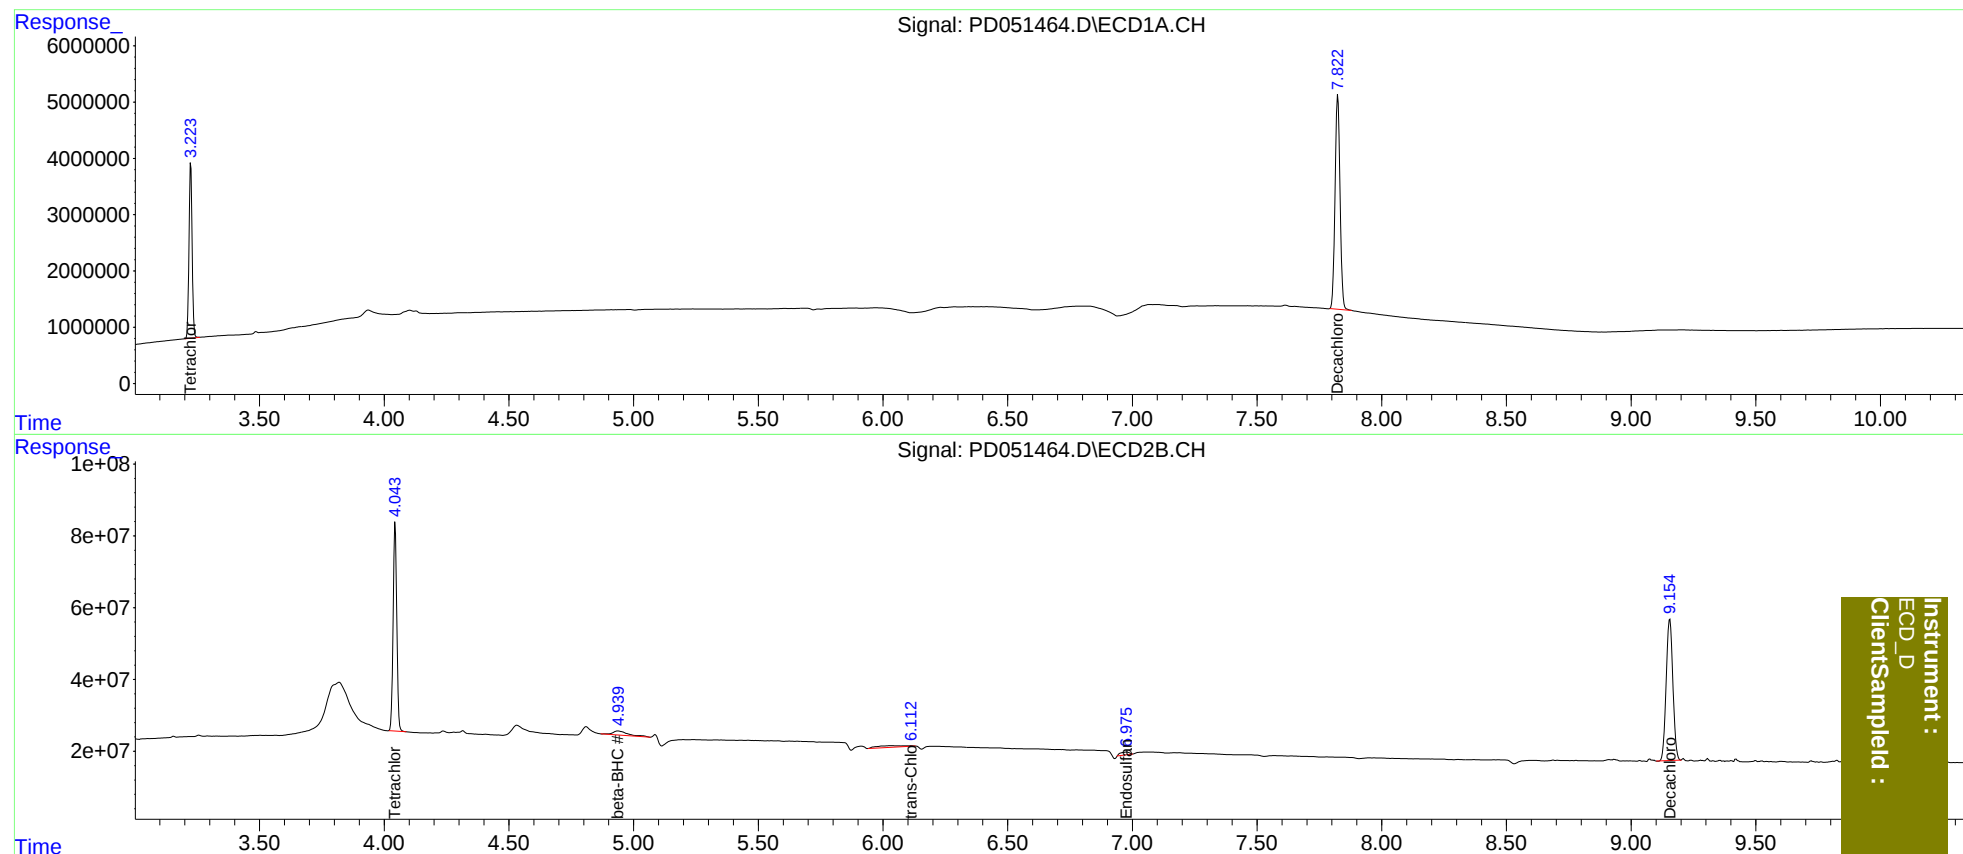


Instrument :
ECD_D
ClientSampleId :

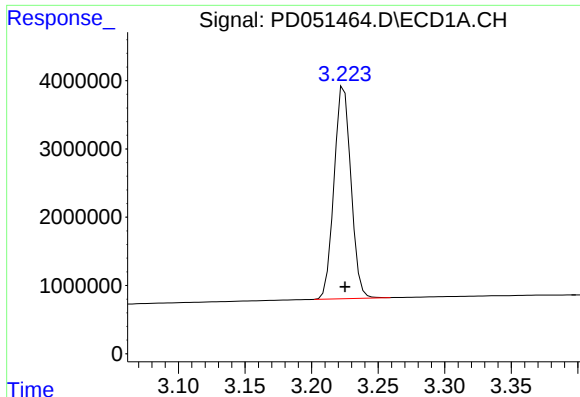

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 27561038
Conc: 19.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

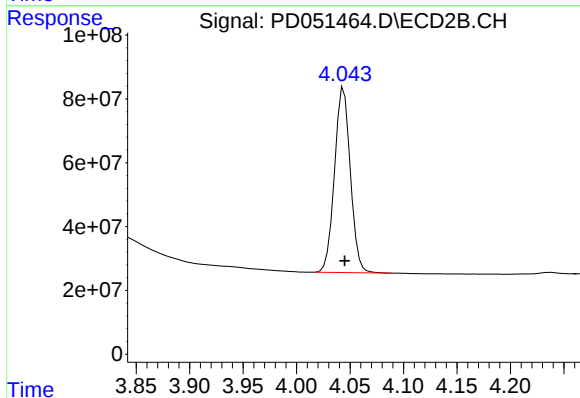


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 596532546
Conc: 19.31 ng/ml

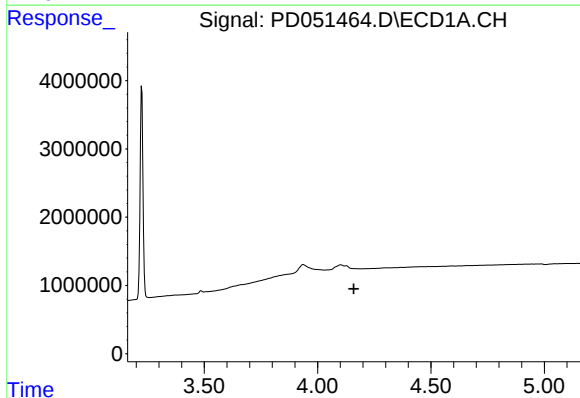


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

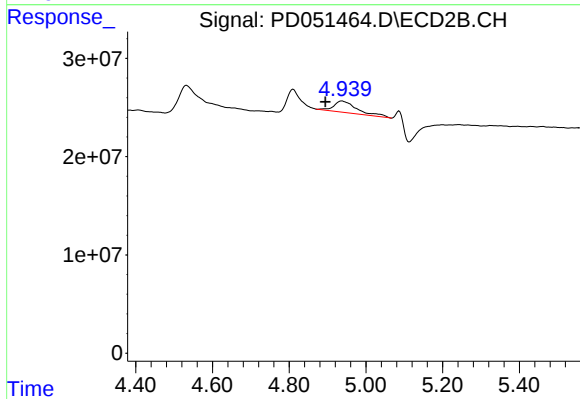

#6 beta-BHC


R.T.: 4.937 min
Delta R.T.: 0.043 min
Response: 49749584
Conc: 2.51 ng/ml

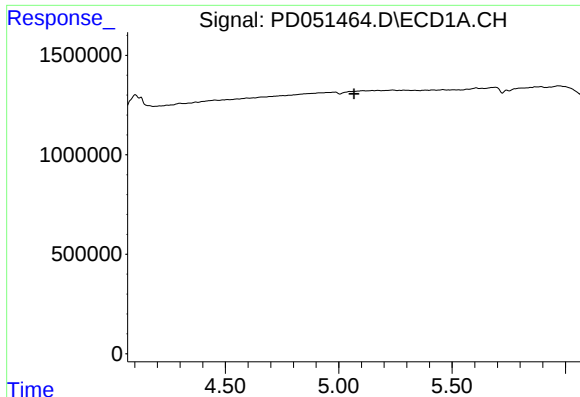

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

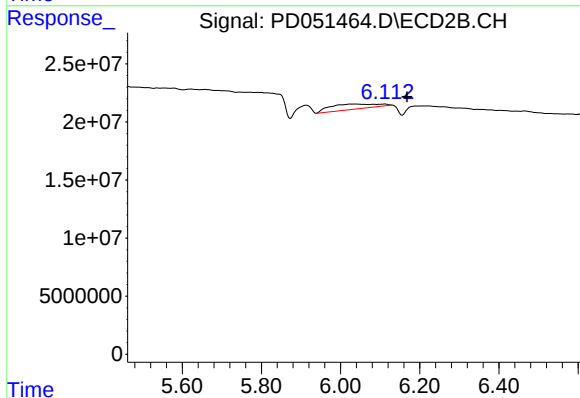


#10 trans-Chlordane

R.T.: 6.113 min
Delta R.T.: -0.055 min
Response: 35366278
Conc: 0.98 ng/ml

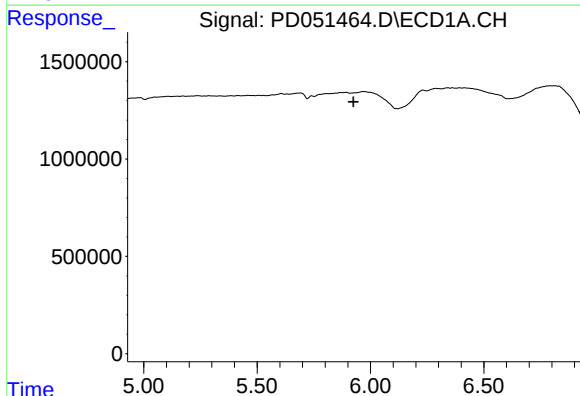


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

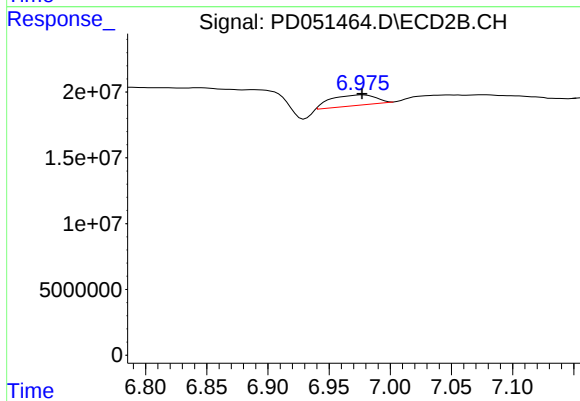

#15 Endosulfan II


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 20381304
Conc: 0.74 ng/ml

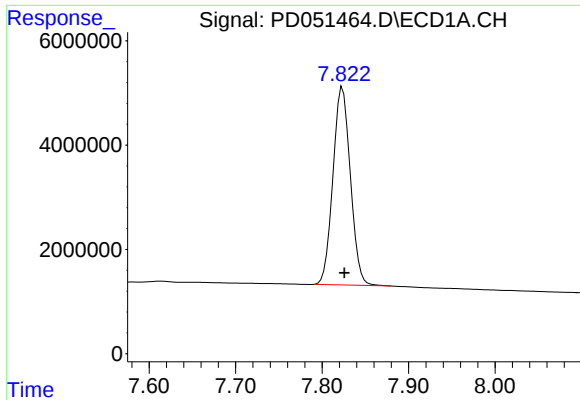

#27 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 52822419
Conc: 43.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

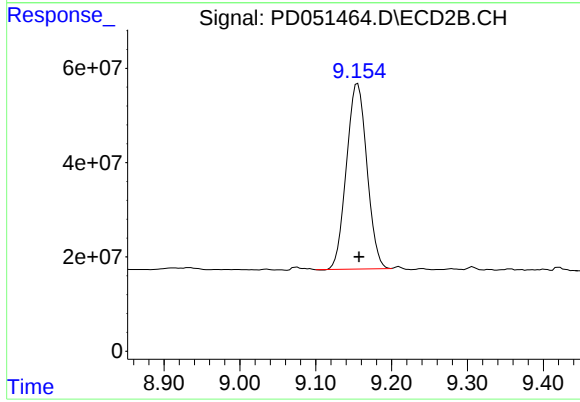

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 737404332
Conc: 38.90 ng/ml