

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030119\
 Data File : PD051471.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 13:24
 Operator : AJ\SJ
 Sample : K1601-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:03:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.044	15849787	345.3E6	11.030	11.176
27)	SA Decachlor...	7.823	9.155	24196783	369.0E6	20.120	19.467
Target Compounds							
2)	A alpha-BHC	0.000	4.463f	0	21144266	N.D.	0.453
6)	B beta-BHC	0.000	4.938f	0	28531648	N.D.	1.438
8)	B Heptachlo...	0.000	5.916	0	54193374	N.D.	1.514
15)	B Endosulfa...	0.000	6.986	0	33128153	N.D.	1.207
20)	A Methoxychlor	0.000	7.646	0	26046403	N.D.	2.460


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030119\
Data File : PD051471.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 13:24
Operator : AJ\SJ
Sample : K1601-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:03:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

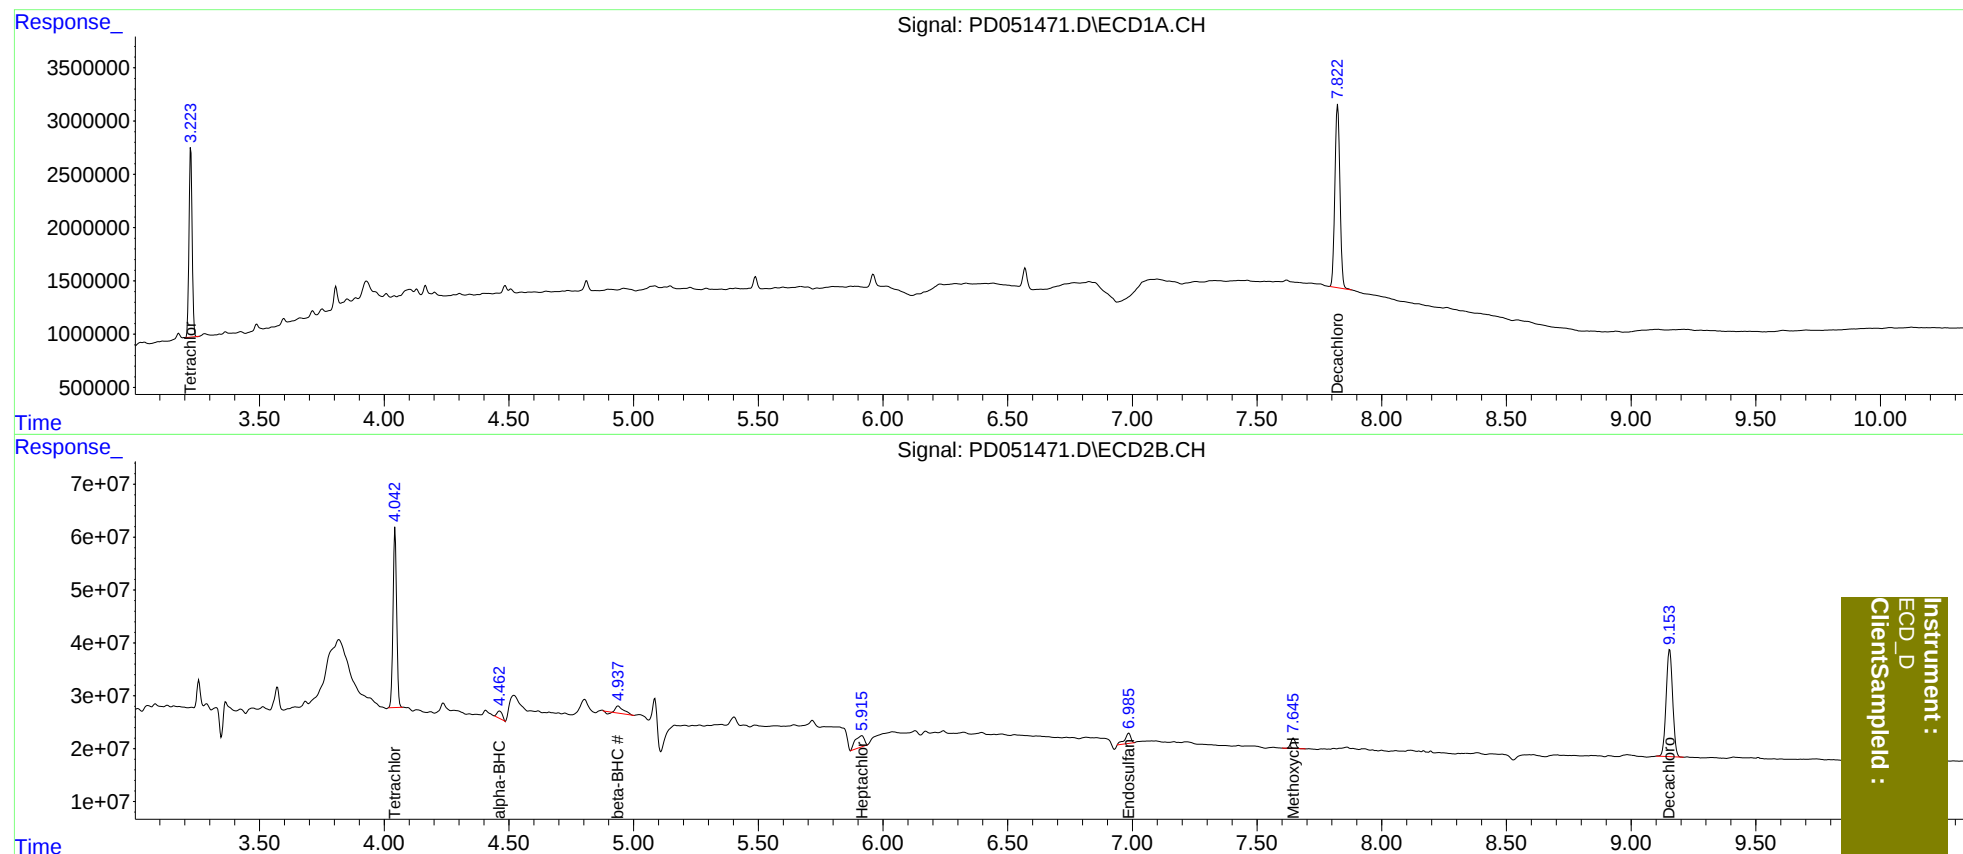


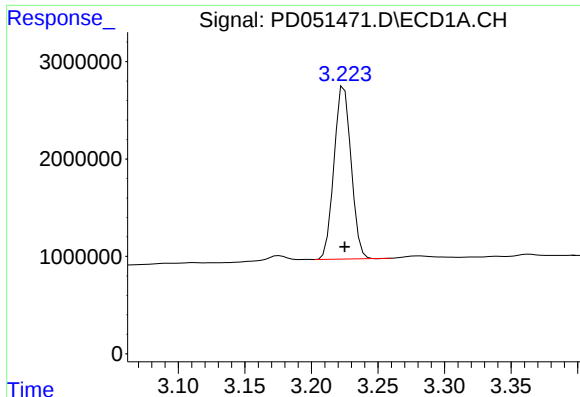

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 15849787
Conc: 11.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

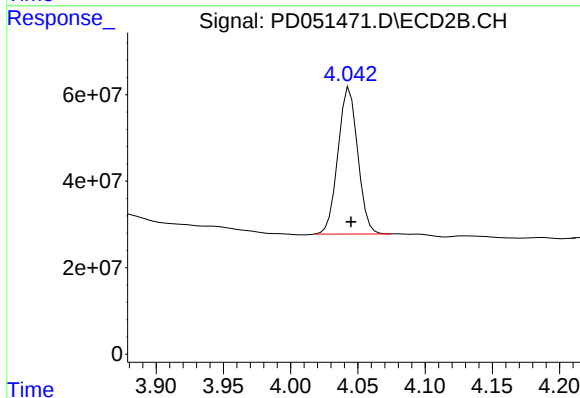


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 345300358
Conc: 11.18 ng/ml

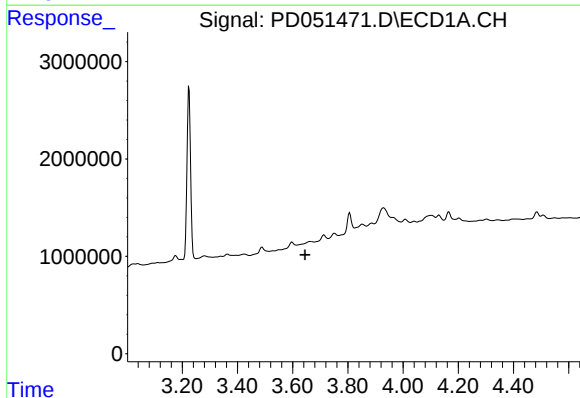


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.645 min
Response: 0
Conc: N.D.

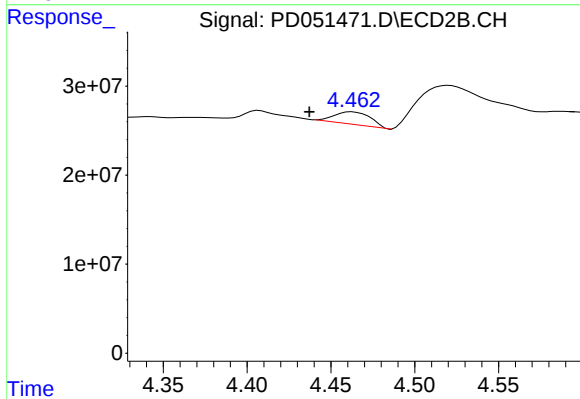

#2 alpha-BHC


R.T.: 4.463 min
Delta R.T.: 0.026 min
Response: 21144266
Conc: 0.45 ng/ml

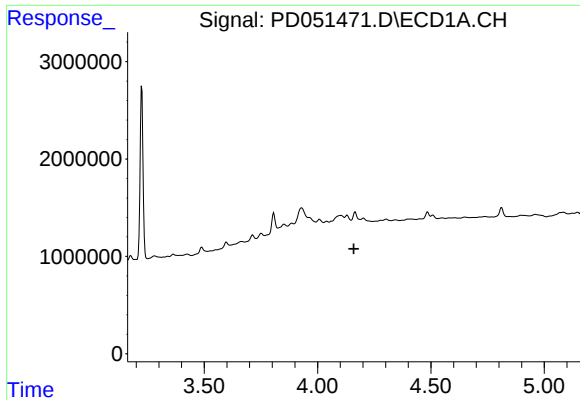

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.159 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

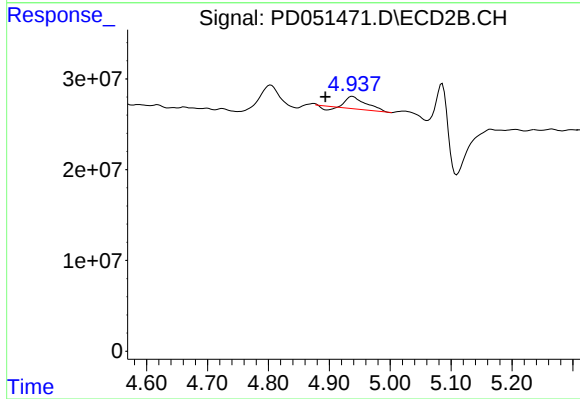


#6 beta-BHC

R.T.: 4.938 min
Delta R.T.: 0.044 min
Response: 28531648
Conc: 1.44 ng/ml

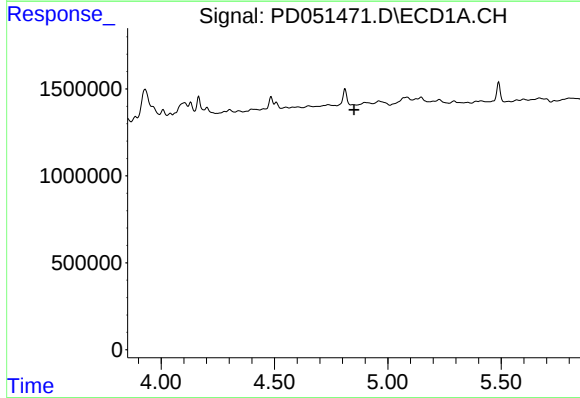


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

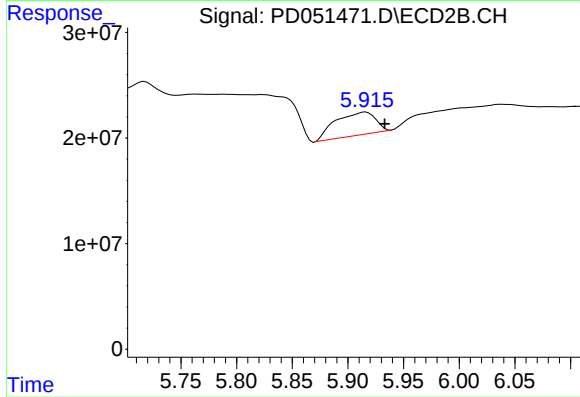

#8 Heptachlor epoxide


R.T.: 5.916 min
Delta R.T.: -0.017 min
Response: 54193374
Conc: 1.51 ng/ml

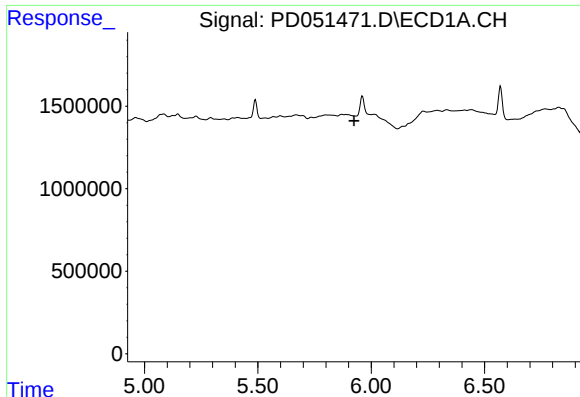

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

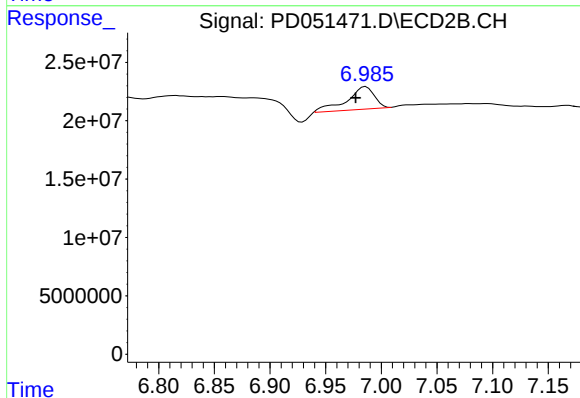


#15 Endosulfan II

R.T.: 6.986 min
Delta R.T.: 0.009 min
Response: 33128153
Conc: 1.21 ng/ml

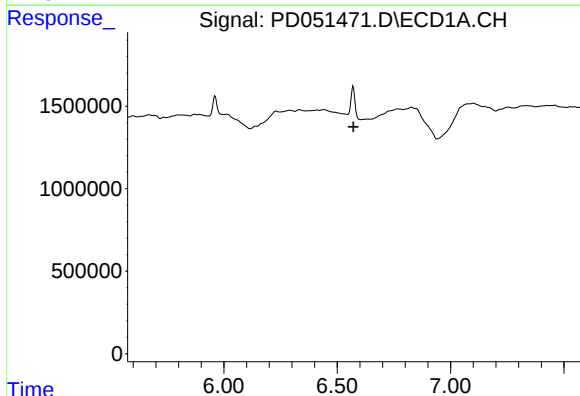


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.572 min
Response: 0
Conc: N.D.

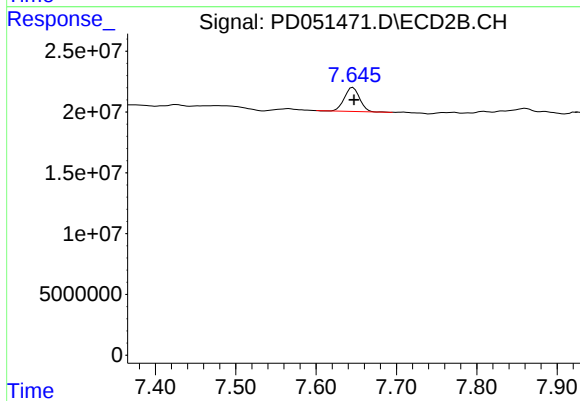

#20 Methoxychlor


R.T.: 7.646 min
Delta R.T.: -0.001 min
Response: 26046403
Conc: 2.46 ng/ml

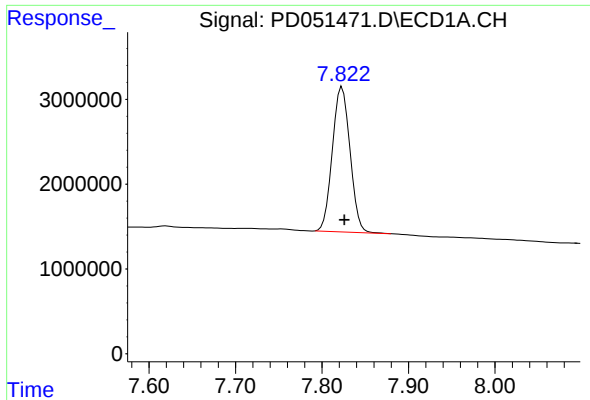

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 24196783
Conc: 20.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

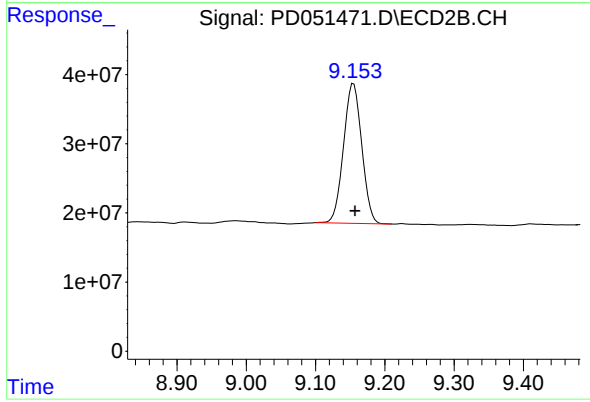

#27 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: -0.002 min
Response: 369048894
Conc: 19.47 ng/ml