

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
 Data File : PD068250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 17:28
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:50:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	21217819	181.4E6	18.100	18.903
2)	SA Decachlor...	8.213	9.372	21979872	112.0E6	18.888	18.886
Target Compounds							
2)	A alpha-BHC	3.889	4.572	14602424	132.8E6	8.510	9.675
3)	MA gamma-BHC...	4.173	4.863	13914004	121.6E6	8.737	9.804
5)	MB Aldrin	0.000	5.726f	0	52835	N.D.	0.004 #
6)	B beta-BHC	4.423	5.026	7268343	58202321	10.359	10.767
7)	B delta-BHC	0.000	5.231f	0	1049291	N.D.	0.084 #
8)	B Heptachlo...	0.000	6.072f	0	1808038	N.D.	0.169 #
9)	A Endosulfan I	0.000	6.472f	0	123281	N.D.	0.013 #
10)	B gamma-Chl...	0.000	6.335	0	2061812	N.D.	0.195 #
11)	B alpha-Chl...	0.000	6.403	0	1353140	N.D.	0.131 #
12)	B 4,4'-DDE	5.617	6.553	580411	6219939	0.426	0.636 #
13)	MA Dieldrin	0.000	6.711	0	3059957	N.D.	0.297 #
14)	MA Endrin	6.006	6.933	57982229	362.4E6	46.936	47.121
15)	B Endosulfa...	6.283	7.136	652099	6898421	0.513	0.840 #
16)	A 4,4'-DDD	6.134	7.044	3010516	22794326	2.539	2.896
17)	MA 4,4'-DDT	6.374	7.347	103.9E6	583.5E6	94.253	82.466
18)	B Endrin al...	6.448	7.262	1136391	8082447	1.240	1.343
20)	A Methoxychlor	6.925	7.800	138.9E6	676.4E6	214.125	194.666
21)	B Endrin ke...	7.154	7.962	2156366	13720032	1.465	1.634
22)	Mirex	7.366f	0.000	150647	0	0.119	N.D. #
24)	Chlordane-2	0.000	5.643f	0	229056	N.D.	0.570 #
25)	Chlordane-3	0.000	6.335	0	2061812	N.D.	1.450 #
26)	Chlordane-4	0.000	6.403	0	1353140	N.D.	0.840 #
27)	Chlordane-5	6.283	0.000	652099	0	13.239	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
Data File : PD068250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 17:28
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PEM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:50:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

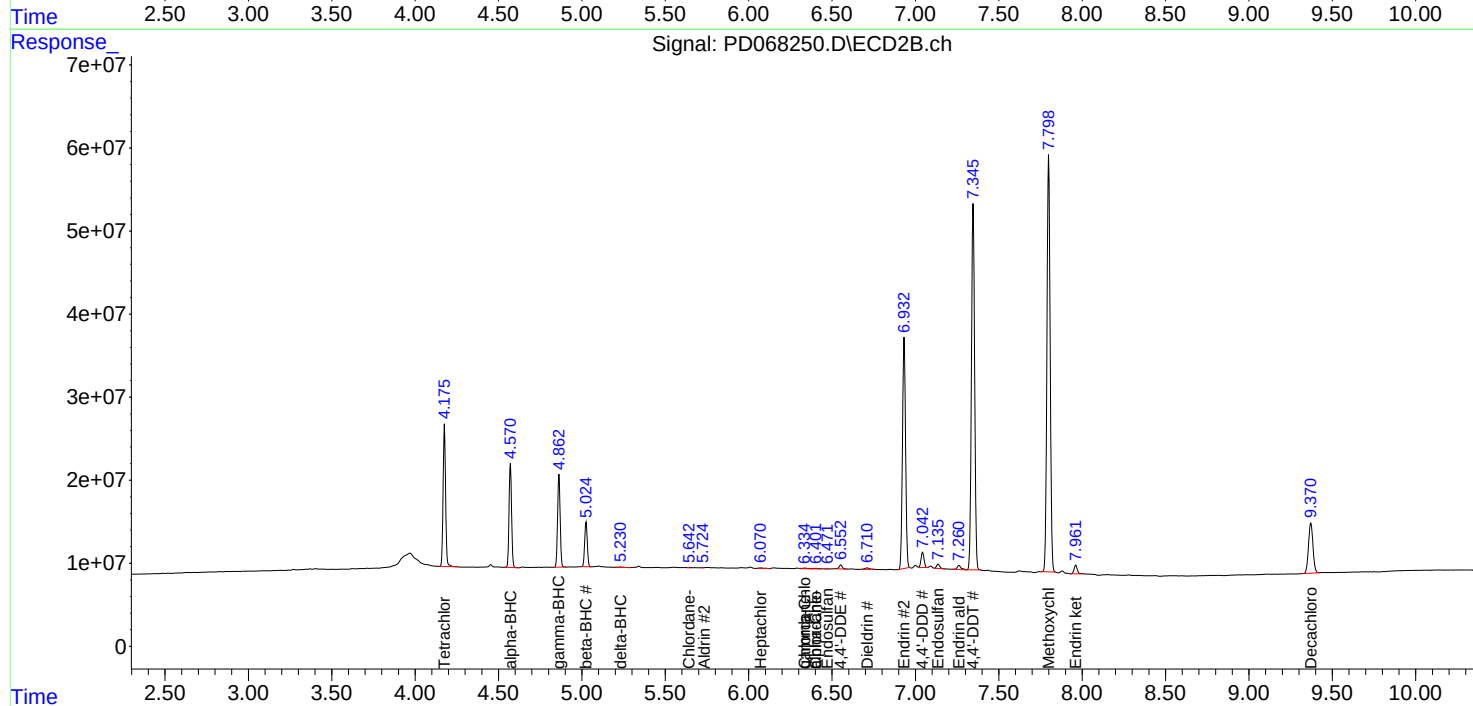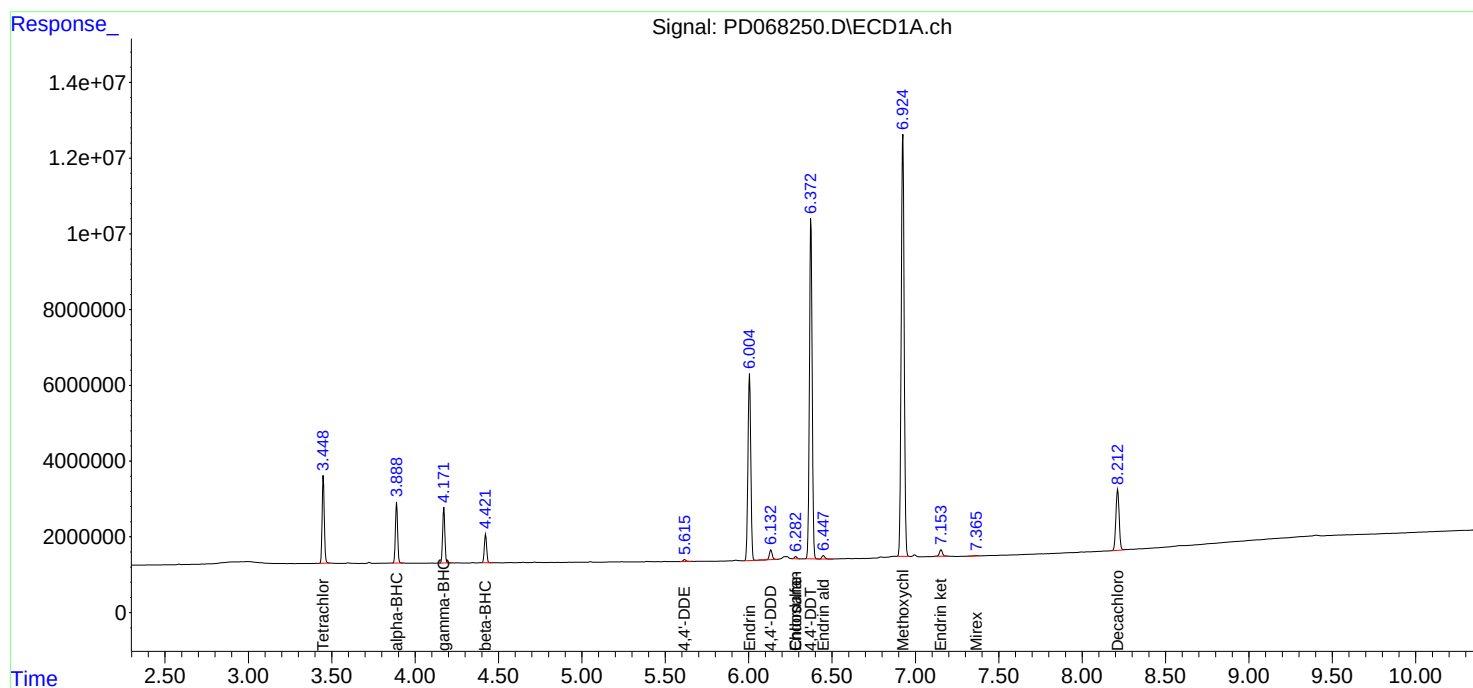


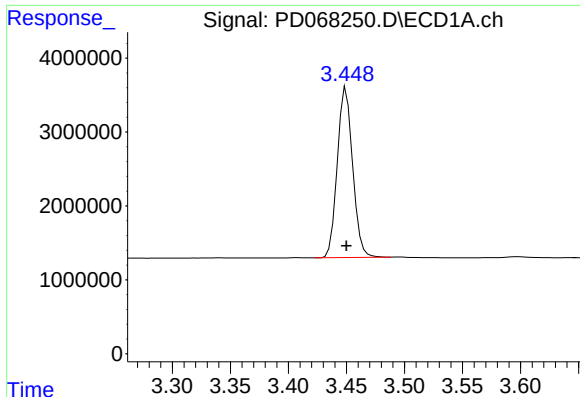

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 21217819
Conc: 18.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

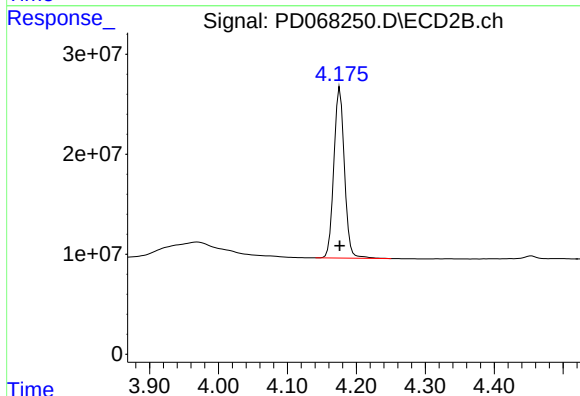


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 181426793
Conc: 18.90 ng/ml

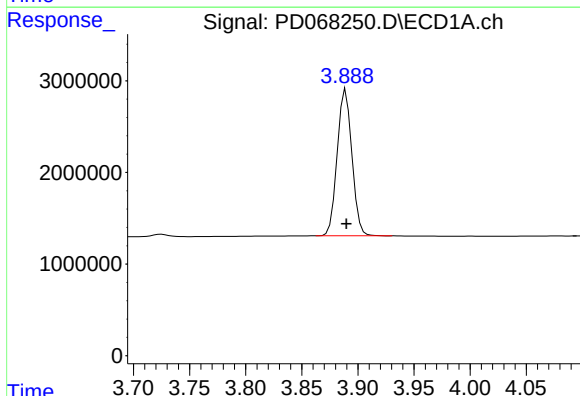


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: 0.000 min
Response: 14602424
Conc: 8.51 ng/ml

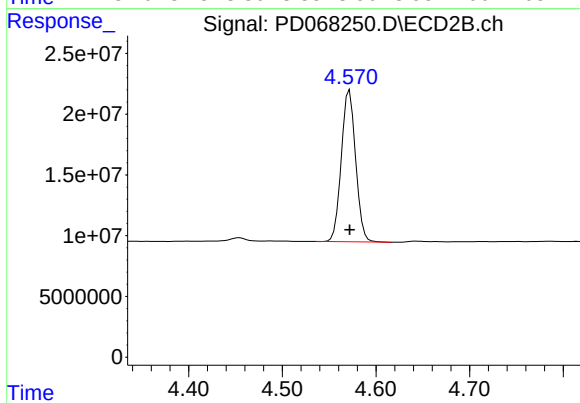

#2 alpha-BHC


R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 132754879
Conc: 9.67 ng/ml

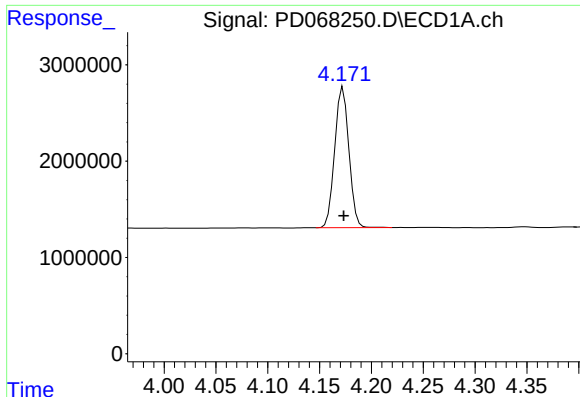

#3 gamma-BHC (Lindane)


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 13914004
Conc: 8.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

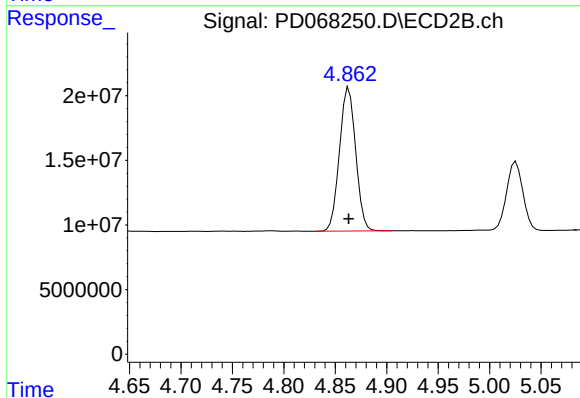


#3 gamma-BHC (Lindane)

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 121567401
Conc: 9.80 ng/ml

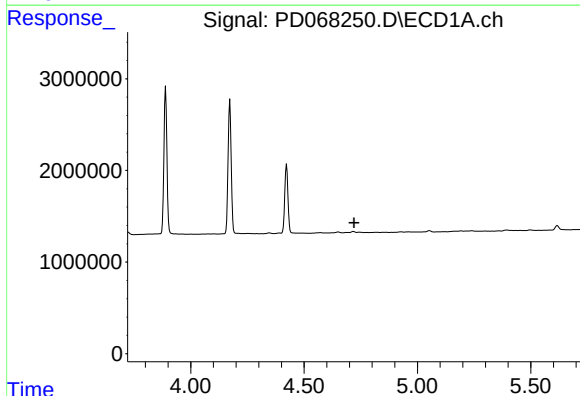


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.720 min
Response: 0
Conc: N.D.

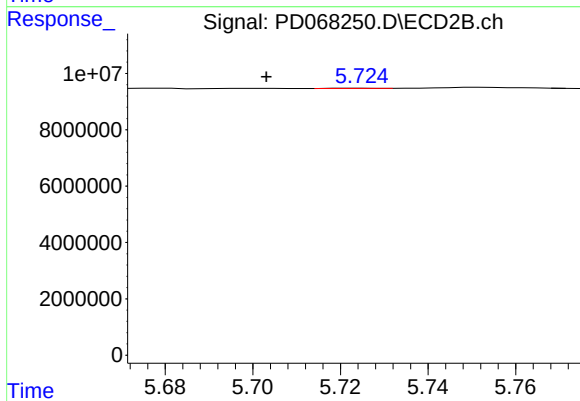

#5 Aldrin


R.T.: 5.726 min
Delta R.T.: 0.023 min
Response: 52835
Conc: 0.00 ng/ml

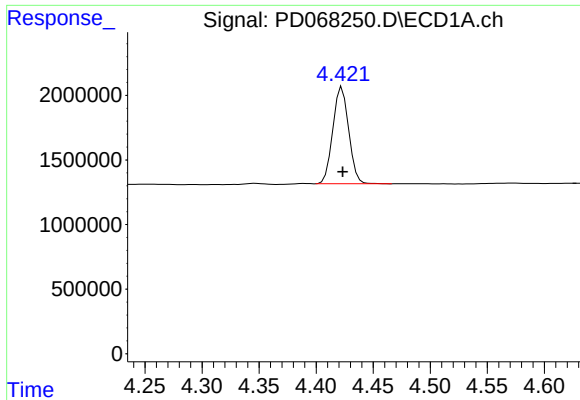

#6 beta-BHC


R.T.: 4.423 min
Delta R.T.: 0.000 min
Response: 7268343
Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

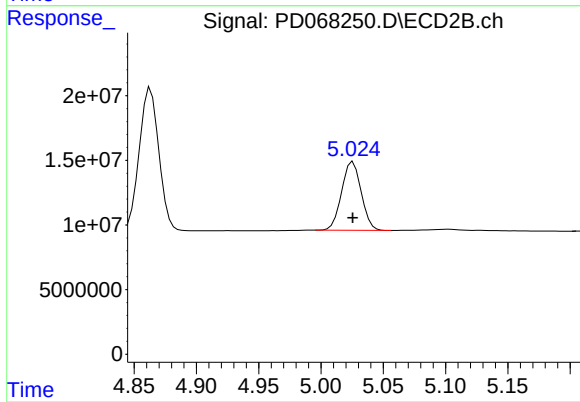


#6 beta-BHC

R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 58202321
Conc: 10.77 ng/ml

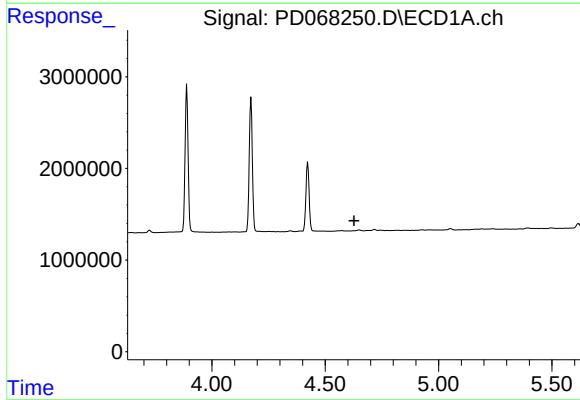


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

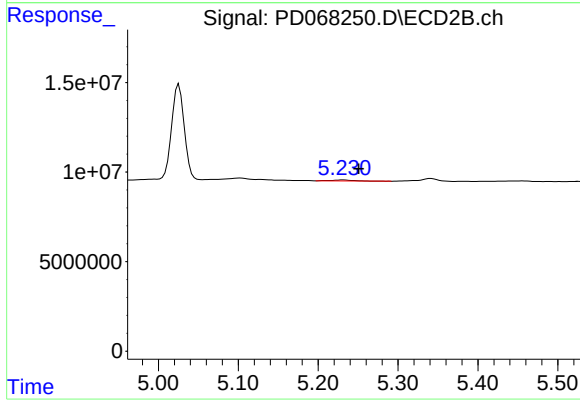

#7 delta-BHC


R.T.: 5.231 min
Delta R.T.: -0.020 min
Response: 1049291
Conc: 0.08 ng/ml

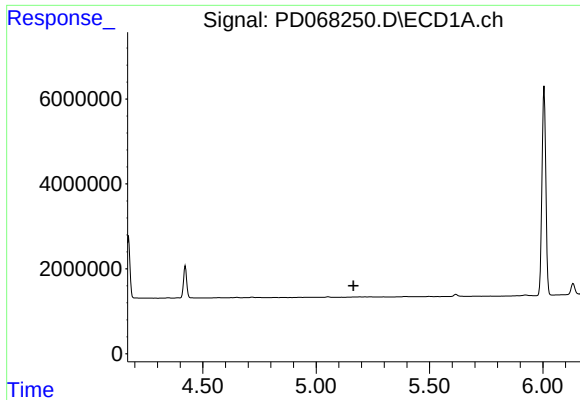

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

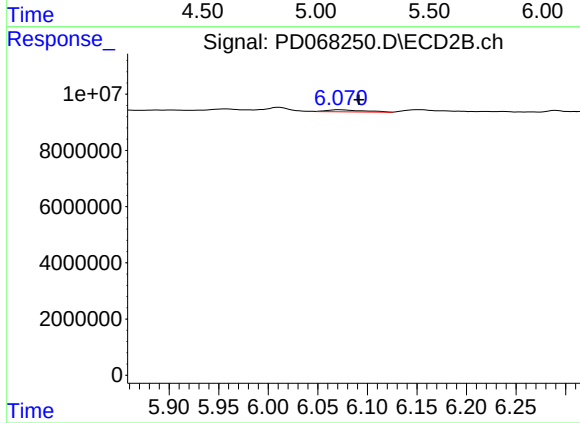


#8 Heptachlor epoxide

R.T.: 6.072 min
Delta R.T.: -0.020 min
Response: 1808038
Conc: 0.17 ng/ml

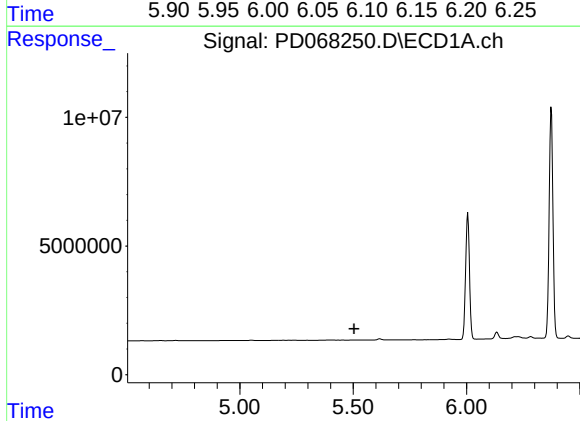


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

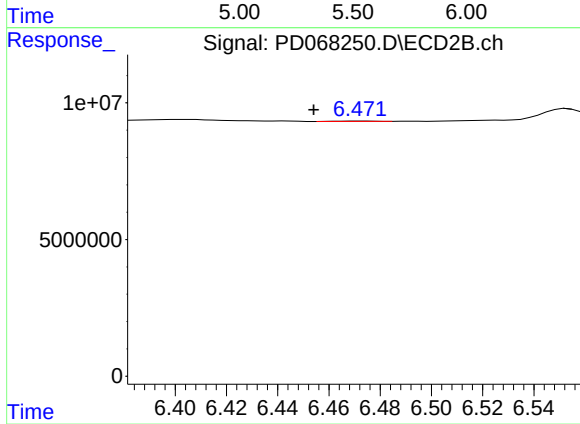

#9 Endosulfan I


R.T.: 6.472 min
Delta R.T.: 0.018 min
Response: 123281
Conc: 0.01 ng/ml

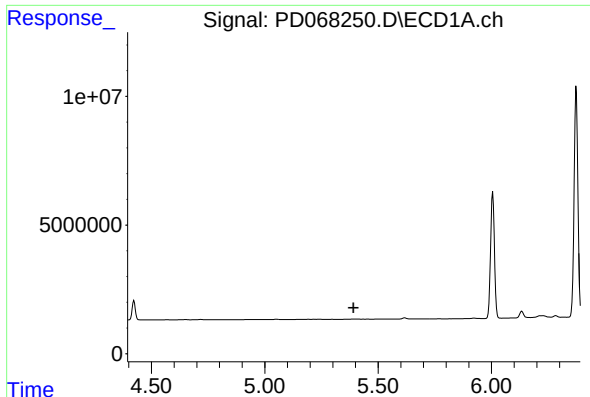

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

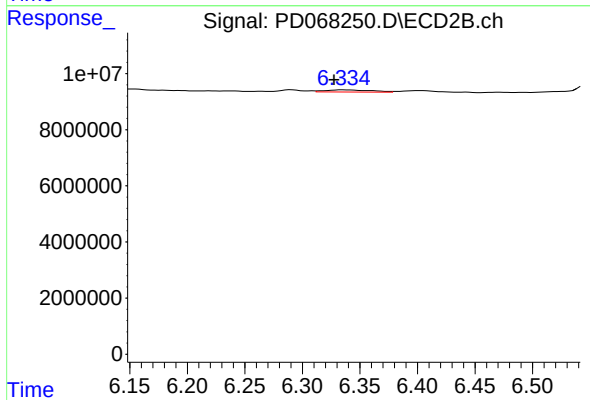


#10 gamma-Chlordane

R.T.: 6.335 min
Delta R.T.: 0.007 min
Response: 2061812
Conc: 0.19 ng/ml

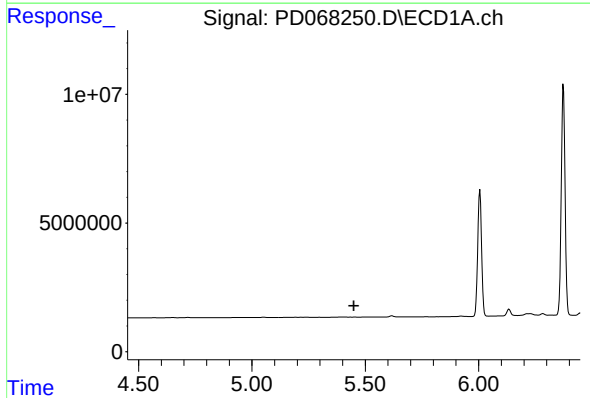


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.450 min
Response: 0
Conc: N.D.

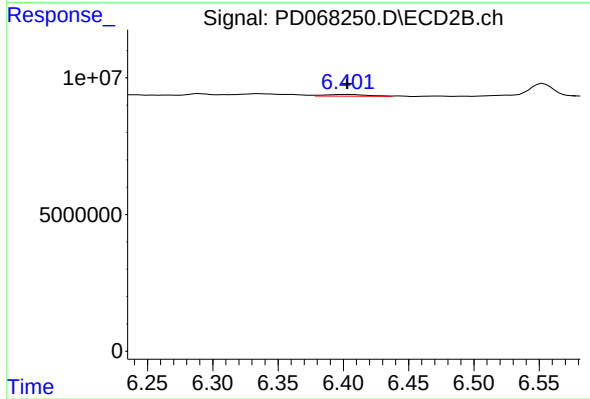

#11 alpha-Chlordane


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 1353140
Conc: 0.13 ng/ml

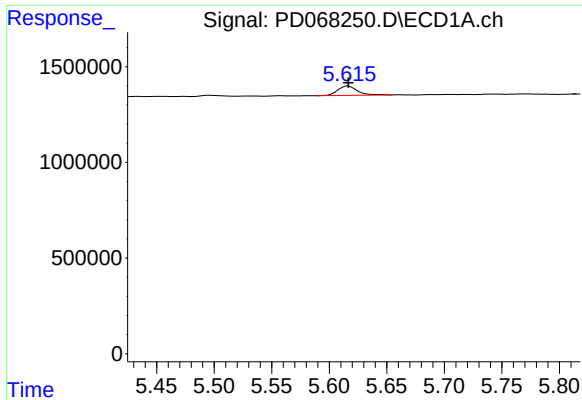

#12 4,4'-DDE


R.T.: 5.617 min
Delta R.T.: 0.000 min
Response: 580411
Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

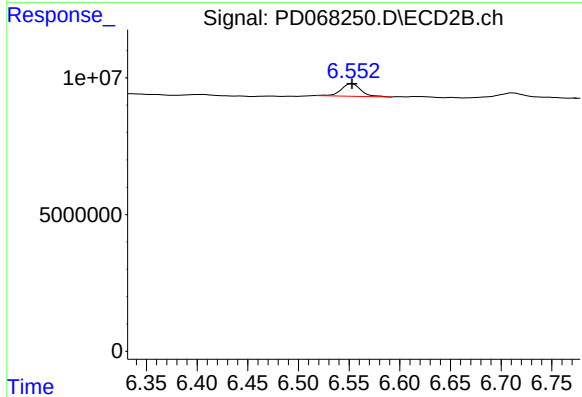


#12 4,4'-DDE

R.T.: 6.553 min
Delta R.T.: 0.000 min
Response: 6219939
Conc: 0.64 ng/ml

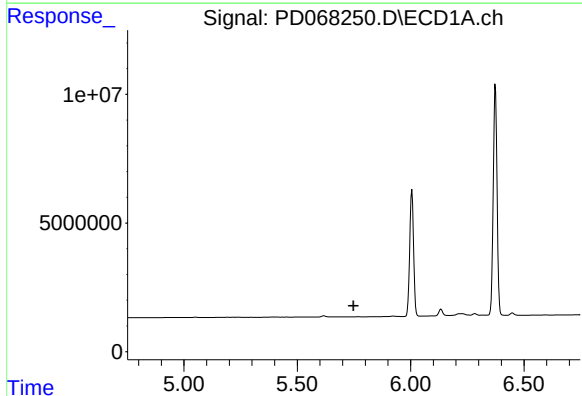


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.748 min
Response: 0
Conc: N.D.

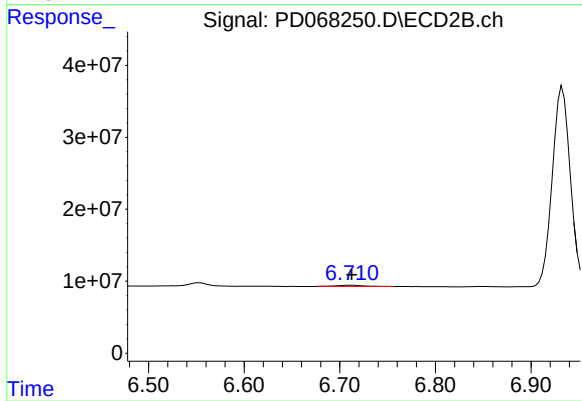

#13 Dieldrin


R.T.: 6.711 min
Delta R.T.: -0.001 min
Response: 3059957
Conc: 0.30 ng/ml

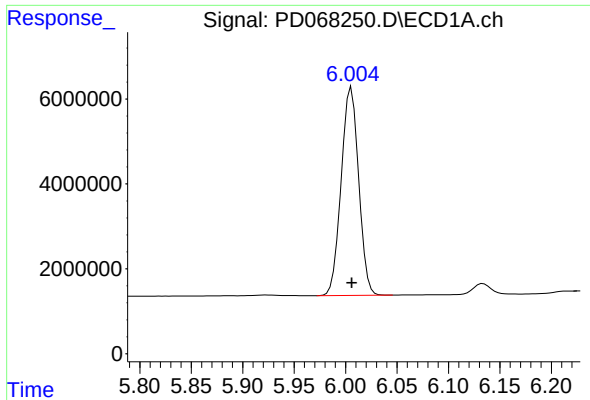

#14 Endrin


R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 57982229
Conc: 46.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

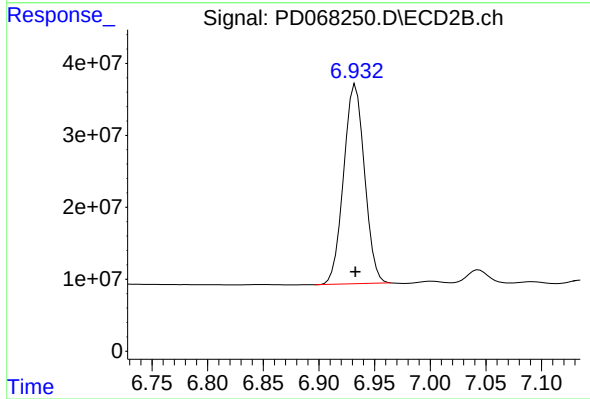


#14 Endrin

R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 362385064
Conc: 47.12 ng/ml

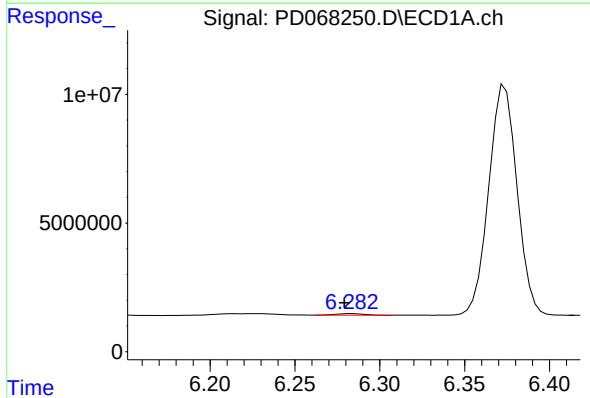


#15 Endosulfan II

R.T.: 6.283 min
Delta R.T.: 0.004 min
Response: 652099
Conc: 0.51 ng/ml

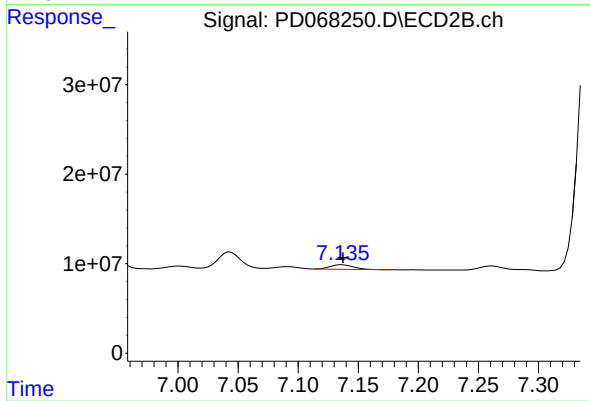

#15 Endosulfan II


R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 6898421
Conc: 0.84 ng/ml

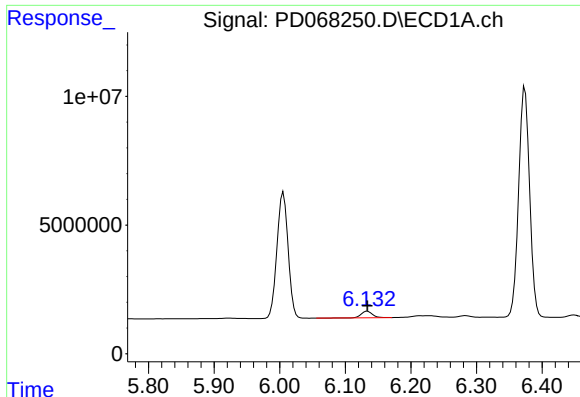

#16 4,4'-DDD


R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 3010516
Conc: 2.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

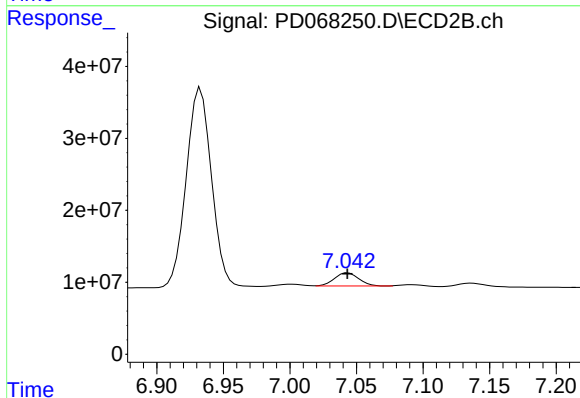


#16 4,4'-DDD

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 22794326
Conc: 2.90 ng/ml

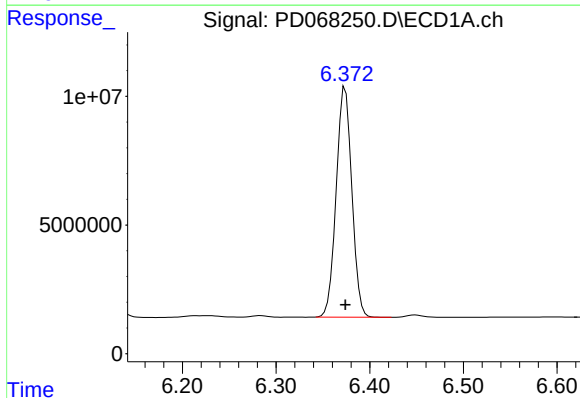


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: 0.000 min
Response: 103939661
Conc: 94.25 ng/ml

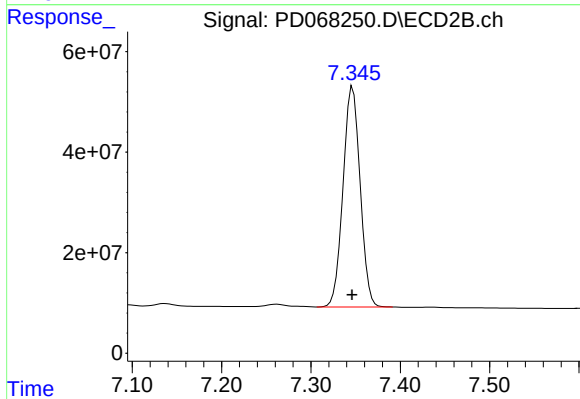

#17 4,4'-DDT


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 583489251
Conc: 82.47 ng/ml

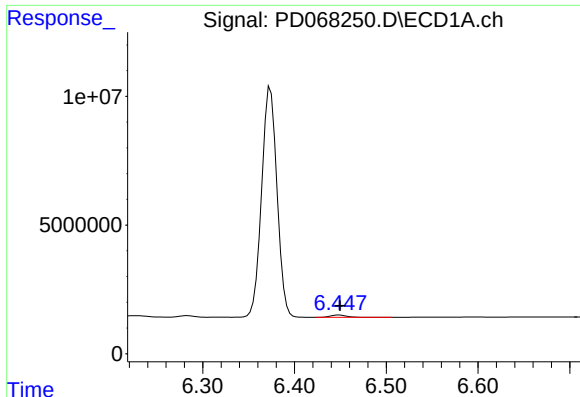

#18 Endrin aldehyde


R.T.: 6.448 min
Delta R.T.: -0.001 min
Response: 1136391
Conc: 1.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

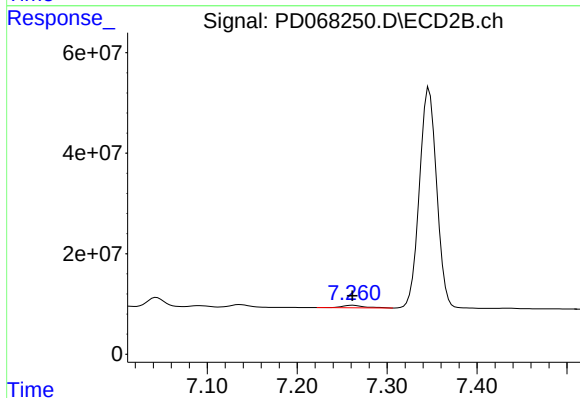


#18 Endrin aldehyde

R.T.: 7.262 min
Delta R.T.: 0.000 min
Response: 8082447
Conc: 1.34 ng/ml

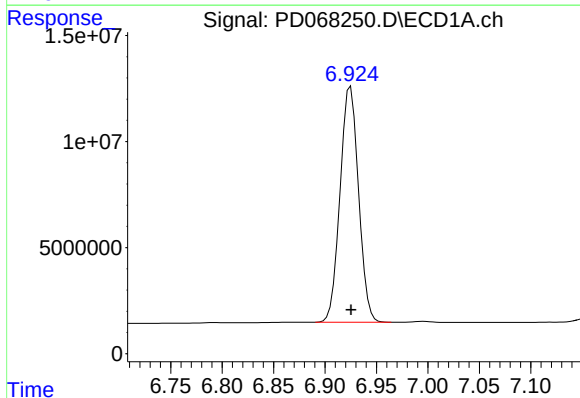


#20 Methoxychlor

R.T.: 6.925 min
Delta R.T.: 0.000 min
Response: 138945134
Conc: 214.12 ng/ml

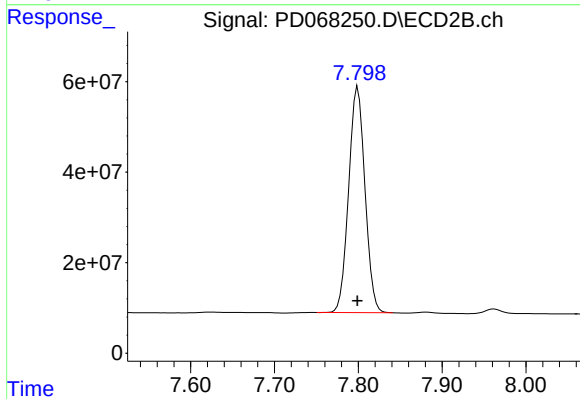

#20 Methoxychlor


R.T.: 7.800 min
Delta R.T.: 0.000 min
Response: 676355225
Conc: 194.67 ng/ml

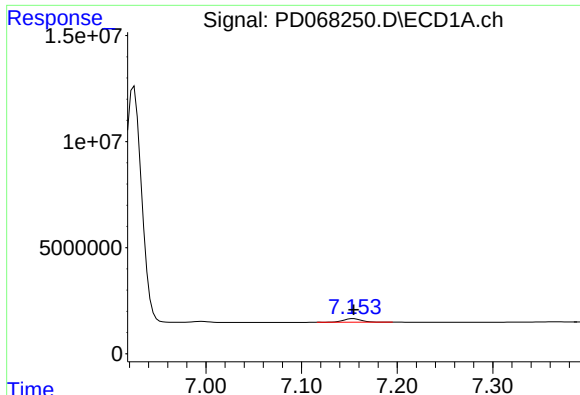

#21 Endrin ketone


R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 2156366
Conc: 1.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

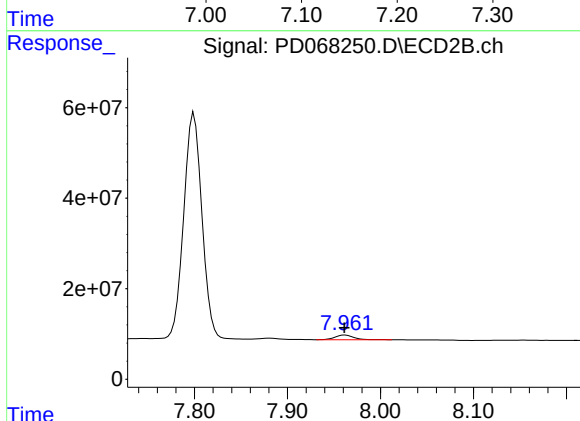


#21 Endrin ketone

R.T.: 7.962 min
Delta R.T.: 0.000 min
Response: 13720032
Conc: 1.63 ng/ml

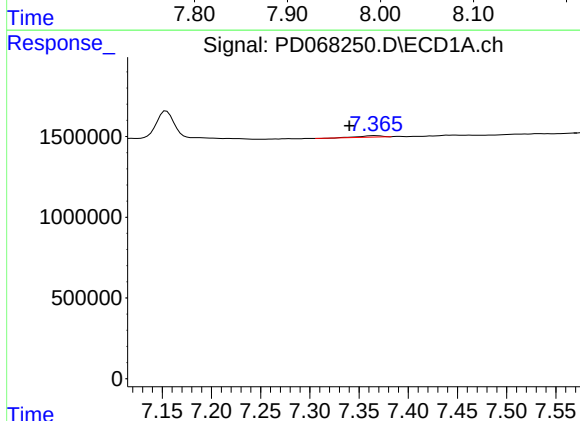


#22 Mirex

R.T.: 7.366 min
Delta R.T.: 0.026 min
Response: 150647
Conc: 0.12 ng/ml

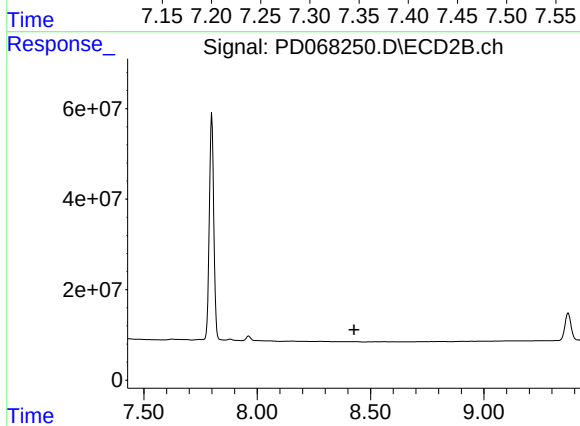

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.428 min
Response: 0
Conc: N.D.

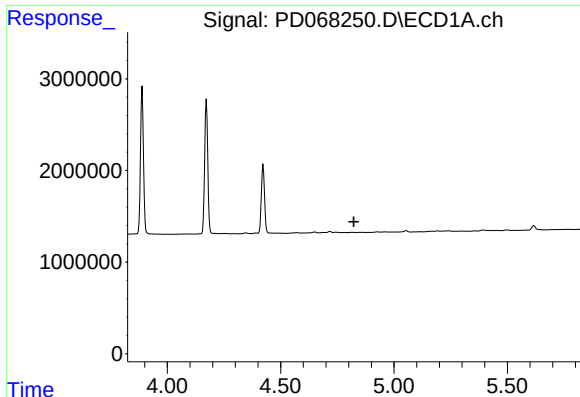

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.822 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

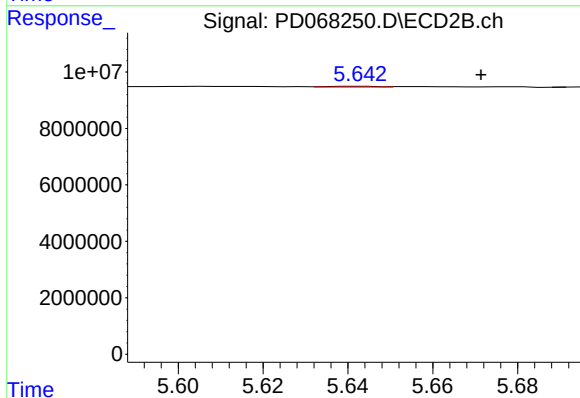


#24 Chlordane-2

R.T.: 5.643 min
Delta R.T.: -0.028 min
Response: 229056
Conc: 0.57 ng/ml

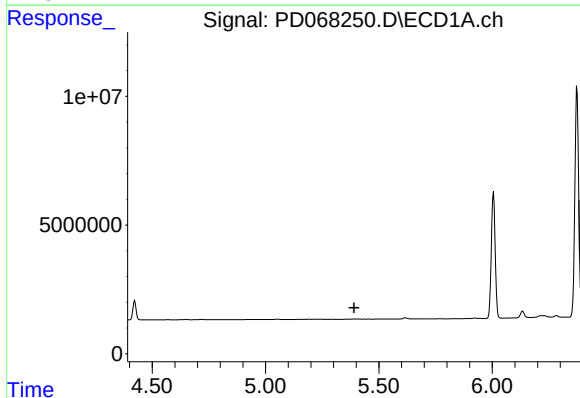


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.391 min
Response: 0
Conc: N.D.

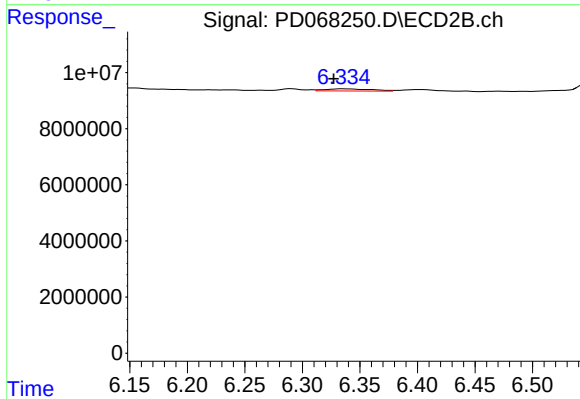

#25 Chlordane-3


R.T.: 6.335 min
Delta R.T.: 0.008 min
Response: 2061812
Conc: 1.45 ng/ml

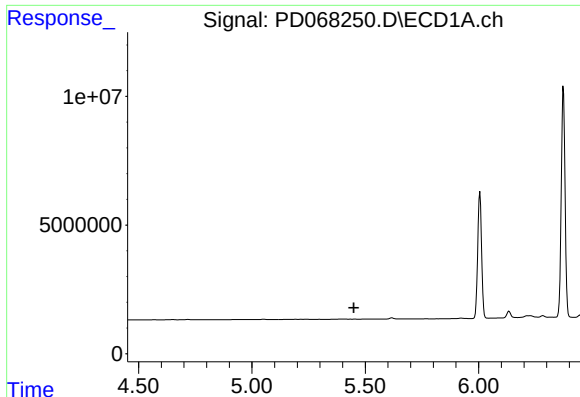

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEM

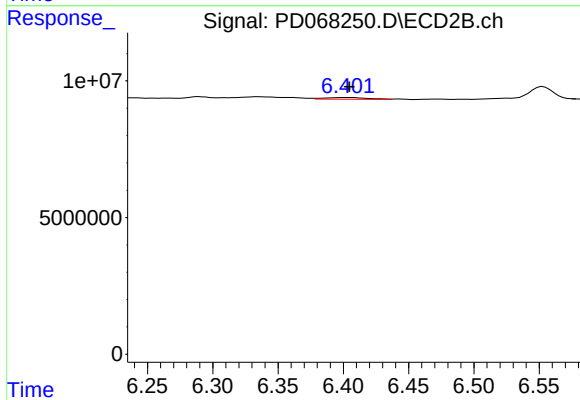


#26 Chlordane-4

R.T.: 6.403 min
Delta R.T.: -0.002 min
Response: 1353140
Conc: 0.84 ng/ml

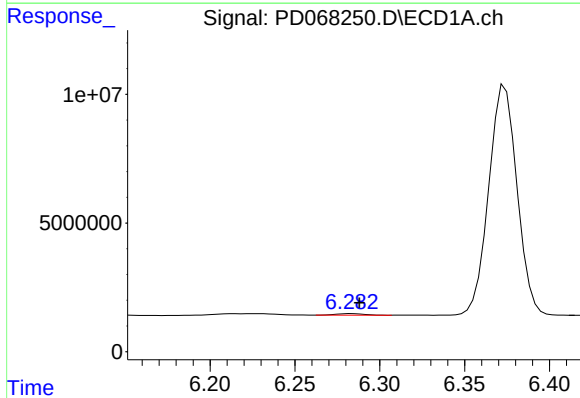


#27 Chlordane-5

R.T.: 6.283 min
Delta R.T.: -0.005 min
Response: 652099
Conc: 13.24 ng/ml

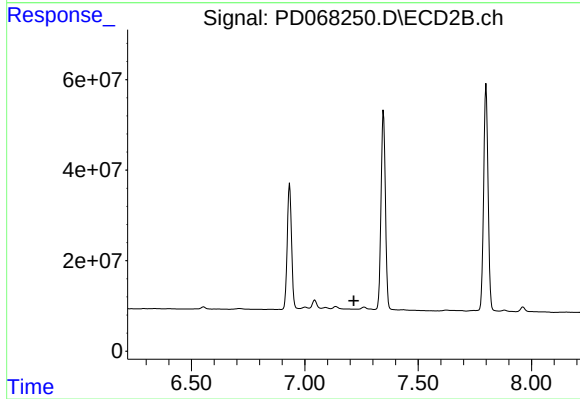

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.216 min
Response: 0
Conc: N.D.

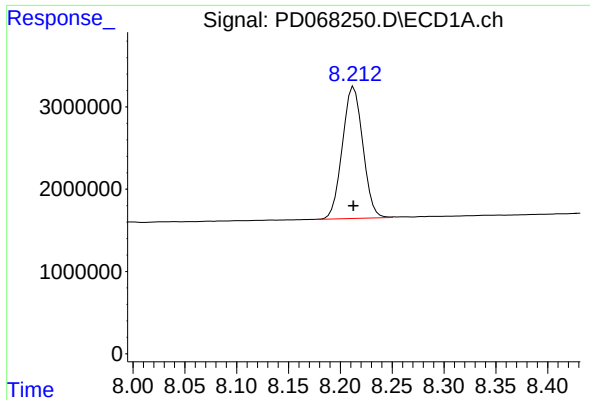

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 21979872
Conc: 18.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

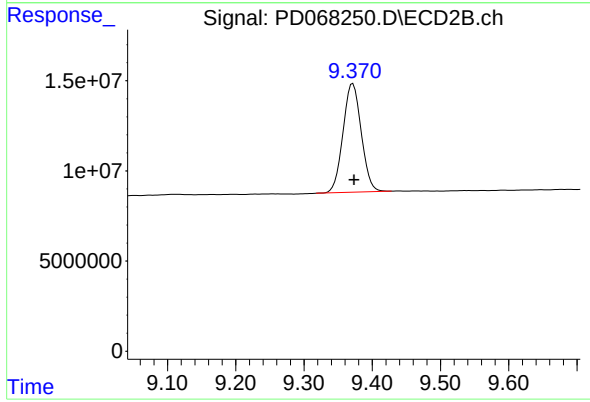

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.002 min
Response: 111970490
Conc: 18.89 ng/ml