

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
 Data File : PD068258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 19:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:38:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:37:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	98513684	651.4E6	69.325	68.269
28)	SA Decachlor...	8.213	9.372	85961399	397.0E6	68.556	66.755
Target Compounds							
23)	Chlordane-1	4.320	5.199	31016233	279.6E6	678.222	677.269
24)	Chlordane-2	4.822	5.672	35611633	267.6E6	667.100	666.285
25)	Chlordane-3	5.391	6.328	102.9E6	981.9E6	682.928	684.771
26)	Chlordane-4	5.450	6.405	87243755	1111.6E6	685.252	682.786
27)	Chlordane-5	6.287	7.217	36329315	196.9E6	682.937	672.680



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
Data File : PD068258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 19:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:38:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:37:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

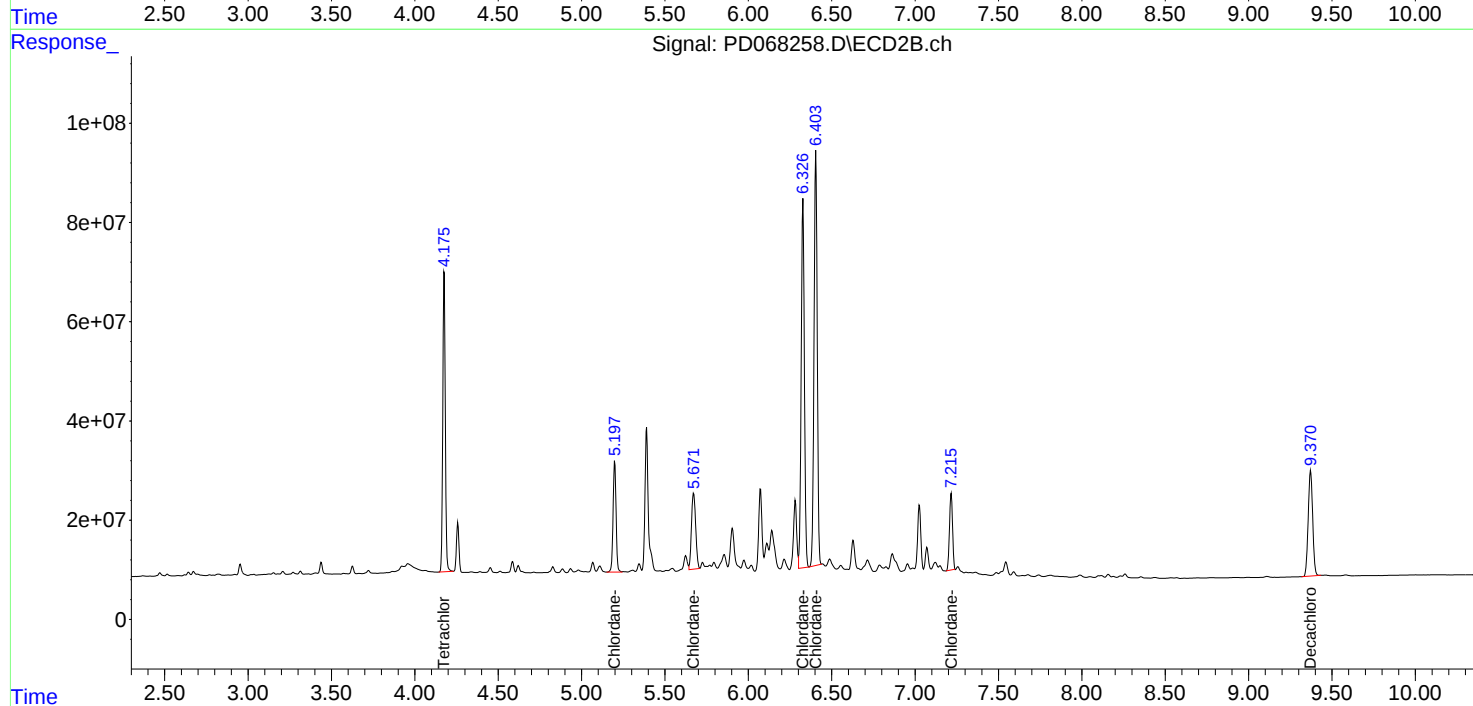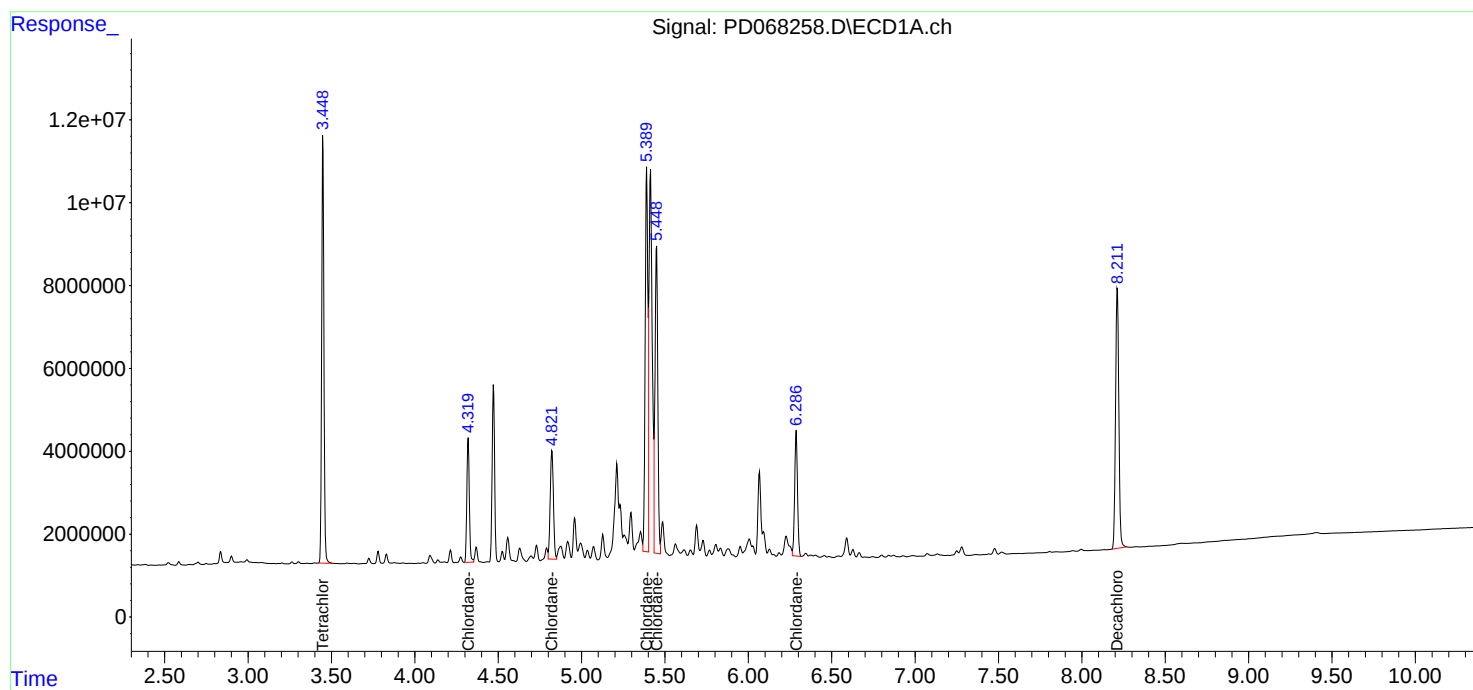


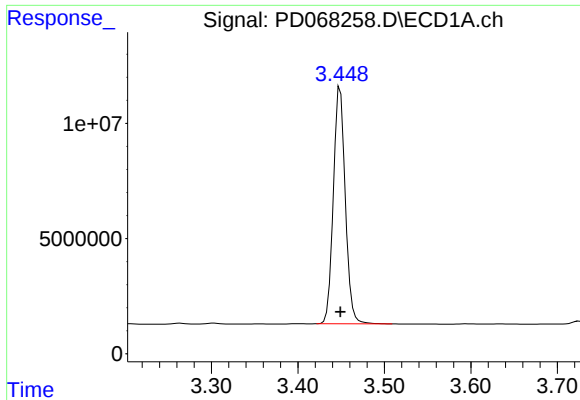

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 98513684
Conc: 69.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

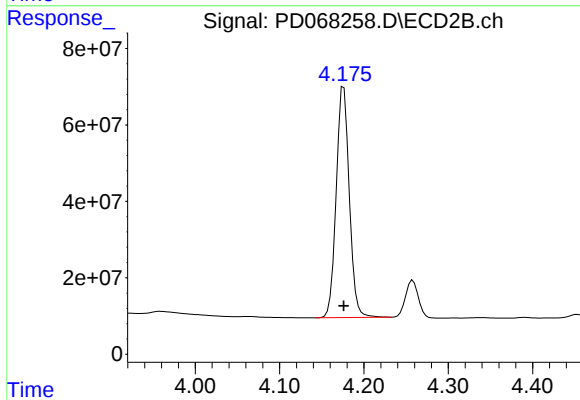


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 651422419
Conc: 68.27 ng/ml

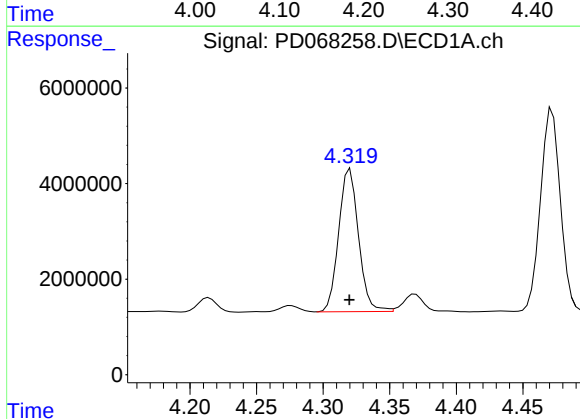


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 31016233
Conc: 678.22 ng/ml

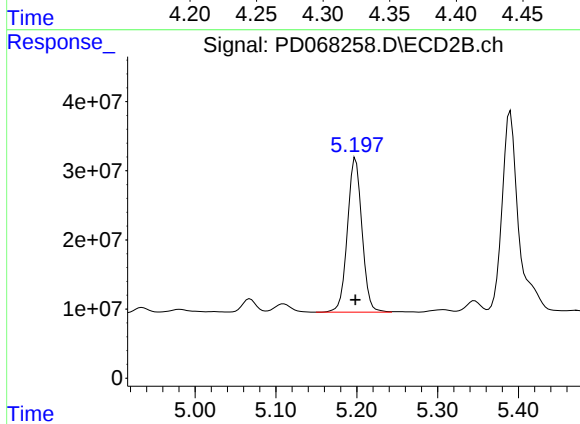

#23 Chlordane-1


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 279582154
Conc: 677.27 ng/ml

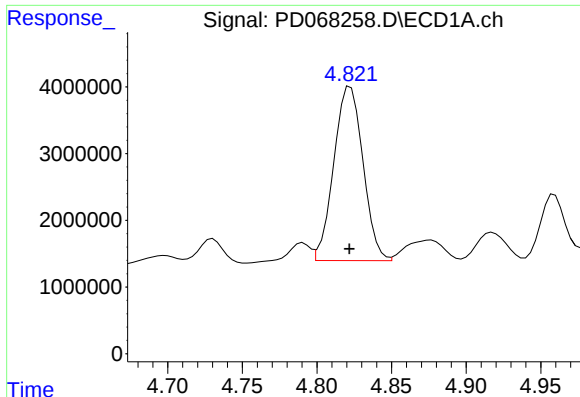

#24 Chlordane-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 35611633
Conc: 667.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

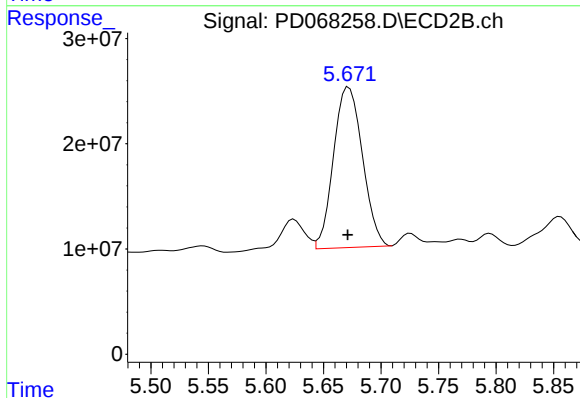


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 267556458
Conc: 666.28 ng/ml

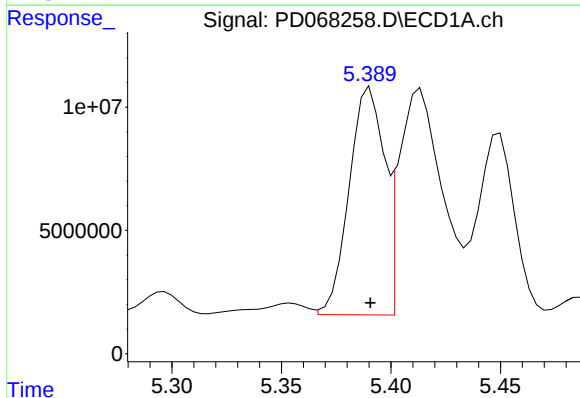


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 102924380
Conc: 682.93 ng/ml

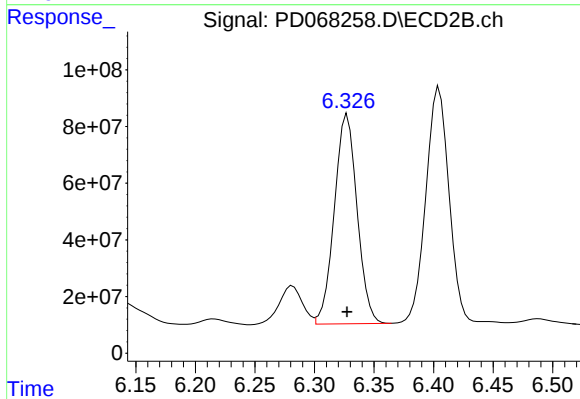

#25 Chlordane-3


R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 981892177
Conc: 684.77 ng/ml

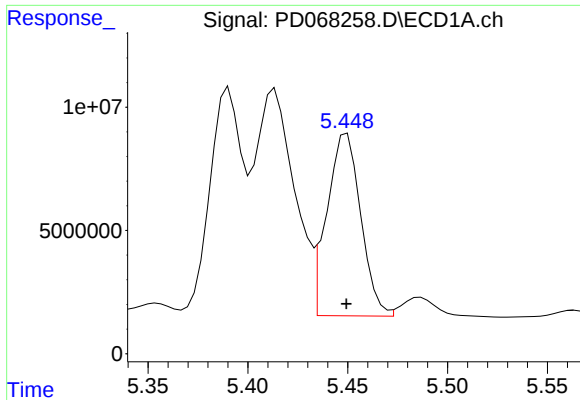

#26 Chlordane-4


R.T.: 5.450 min
Delta R.T.: 0.000 min
Response: 87243755
Conc: 685.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

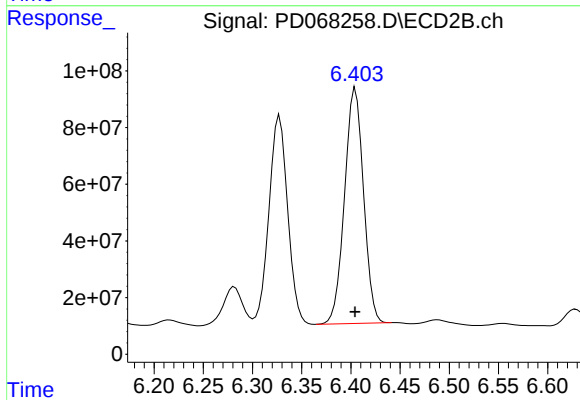


#26 Chlordane-4

R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 1111568593
Conc: 682.79 ng/ml

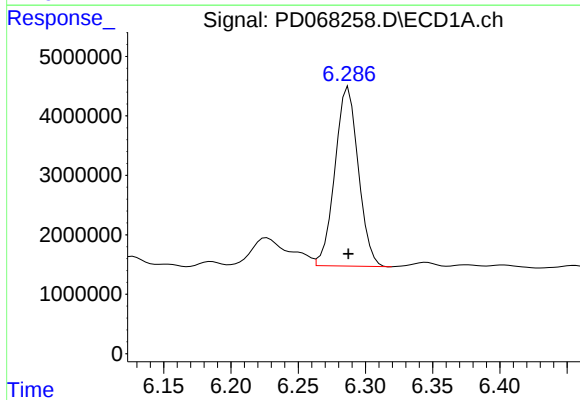


#27 Chlordane-5

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 36329315
Conc: 682.94 ng/ml

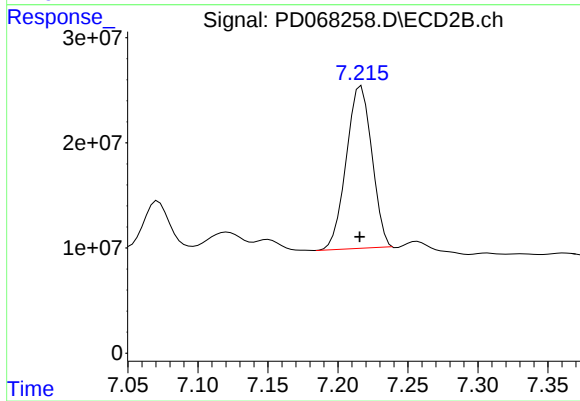

#27 Chlordane-5


R.T.: 7.217 min
Delta R.T.: 0.001 min
Response: 196899899
Conc: 672.68 ng/ml

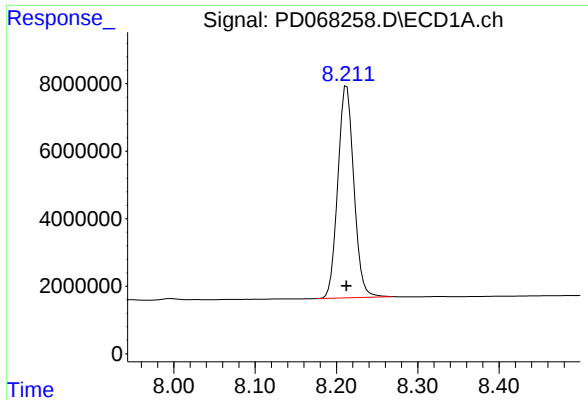

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 85961399
Conc: 68.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

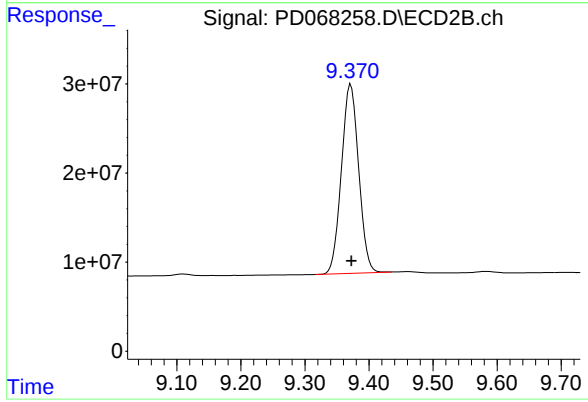

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 396964295
Conc: 66.75 ng/ml