

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
 Data File : PD068257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 19:06
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:38:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:37:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	138.9E6	895.8E6	97.750	93.878
28)	SA Decachlor...	8.212	9.372	116.2E6	537.1E6	92.639	90.328
Target Compounds							
23)	Chlordane-1	4.320	5.199	43440319	383.1E6	949.895	928.051
24)	Chlordane-2	4.822	5.671	48667786	360.8E6	911.676	898.586
25)	Chlordane-3	5.391	6.327	148.5E6	1358.3E6	985.554	947.299
26)	Chlordane-4	5.449	6.405	122.5E6	1529.3E6	962.538	939.372
27)	Chlordane-5	6.288	7.216	50848405	272.3E6	955.874	930.178



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
Data File : PD068257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 19:06
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:38:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:37:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

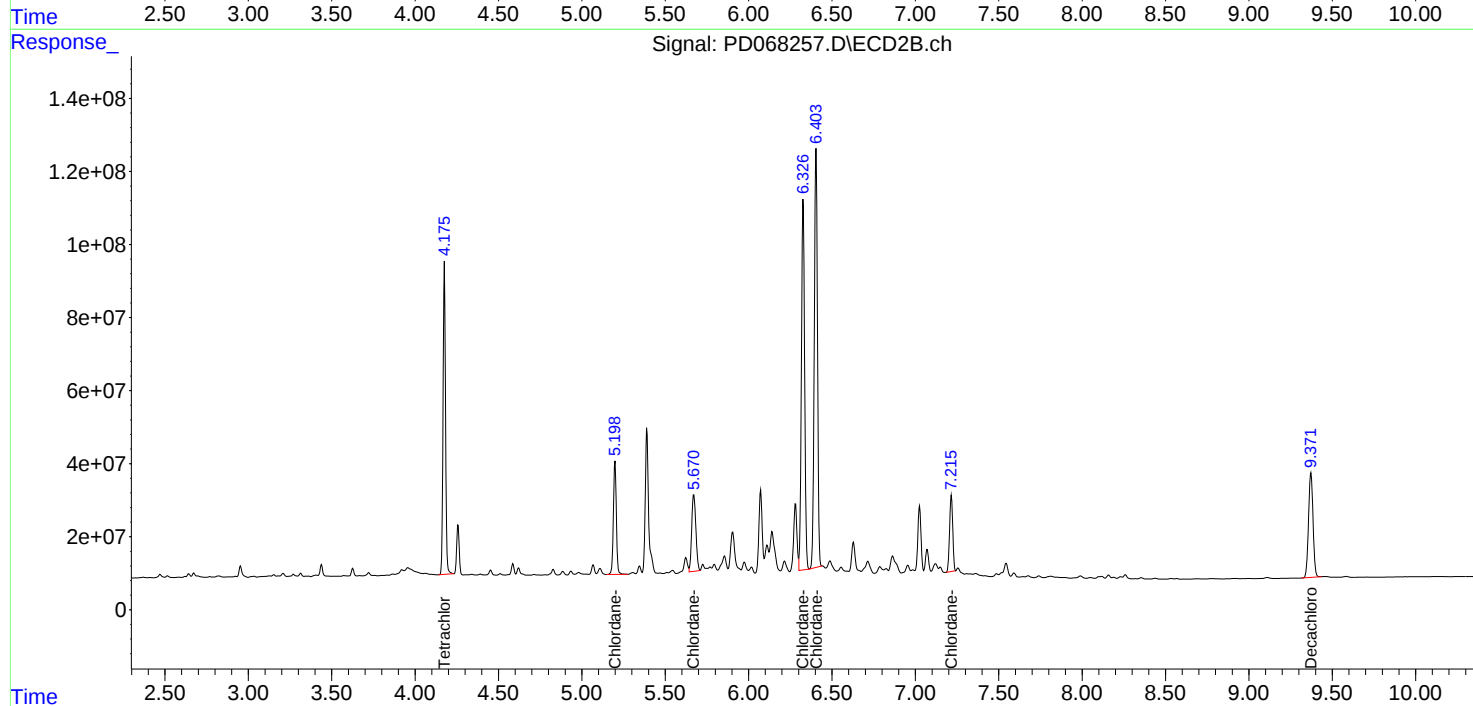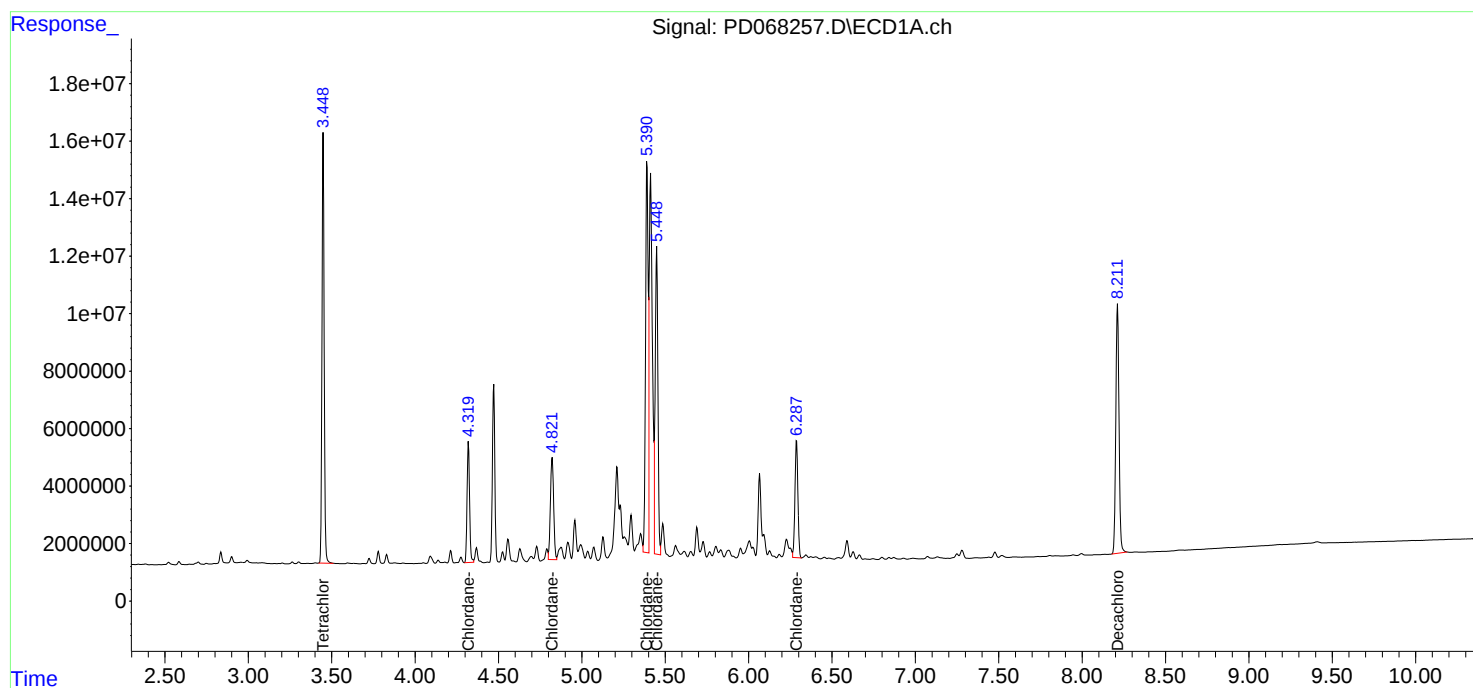


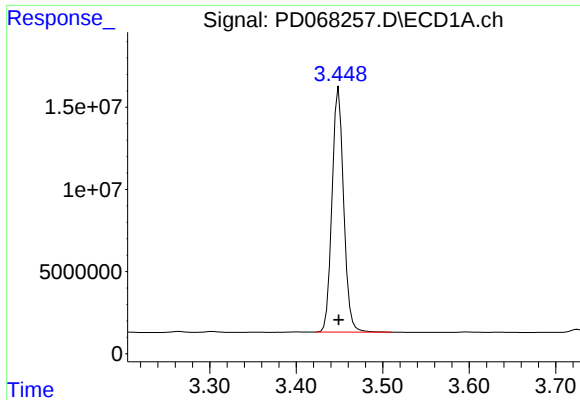

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 138907584
Conc: 97.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

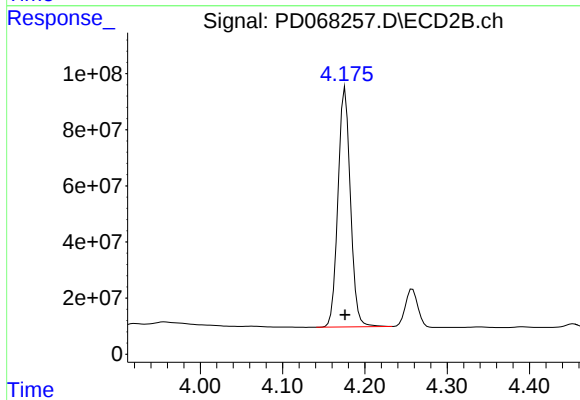


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 895787766
Conc: 93.88 ng/ml

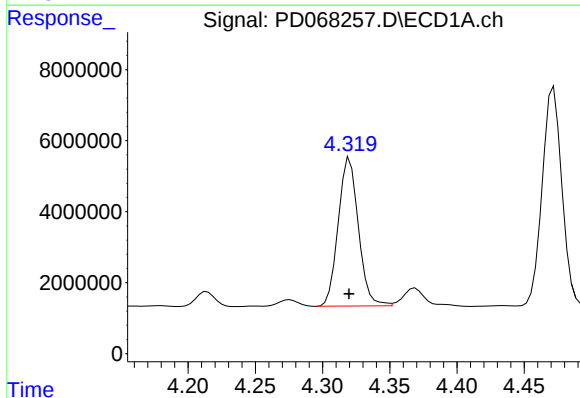


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 43440319
Conc: 949.90 ng/ml

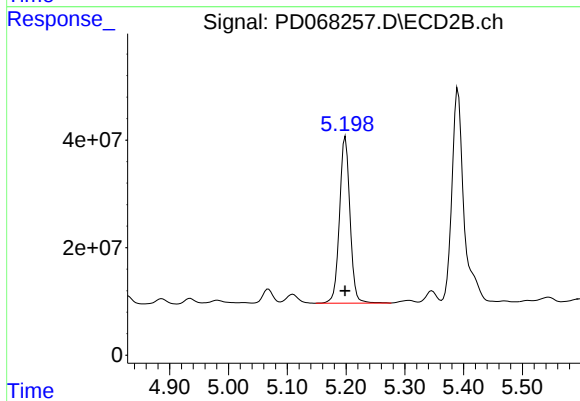

#23 Chlordane-1


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 383107062
Conc: 928.05 ng/ml

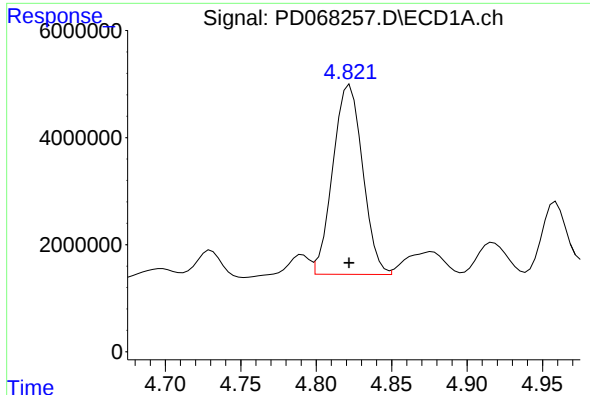

#24 Chlordane-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 48667786
Conc: 911.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

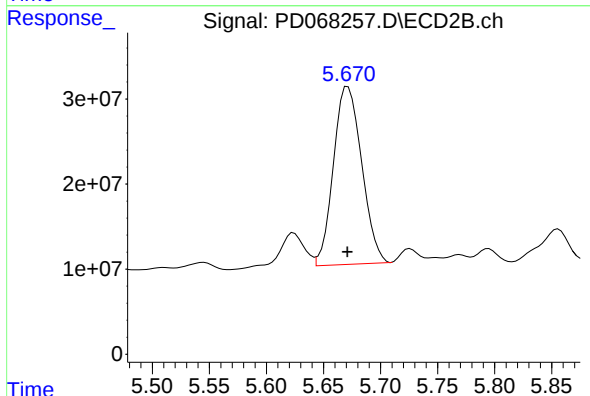


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 360840331
Conc: 898.59 ng/ml

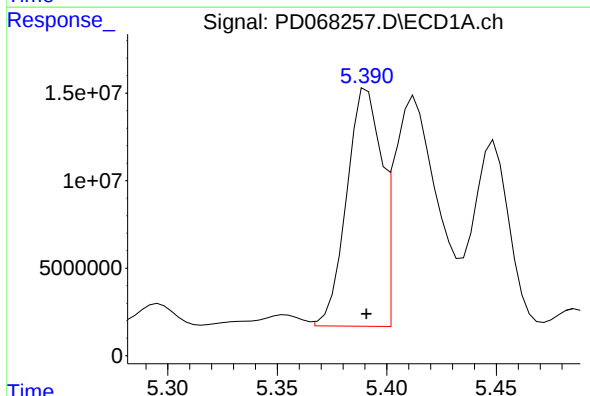


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 148533294
Conc: 985.55 ng/ml

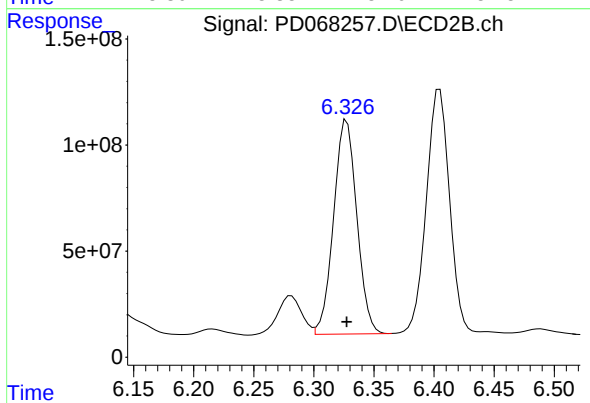

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 1358330865
Conc: 947.30 ng/ml

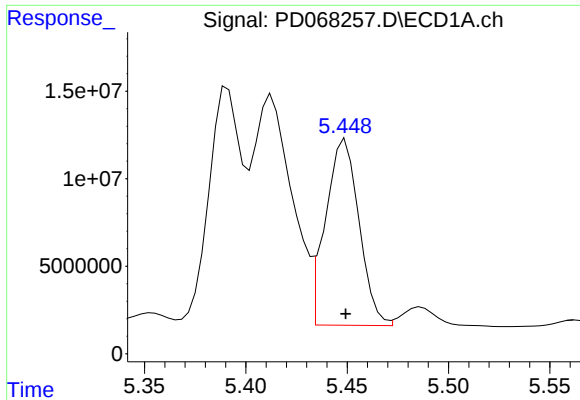

#26 Chlordane-4


R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 122546662
Conc: 962.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

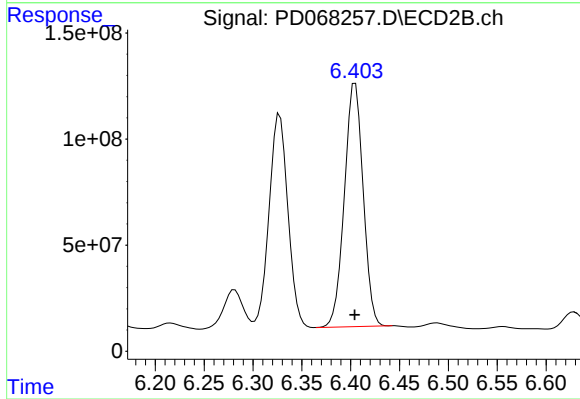


#26 Chlordane-4

R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 1529287933
Conc: 939.37 ng/ml

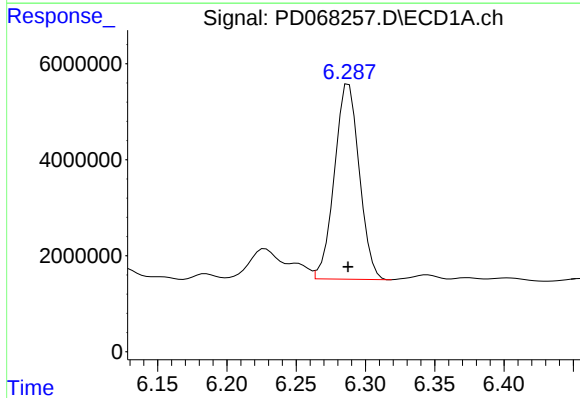


#27 Chlordane-5

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 50848405
Conc: 955.87 ng/ml

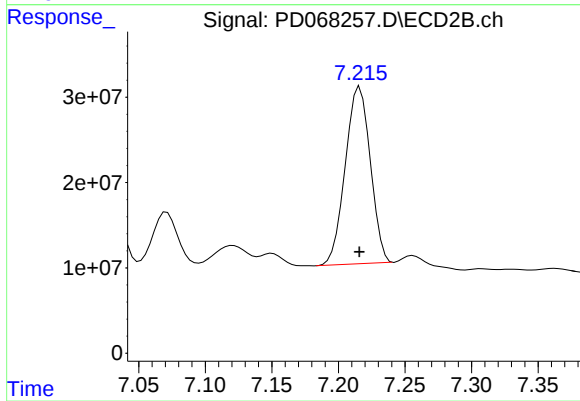

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 272272215
Conc: 930.18 ng/ml

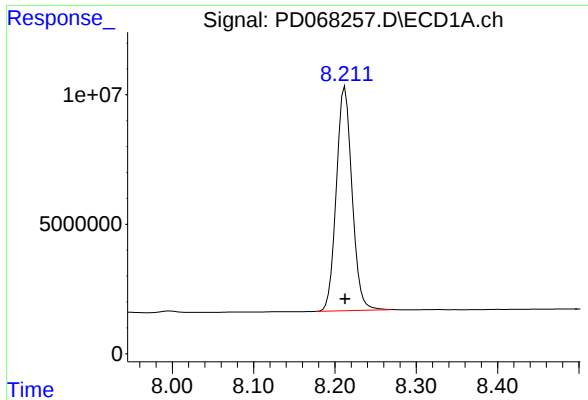

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 116158957
Conc: 92.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

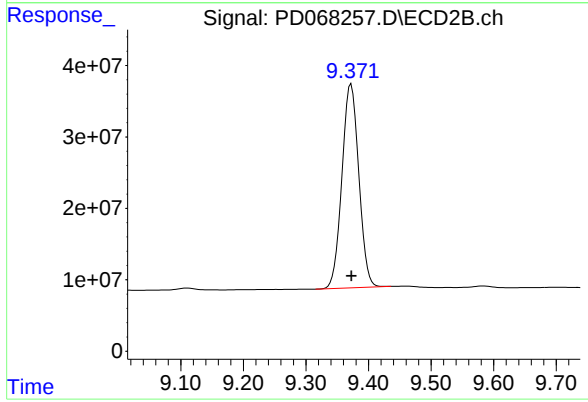

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 537147524
Conc: 90.33 ng/ml