

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
 Data File : PD068259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 19:34
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:38:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:37:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	71052396	477.1E6	50.000	50.000
28)	SA Decachlor...	8.212	9.373	62694116	297.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.320	5.198	22865852	206.4E6	500.000	500.000
24)	Chlordane-2	4.822	5.671	26691379	200.8E6	500.000	500.000
25)	Chlordane-3	5.391	6.327	75355194	716.9E6	500.000	500.000
26)	Chlordane-4	5.449	6.404	63658121	814.0E6	500.000	500.000
27)	Chlordane-5	6.287	7.216	26597850	146.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
Data File : PD068259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 19:34
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:38:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:37:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

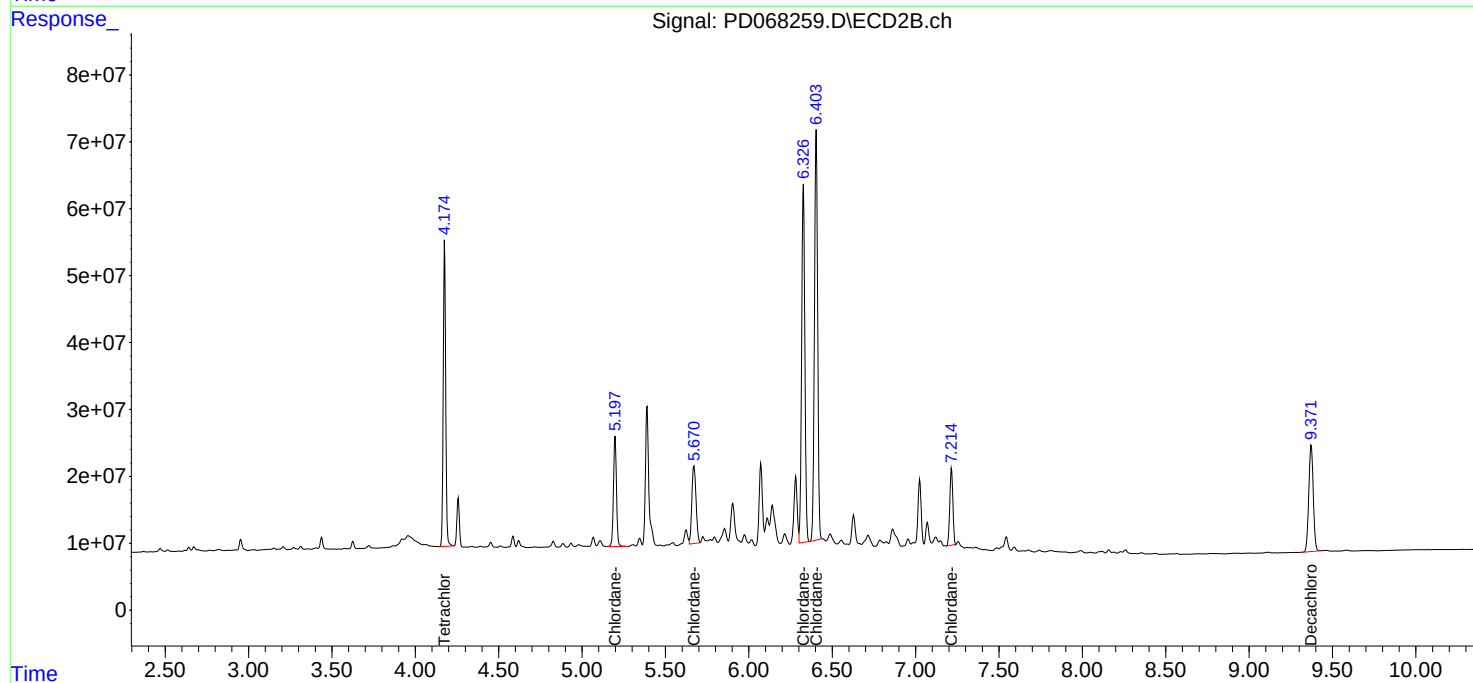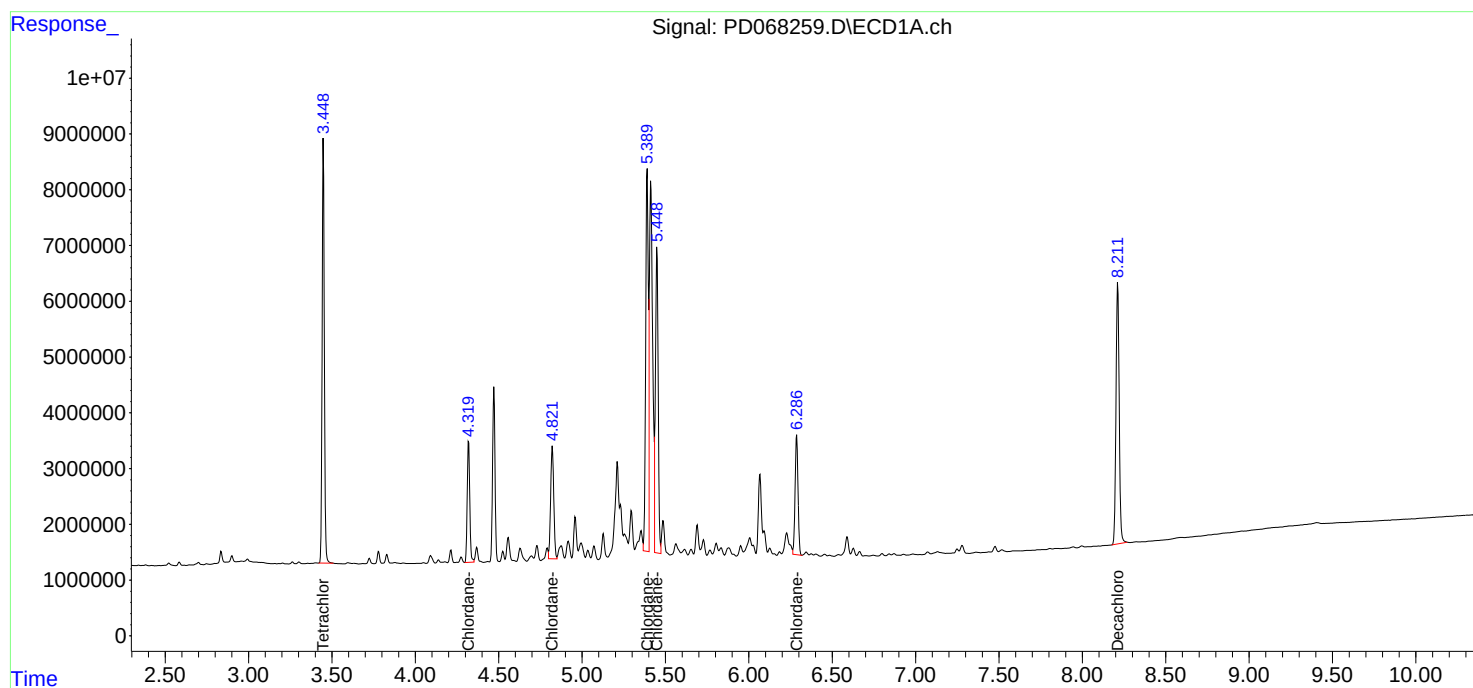


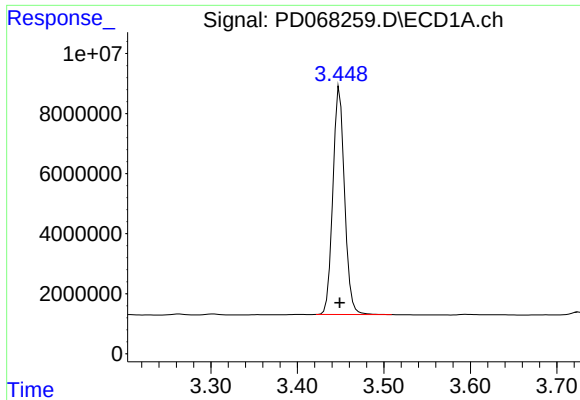

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 71052396
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

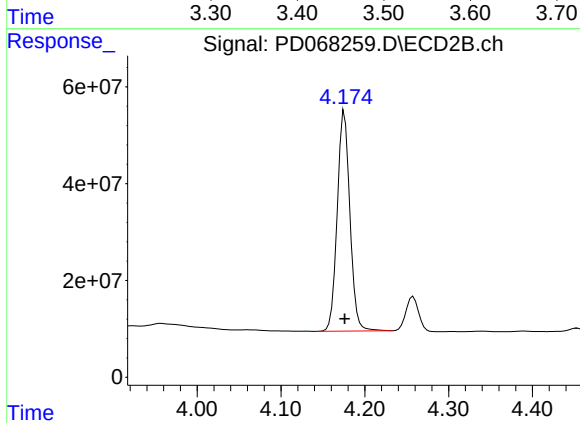


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 477102150
Conc: 50.00 ng/ml

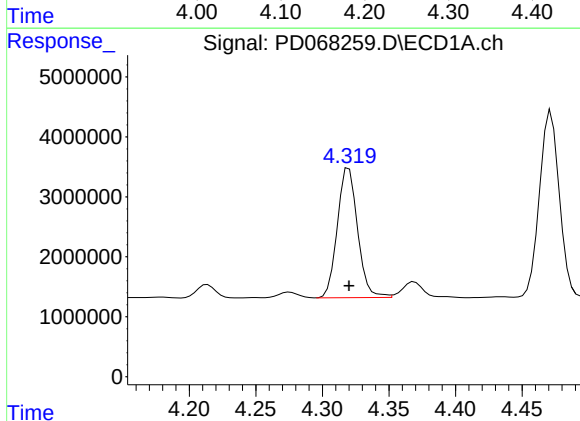


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 22865852
Conc: 500.00 ng/ml

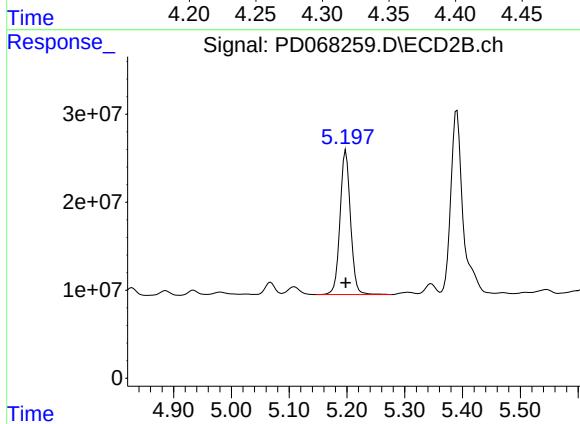

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 206404179
Conc: 500.00 ng/ml

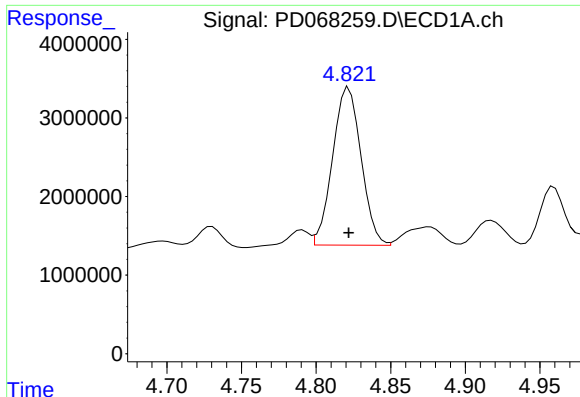

#24 Chlordane-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 26691379
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

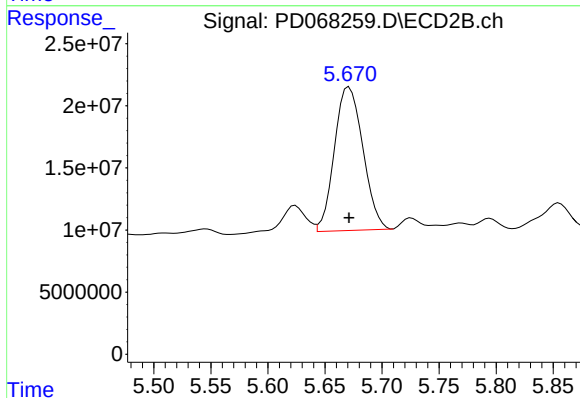


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 200782298
Conc: 500.00 ng/ml

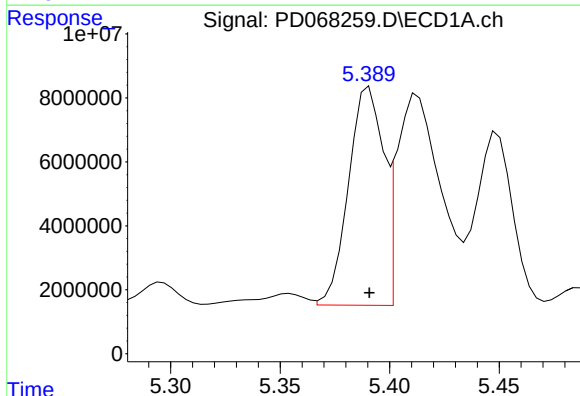


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 75355194
Conc: 500.00 ng/ml

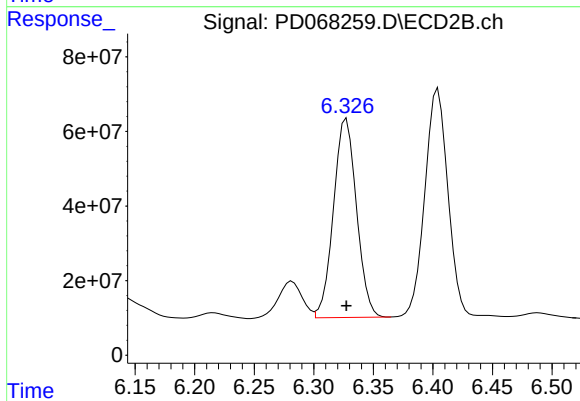

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 716949523
Conc: 500.00 ng/ml

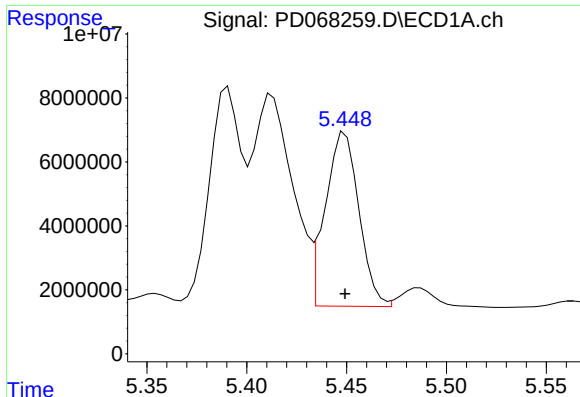

#26 Chlordane-4


R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 63658121
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

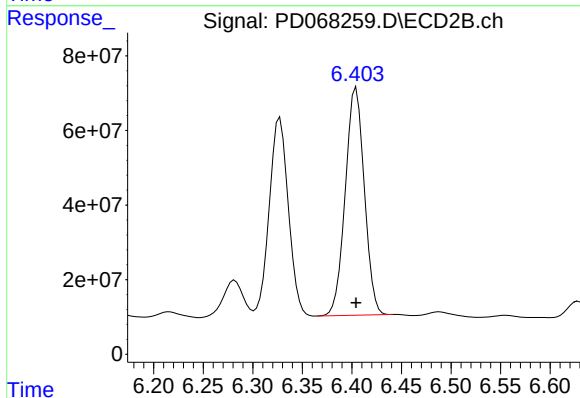


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 813994995
Conc: 500.00 ng/ml

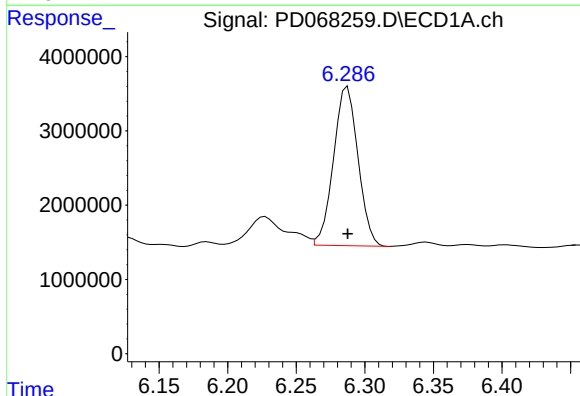


#27 Chlordane-5

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 26597850
Conc: 500.00 ng/ml

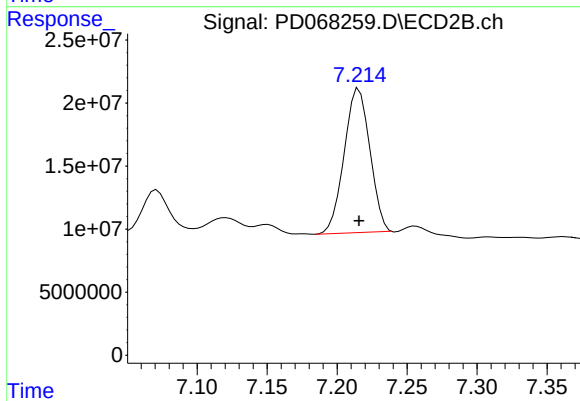

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 146354838
Conc: 500.00 ng/ml

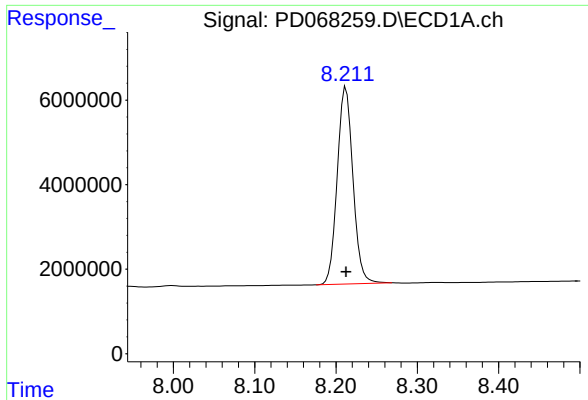

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 62694116
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

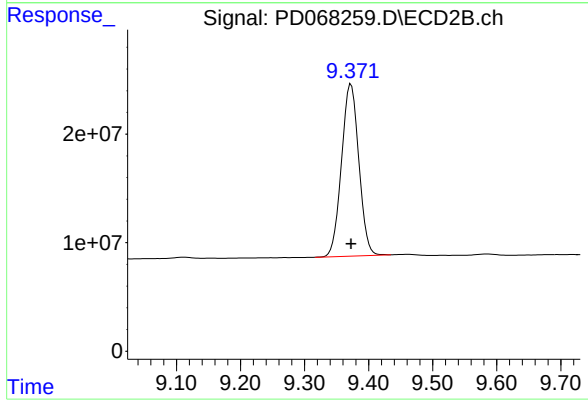

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 297331397
Conc: 50.00 ng/ml