

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
 Data File : PD068260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 19:48
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:38:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:37:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	33184231	243.3E6	23.352	25.500
28)	SA Decachlor...	8.212	9.372	30279790	151.4E6	24.149	25.452
Target Compounds							
23)	Chlordane-1	4.320	5.198	10989519	105.0E6	240.304	254.340
24)	Chlordane-2	4.823	5.671	13480757	105.0E6	252.530	261.574
25)	Chlordane-3	5.391	6.327	34727556	358.9E6	230.426	250.268
26)	Chlordane-4	5.449	6.404	30228836	410.1E6	237.431	251.926
27)	Chlordane-5	6.288	7.216	12613485	73611335	237.115	251.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
Data File : PD068260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 19:48
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:38:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:37:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

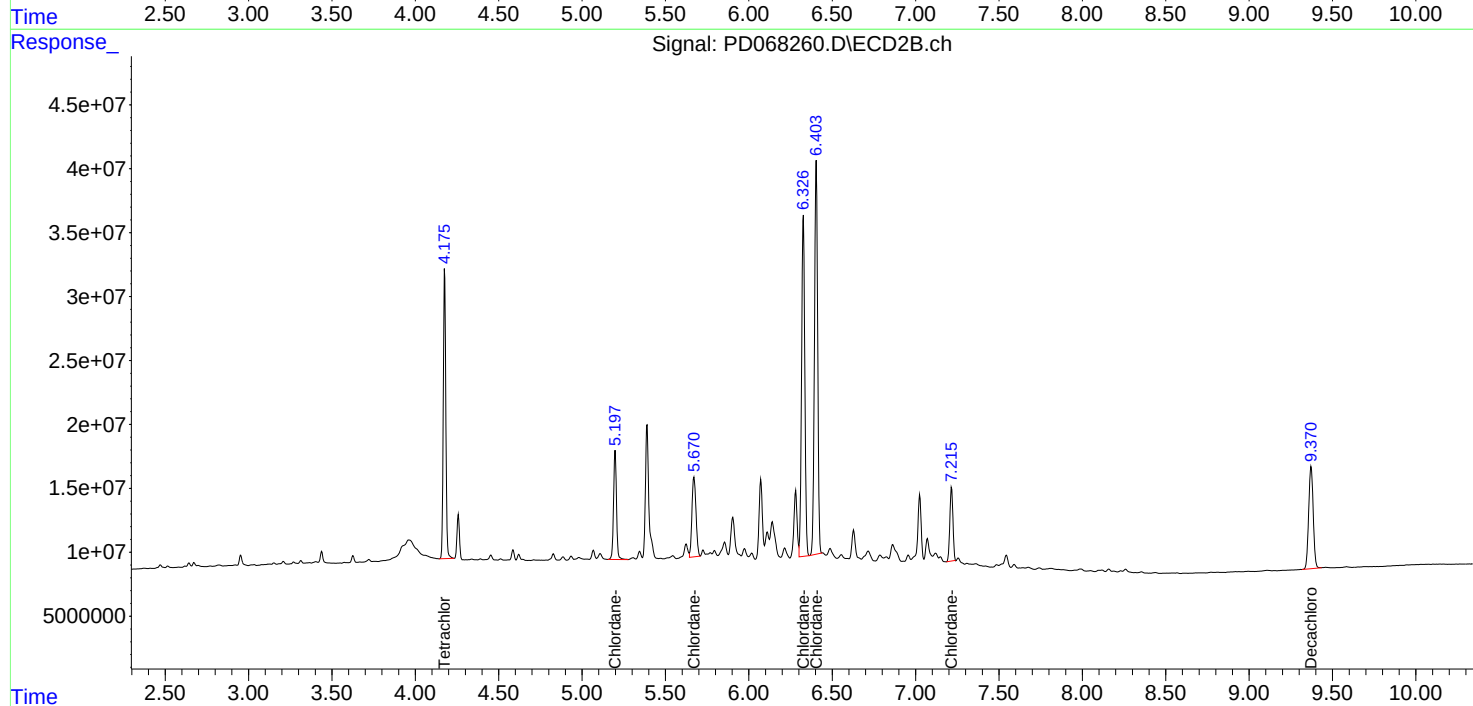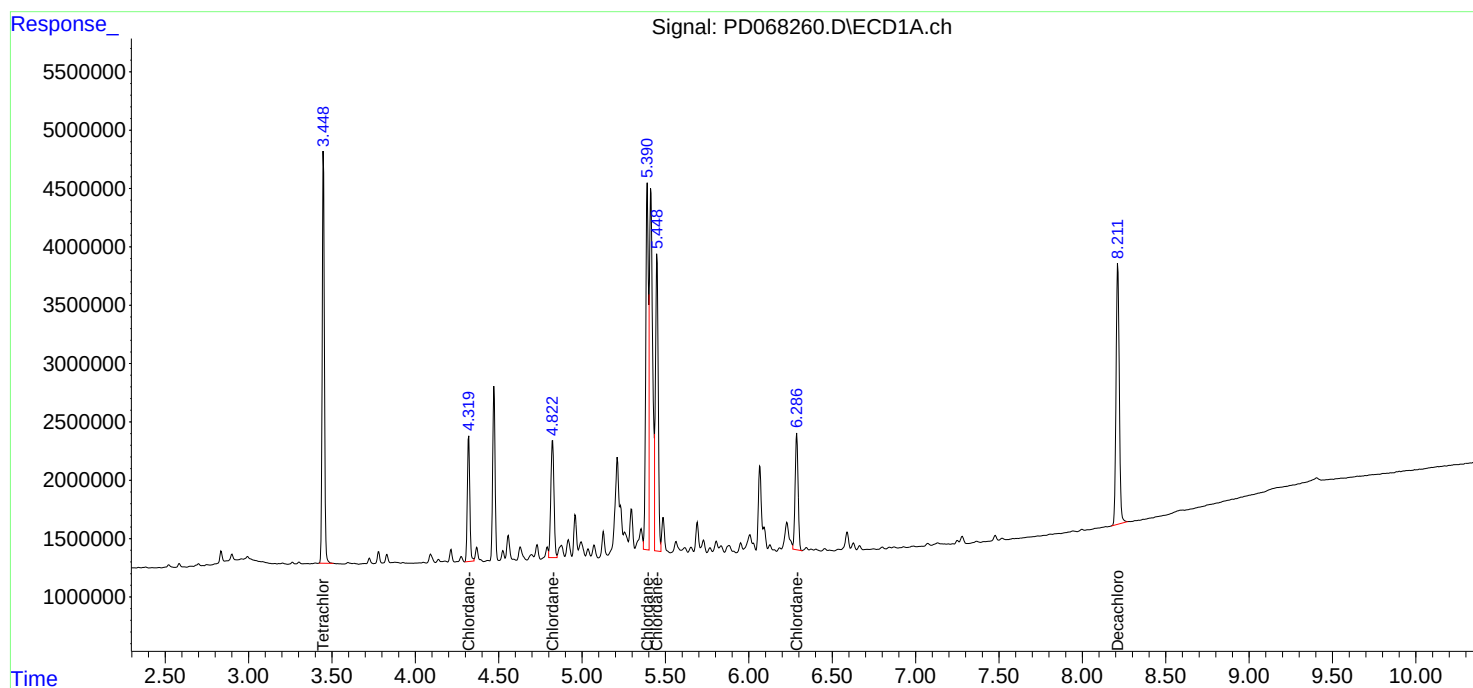


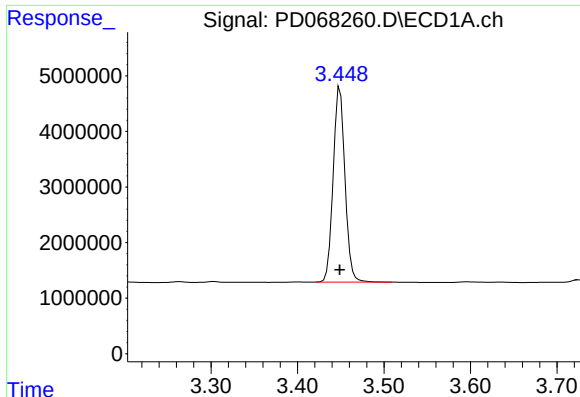

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 33184231
Conc: 23.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

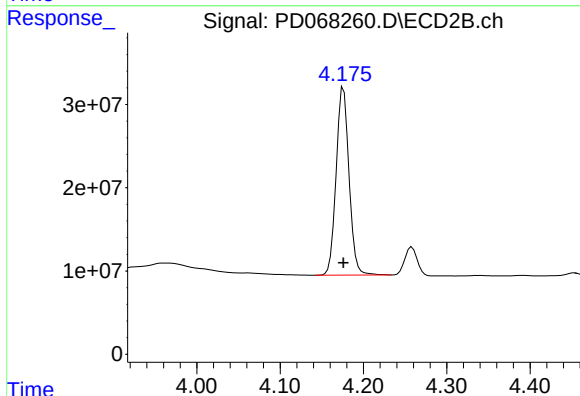


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 243322017
Conc: 25.50 ng/ml

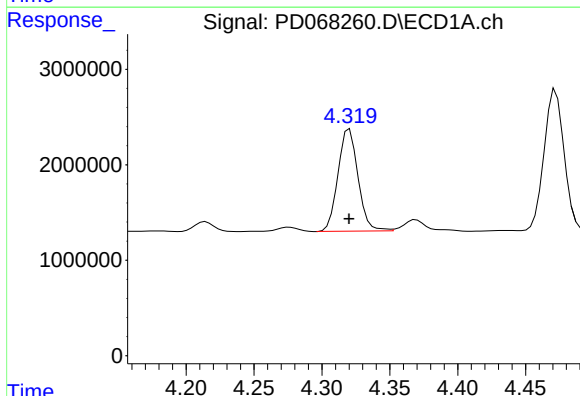


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 10989519
Conc: 240.30 ng/ml

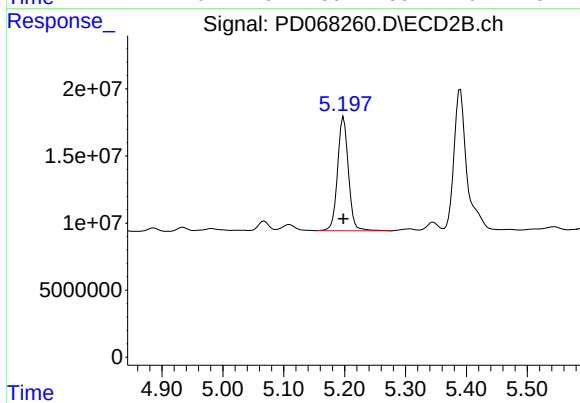

#23 Chlordane-1


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 104993795
Conc: 254.34 ng/ml

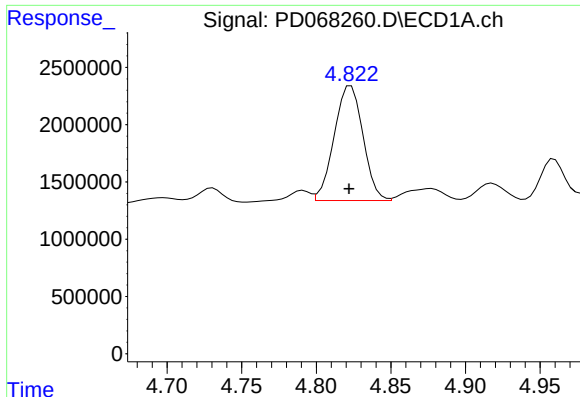

#24 Chlordane-2


R.T.: 4.823 min
Delta R.T.: 0.001 min
Response: 13480757
Conc: 252.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

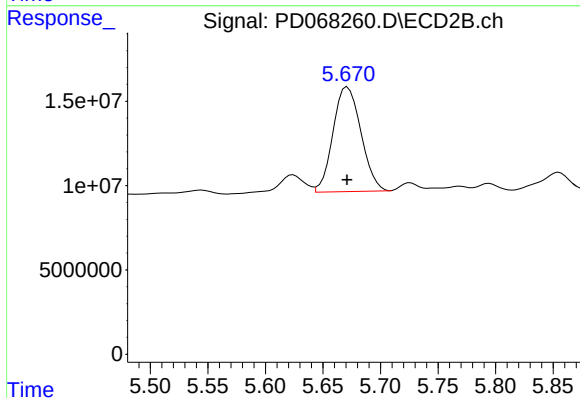


#24 Chlordane-2

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 105038941
Conc: 261.57 ng/ml

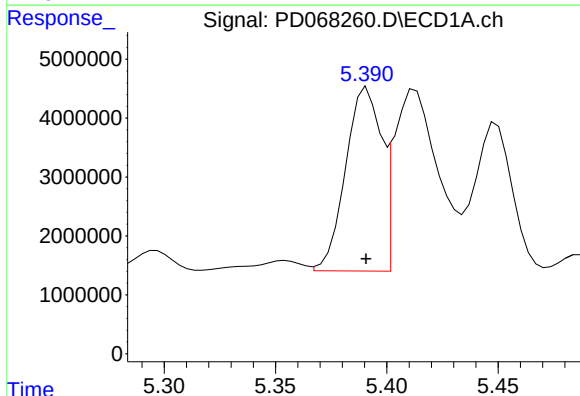


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 34727556
Conc: 230.43 ng/ml

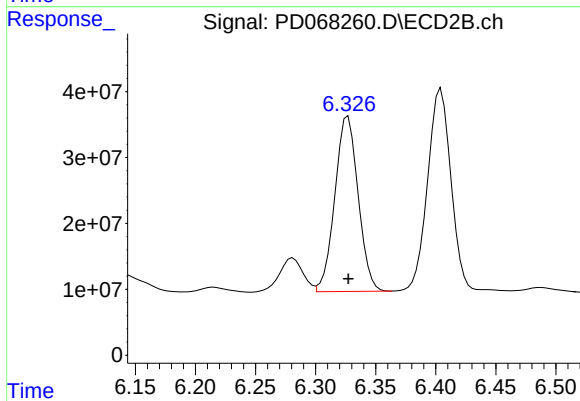

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 358858780
Conc: 250.27 ng/ml

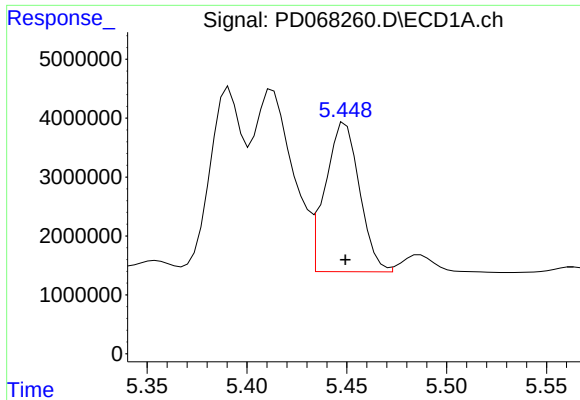

#26 Chlordane-4


R.T.: 5.449 min
Delta R.T.: 0.000 min
Response: 30228836
Conc: 237.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

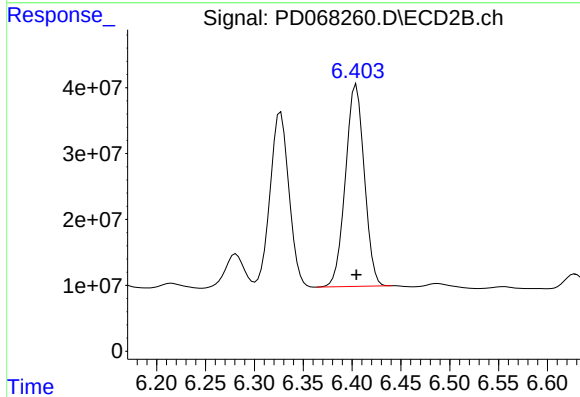


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 410132485
Conc: 251.93 ng/ml

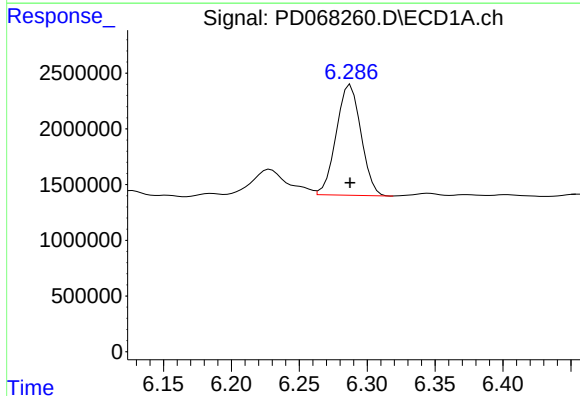


#27 Chlordane-5

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 12613485
Conc: 237.11 ng/ml

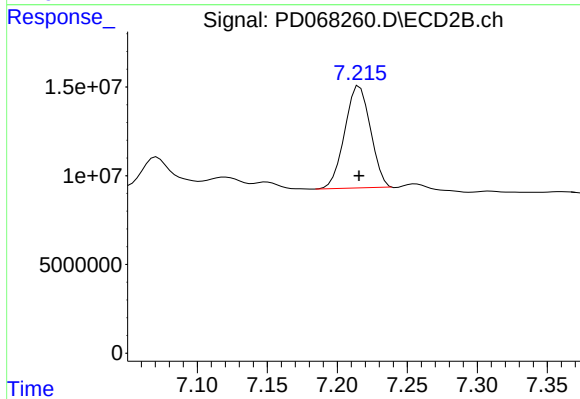

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 73611335
Conc: 251.48 ng/ml

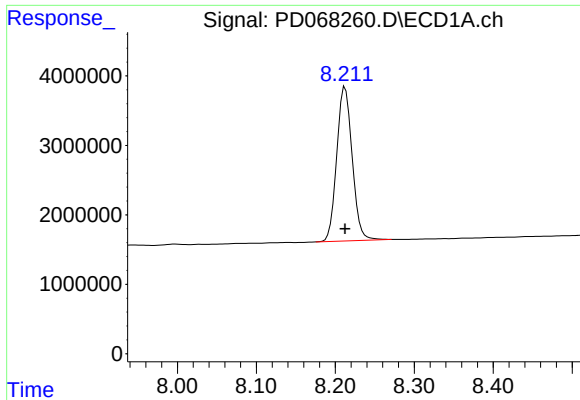

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 30279790
Conc: 24.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

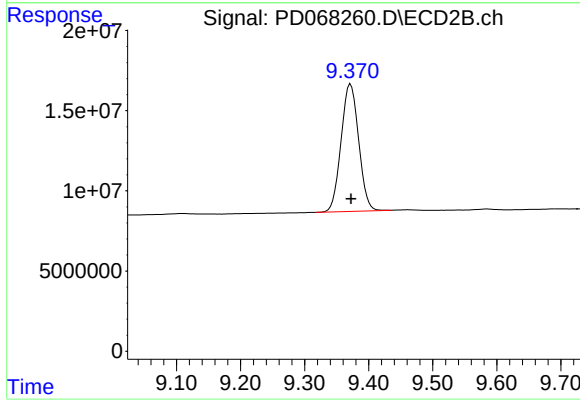

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: 0.000 min
Response: 151355769
Conc: 25.45 ng/ml