

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
 Data File : PD068268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 21:40
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD030122CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 06:43:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:43:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	73992239	481.1E6	54.831	50.833
28)	SA Decachlor...	8.213	9.373	64410740	296.9E6	52.706	50.391
Target Compounds							
23)	Chlordane-1	4.320	5.199	23861014	206.9E6	546.967	510.990
24)	Chlordane-2	4.823	5.672	27914443	201.3E6	540.698	500.792
25)	Chlordane-3	5.391	6.327	77878083	717.1E6	544.349	504.279
26)	Chlordane-4	5.450	6.404	66421712	812.8E6	543.685	504.261
27)	Chlordane-5	6.288	7.216	27381695	145.7E6	555.900	507.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030122\
Data File : PD068268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 21:40
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD030122CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 06:43:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:43:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

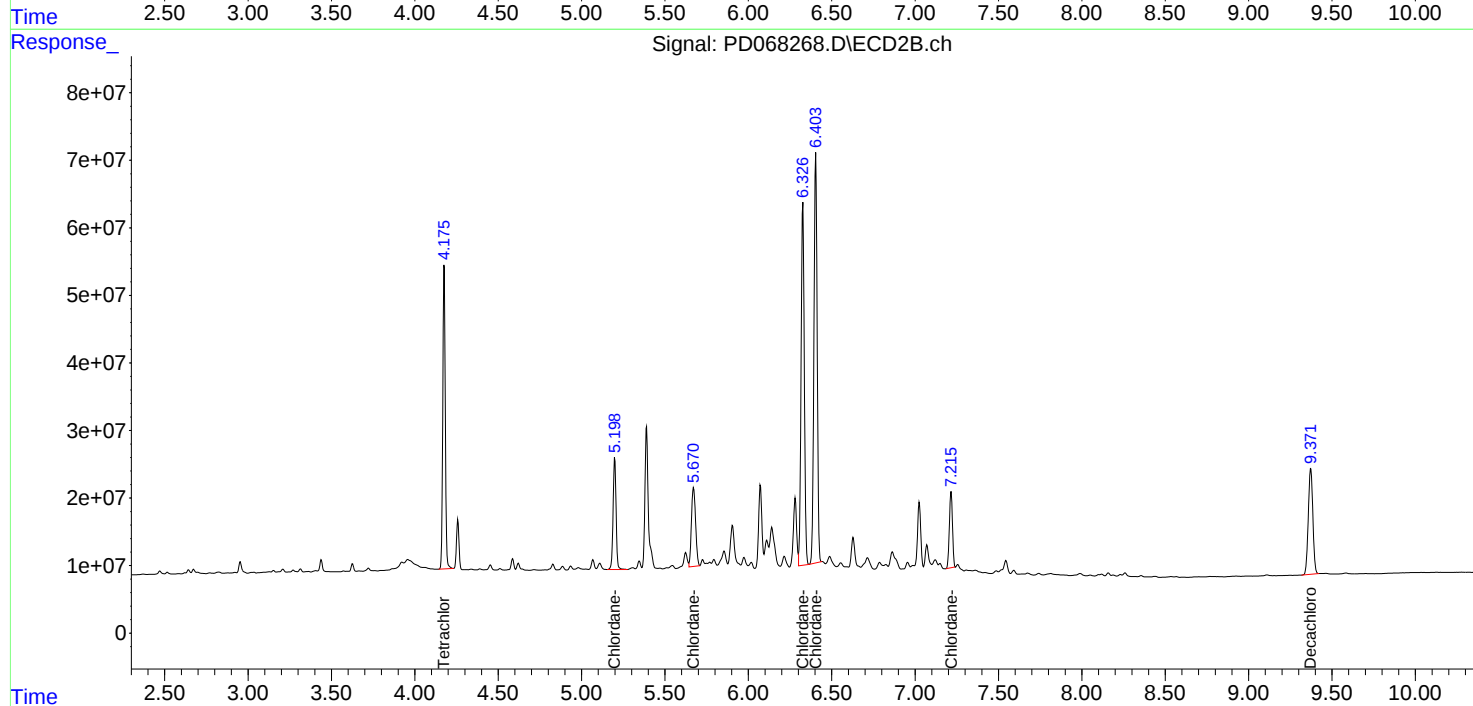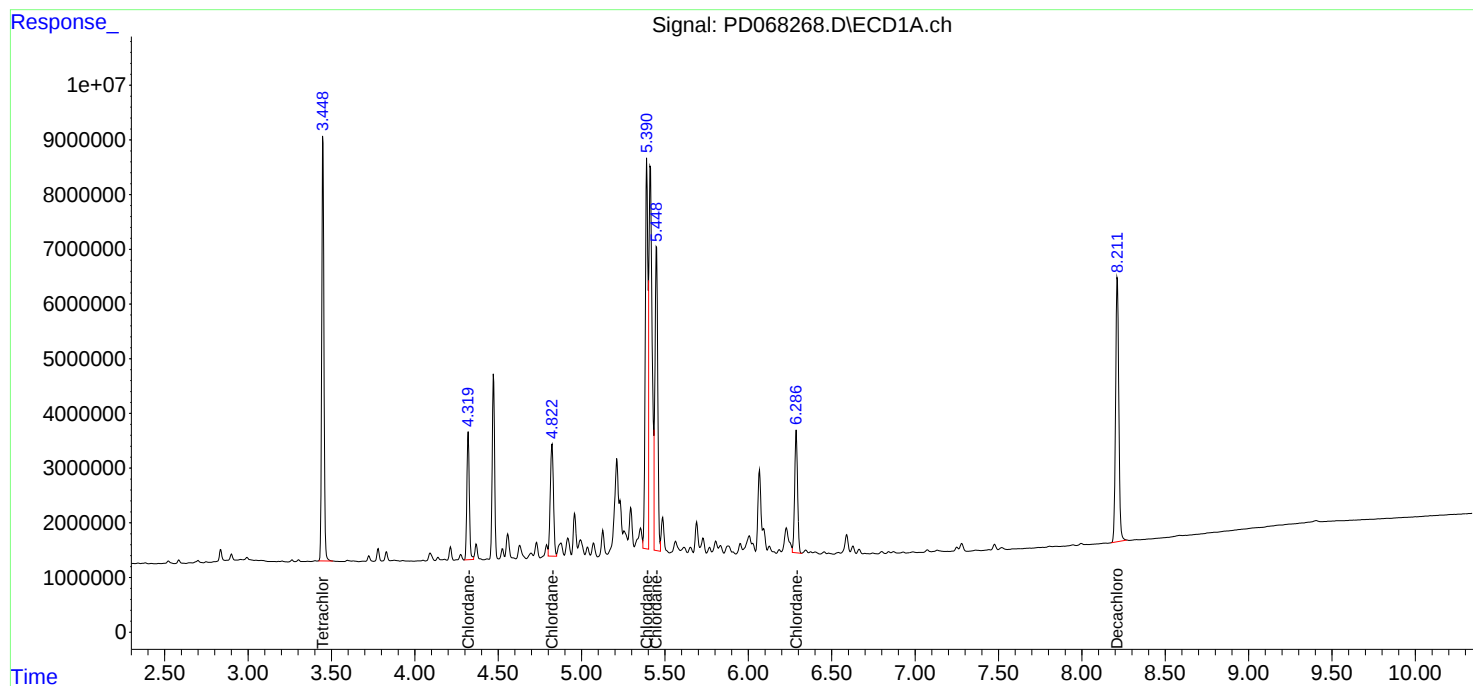


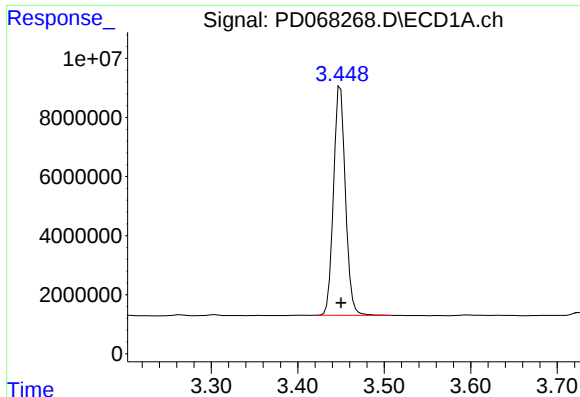

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 73992239
Conc: 54.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030122CHLOR

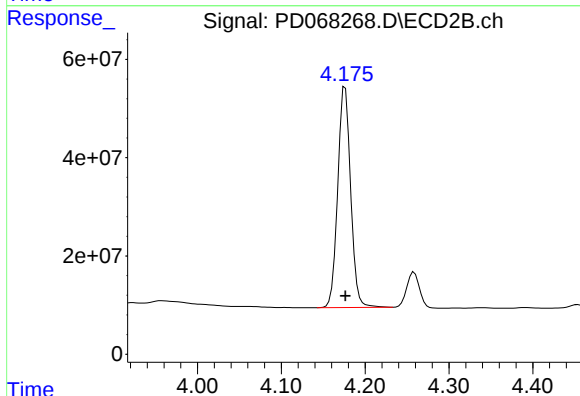


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 481055263
Conc: 50.83 ng/ml

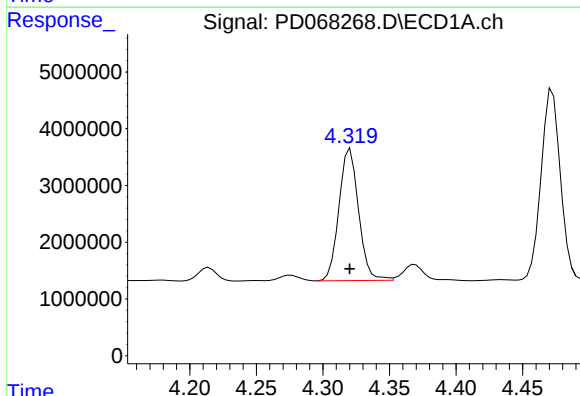


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 23861014
Conc: 546.97 ng/ml

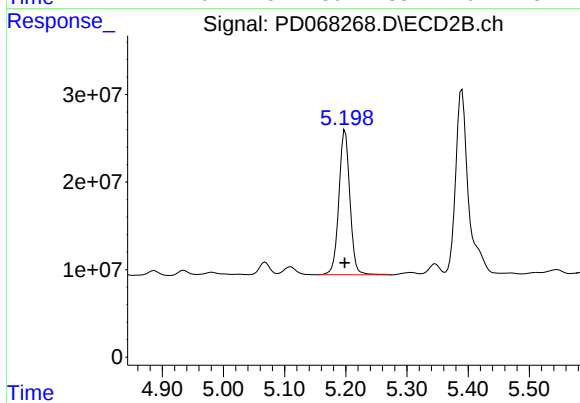

#23 Chlordane-1


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 206947667
Conc: 510.99 ng/ml

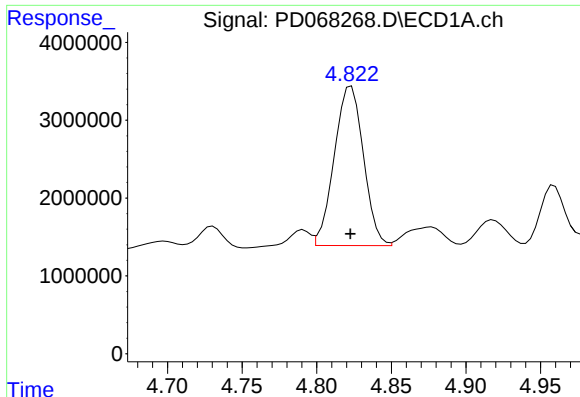

#24 Chlordane-2


R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 27914443
Conc: 540.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030122CHLOR

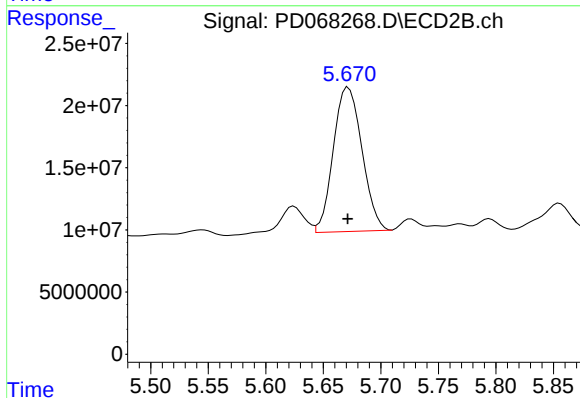


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 201326017
Conc: 500.79 ng/ml

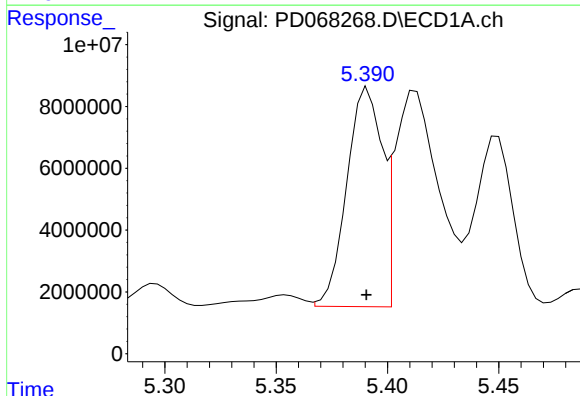


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 77878083
Conc: 544.35 ng/ml

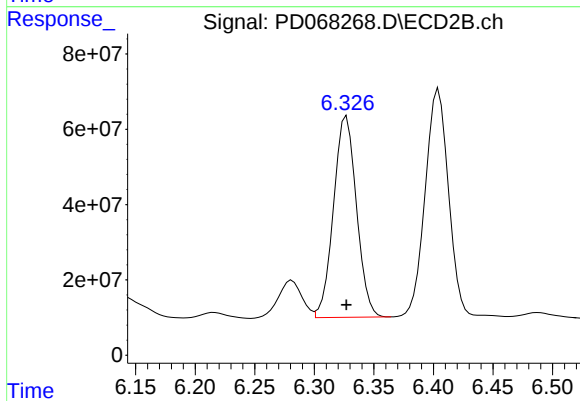

#25 Chlordane-3


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 717128817
Conc: 504.28 ng/ml

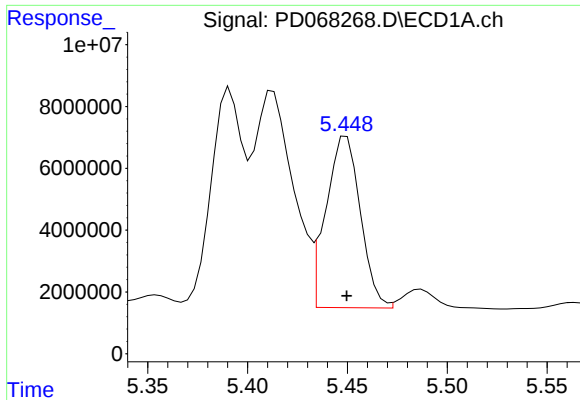

#26 Chlordane-4


R.T.: 5.450 min
Delta R.T.: 0.000 min
Response: 66421712
Conc: 543.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030122CHLOR

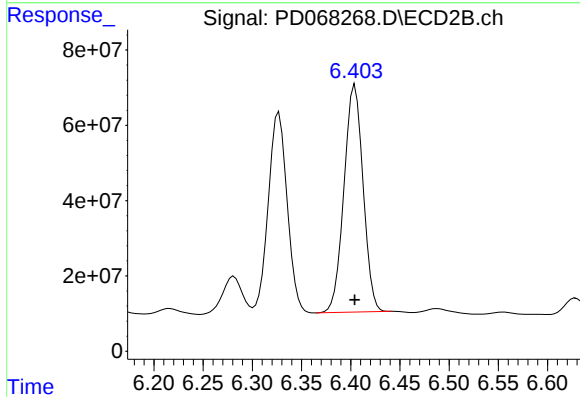


#26 Chlordane-4

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 812753013
Conc: 504.26 ng/ml

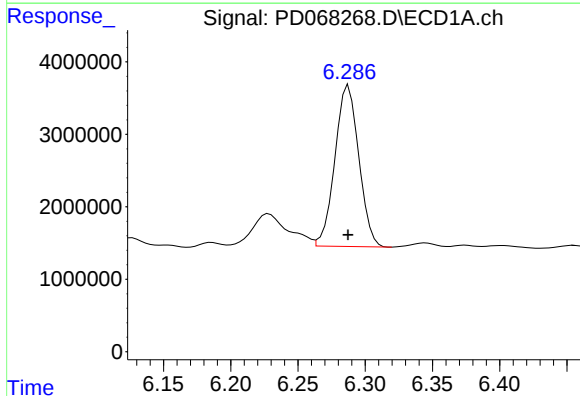


#27 Chlordane-5

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 27381695
Conc: 555.90 ng/ml

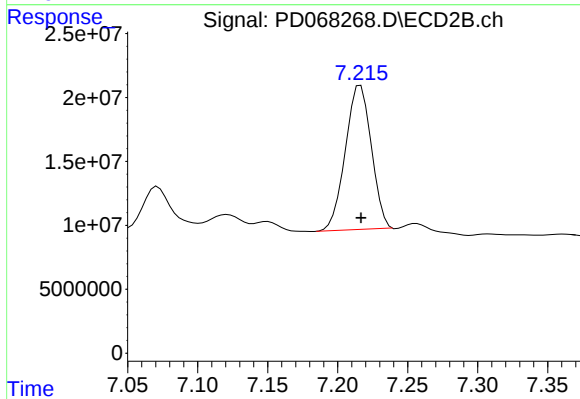

#27 Chlordane-5


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 145676124
Conc: 507.88 ng/ml

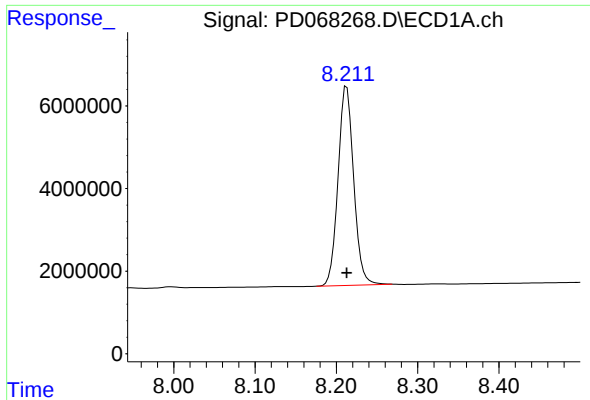

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 64410740
Conc: 52.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030122CHLOR

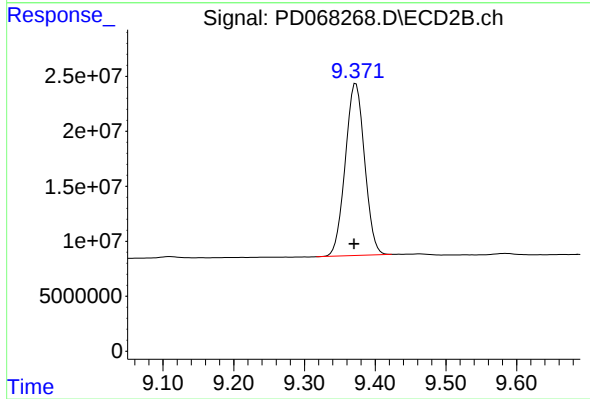

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.002 min
Response: 296852866
Conc: 50.39 ng/ml