

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
 Data File : PD074064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 20:40
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 01:02:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 00:56:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.774	173.7E6	110.4E6	74.734	74.872
28)	SA Decachlor...	9.098	7.929	189.0E6	89274810	74.378	74.141
Target Compounds							
23)	Chlordane-1	4.719	3.776	88865338	37183885	750.540	745.739
24)	Chlordane-2	5.249	4.353	94021735	42245232	744.745	740.947
25)	Chlordane-3	5.963	4.985	390.6E6	128.2E6	748.492	749.873
26)	Chlordane-4	6.045	5.049	470.7E6	121.3E6	747.375	747.149
27)	Chlordane-5	6.897	5.946	81046754	45980884	744.192	745.468



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
Data File : PD074064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 20:40
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 01:02:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 00:56:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

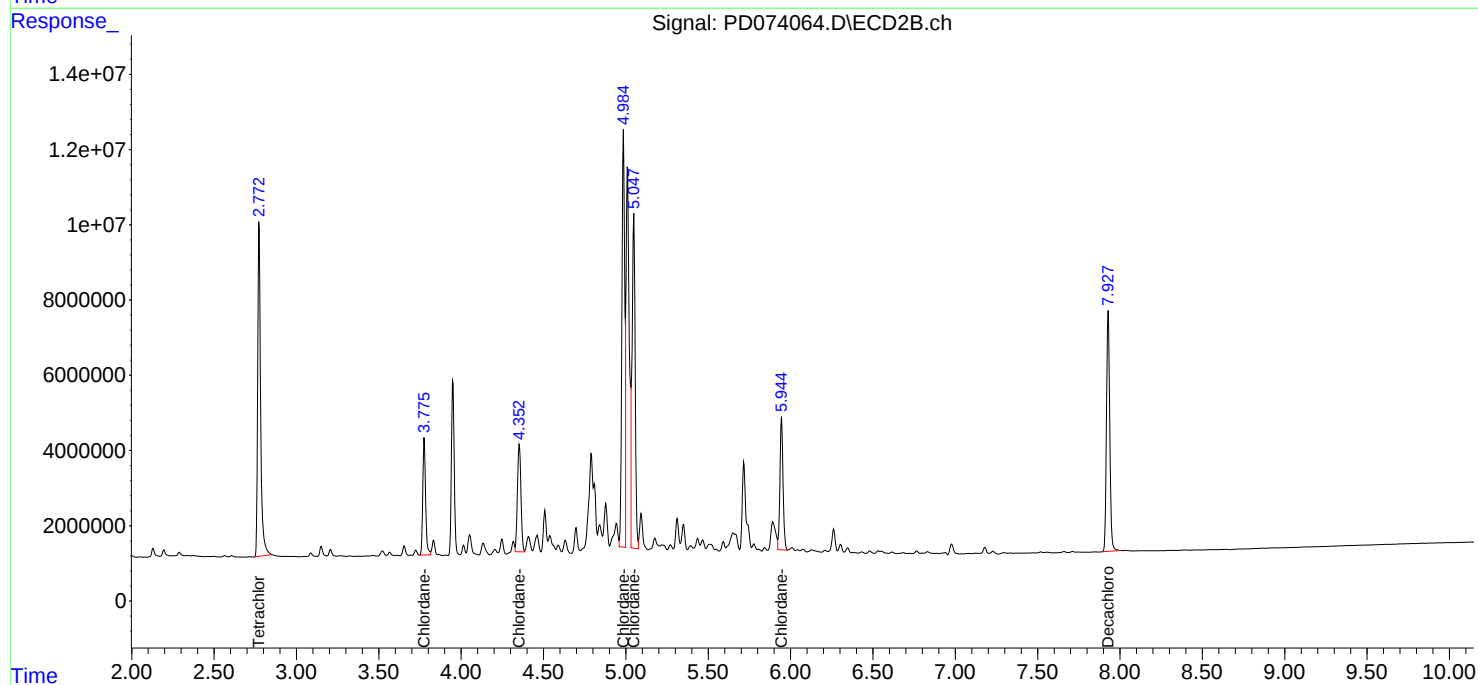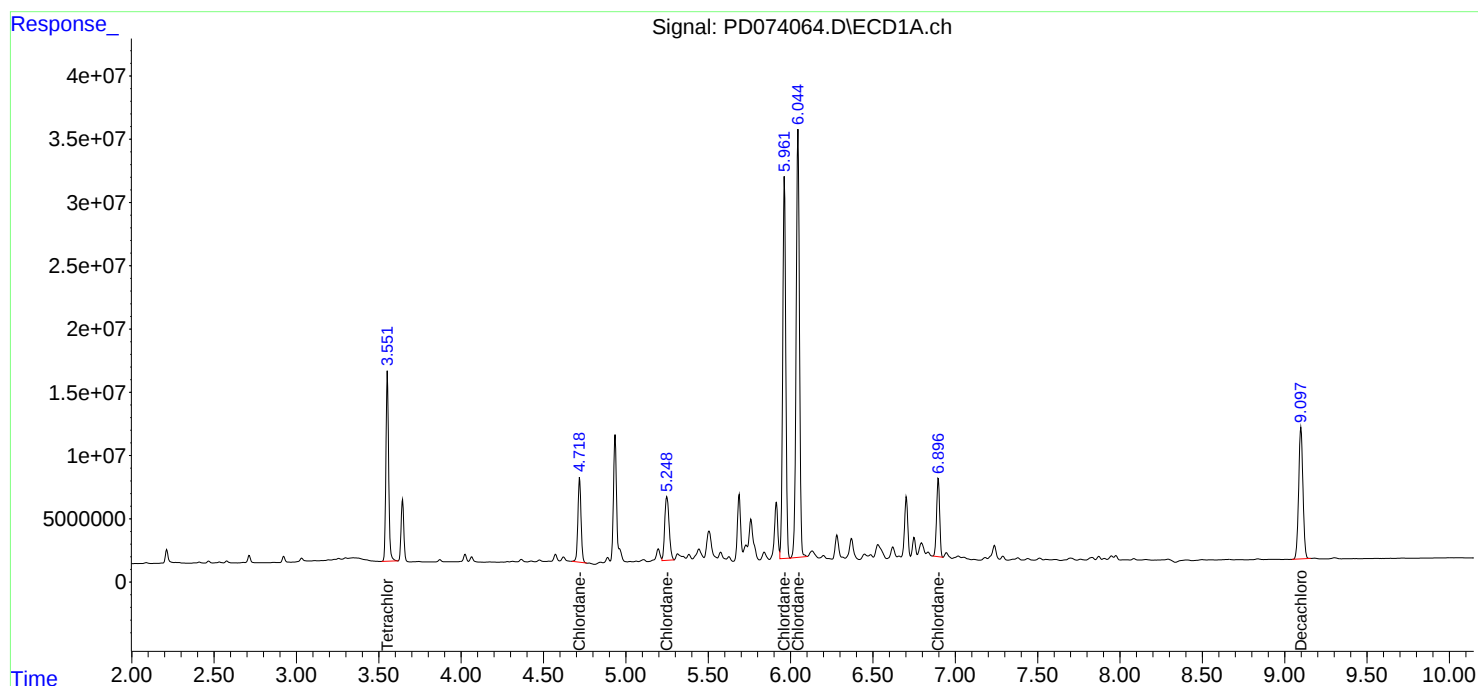


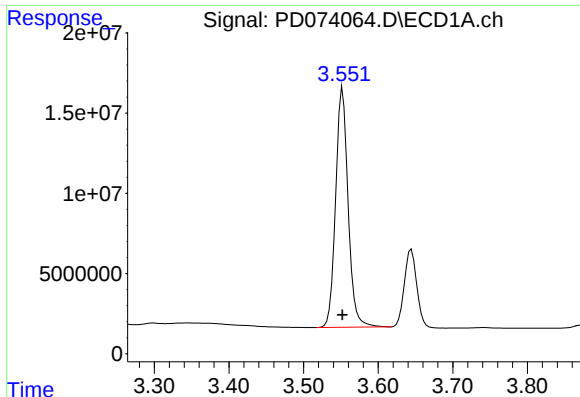

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 173685290
Conc: 74.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

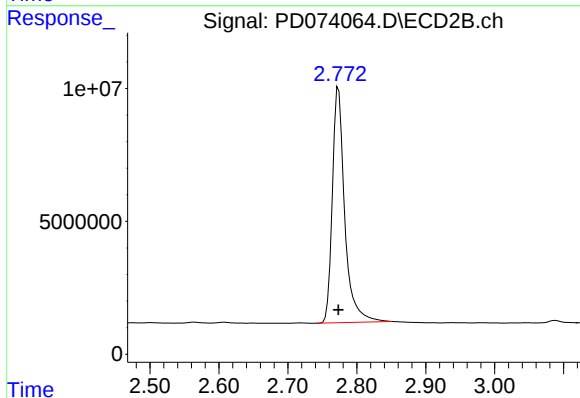


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 110374611
Conc: 74.87 ng/ml

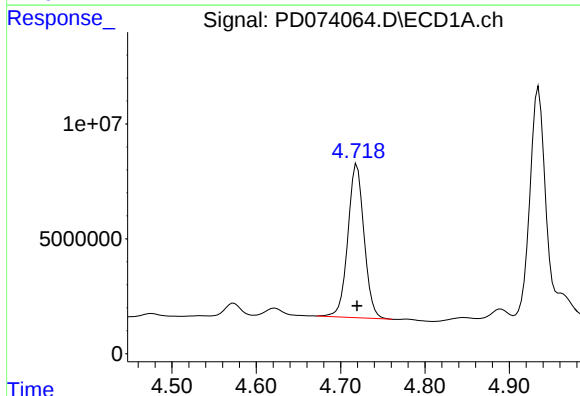


#23 Chlordane-1

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 88865338
Conc: 750.54 ng/ml

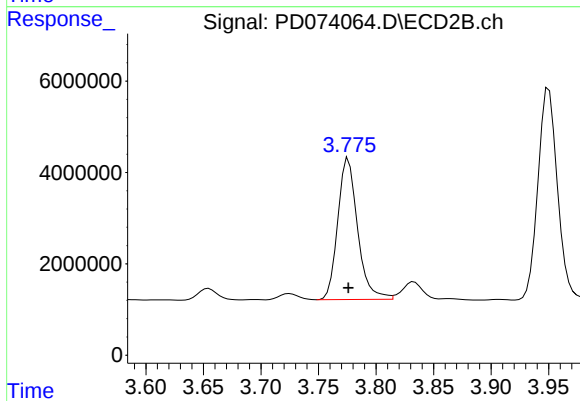

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 37183885
Conc: 745.74 ng/ml

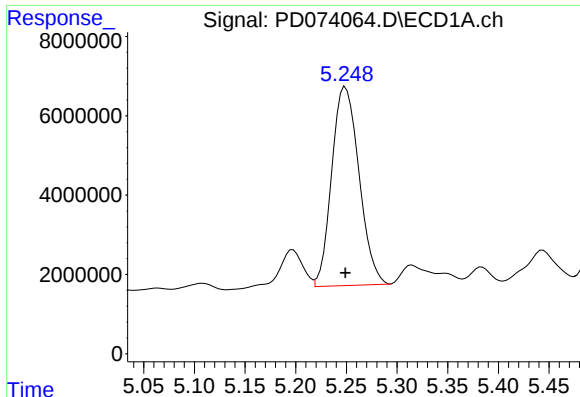

#24 Chlordane-2


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 94021735
Conc: 744.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

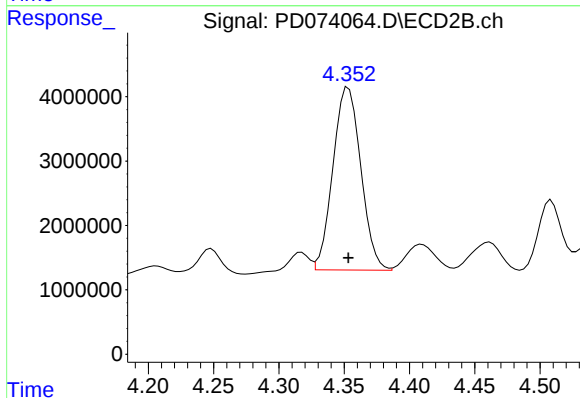


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 42245232
Conc: 740.95 ng/ml

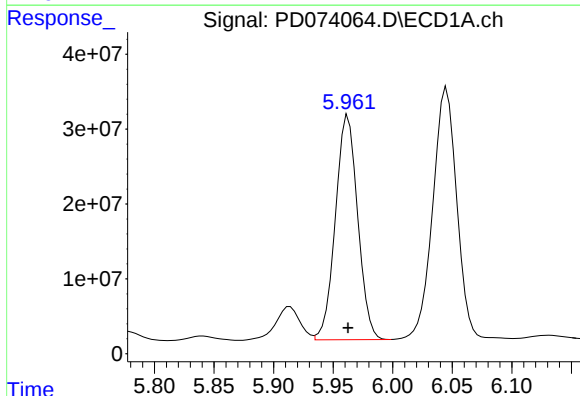


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 390594877
Conc: 748.49 ng/ml

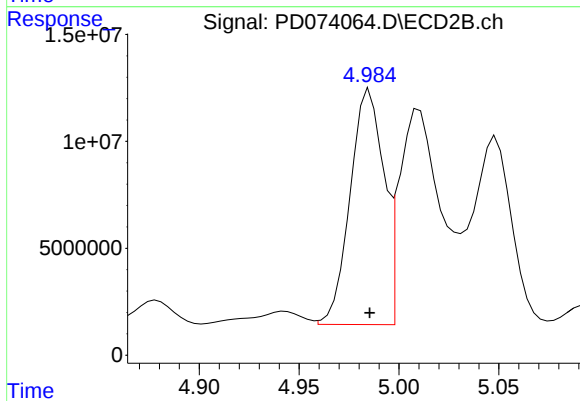

#25 Chlordane-3


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 128186341
Conc: 749.87 ng/ml

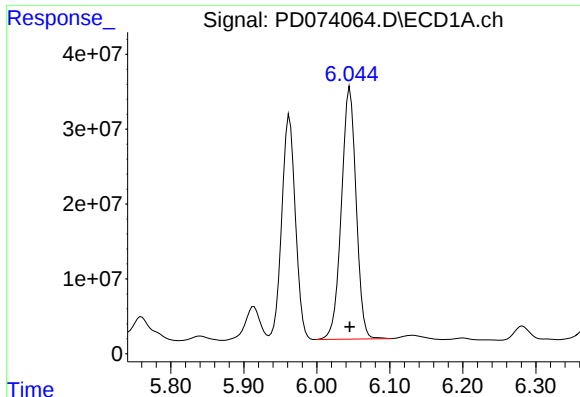

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 470749059
Conc: 747.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

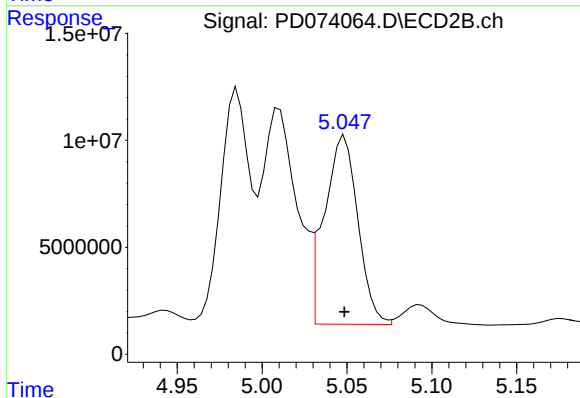


#26 Chlordane-4

R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 121273586
Conc: 747.15 ng/ml

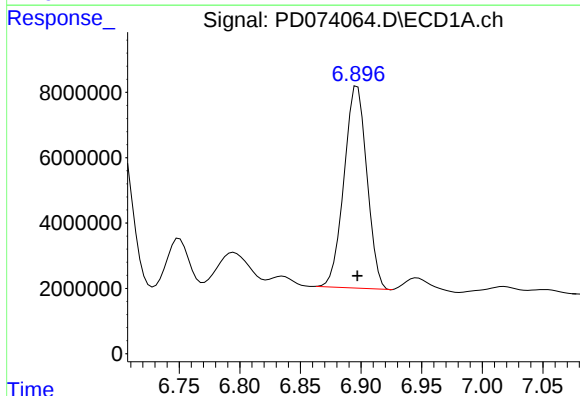


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 81046754
Conc: 744.19 ng/ml

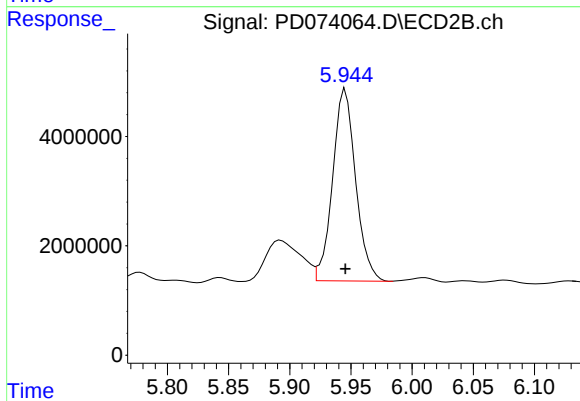

#27 Chlordane-5


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 45980884
Conc: 745.47 ng/ml

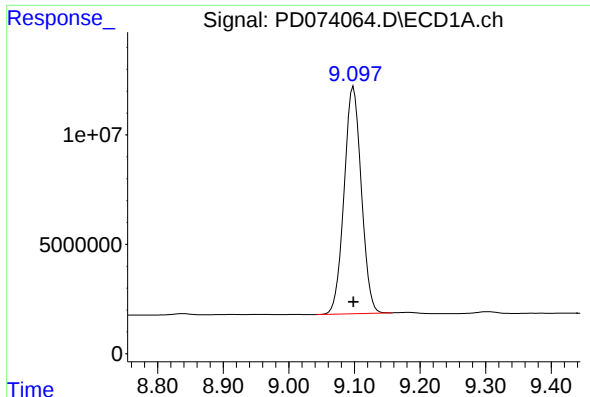

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 189030605
Conc: 74.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

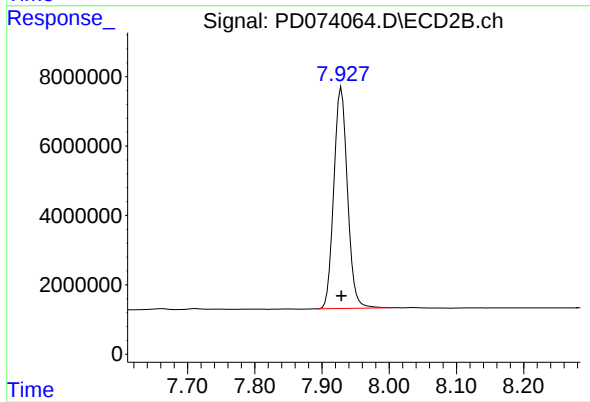

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 89274810
Conc: 74.14 ng/ml