

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
 Data File : PD074065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 20:53
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:57:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 00:56:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.774	117.6E6	74583068	50.000	50.000
28)	SA Decachlor...	9.098	7.929	132.9E6	62789608	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.719	3.776	60281133	25423285	500.000	500.000
24)	Chlordane-2	5.250	4.353	65785432	29938300	500.000	500.000
25)	Chlordane-3	5.962	4.985	261.0E6	86232781	500.000	500.000
26)	Chlordane-4	6.045	5.049	316.9E6	82340799	500.000	500.000
27)	Chlordane-5	6.897	5.946	55340382	31658868	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
Data File : PD074065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 20:53
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:57:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 00:56:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

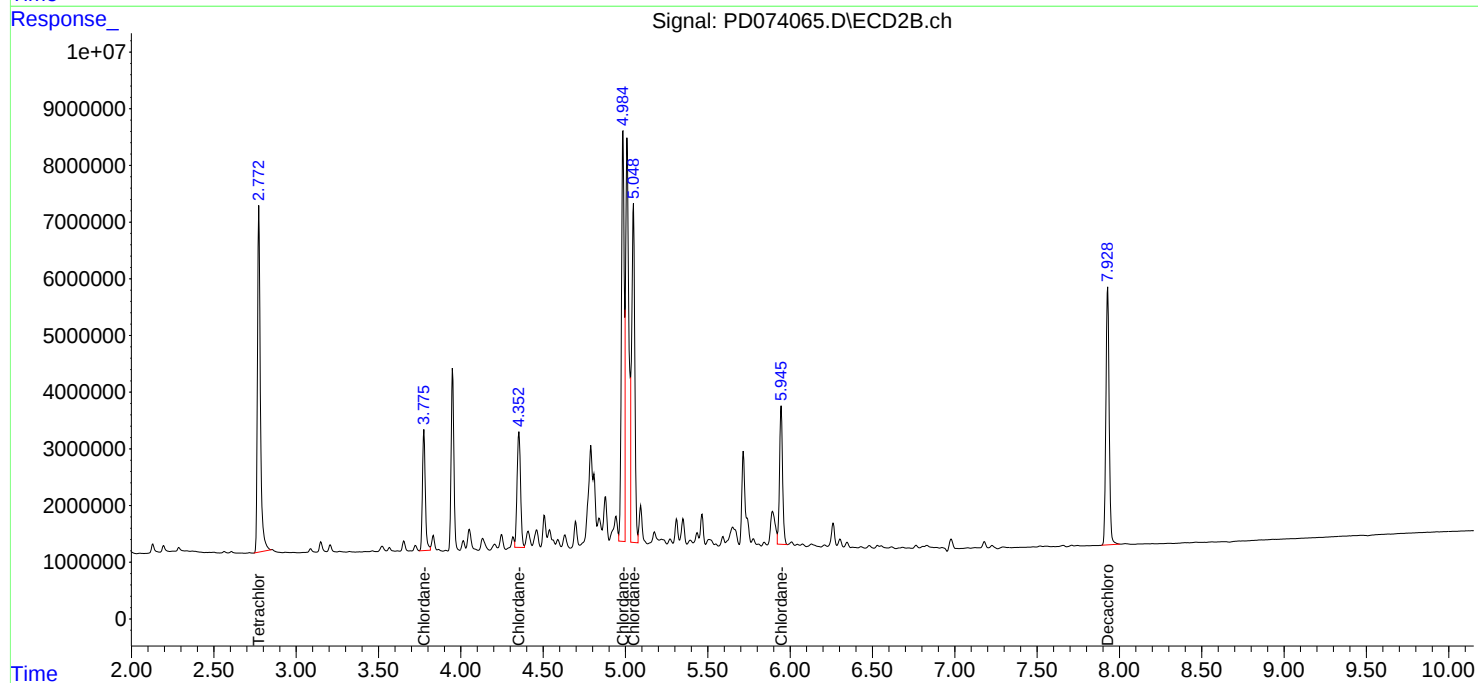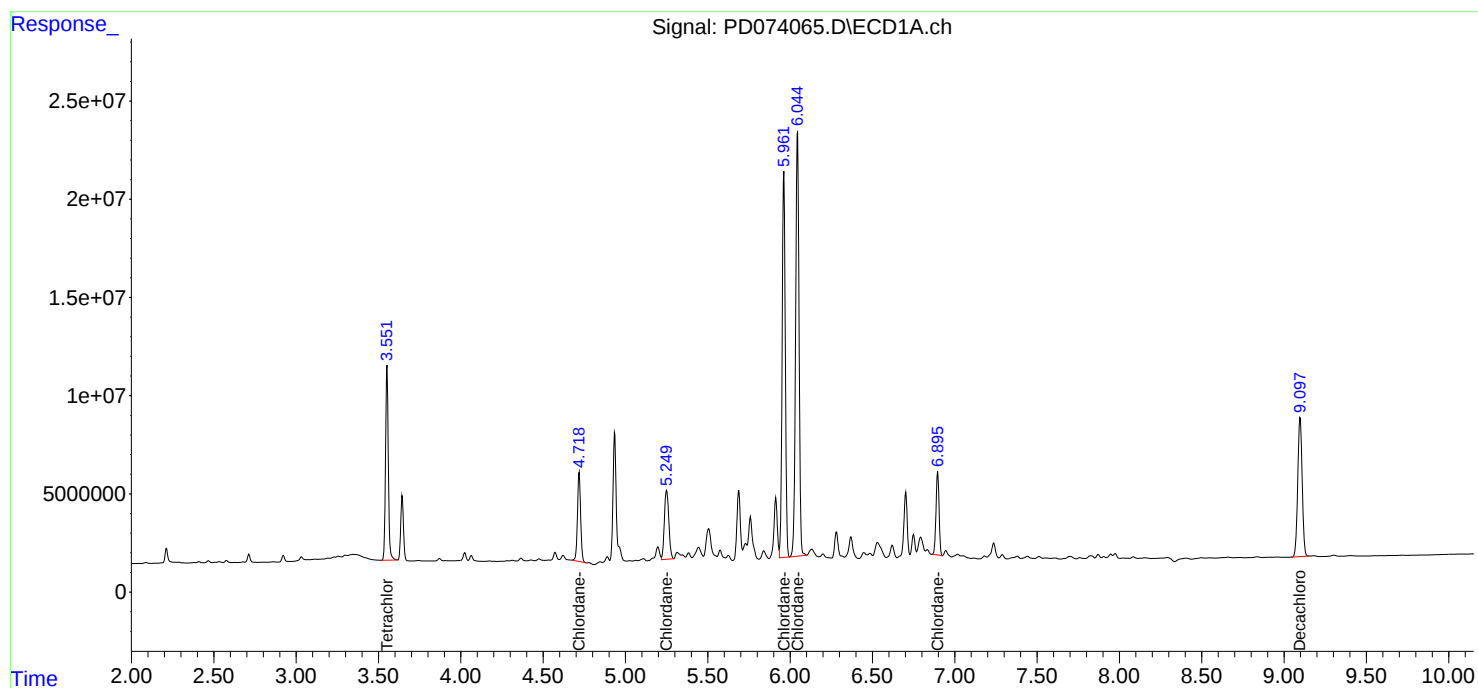


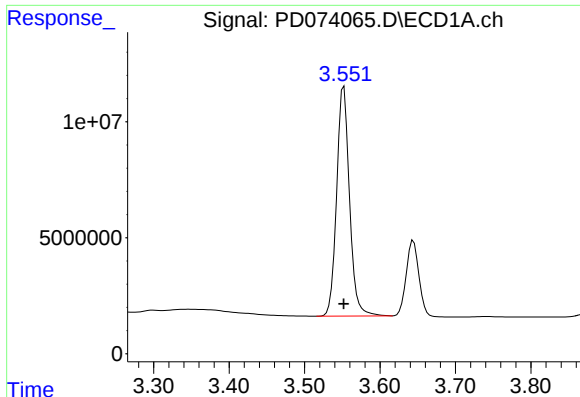

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 117573215
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

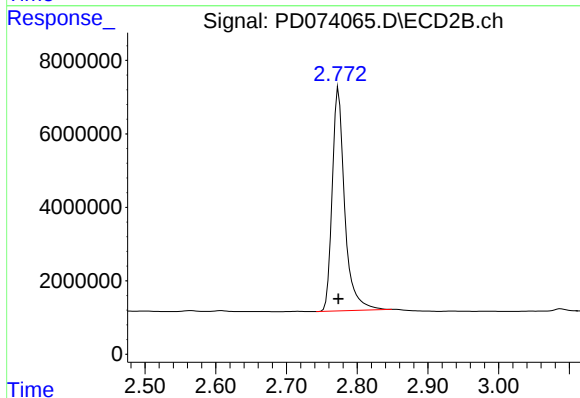


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 74583068
Conc: 50.00 ng/ml

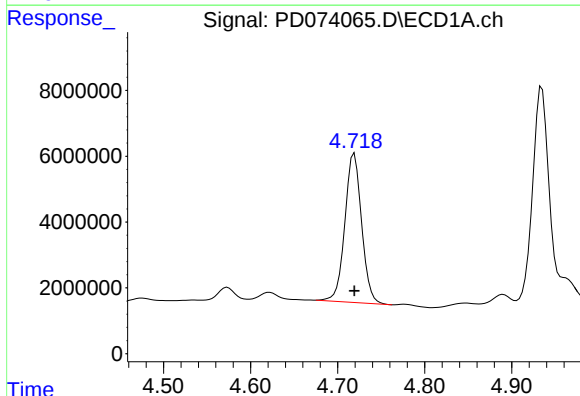


#23 Chlordane-1

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 60281133
Conc: 500.00 ng/ml

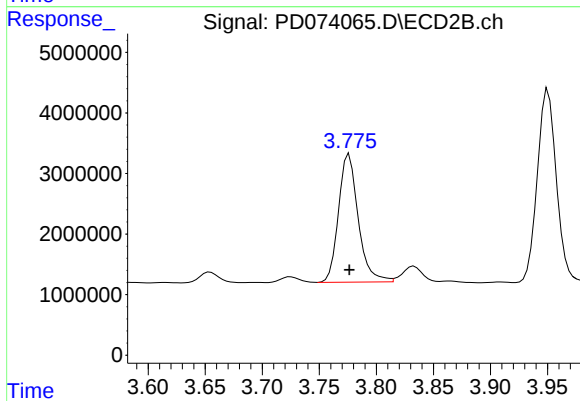

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 25423285
Conc: 500.00 ng/ml

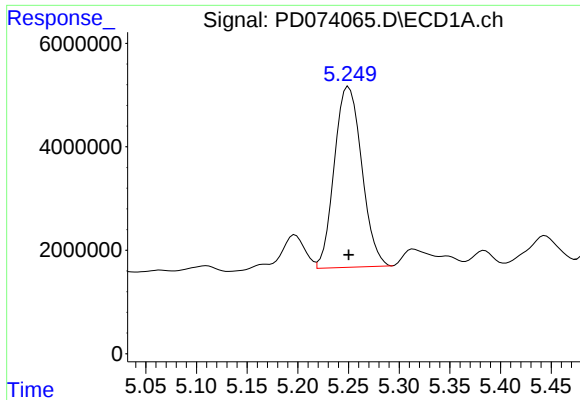

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 65785432
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

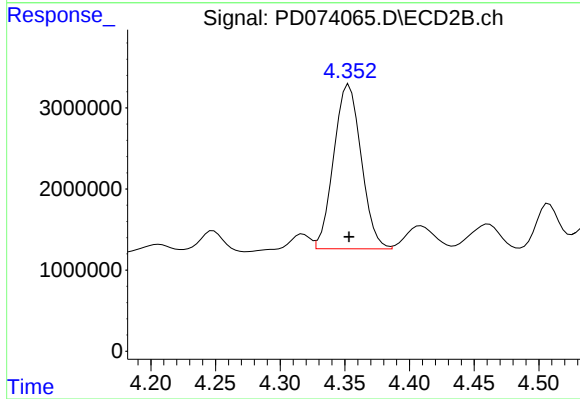


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 29938300
Conc: 500.00 ng/ml

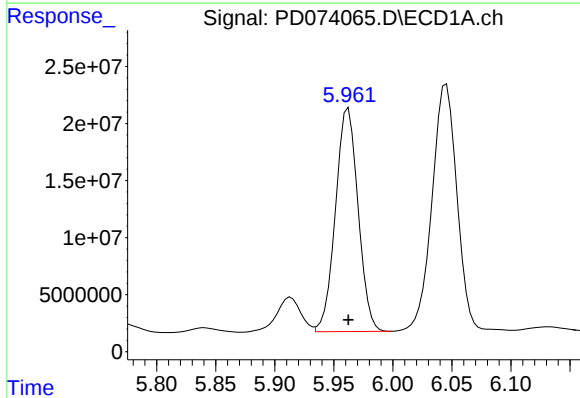


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 261035037
Conc: 500.00 ng/ml

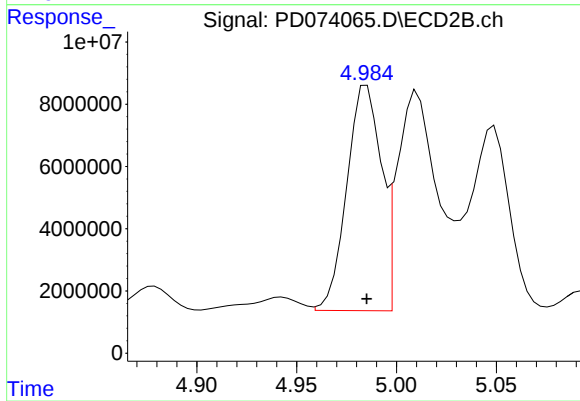

#25 Chlordane-3


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 86232781
Conc: 500.00 ng/ml

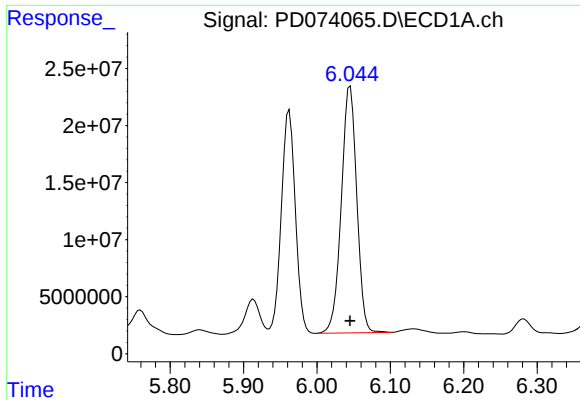

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 316931969
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

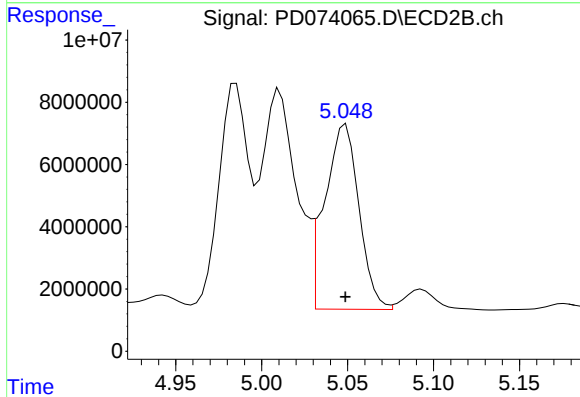


#26 Chlordane-4

R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 82340799
Conc: 500.00 ng/ml

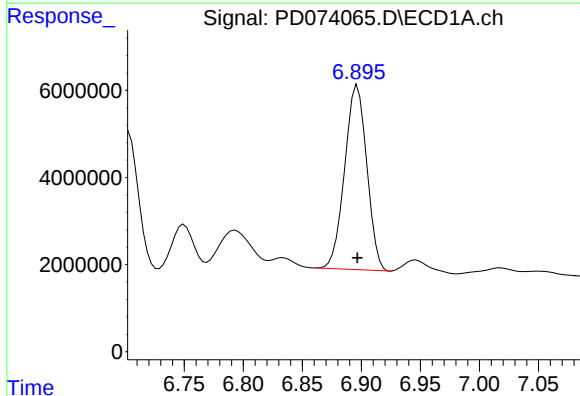


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 55340382
Conc: 500.00 ng/ml

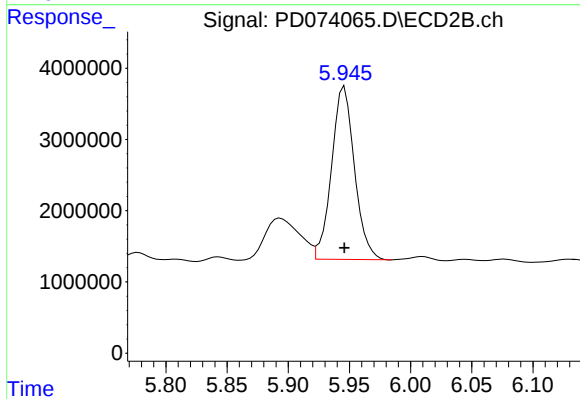

#27 Chlordane-5


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 31658868
Conc: 500.00 ng/ml

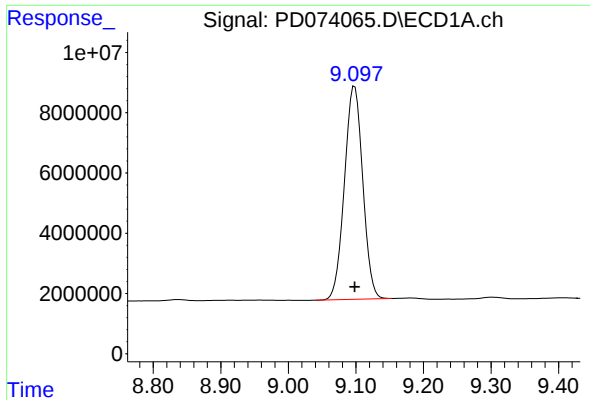

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 132946340
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

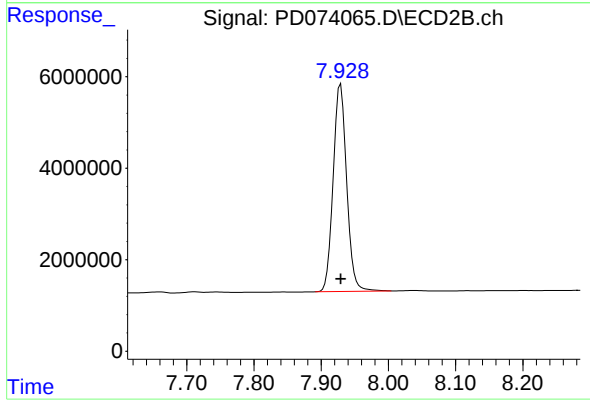

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 62789608
Conc: 50.00 ng/ml