

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
 Data File : PD074057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 19:05
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 01:45:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	53070768	27832030	23.164	23.498
28)	SA Decachlor...	9.100	7.930	62617671	28815897	23.492	23.535
Target Compounds							
9)	A Endosulfan I	6.092	5.105	32094143	16104628	11.108	11.482
10)	B gamma-Chl...	5.962	4.985	33417613	17570872	10.916	11.530
12)	B 4,4'-DDE	6.214	5.240	61752699	31007473	21.742	22.353
13)	MA Dieldrin	6.369	5.370	68216959	33976226	22.485	23.008
19)	B Endosulfa...	7.182	6.342	54092850	25221783	21.000	20.793
20)	A Methoxychlor	7.522	6.622	160.6E6	70004276	108.129	107.022
21)	B Endrin ke...	7.669	6.849	67128058	33126539	22.896	22.792



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
Data File : PD074057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 19:05
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 01:45:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

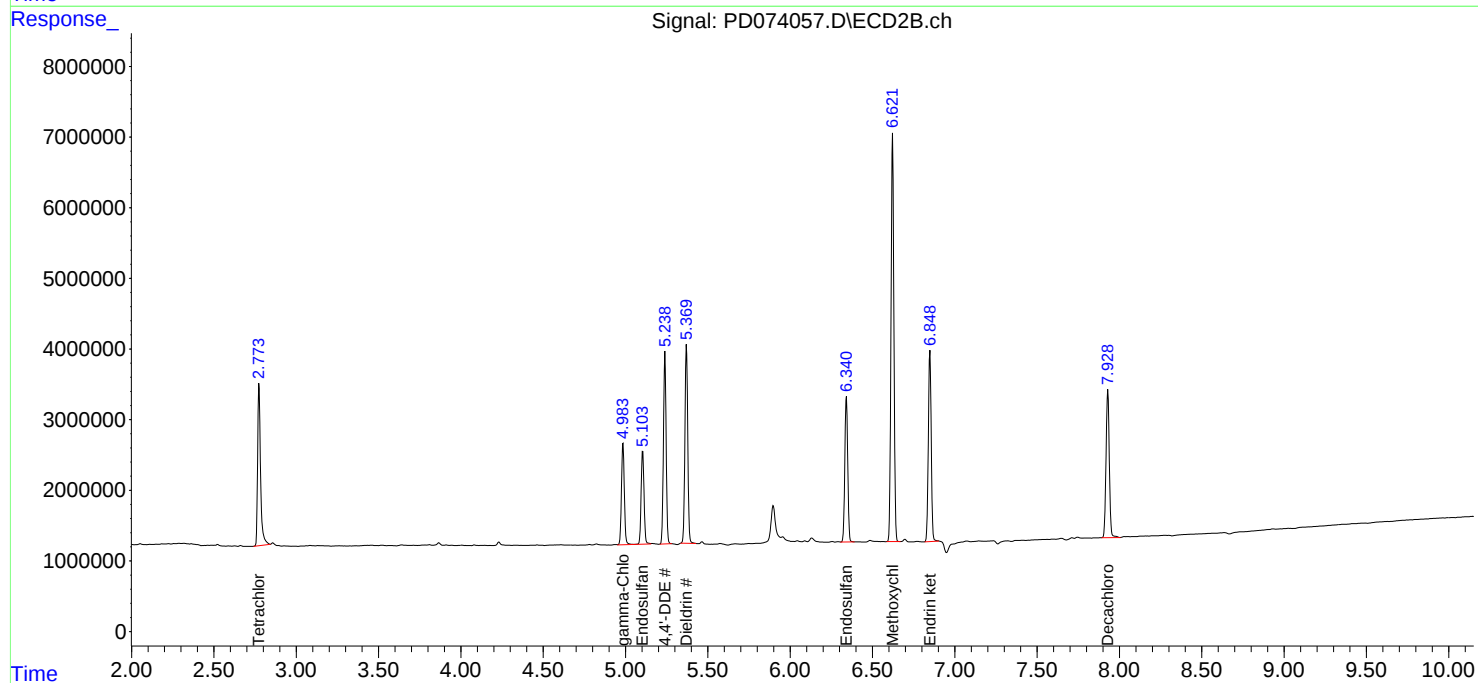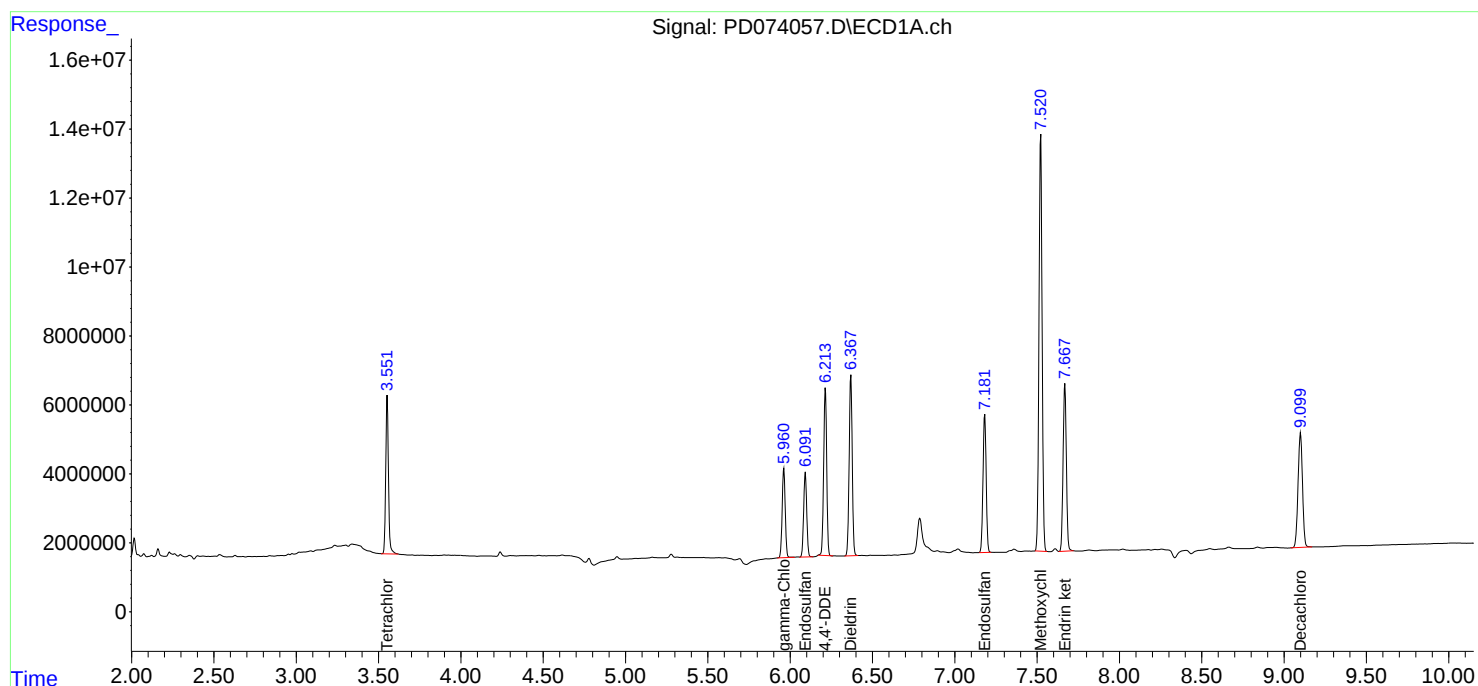


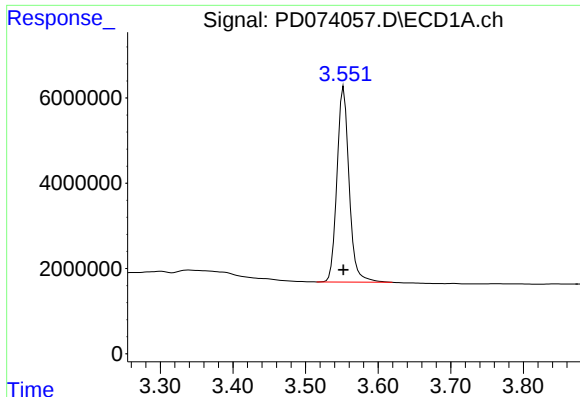

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 53070768
Conc: 23.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

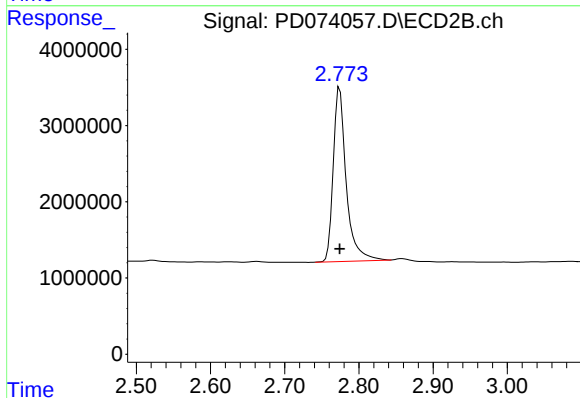


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 27832030
Conc: 23.50 ng/ml

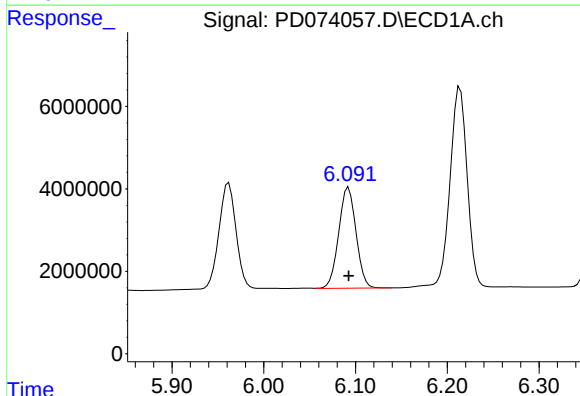


#9 Endosulfan I

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 32094143
Conc: 11.11 ng/ml

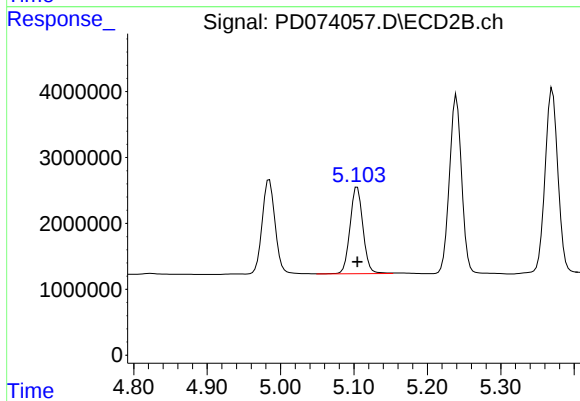

#9 Endosulfan I


R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 16104628
Conc: 11.48 ng/ml

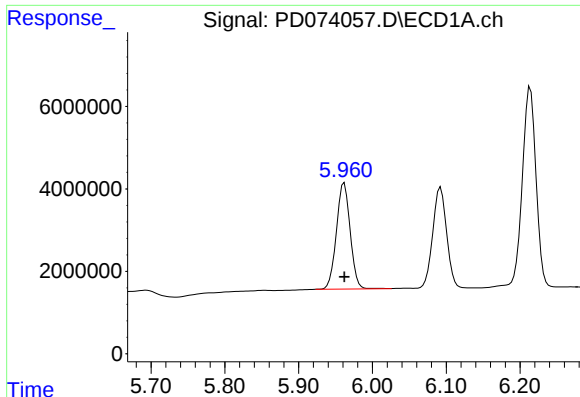

#10 gamma-Chlordane


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 33417613
Conc: 10.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

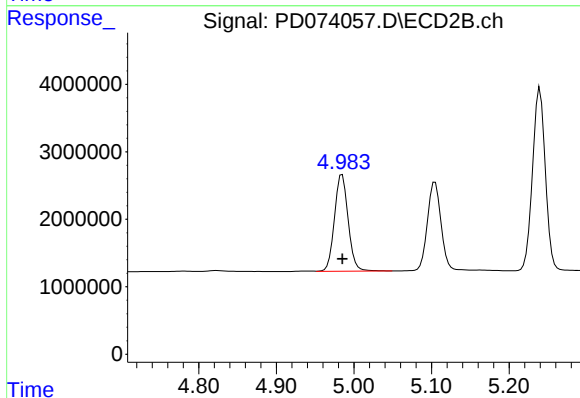


#10 gamma-Chlordane

R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 17570872
Conc: 11.53 ng/ml

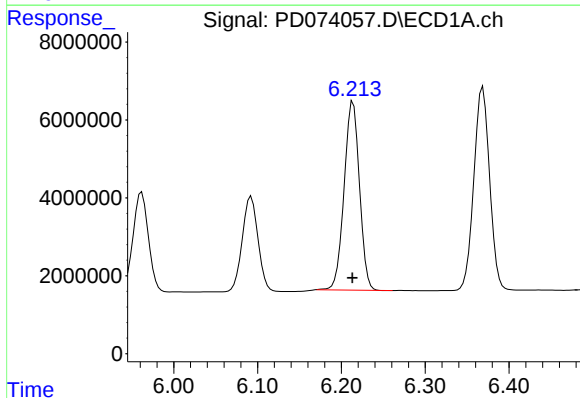


#12 4,4'-DDE

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 61752699
Conc: 21.74 ng/ml

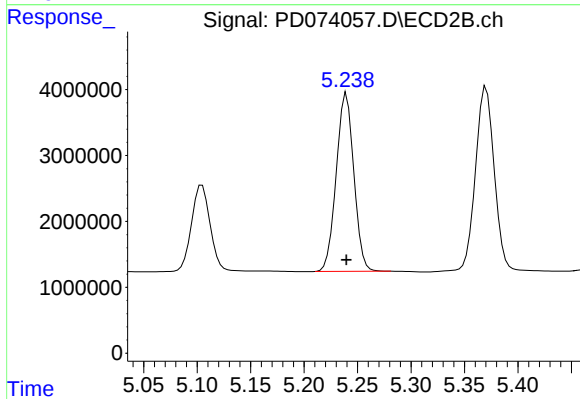

#12 4,4'-DDE


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 31007473
Conc: 22.35 ng/ml

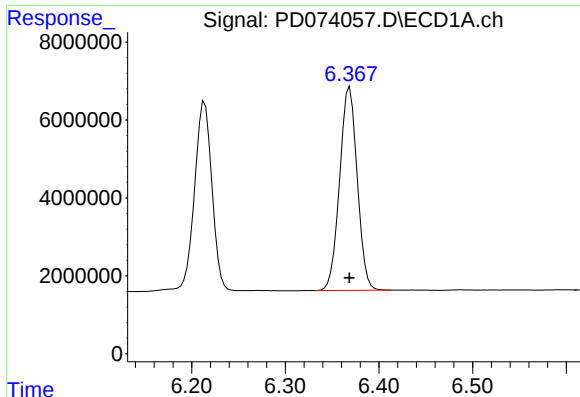

#13 Dieldrin


R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 68216959
Conc: 22.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

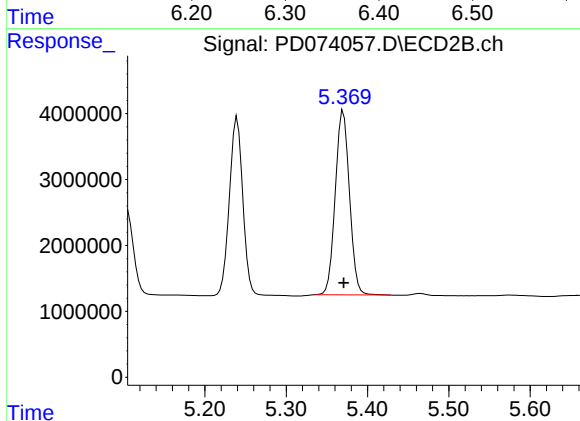


#13 Dieldrin

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 33976226
Conc: 23.01 ng/ml

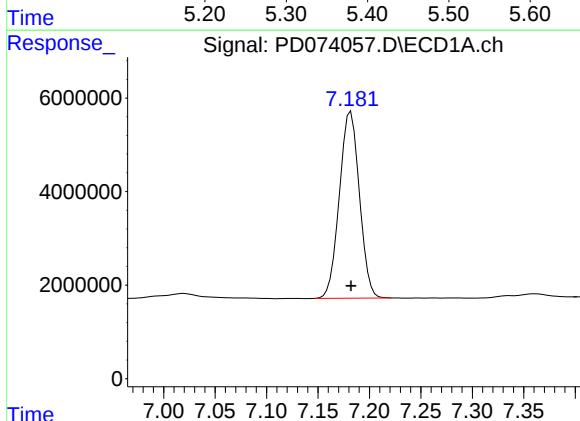


#19 Endosulfan Sulfate

R.T.: 7.182 min
Delta R.T.: 0.000 min
Response: 54092850
Conc: 21.00 ng/ml

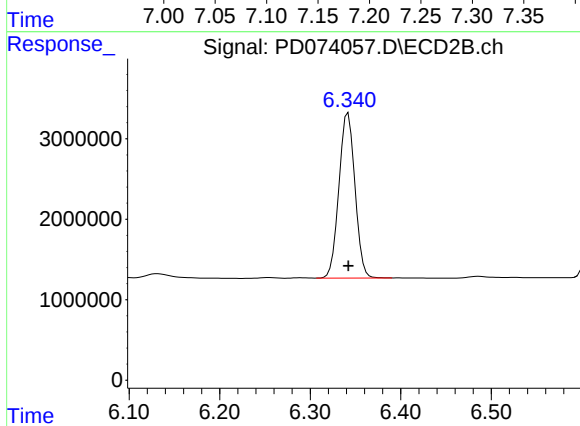

#19 Endosulfan Sulfate


R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 25221783
Conc: 20.79 ng/ml

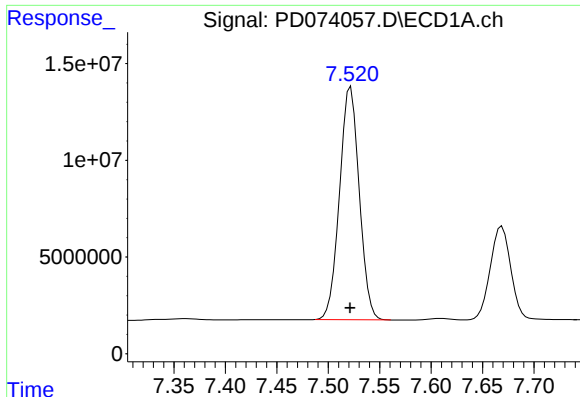

#20 Methoxychlor


R.T.: 7.522 min
Delta R.T.: 0.000 min
Response: 160587806
Conc: 108.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

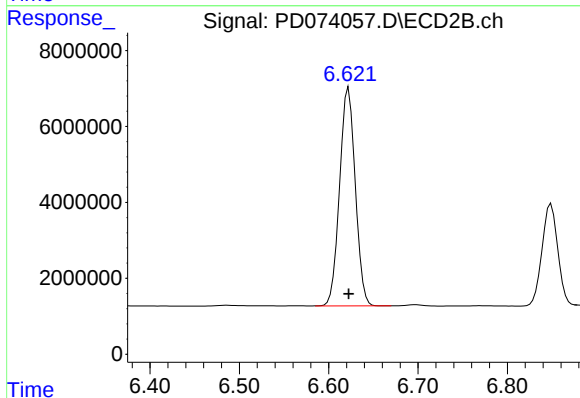


#20 Methoxychlor

R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 70004276
Conc: 107.02 ng/ml

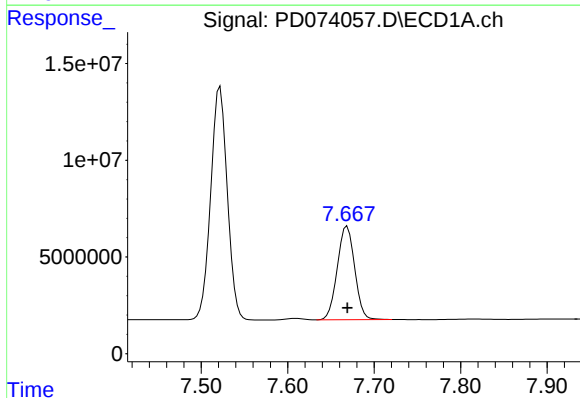


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 67128058
Conc: 22.90 ng/ml

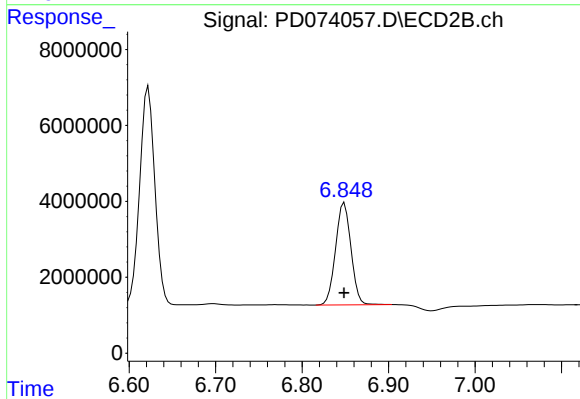

#21 Endrin ketone


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 33126539
Conc: 22.79 ng/ml

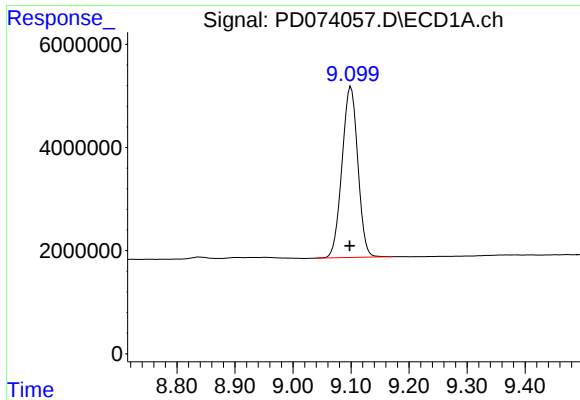

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.002 min
Response: 62617671
Conc: 23.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

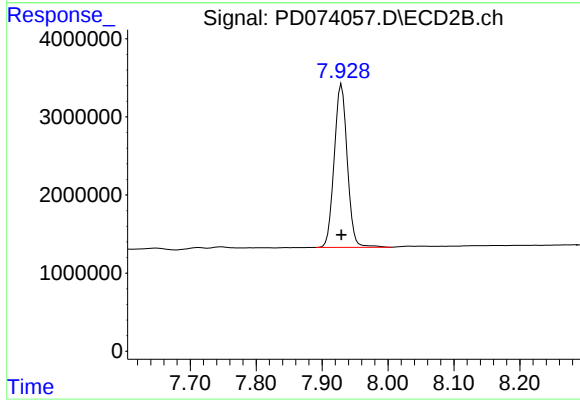

#28 Decachlorobiphenyl

R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 28815897
Conc: 23.54 ng/ml