

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
 Data File : PD074063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 20:26
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:59:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 00:56:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.774	230.5E6	145.9E6	98.999	98.900
28)	SA Decachlor...	9.099	7.929	244.5E6	116.6E6	95.811	96.302
Target Compounds							
23)	Chlordane-1	4.720	3.776	116.2E6	49160274	981.388	983.138
24)	Chlordane-2	5.250	4.353	121.8E6	54842097	961.468	956.114
25)	Chlordane-3	5.963	4.986	522.7E6	169.5E6	1000.569	991.184
26)	Chlordane-4	6.045	5.049	628.1E6	160.6E6	995.416	987.345
27)	Chlordane-5	6.897	5.946	108.0E6	60416124	987.621	976.550



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
Data File : PD074063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 20:26
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:59:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 00:56:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

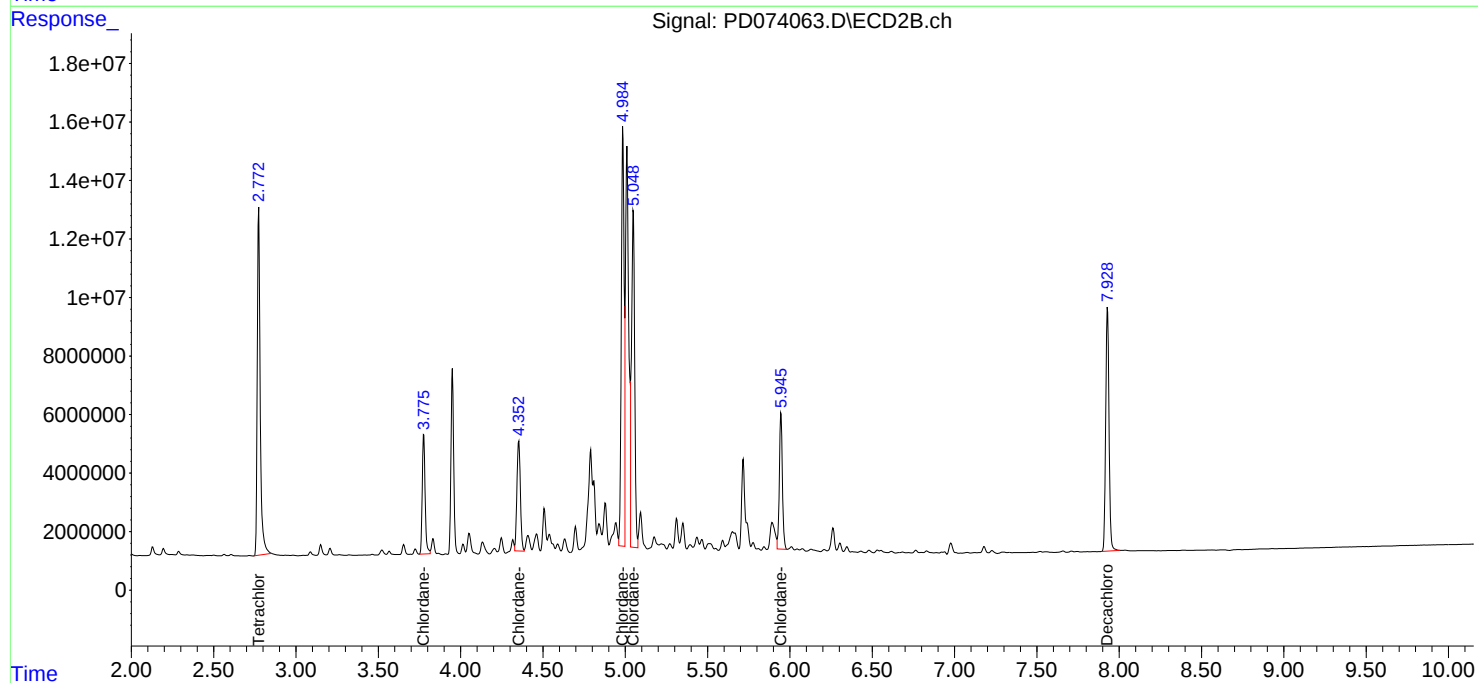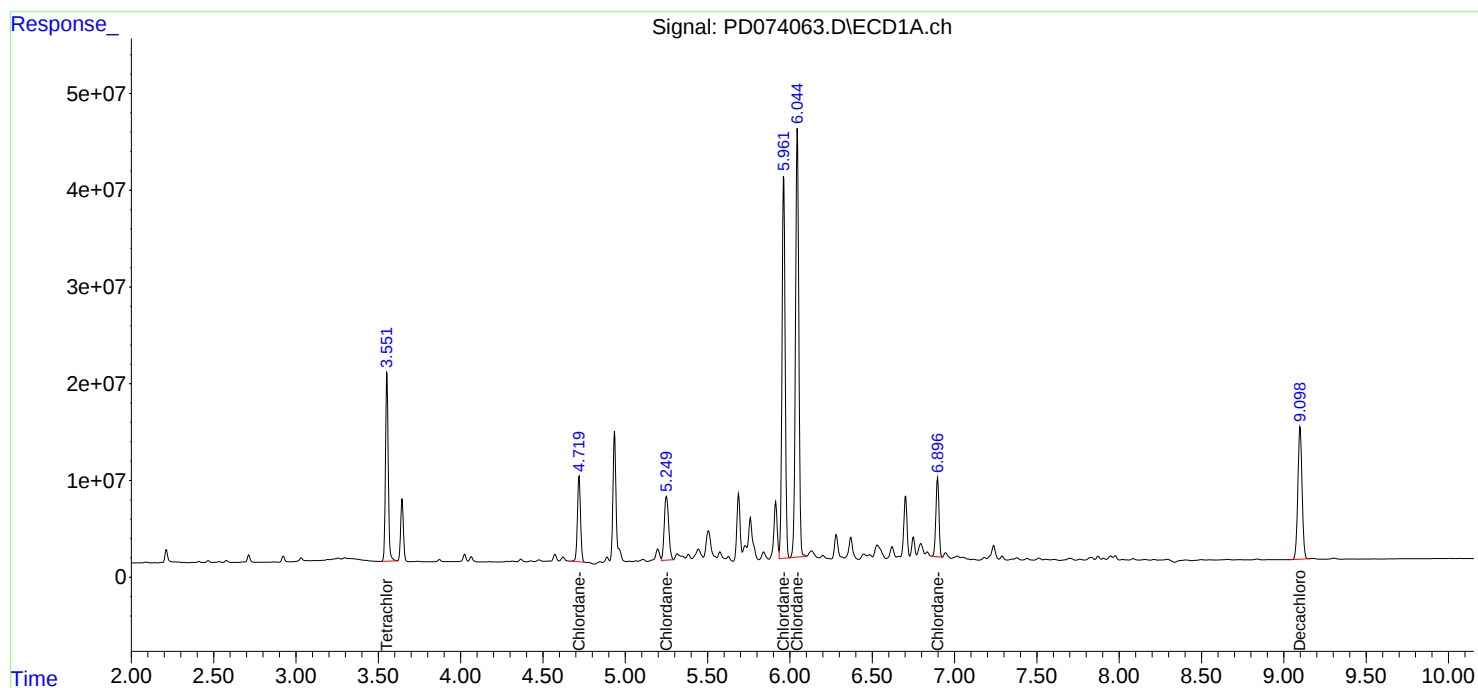


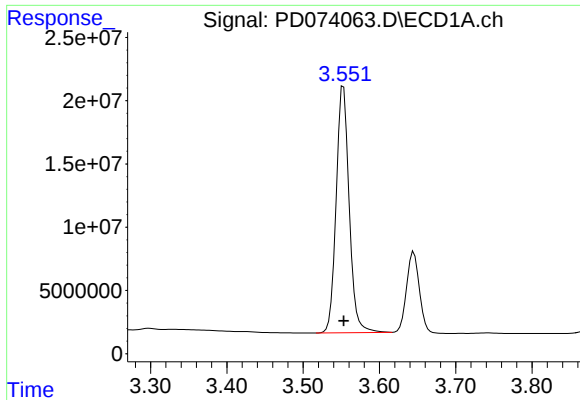

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 230487295
Conc: 99.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

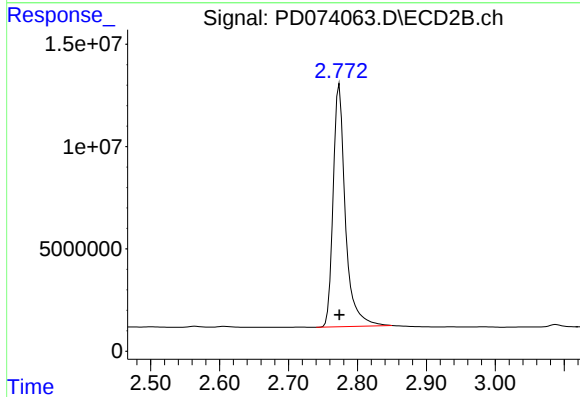


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 145920653
Conc: 98.90 ng/ml

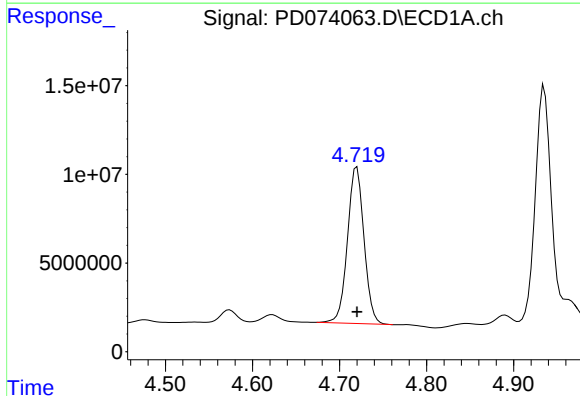


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 116156393
Conc: 981.39 ng/ml

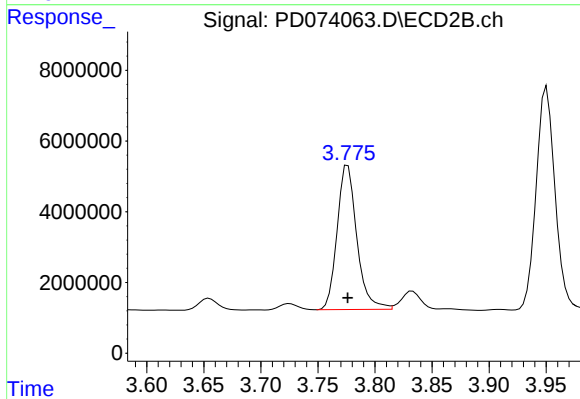

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 49160274
Conc: 983.14 ng/ml

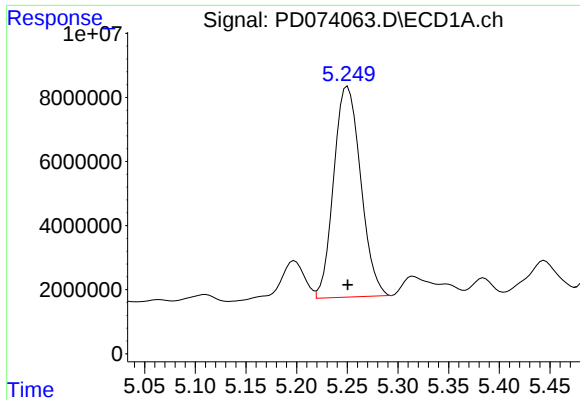

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 121807566
Conc: 961.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

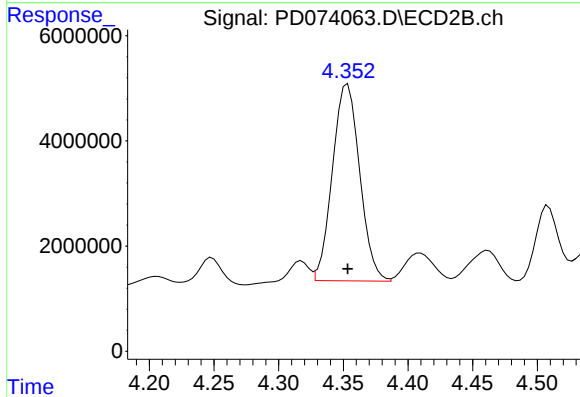


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 54842097
Conc: 956.11 ng/ml

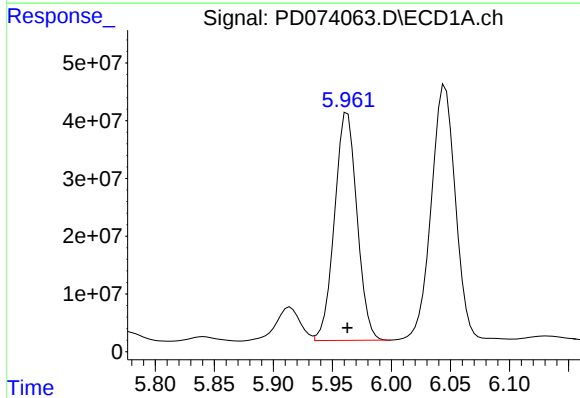


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 522664635
Conc: 1000.57 ng/ml

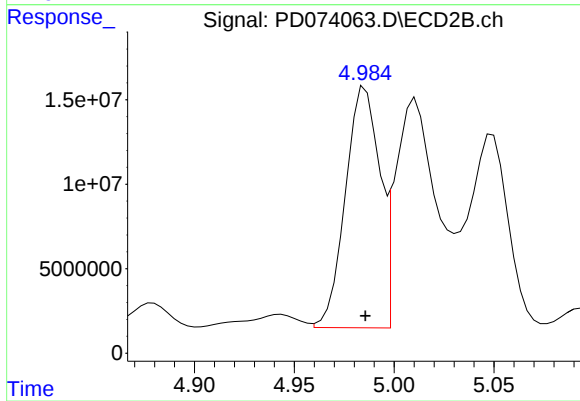

#25 Chlordane-3


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 169451216
Conc: 991.18 ng/ml

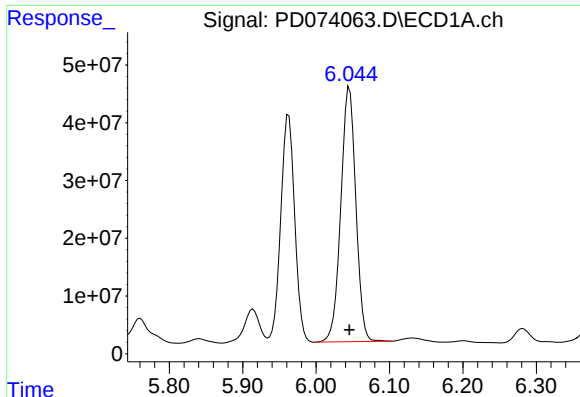

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 628079564
Conc: 995.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

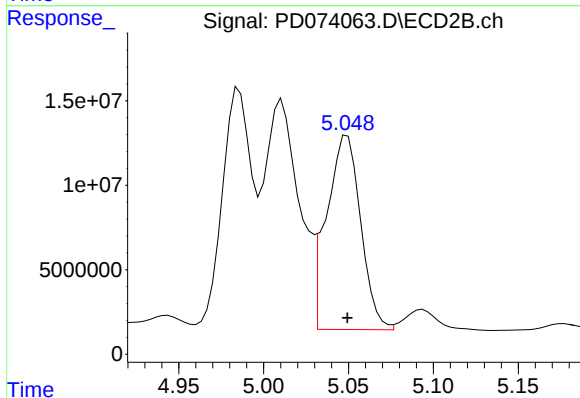


#26 Chlordane-4

R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 160565442
Conc: 987.34 ng/ml

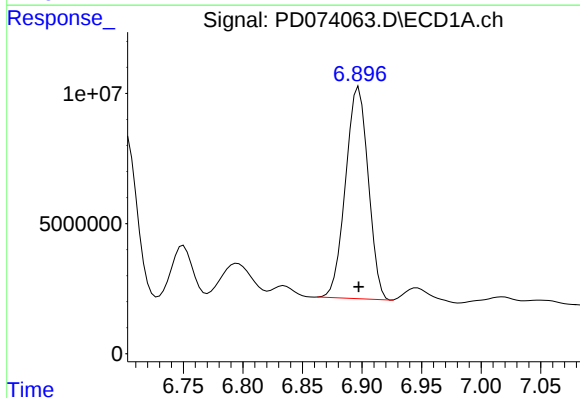


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: 0.000 min
Response: 107973981
Conc: 987.62 ng/ml

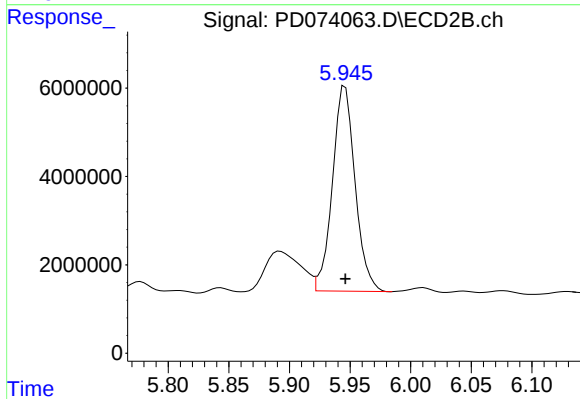

#27 Chlordane-5


R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 60416124
Conc: 976.55 ng/ml

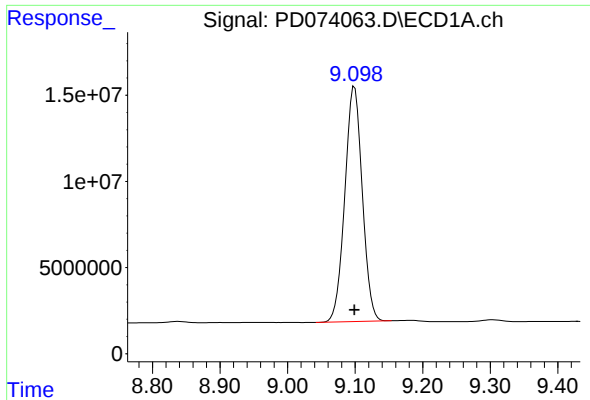

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 244511643
Conc: 95.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

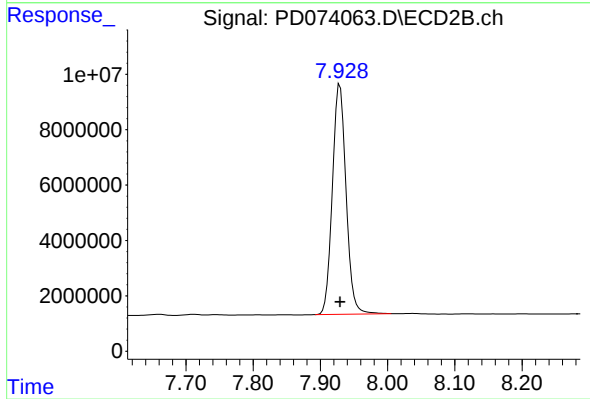

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 116623208
Conc: 96.30 ng/ml