

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
 Data File : PD074074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2023 22:54
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD030123CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 01:08:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:07:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.773	120.0E6	75610277	51.082	50.850
28)	SA Decachlor...	9.098	7.929	136.1E6	64006096	49.819	49.969
Target Compounds							
23)	Chlordane-1	4.719	3.776	62978896	26040936	510.323	517.426
24)	Chlordane-2	5.250	4.353	68396943	30345513	506.500	506.982
25)	Chlordane-3	5.962	4.985	270.9E6	87238250	529.474	513.400
26)	Chlordane-4	6.045	5.049	327.5E6	83257471	522.784	512.155
27)	Chlordane-5	6.896	5.945	57165540	32031926	516.646	498.105



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030123\
Data File : PD074074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2023 22:54
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD030123CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 01:08:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:07:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

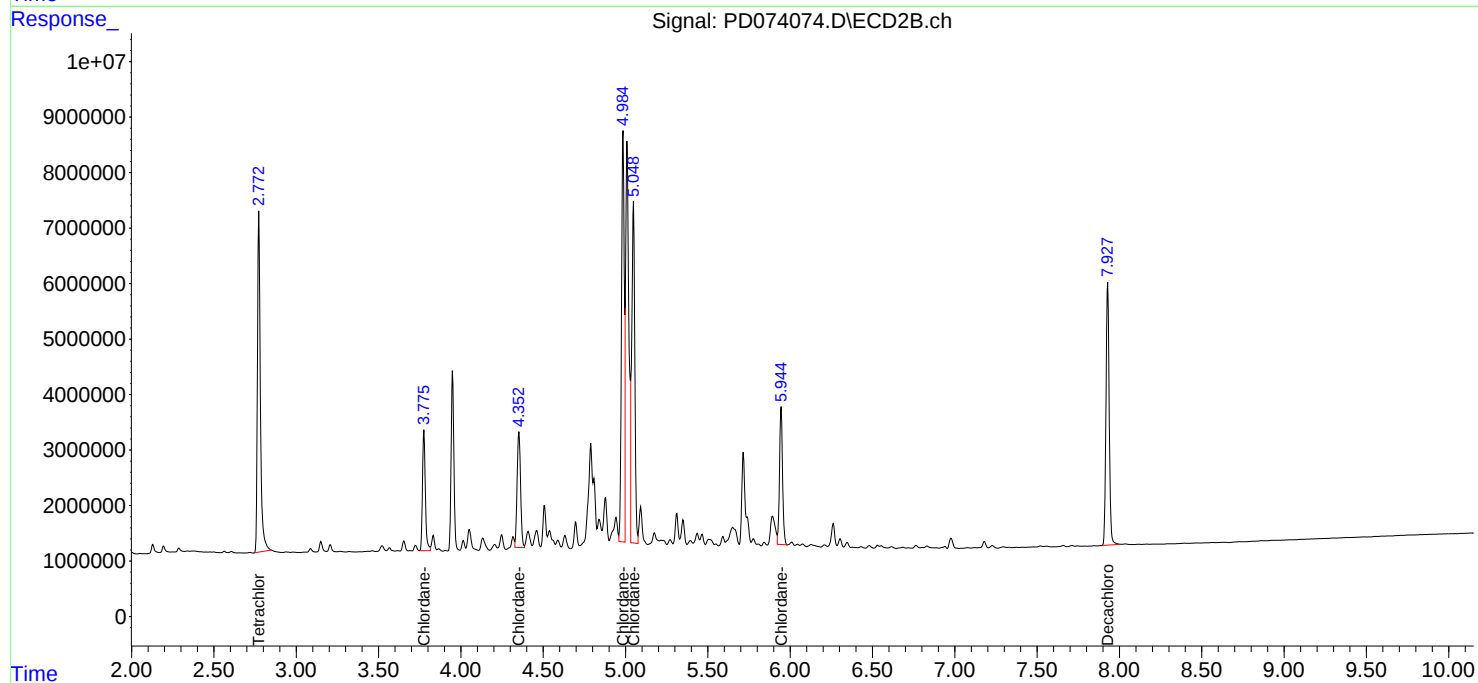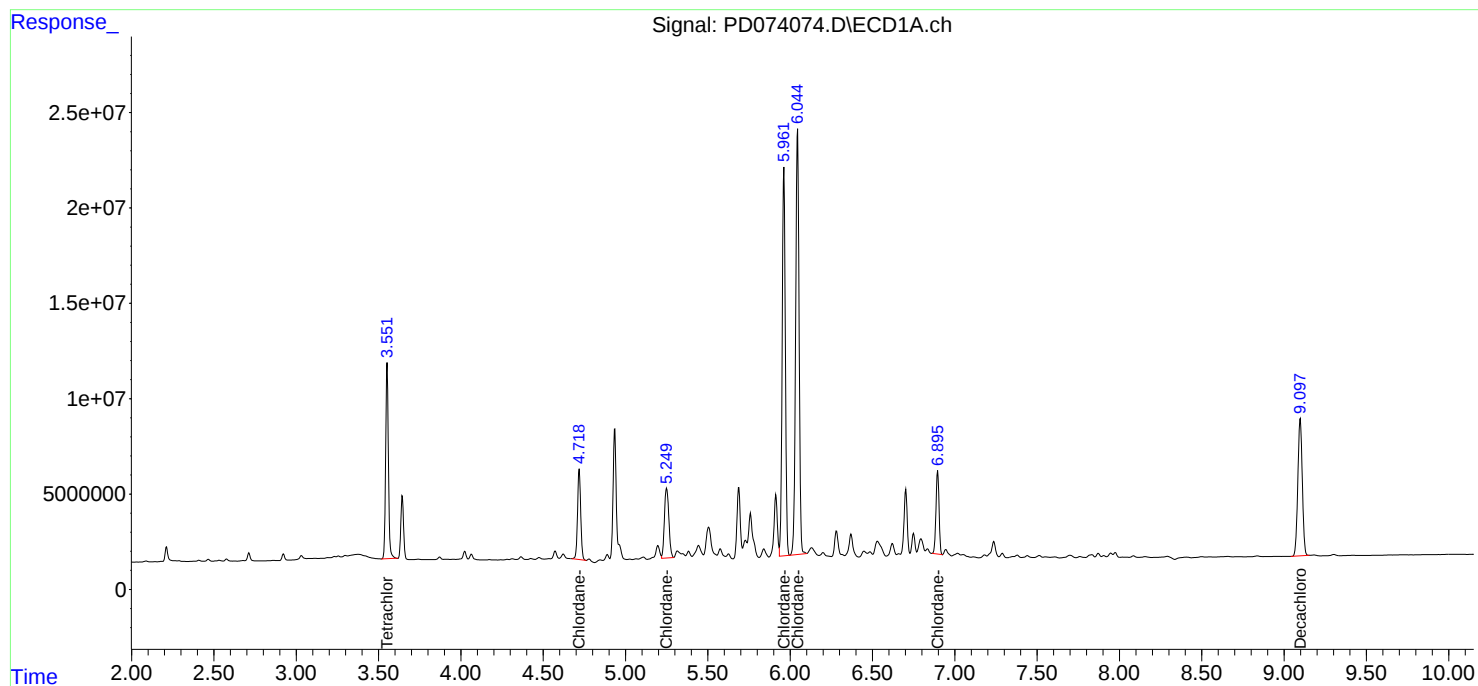


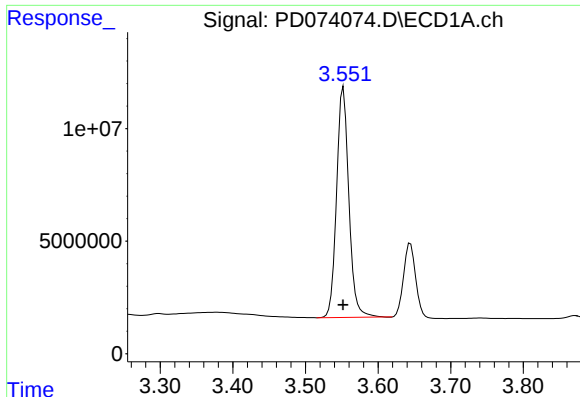

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 119970607
Conc: 51.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030123CHLOR

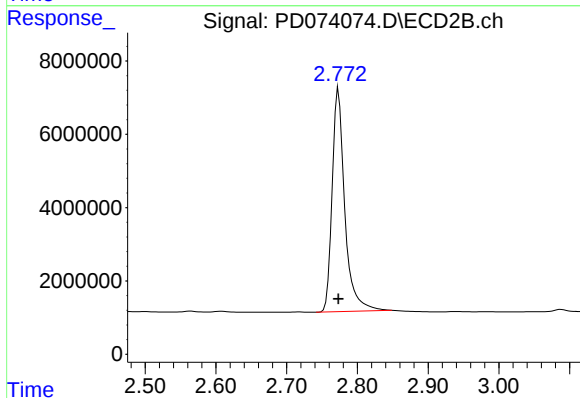


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 75610277
Conc: 50.85 ng/ml

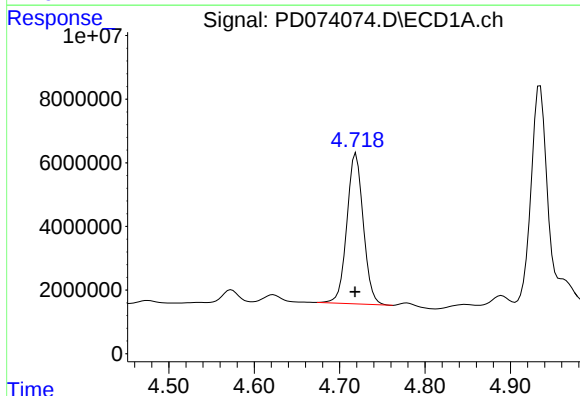


#23 Chlordane-1

R.T.: 4.719 min
Delta R.T.: 0.001 min
Response: 62978896
Conc: 510.32 ng/ml

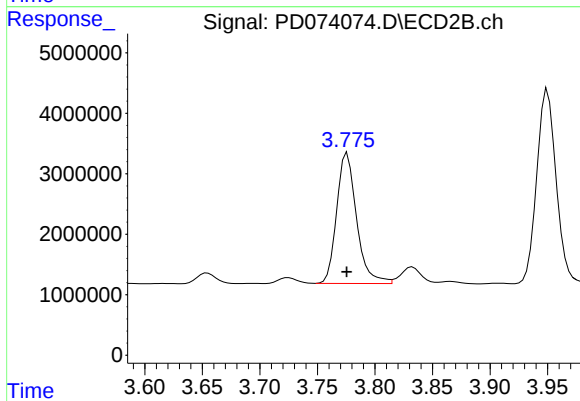

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 26040936
Conc: 517.43 ng/ml

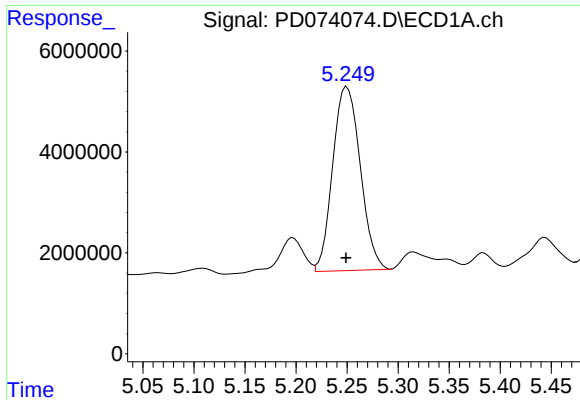

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 68396943
Conc: 506.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030123CHLOR

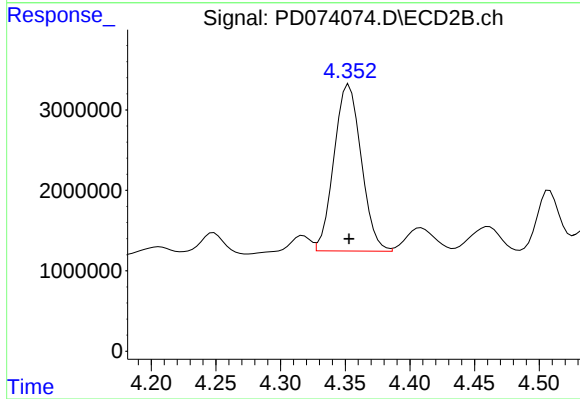


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 30345513
Conc: 506.98 ng/ml

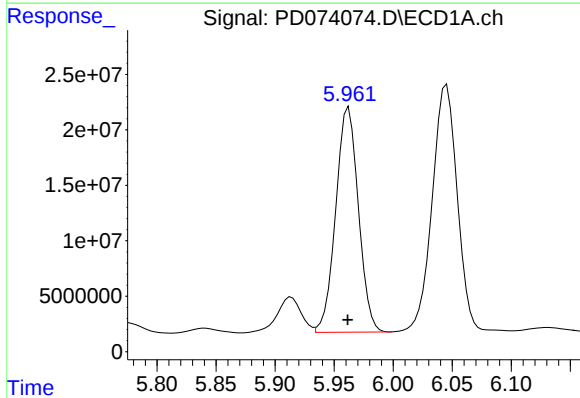


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 270855714
Conc: 529.47 ng/ml

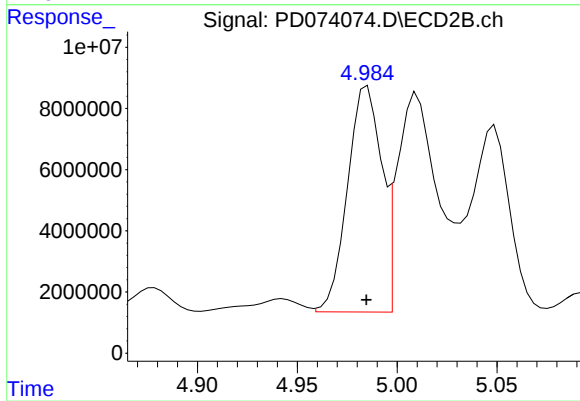

#25 Chlordane-3


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 87238250
Conc: 513.40 ng/ml

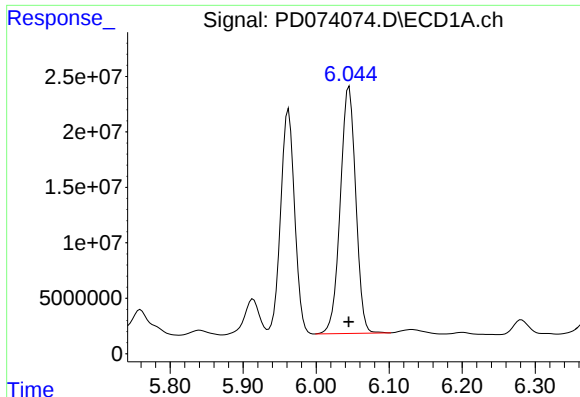

#26 Chlordane-4


R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 327533768
Conc: 522.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030123CHLOR

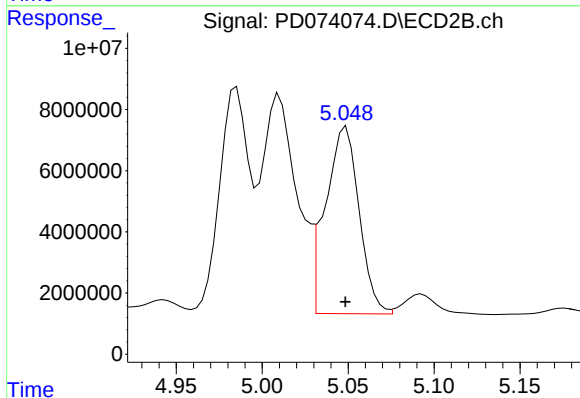


#26 Chlordane-4

R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 83257471
Conc: 512.15 ng/ml

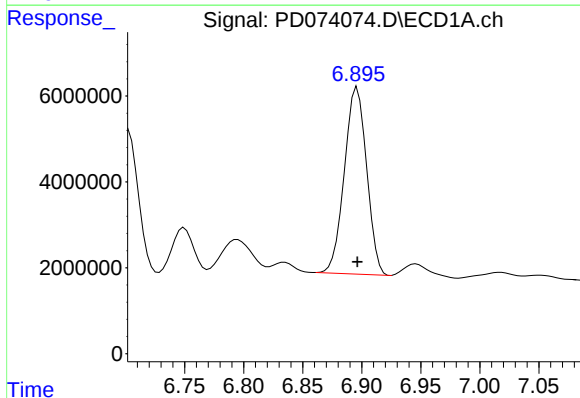


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 57165540
Conc: 516.65 ng/ml

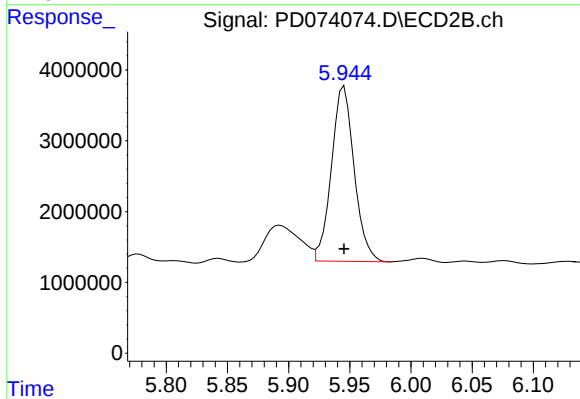

#27 Chlordane-5


R.T.: 5.945 min
Delta R.T.: 0.000 min
Response: 32031926
Conc: 498.11 ng/ml

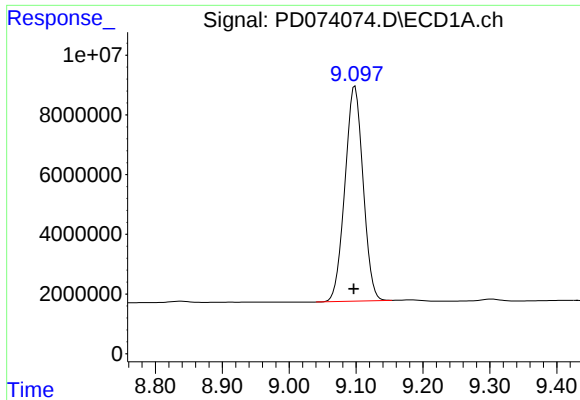

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.002 min
Response: 136142139
Conc: 49.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030123CHLOR

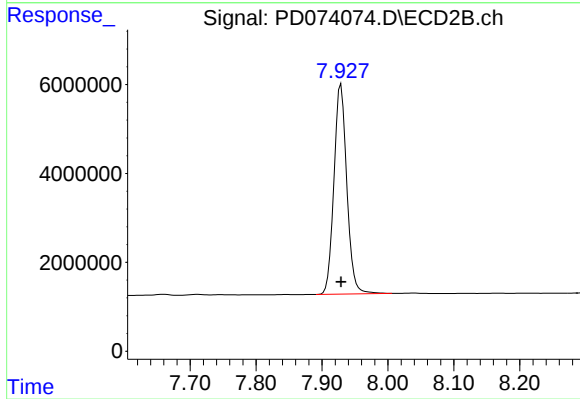

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 64006096
Conc: 49.97 ng/ml