

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030124\
 Data File : PD081854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2024 12:01
 Operator : AR\AJ
 Sample : P1647-07MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSK4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/04/2024
 Supervised By :Ankita Jodhani 03/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 19:43:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.791	17415594	32025630	12.739	13.063
27)	SA Decachlor...	9.105	7.923	31397157	43697554	16.273	17.615m
Target Compounds							
2)	A alpha-BHC	4.019	3.291	118.6E6	198.0E6	50.788m	51.496m
3)	MA gamma-BHC...	4.354	3.622	106.8E6	176.9E6	46.207	48.840
4)	MA Heptachlor	4.946	3.962	117.1E6	175.1E6	47.762	49.368
5)	MB Aldrin	5.289	4.241	114.1E6	165.9E6	48.238	48.985m
6)	B beta-BHC	4.548	3.917	49453468	77028390	47.587	45.587
7)	B delta-BHC	4.797	4.147	117.9E6	184.6E6	49.759	49.292
8)	B Heptachlo...	5.715	4.743	102.6E6	156.6E6	45.296	48.798
9)	A Endosulfan I	6.102	5.113	98613992	147.7E6	46.833	49.343
10)	B trans-Chl...	5.971	4.993	100.6E6	154.1E6	45.961	49.377
11)	B cis-Chlor...	6.050	5.057	103.1E6	154.7E6	45.760	48.279
12)	B 4,4'-DDE	6.222	5.245	200.9E6	297.4E6	93.585	100.570
13)	MA Dieldrin	6.377	5.377	211.2E6	320.7E6	95.109	97.650
14)	MA Endrin	6.608	5.651	175.6E6	283.4E6	93.595	98.647m
15)	B Endosulfa...	6.826	5.944	181.9E6	278.9E6	94.235	98.821
16)	A 4,4'-DDD	6.739	5.798	157.4E6	244.8E6	94.763	97.132
17)	MA 4,4'-DDT	7.054	6.049	172.8E6	258.3E6	99.480	100.035
18)	B Endrin al...	6.955	6.124	129.2E6	195.5E6	86.480	90.213
19)	B Endosulfa...	7.190	6.344	173.8E6	261.8E6	94.943	97.605m
20)	A Methoxychlor	7.528	6.623	438.3E6	620.7E6	477.847	464.601
21)	B Endrin ke...	7.676	6.851	195.9E6	296.3E6	101.332	98.818

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030124\
Data File : PD081854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2024 12:01
Operator : AR\AJ
Sample : P1647-07MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 19:43:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

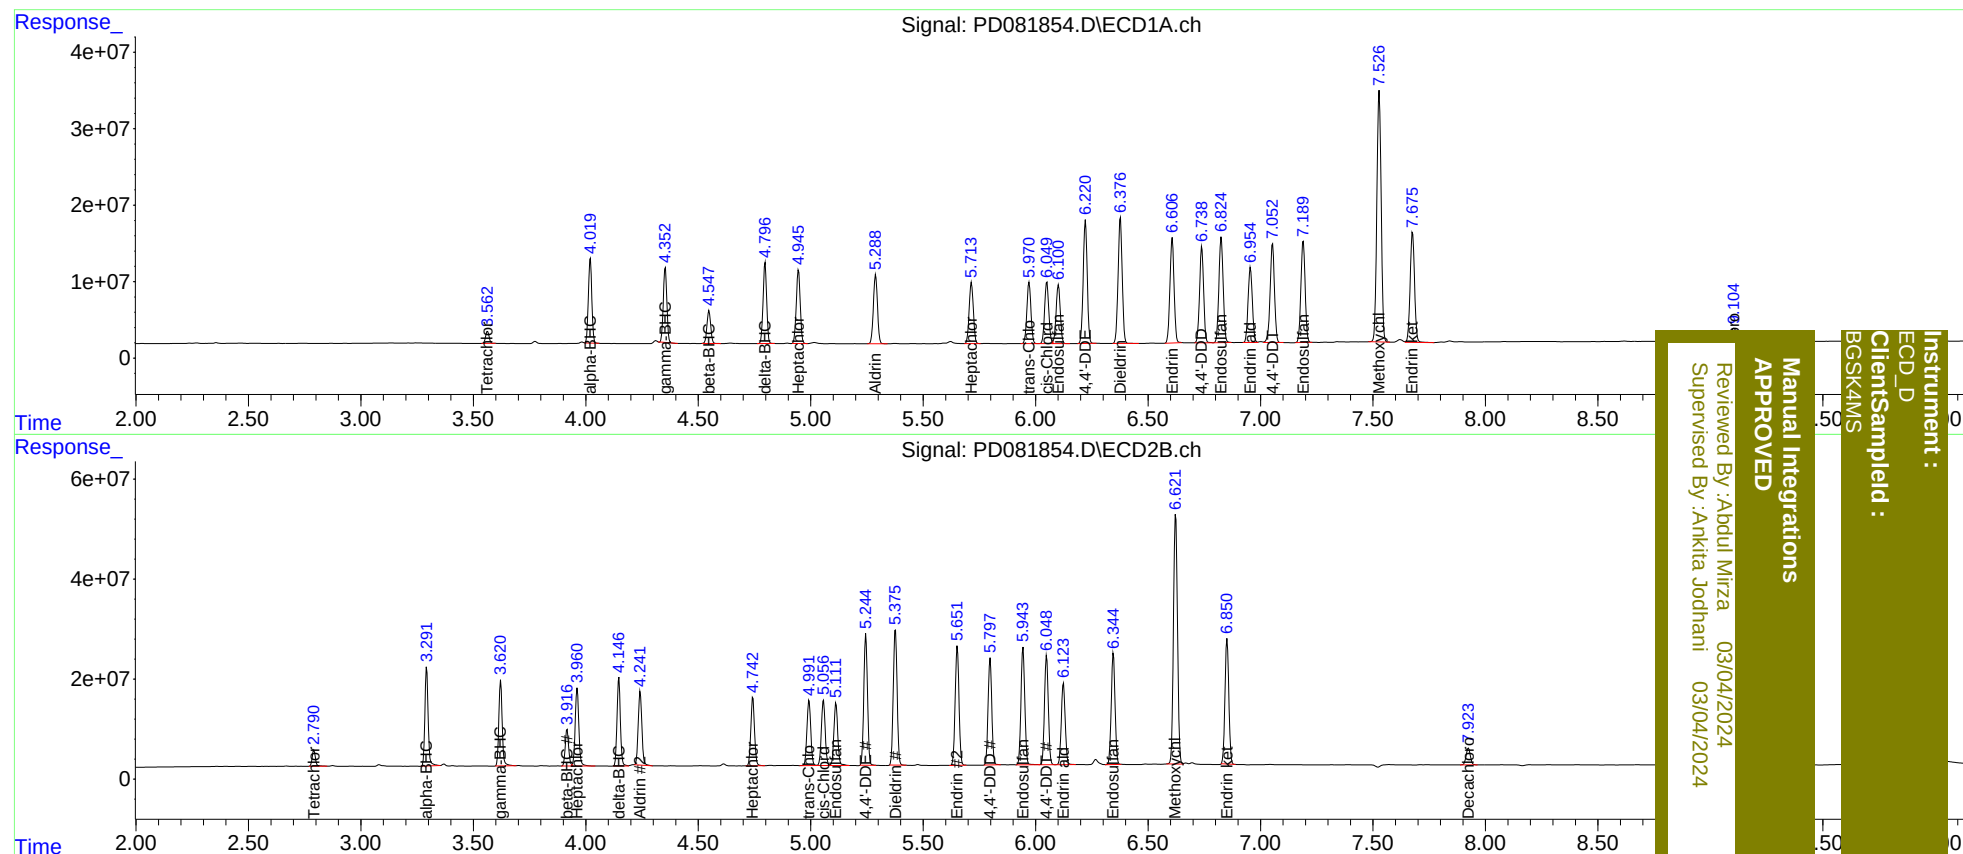

Instrument :
ECD_D
ClientSampled :
BSK4MS
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 03/04/2024
Supervised By :Ankita Jodhani 03/04/2024