

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030124\
 Data File : PD081885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2024 18:54
 Operator : AR\AJ
 Sample : P1603-21
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSY2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/04/2024
 Supervised By :Ankita Jodhani 03/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 19:50:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.791	15110973	28032941	11.053	11.435
27)	SA Decachlor...	9.106	7.923	21306085	31714784	11.043m	12.785m
Target Compounds							
5)	MB Aldrin	5.291	4.242	2735375	3657982	1.157	1.080
10)	B trans-Chl...	5.971	4.993	4201530	5715925	1.919	1.832
11)	B cis-Chlor...	6.055	5.057	15145373	10616269	6.724	3.314 #
13)	MA Dieldrin	6.378	5.377	123.4E6	191.5E6	55.583	58.318

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030124\
Data File : PD081885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2024 18:54
Operator : AR\AJ
Sample : P1603-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 19:50:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

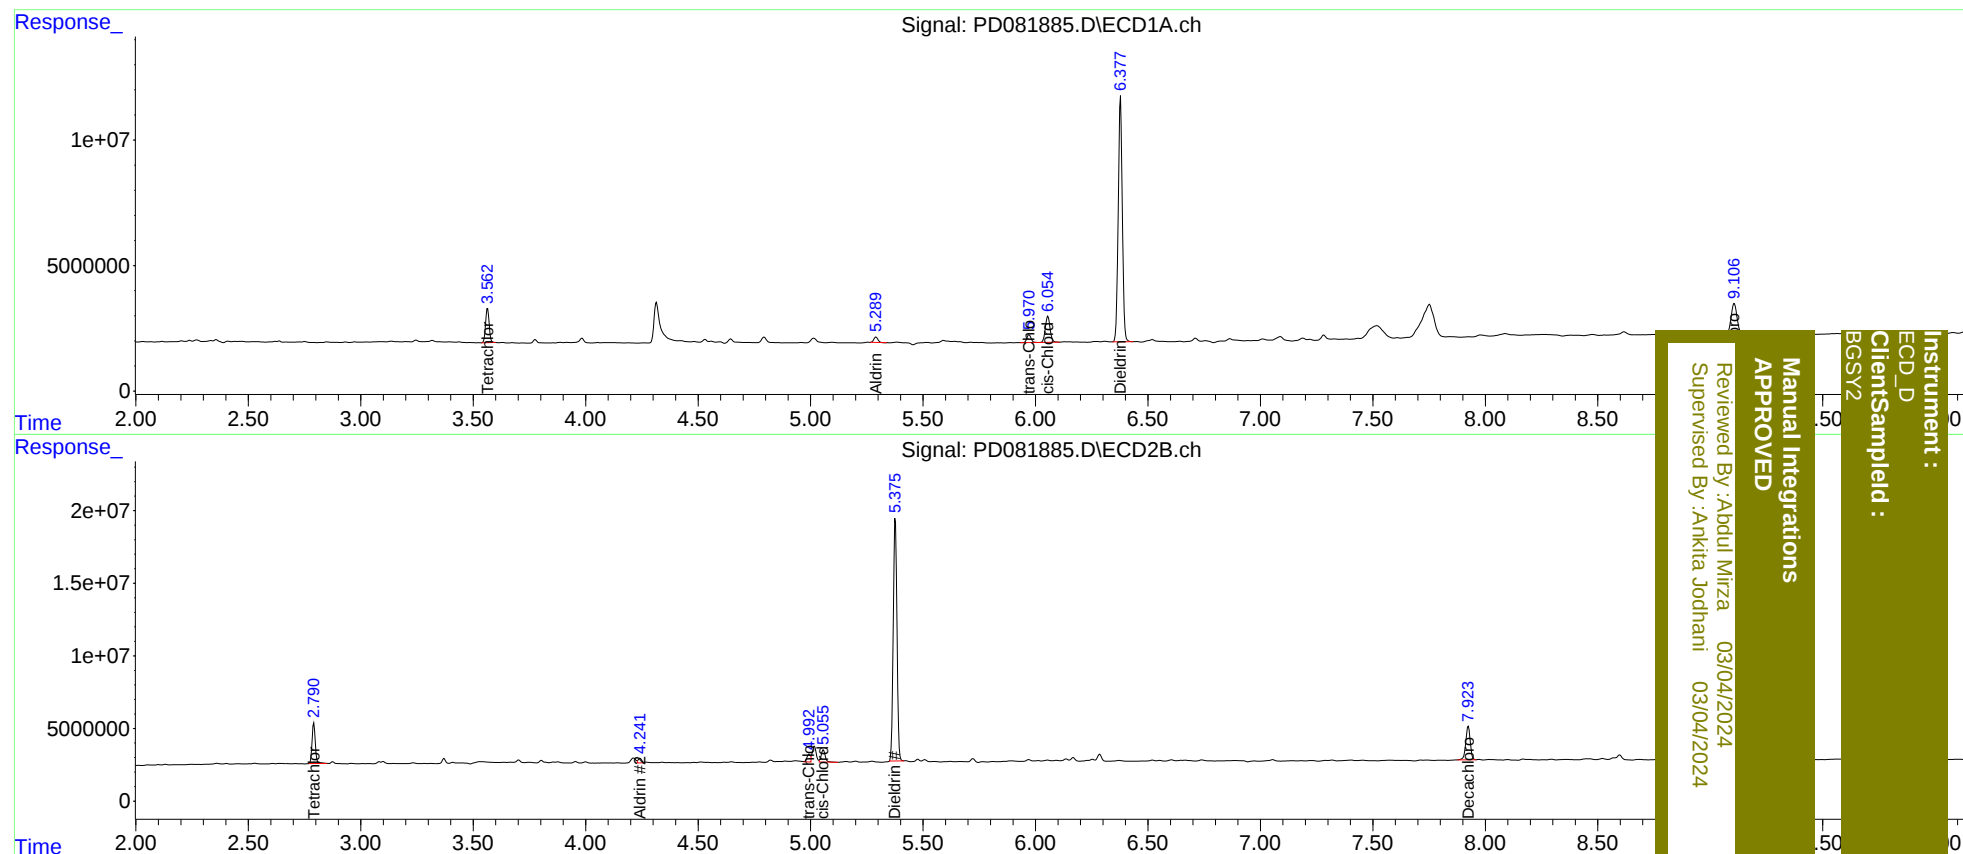

Reviewed By: Abdul Mirza 03/04/2024
Supervised By: Ankita Jodhani 03/04/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGSY2