

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051479.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 16:53
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 03:01:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	25478212	594.4E6	19.215	20.728
28)	SA Decachlor...	7.823	9.156	23741840	388.7E6	20.887	21.279
Target Compounds							
3)	MA gamma-BHC...	3.931f	4.737	1024394	816853	0.490	0.021 #
4)	MA Heptachlor	0.000	5.254f	0	7047928	N.D.	0.184 #
7)	B delta-BHC	0.000	5.086f	0	40302220	N.D.	1.173 #
8)	B Heptachlo...	0.000	5.917	0	3118175	N.D.	0.097 #
10)	B gamma-Chl...	0.000	6.174	0	14179707	N.D.	0.443 #
11)	B alpha-Chl...	0.000	6.240	0	3639094	N.D.	0.115 #
15)	B Endosulfa...	0.000	6.973	0	8892959	N.D.	0.345 #
25)	Chlordane-3	0.000	6.174	0	14179707	N.D.	3.184 #
26)	Chlordane-4	0.000	6.240	0	3639094	N.D.	0.695 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051479.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 16:53
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 03:01:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

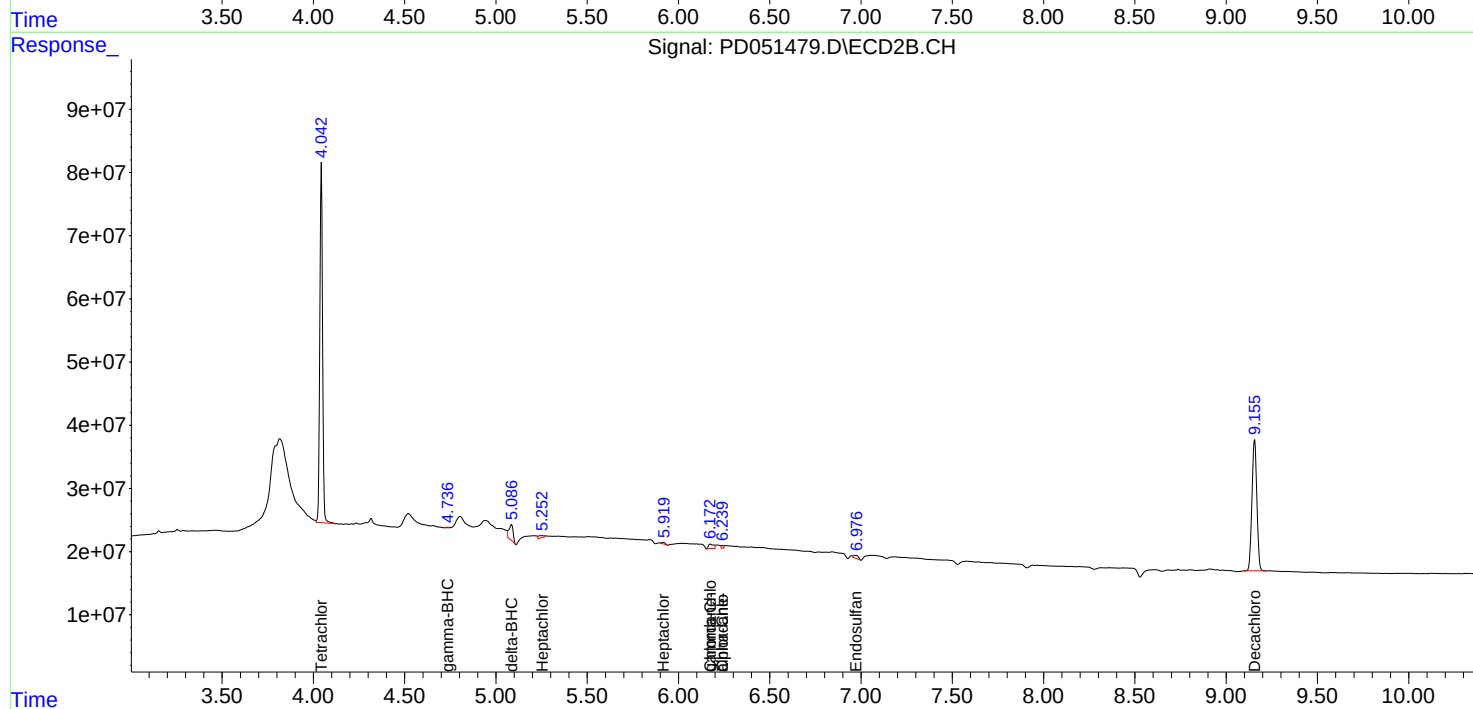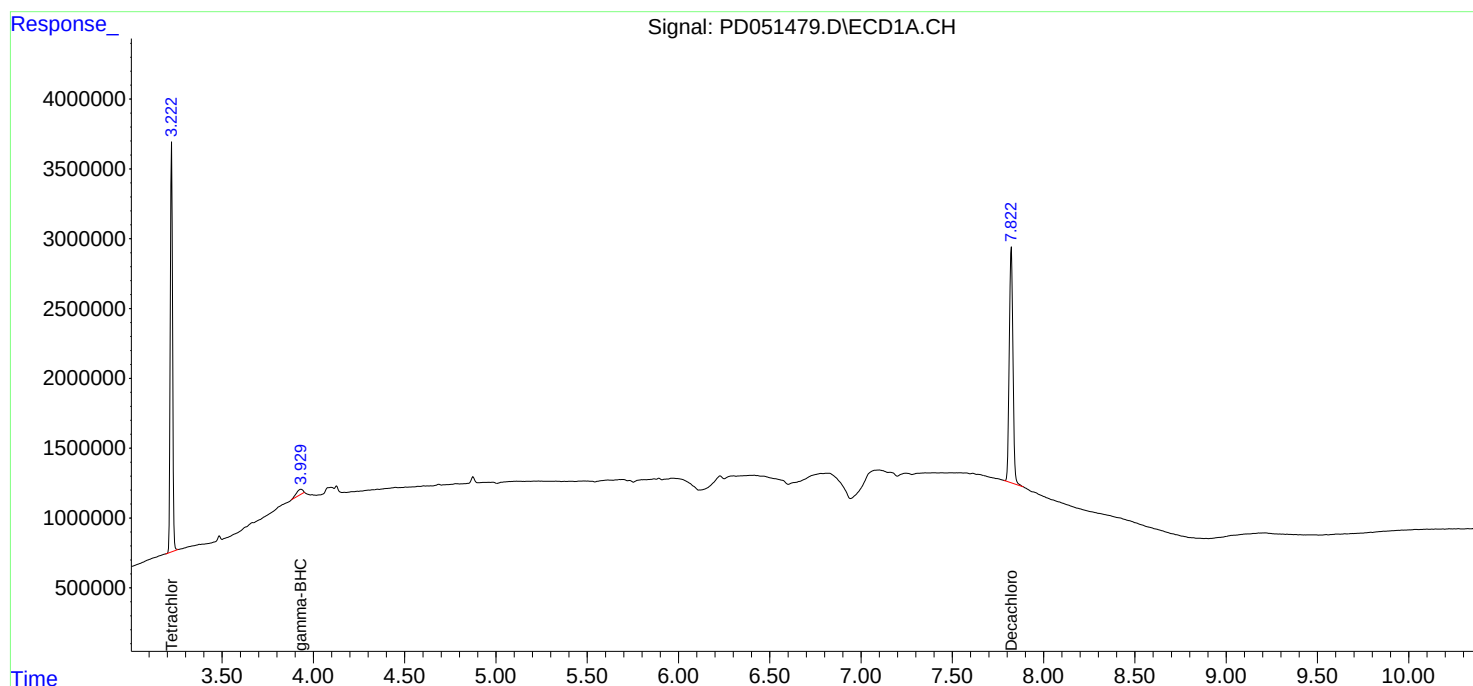


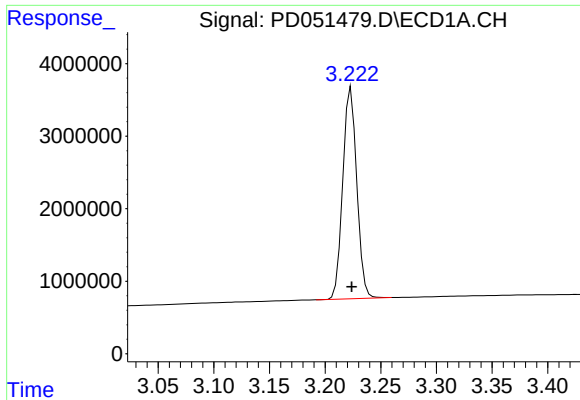

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 25478212
Conc: 19.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

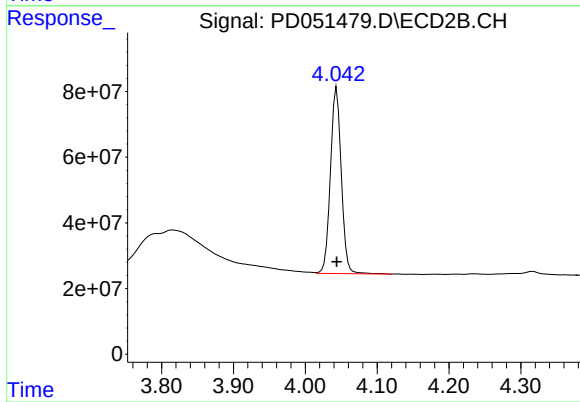


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 594407428
Conc: 20.73 ng/ml

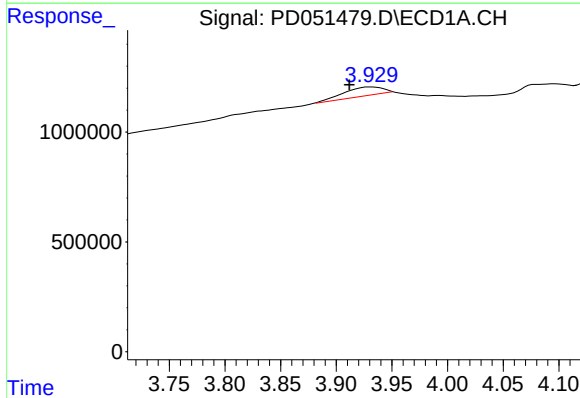


#3 gamma-BHC (Lindane)

R.T.: 3.931 min
Delta R.T.: 0.019 min
Response: 1024394
Conc: 0.49 ng/ml

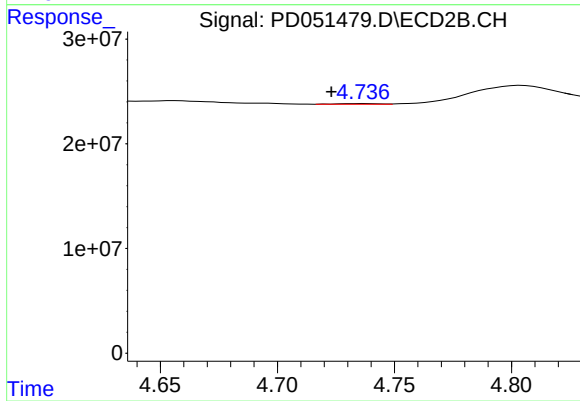

#3 gamma-BHC (Lindane)


R.T.: 4.737 min
Delta R.T.: 0.014 min
Response: 816853
Conc: 0.02 ng/ml

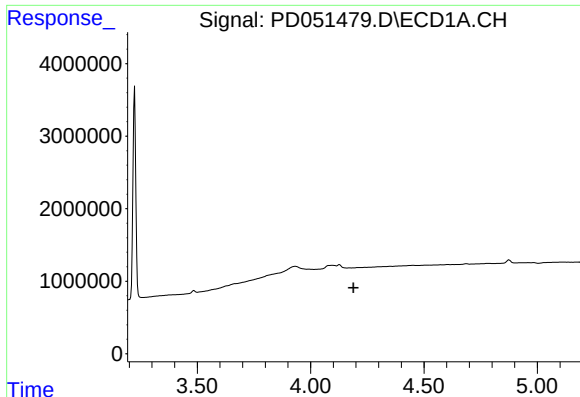

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

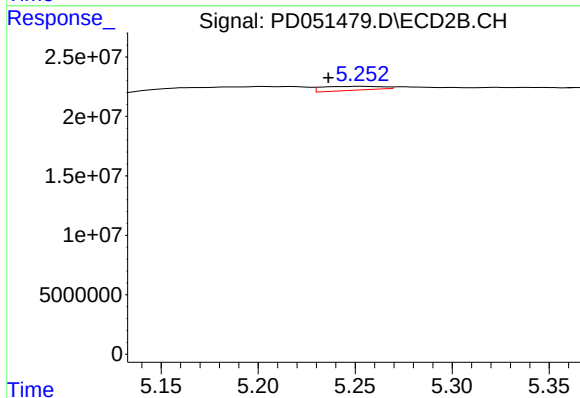


#4 Heptachlor

R.T.: 5.254 min
Delta R.T.: 0.018 min
Response: 7047928
Conc: 0.18 ng/ml

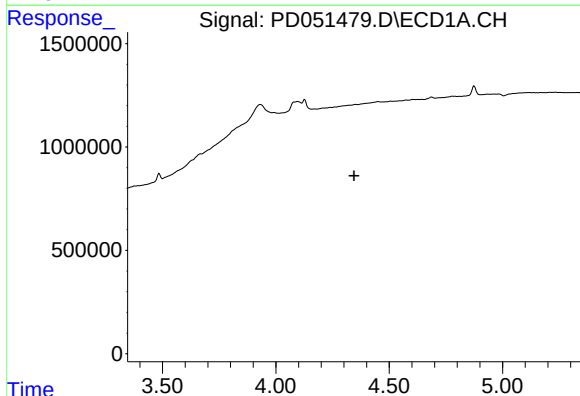


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

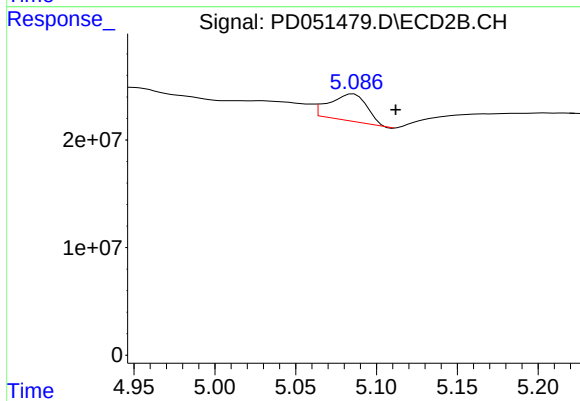

#7 delta-BHC


R.T.: 5.086 min
Delta R.T.: -0.026 min
Response: 40302220
Conc: 1.17 ng/ml

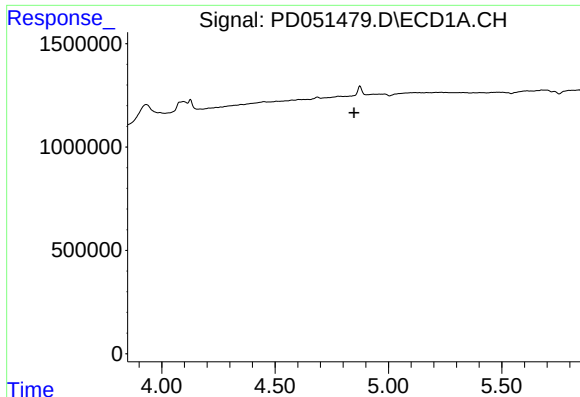

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.849 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

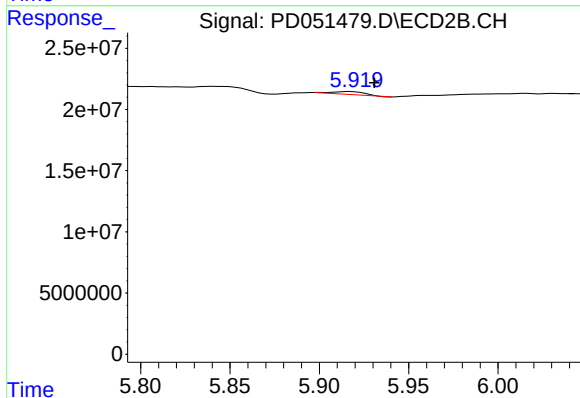


#8 Heptachlor epoxide

R.T.: 5.917 min
Delta R.T.: -0.013 min
Response: 3118175
Conc: 0.10 ng/ml

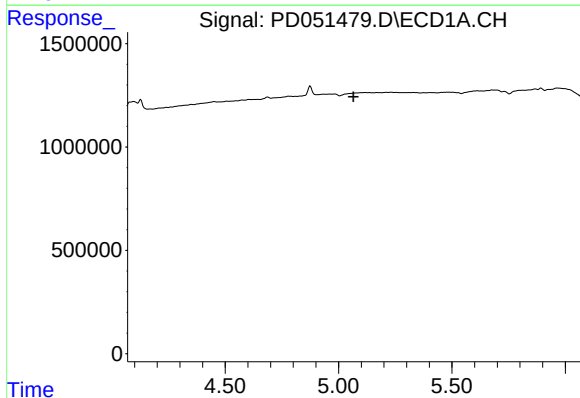


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

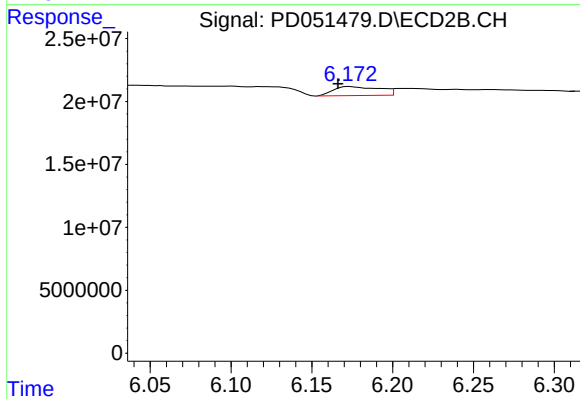

#10 gamma-Chlordane


R.T.: 6.174 min
Delta R.T.: 0.007 min
Response: 14179707
Conc: 0.44 ng/ml

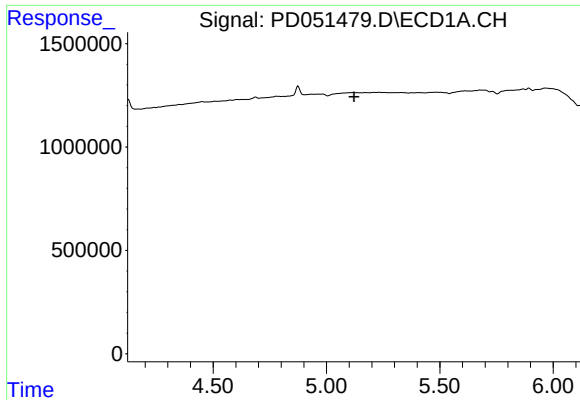

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.122 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

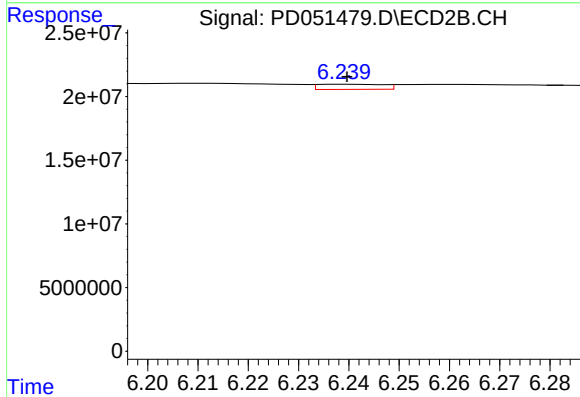


#11 alpha-Chlordane

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 3639094
Conc: 0.11 ng/ml

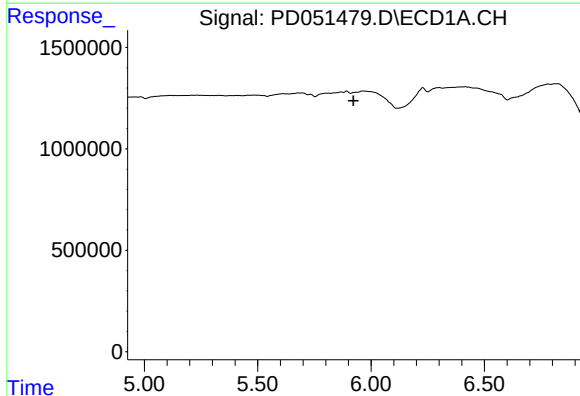


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.923 min
Response: 0
Conc: N.D.

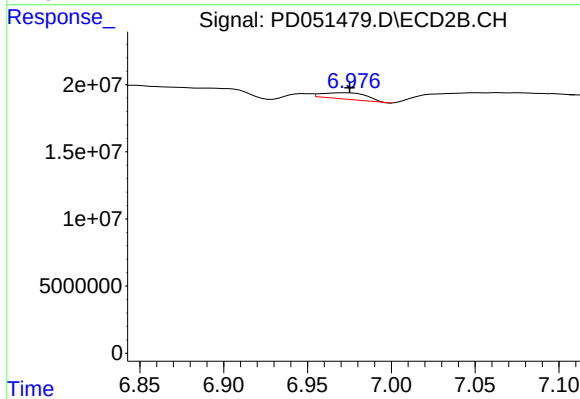

#15 Endosulfan II


R.T.: 6.973 min
Delta R.T.: -0.002 min
Response: 8892959
Conc: 0.35 ng/ml

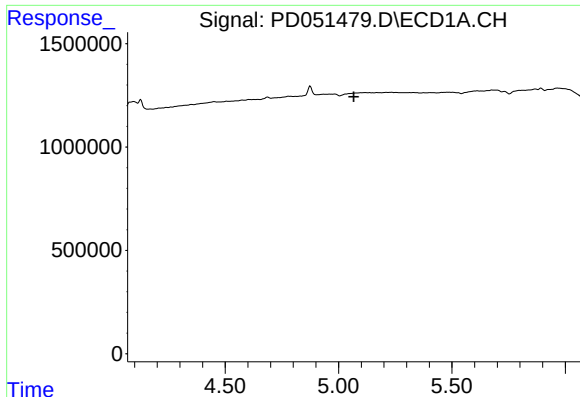

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

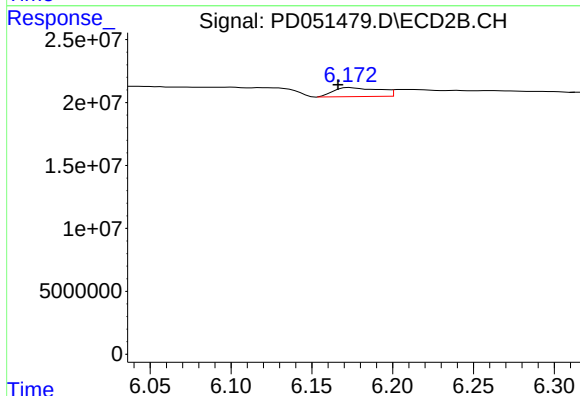


#25 Chlordane-3

R.T.: 6.174 min
Delta R.T.: 0.007 min
Response: 14179707
Conc: 3.18 ng/ml

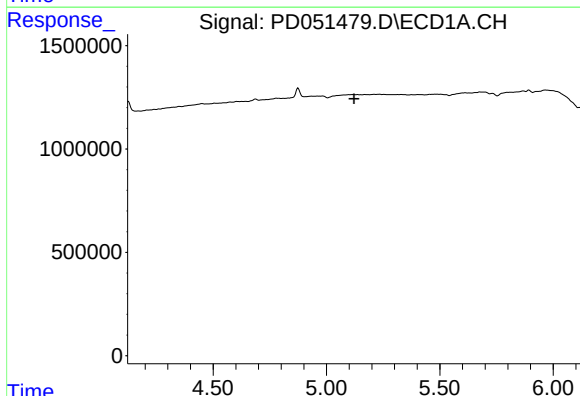


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.122 min
Response: 0
Conc: N.D.

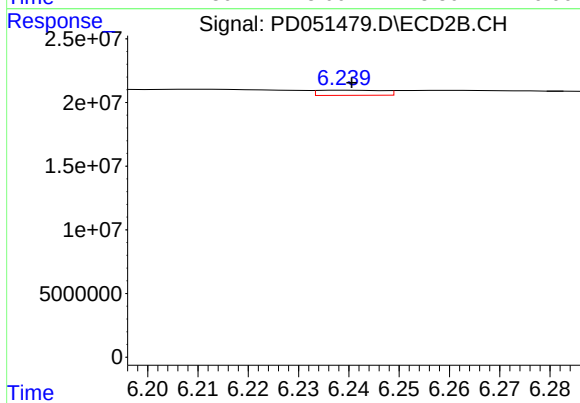

#26 Chlordane-4


R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 3639094
Conc: 0.69 ng/ml

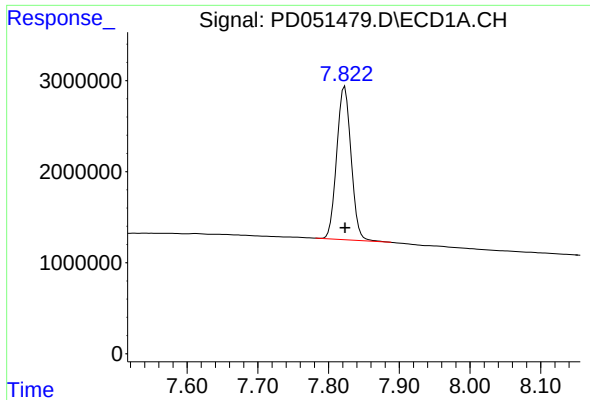

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 23741840
Conc: 20.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

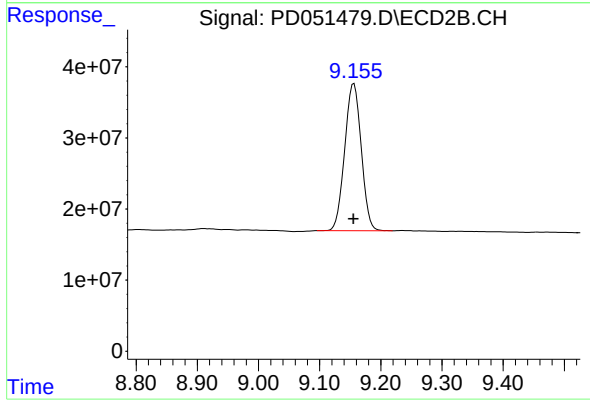

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 388713350
Conc: 21.28 ng/ml