

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051487.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 18:45
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 23:29:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:29:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	131.7E6	2385.9E6	97.611	89.550
28)	SA Decachlor...	7.824	9.155	95080861	1473.0E6	89.188	88.078
Target Compounds							
23)	Chlordane-1	4.046	5.047	64682100	1348.5E6	984.213	896.136
24)	Chlordane-2	4.526	5.517	72959862	1189.5E6	921.597	866.302
25)	Chlordane-3	5.067	6.166	237.2E6	3941.2E6	988.489	901.277
26)	Chlordane-4	5.122	6.241	224.0E6	4580.4E6	968.367	893.354
27)	Chlordane-5	5.927	7.049	72008987	891.8E6	962.684	897.774



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051487.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 18:45
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:29:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:29:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

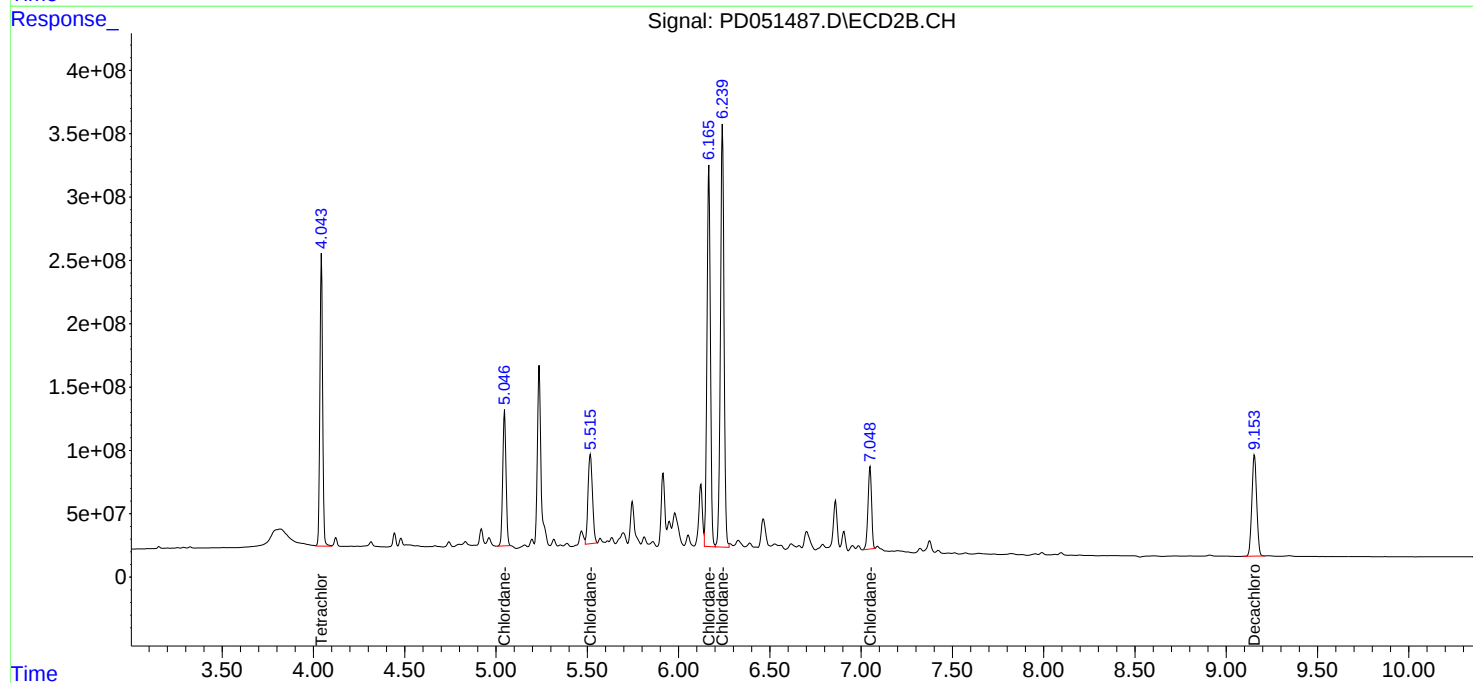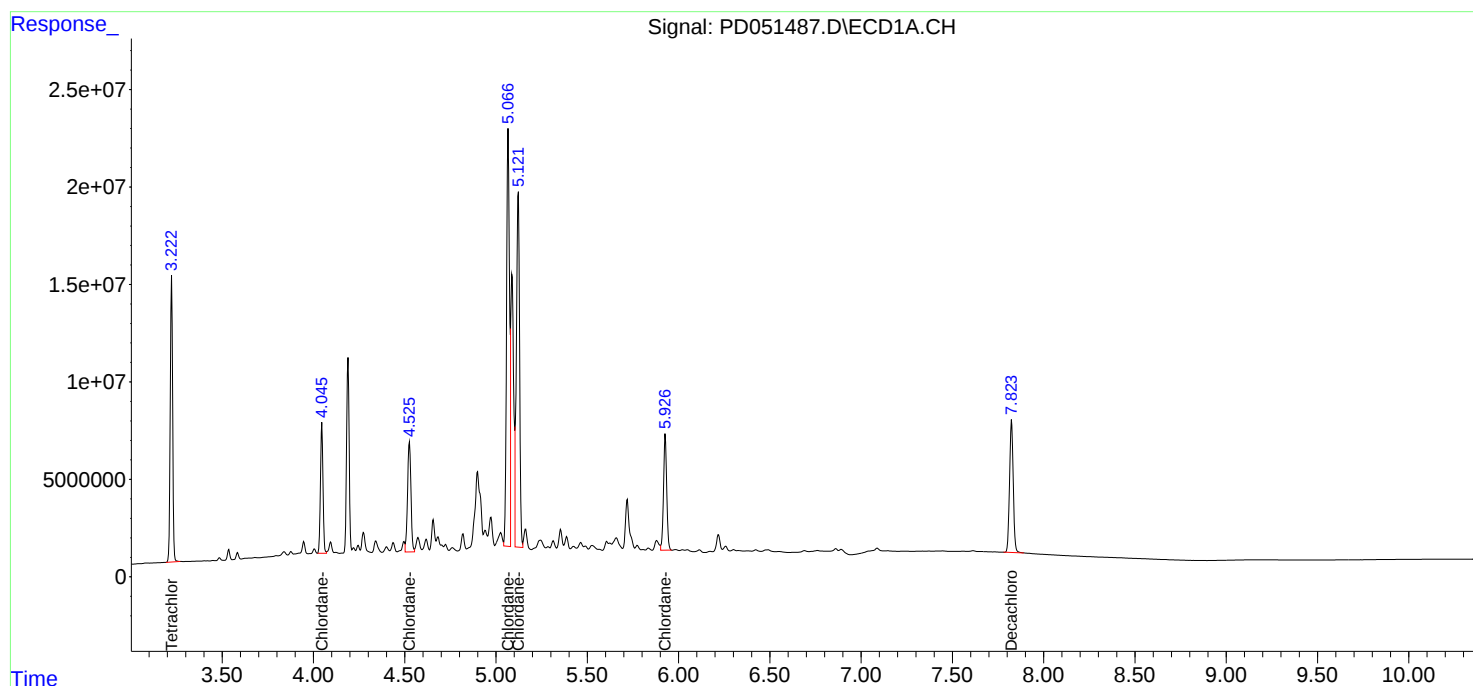


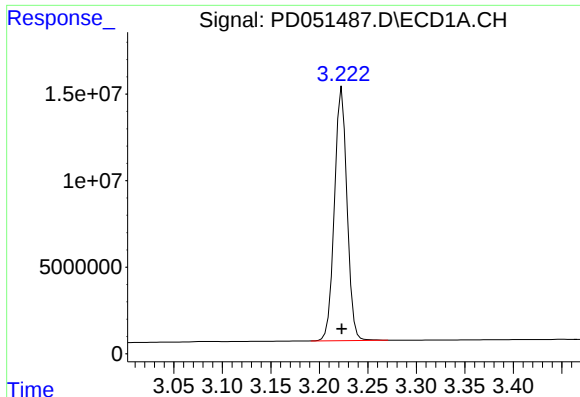

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 131731493
Conc: 97.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

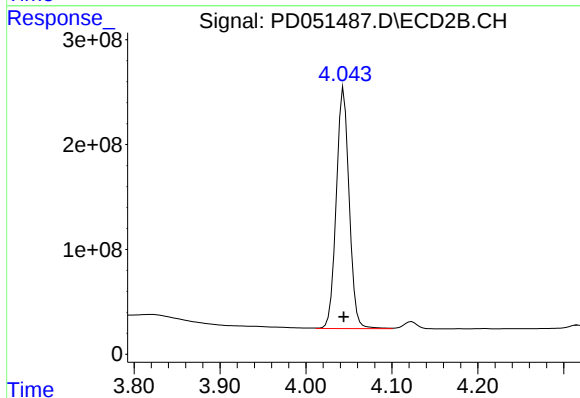


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 2385892226
Conc: 89.55 ng/ml

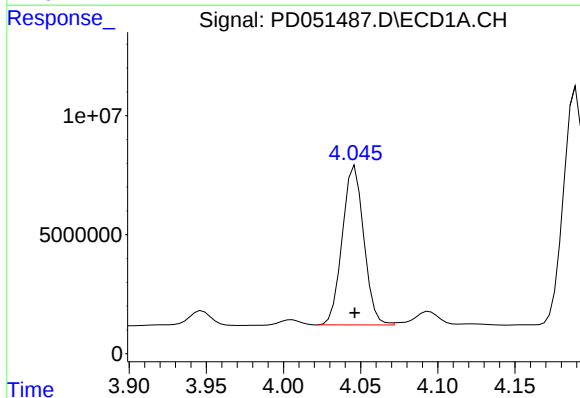


#23 Chlordane-1

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 64682100
Conc: 984.21 ng/ml

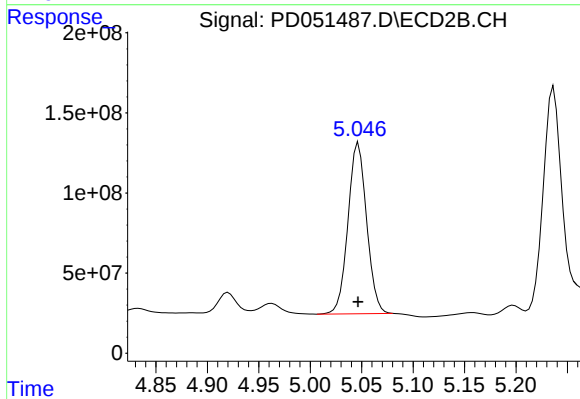

#23 Chlordane-1


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 1348490293
Conc: 896.14 ng/ml

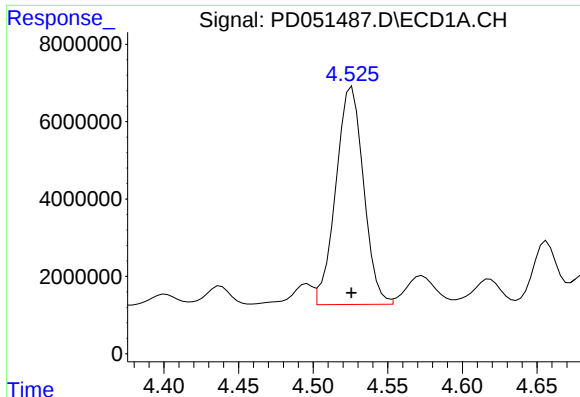

#24 Chlordane-2


R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 72959862
Conc: 921.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

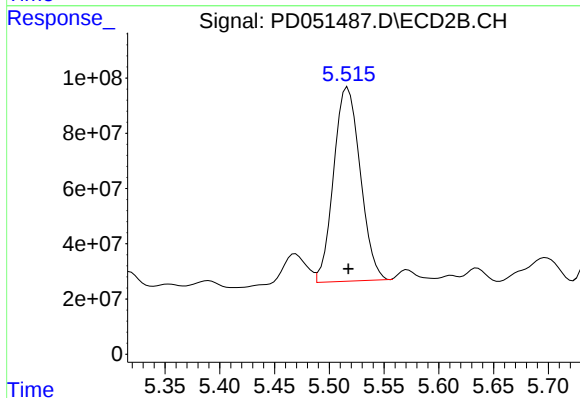


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 1189541874
Conc: 866.30 ng/ml

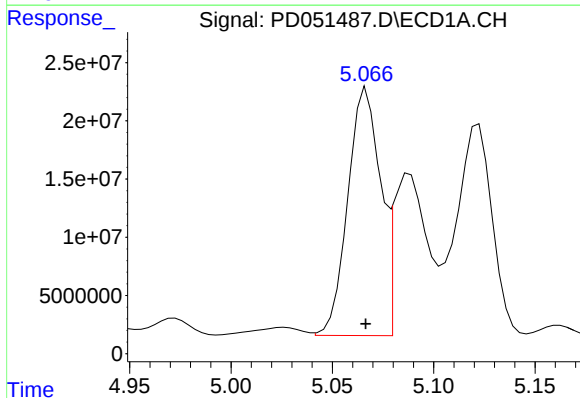


#25 Chlordane-3

R.T.: 5.067 min
Delta R.T.: 0.000 min
Response: 237161433
Conc: 988.49 ng/ml

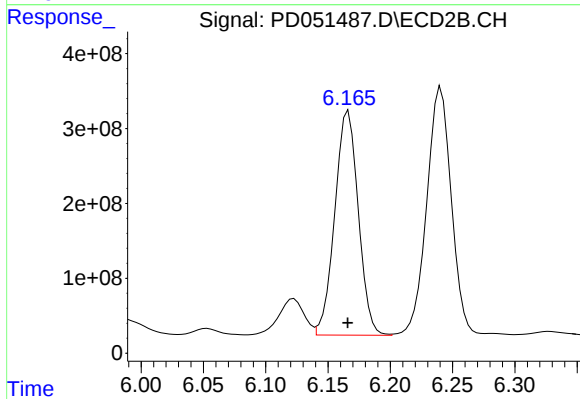

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 3941170253
Conc: 901.28 ng/ml

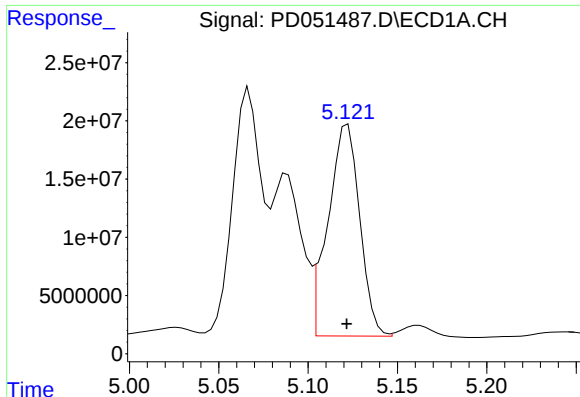

#26 Chlordane-4


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 223984248
Conc: 968.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

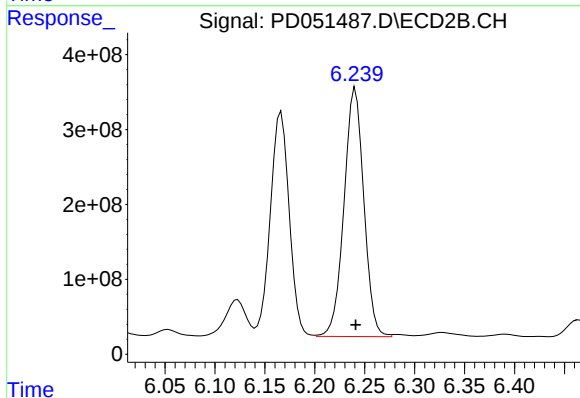


#26 Chlordane-4

R.T.: 6.241 min
Delta R.T.: 0.000 min
Response: 4580409017
Conc: 893.35 ng/ml

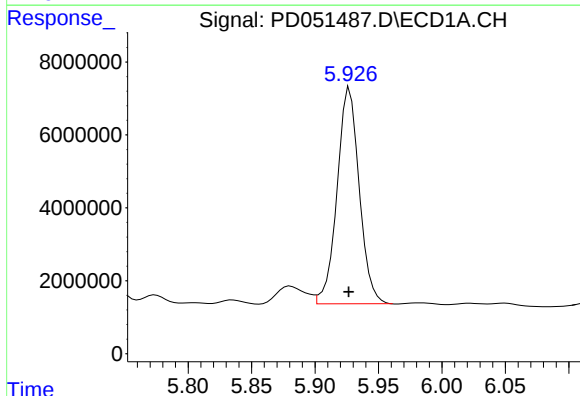


#27 Chlordane-5

R.T.: 5.927 min
Delta R.T.: 0.001 min
Response: 72008987
Conc: 962.68 ng/ml

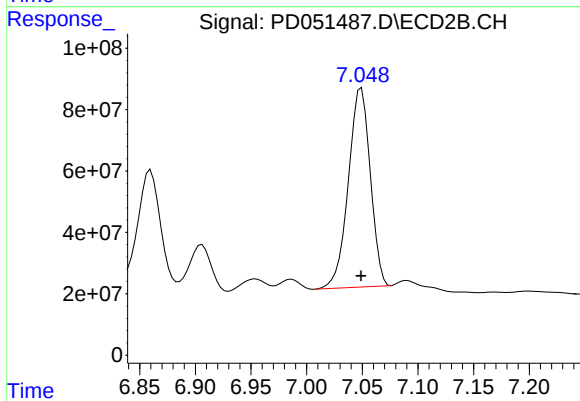

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 891791081
Conc: 897.77 ng/ml

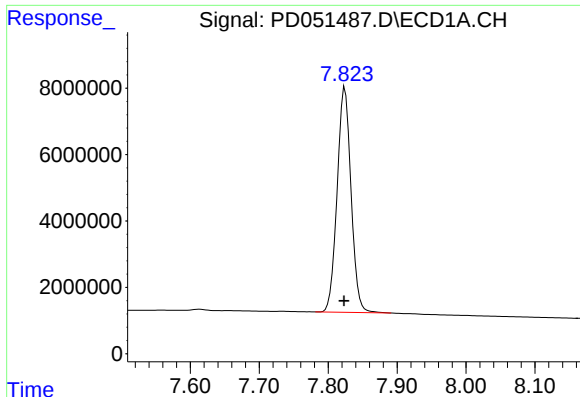

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.002 min
Response: 95080861
Conc: 89.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

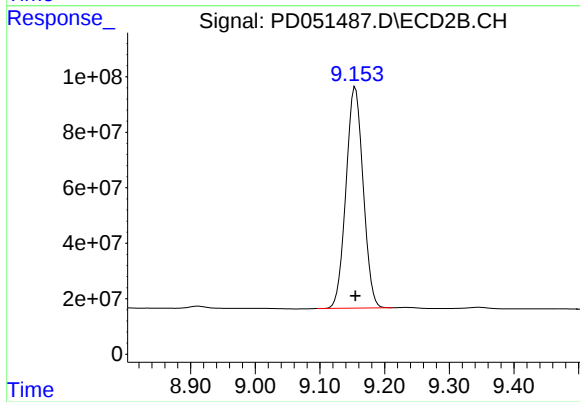

#28 Decachlorobiphenyl

R.T.: 9.155 min
Delta R.T.: 0.000 min
Response: 1473015798
Conc: 88.08 ng/ml