

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051490.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 19:27
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 23:30:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:29:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	32271867	700.3E6	23.913	26.284
28)	SA Decachlor...	7.823	9.156	28469214	452.1E6	26.705	27.032
Target Compounds							
23)	Chlordane-1	4.046	5.046	16131896	394.9E6	245.465	262.405
24)	Chlordane-2	4.525	5.516	19965656	373.3E6	252.198	271.830
25)	Chlordane-3	5.066	6.165	57512165	1149.6E6	239.711	262.900
26)	Chlordane-4	5.122	6.240	55845382	1345.6E6	241.440	262.439
27)	Chlordane-5	5.926	7.049	18445575	261.1E6	246.598	262.843



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051490.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 19:27
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:30:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:29:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

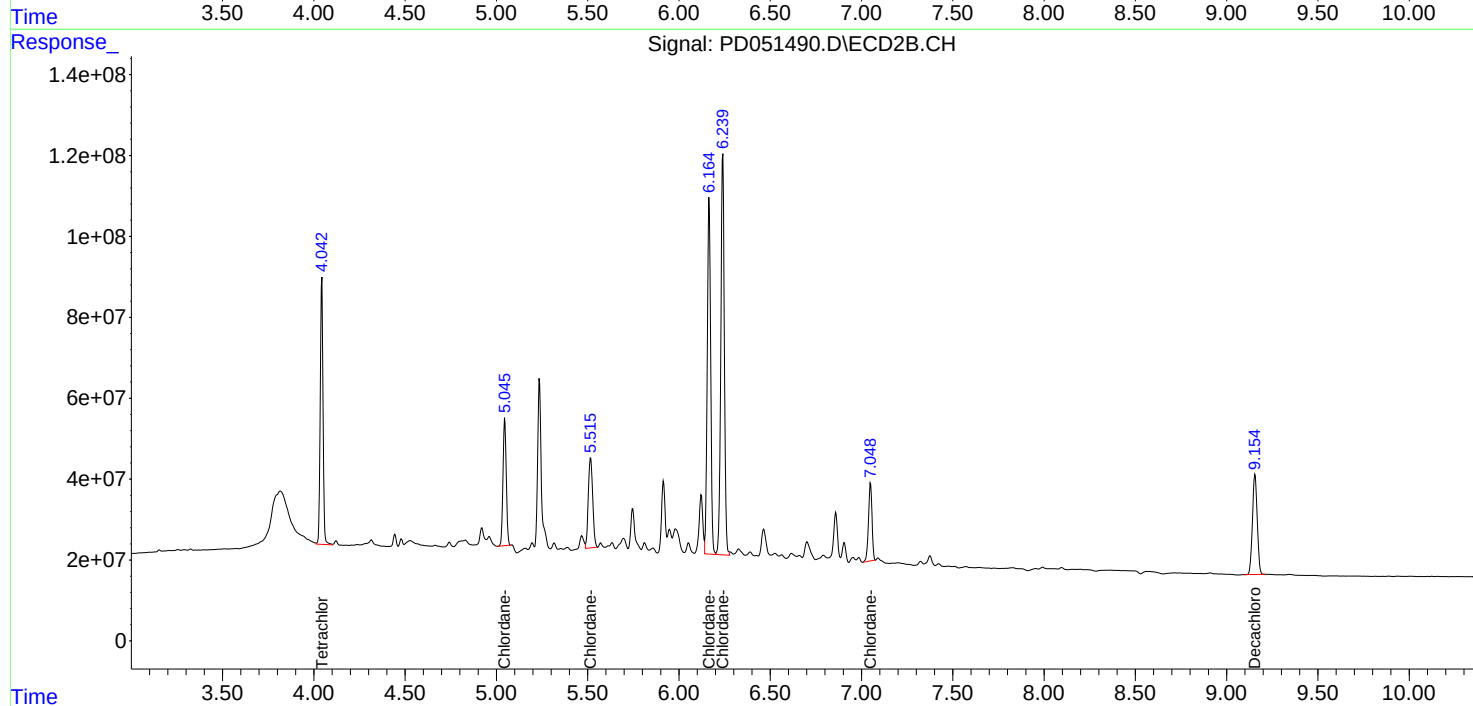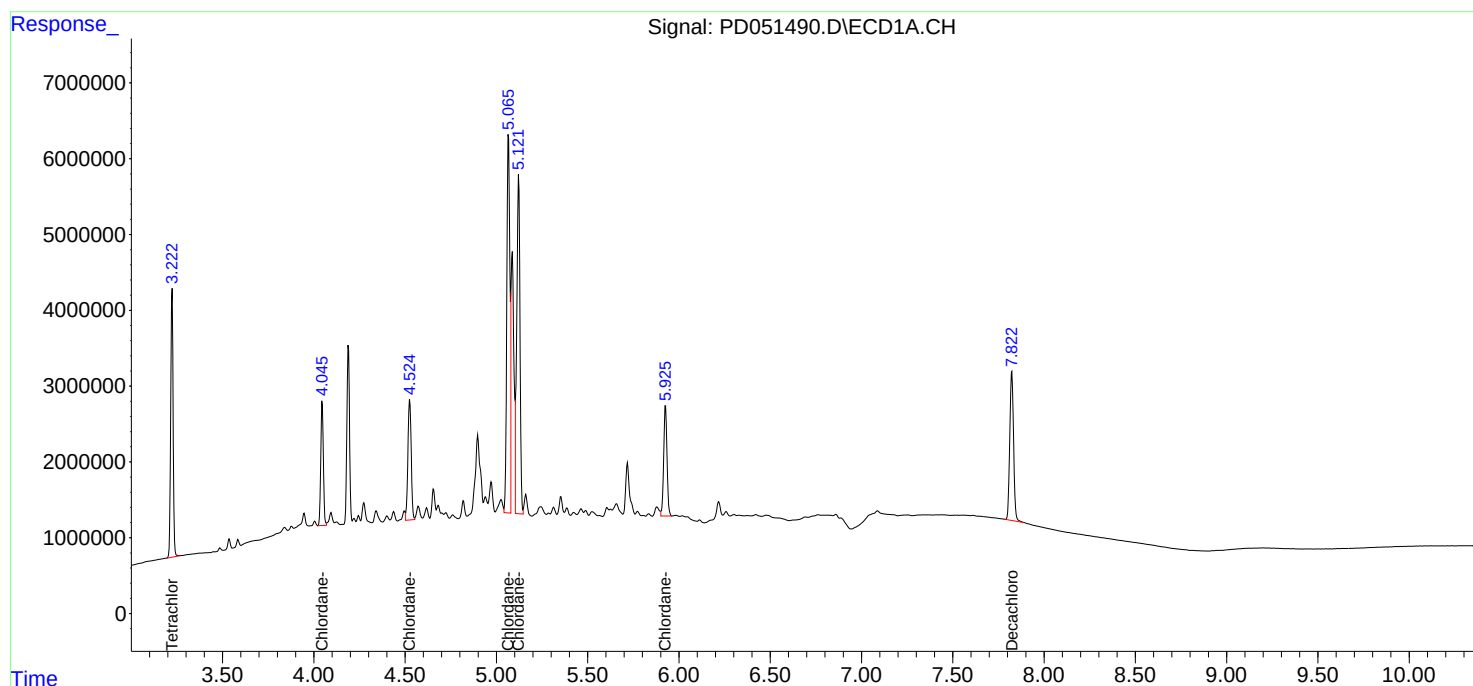


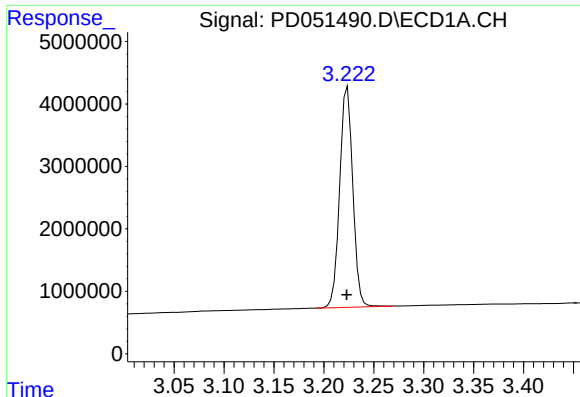

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 32271867
Conc: 23.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

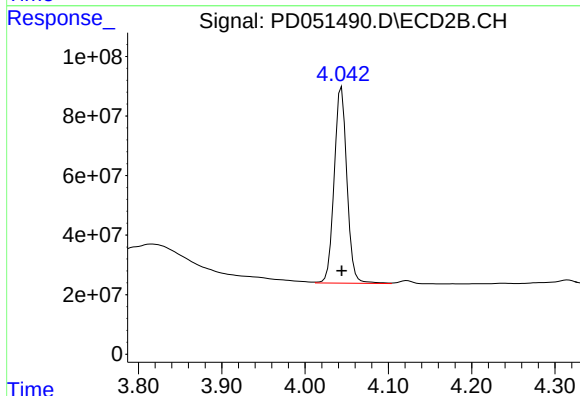


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 700277759
Conc: 26.28 ng/ml

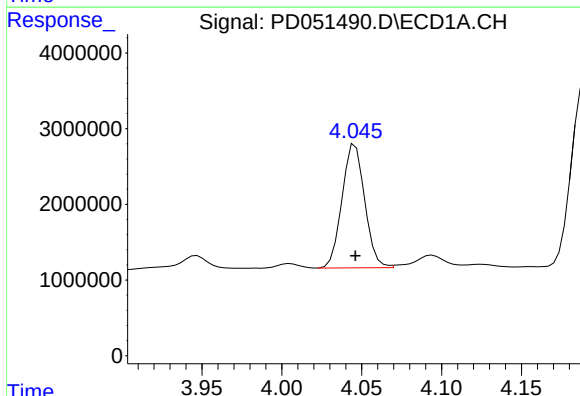


#23 Chlordane-1

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 16131896
Conc: 245.47 ng/ml

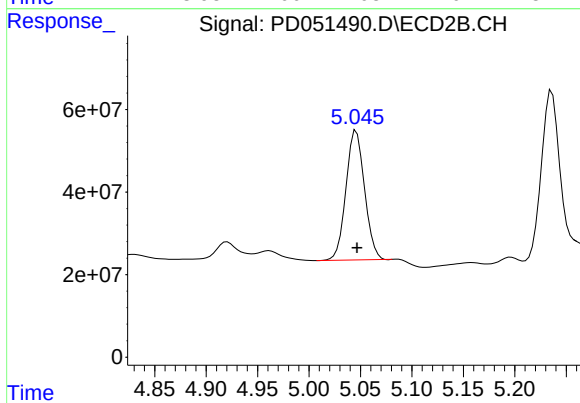

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 394862838
Conc: 262.41 ng/ml

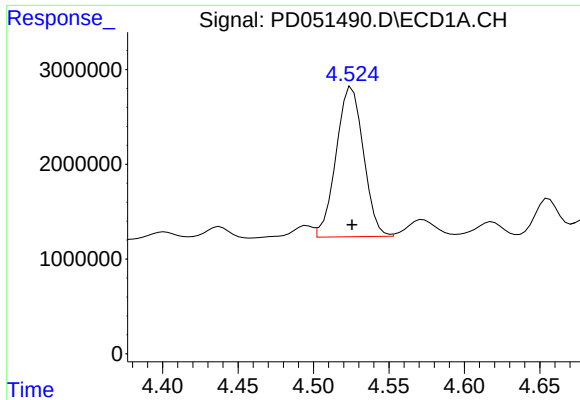

#24 Chlordane-2


R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 19965656
Conc: 252.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

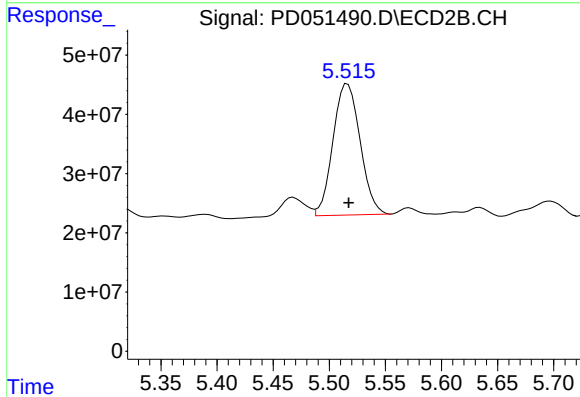


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 373257183
Conc: 271.83 ng/ml

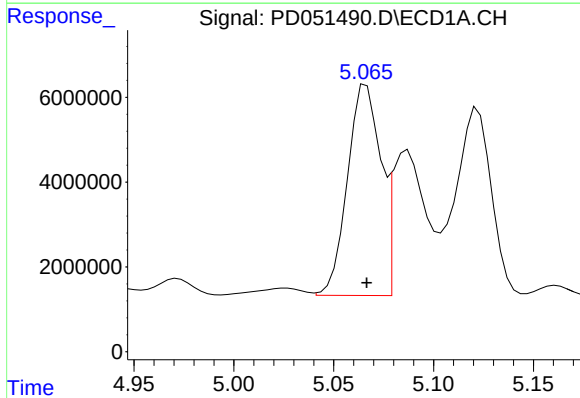


#25 Chlordane-3

R.T.: 5.066 min
Delta R.T.: 0.000 min
Response: 57512165
Conc: 239.71 ng/ml

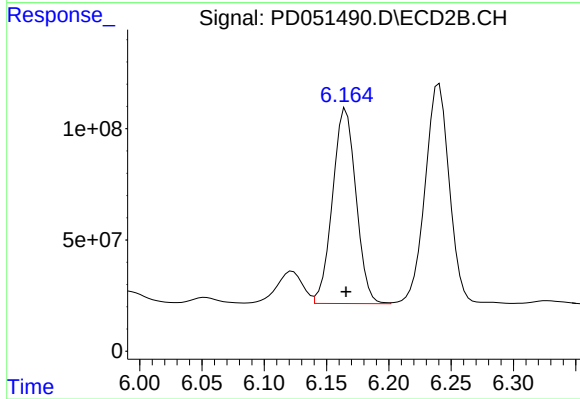

#25 Chlordane-3


R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 1149626410
Conc: 262.90 ng/ml

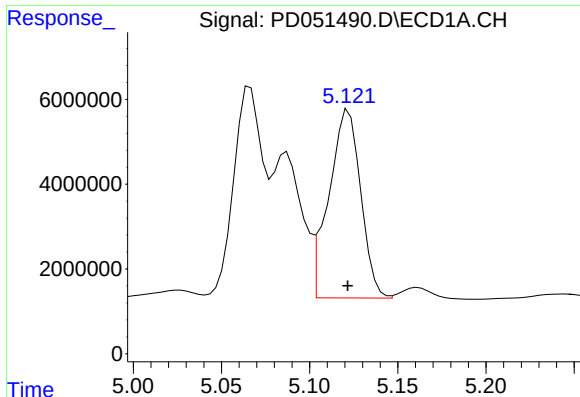

#26 Chlordane-4


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 55845382
Conc: 241.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

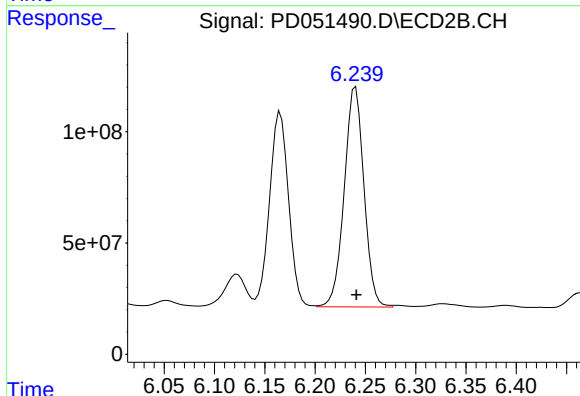


#26 Chlordane-4

R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 1345578099
Conc: 262.44 ng/ml

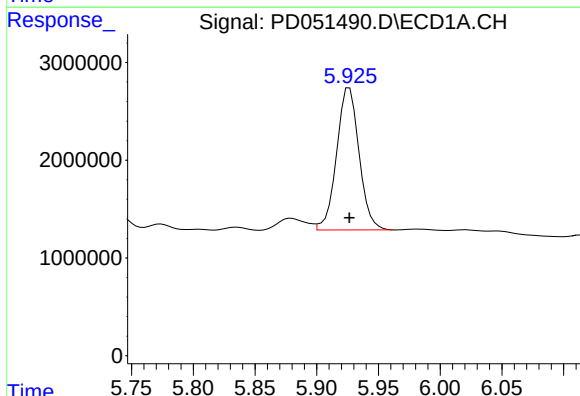


#27 Chlordane-5

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 18445575
Conc: 246.60 ng/ml

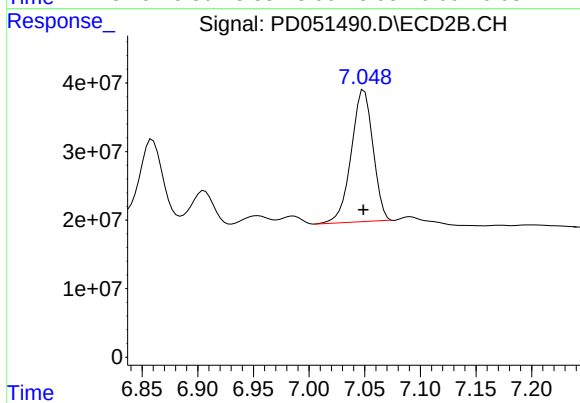

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 261091144
Conc: 262.84 ng/ml

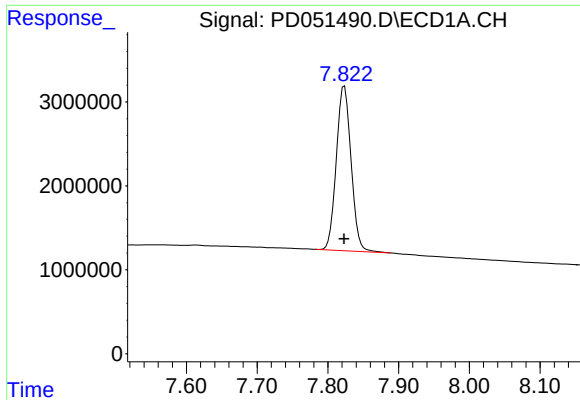

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 28469214
Conc: 26.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

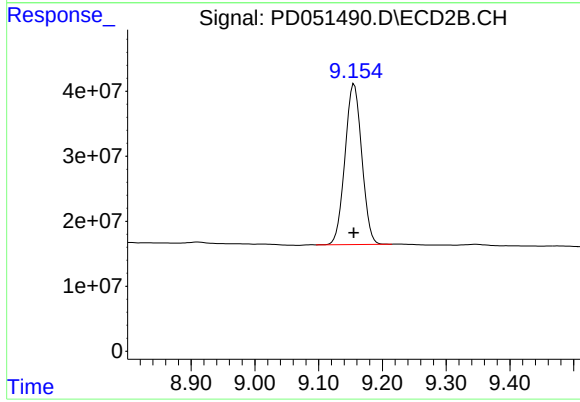

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 452079314
Conc: 27.03 ng/ml