

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051491.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 19:41
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 23:30:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:29:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.043	6341241	169.0E6	4.699	6.344 #
28)	SA Decachlor...	7.824	9.156	6473370	110.3E6	6.072	6.596
Target Compounds							
23)	Chlordane-1	4.045	5.046	2987490	90190312	45.458	59.936 #
24)	Chlordane-2	4.525	5.517	4175684	88049190	52.745	64.123
25)	Chlordane-3	5.066	6.166	10662139	262.2E6	44.440	59.971 #
26)	Chlordane-4	5.121	6.241	10435548	314.9E6	45.117	61.417 #
27)	Chlordane-5	5.926	7.049	3308183	58716416	44.227	59.110 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051491.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 19:41
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:30:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:29:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

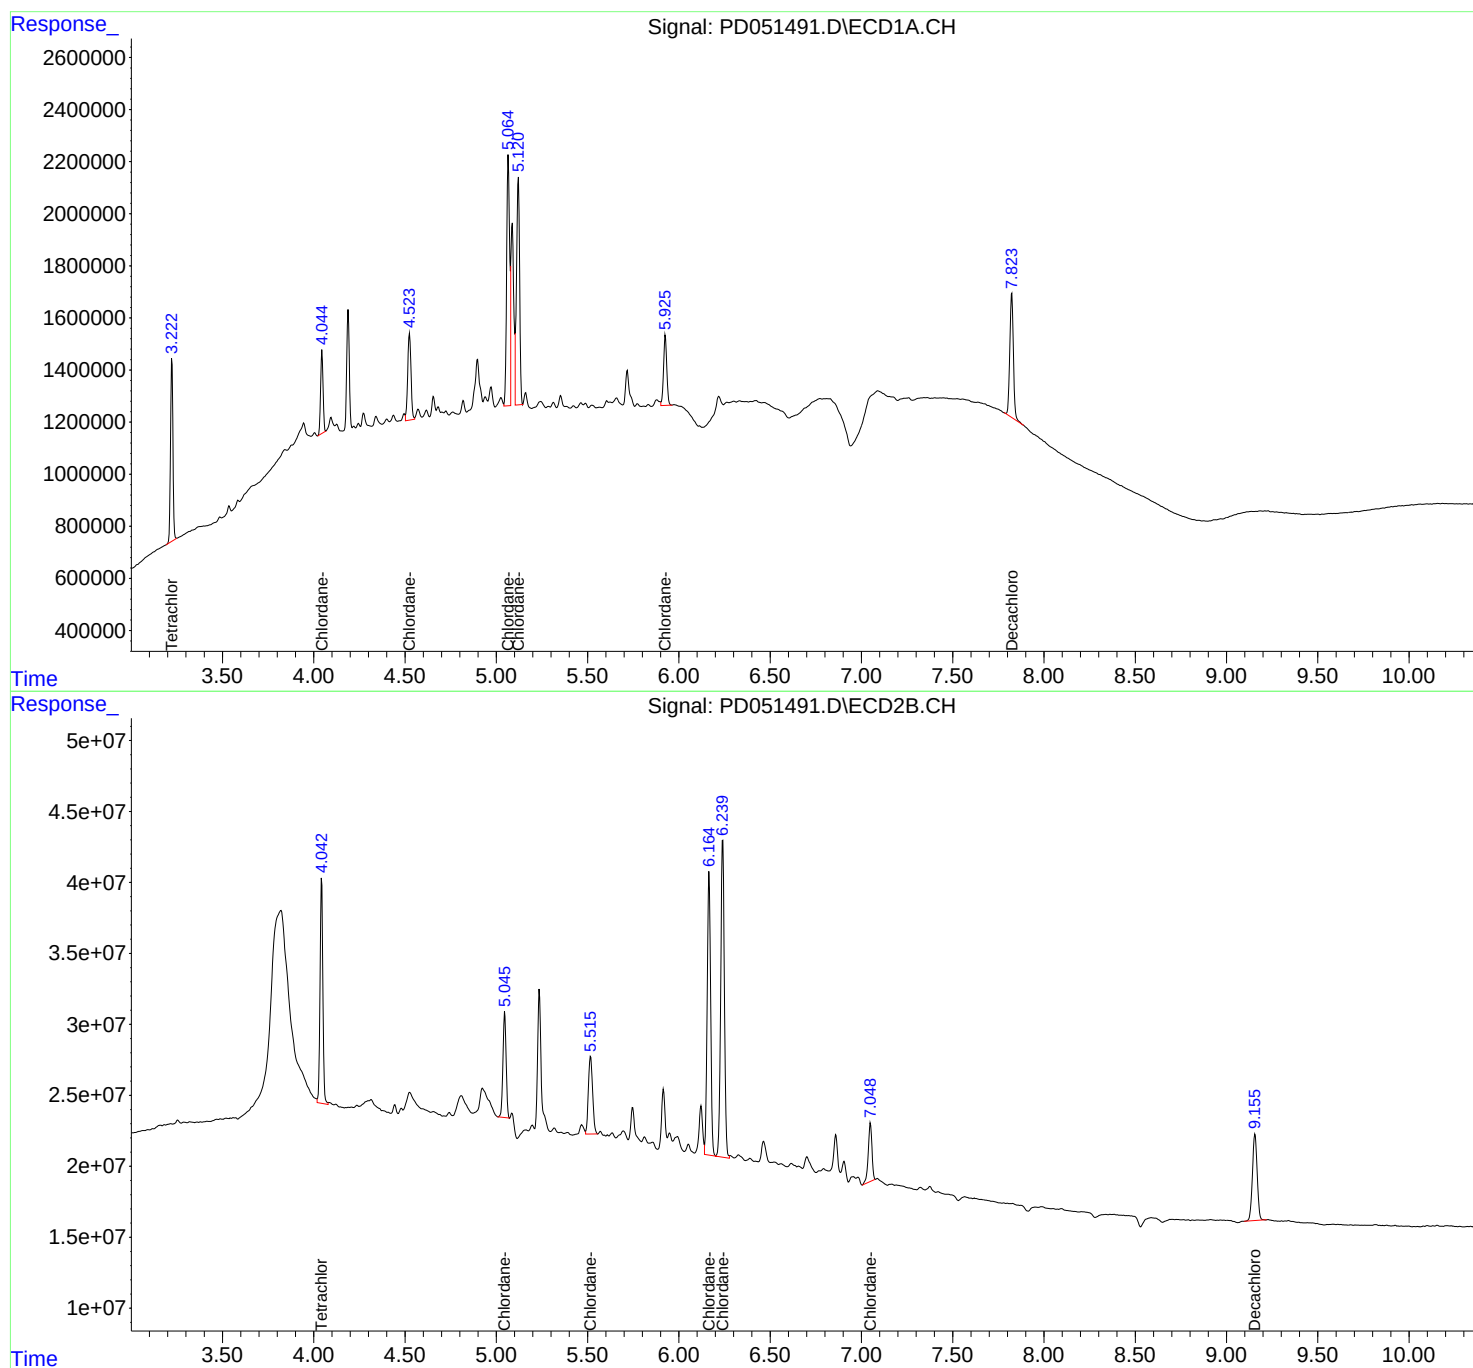


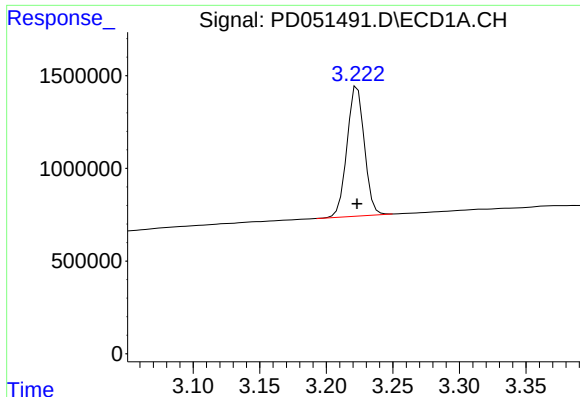

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 6341241
Conc: 4.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

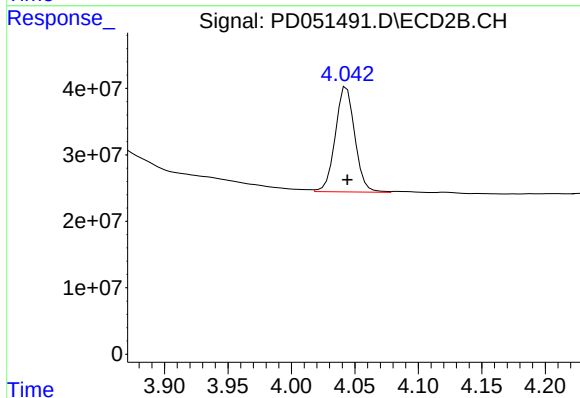


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 169036544
Conc: 6.34 ng/ml

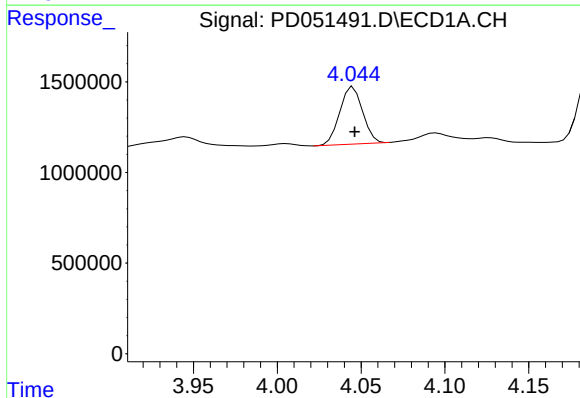


#23 Chlordane-1

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 2987490
Conc: 45.46 ng/ml

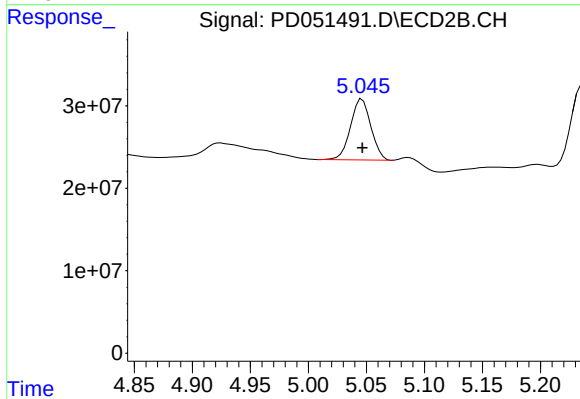

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 90190312
Conc: 59.94 ng/ml

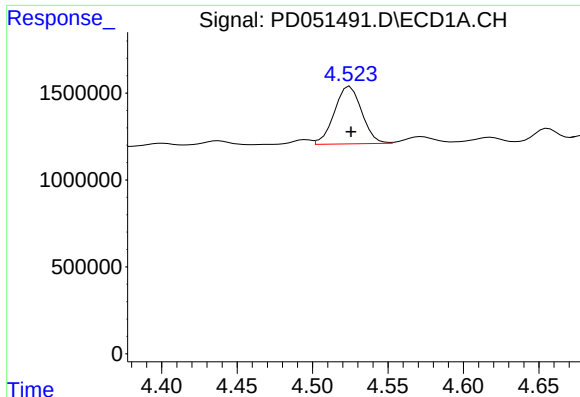

#24 Chlordane-2


R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 4175684
Conc: 52.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

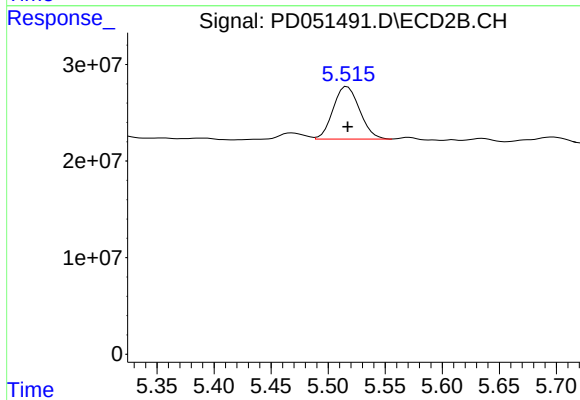


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 88049190
Conc: 64.12 ng/ml

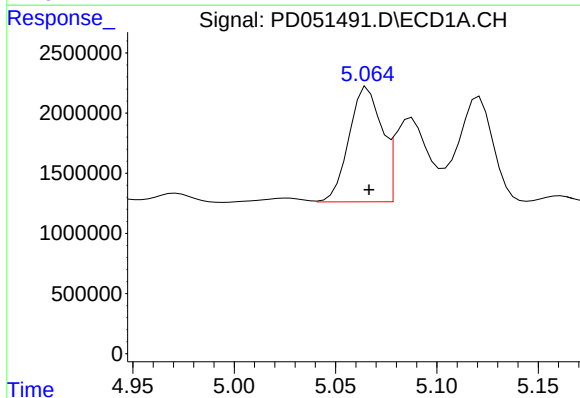


#25 Chlordane-3

R.T.: 5.066 min
Delta R.T.: 0.000 min
Response: 10662139
Conc: 44.44 ng/ml

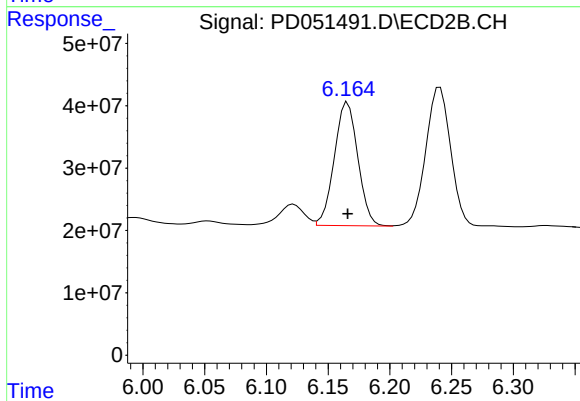

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 262245513
Conc: 59.97 ng/ml

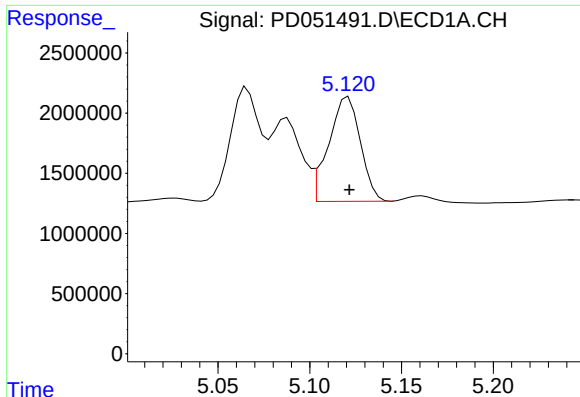

#26 Chlordane-4


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 10435548
Conc: 45.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

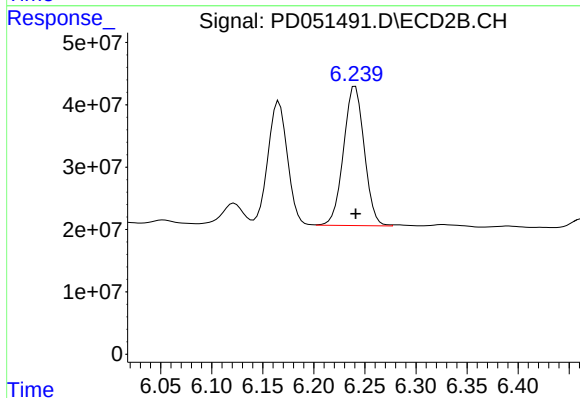


#26 Chlordane-4

R.T.: 6.241 min
Delta R.T.: 0.000 min
Response: 314897104
Conc: 61.42 ng/ml

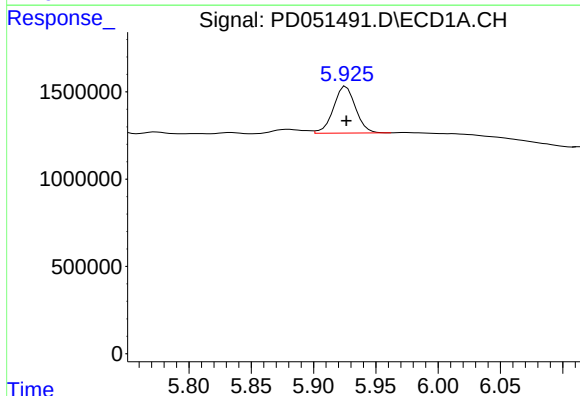


#27 Chlordane-5

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 3308183
Conc: 44.23 ng/ml

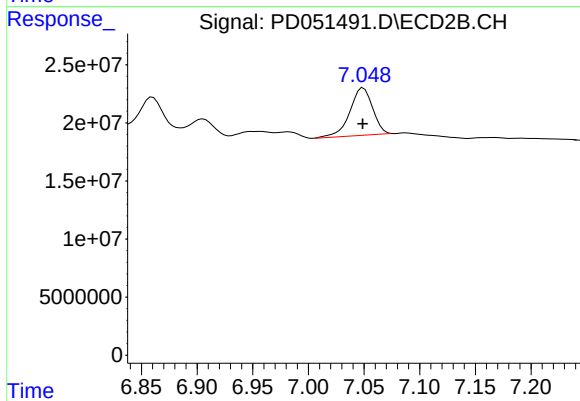

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 58716416
Conc: 59.11 ng/ml

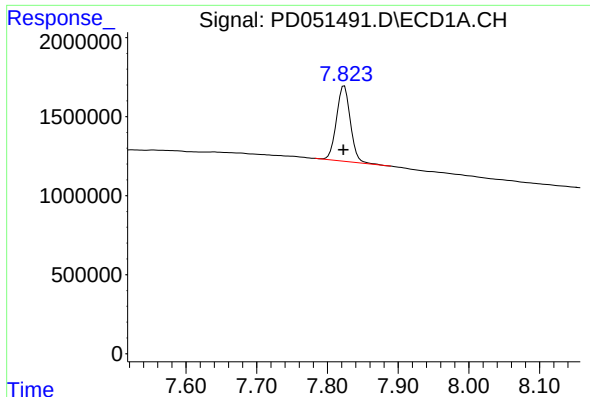

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.001 min
Response: 6473370
Conc: 6.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

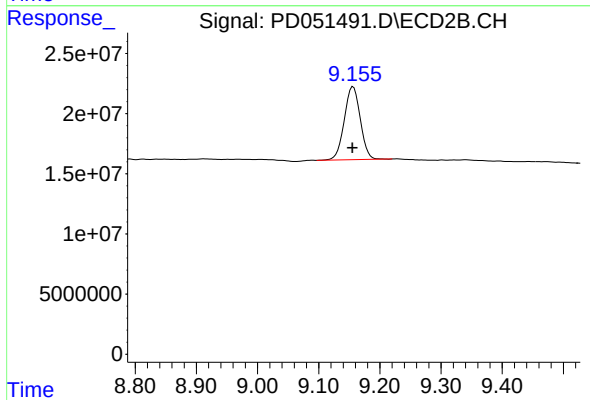

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.001 min
Response: 110308458
Conc: 6.60 ng/ml