

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051500.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 21:46
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 03:02:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	26081190	621.7E6	19.670	21.679
28)	SA Decachlor...	7.823	9.157	24614513	407.8E6	21.655	22.326
Target Compounds							
3)	MA gamma-BHC...	3.937f	0.000	449407	0	0.215	N.D. #
4)	MA Heptachlor	0.000	5.239	0	1447204	N.D.	0.038 #
7)	B delta-BHC	0.000	5.088f	0	27899111	N.D.	0.812 #
8)	B Heptachlo...	4.875f	5.925	557747	18854903	0.284	0.588 #
10)	B gamma-Chl...	0.000	6.169	0	36233882	N.D.	1.133 #
13)	MA Dieldrin	0.000	6.540	0	2843153	N.D.	0.092 #
15)	B Endosulfa...	0.000	6.977	0	2914633	N.D.	0.113 #
23)	Chlordane-1	0.000	5.031f	0	8136856	N.D.	5.314 #
25)	Chlordane-3	0.000	6.169	0	36233882	N.D.	8.137 #
27)	Chlordane-5	0.000	7.056	0	165706	N.D.	0.164 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051500.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 21:46
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 03:02:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

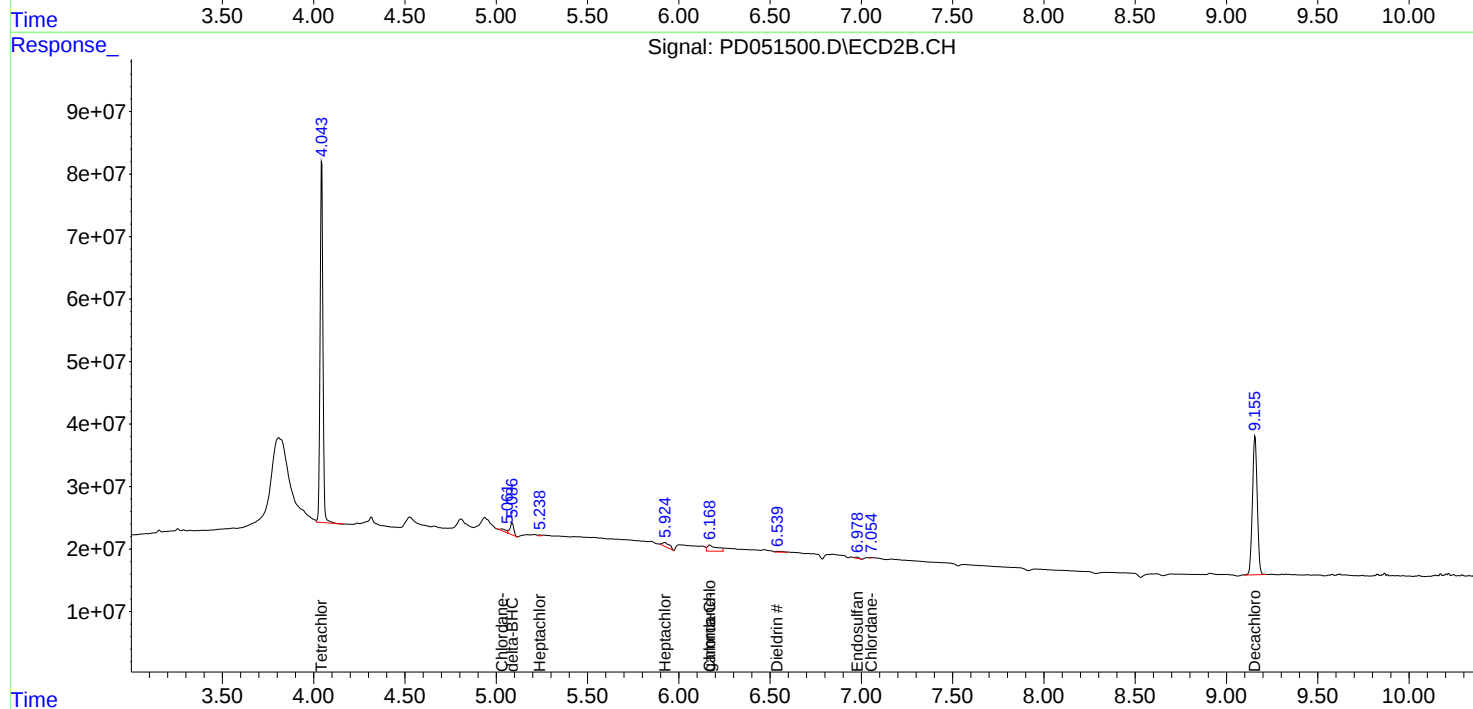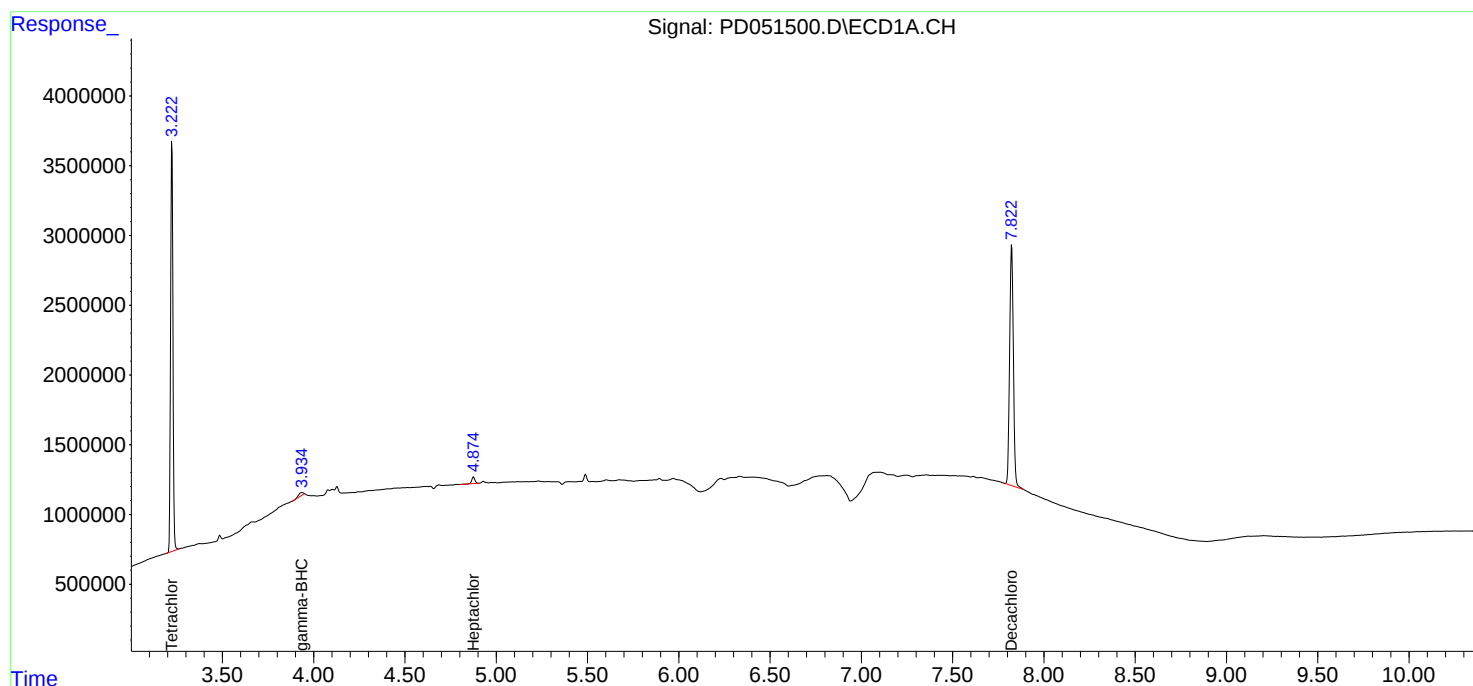


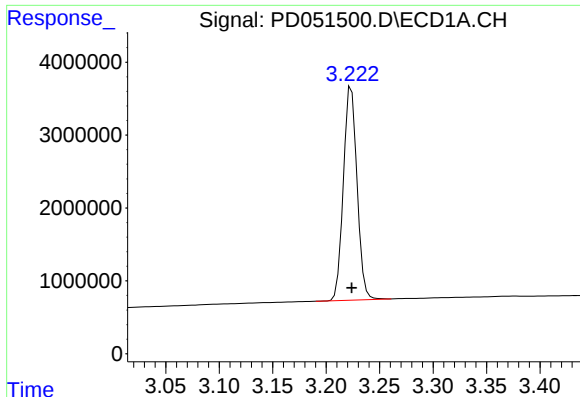

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 26081190
Conc: 19.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

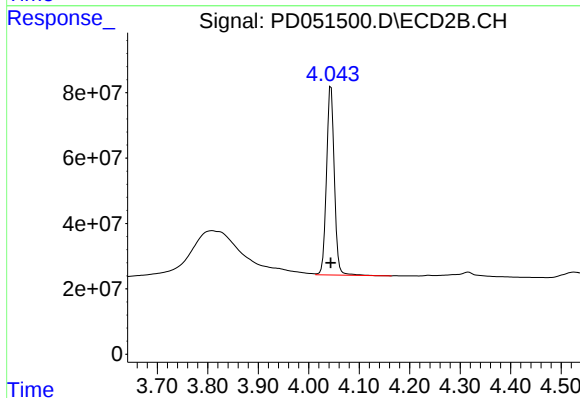


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 621687956
Conc: 21.68 ng/ml

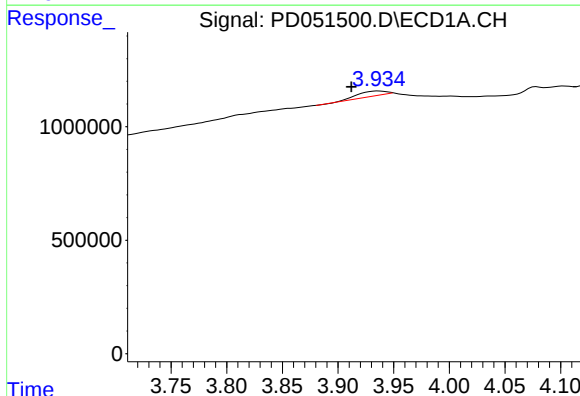


#3 gamma-BHC (Lindane)

R.T.: 3.937 min
Delta R.T.: 0.025 min
Response: 449407
Conc: 0.22 ng/ml

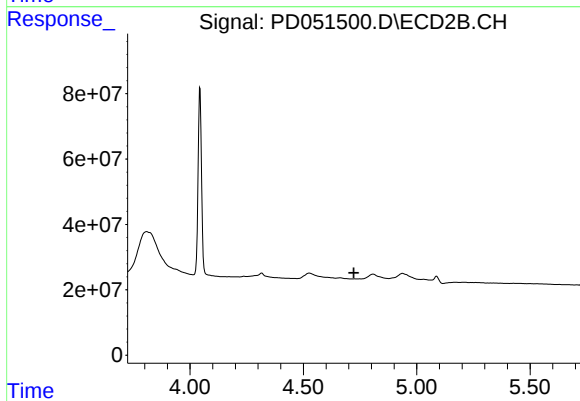

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

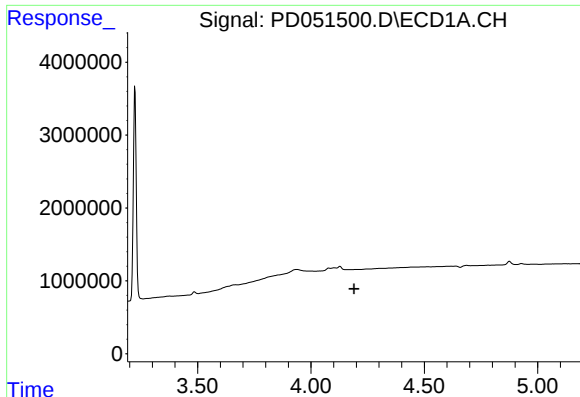

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

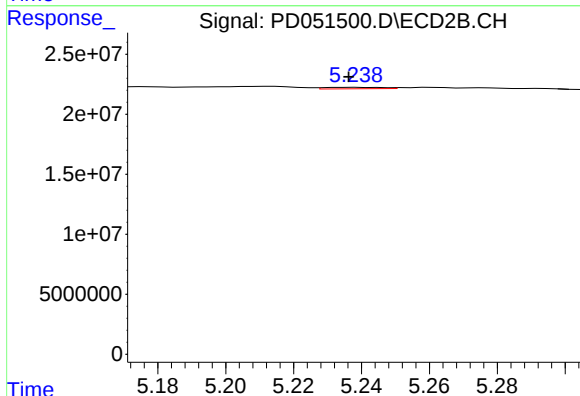


#4 Heptachlor

R.T.: 5.239 min
Delta R.T.: 0.003 min
Response: 1447204
Conc: 0.04 ng/ml

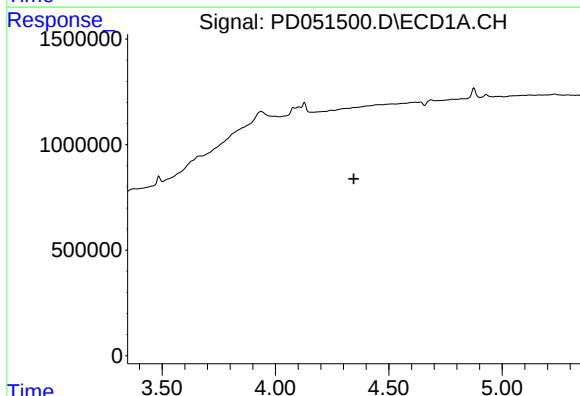


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

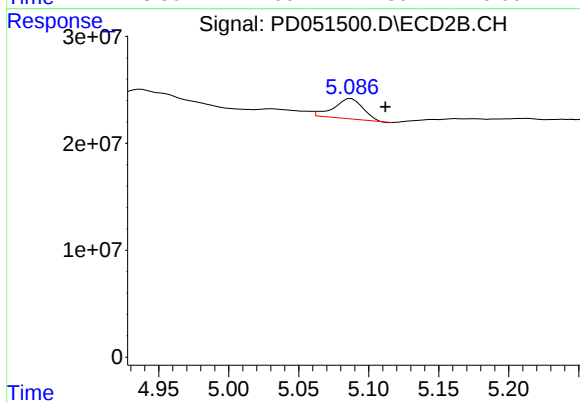

#7 delta-BHC


R.T.: 5.088 min
Delta R.T.: -0.024 min
Response: 27899111
Conc: 0.81 ng/ml

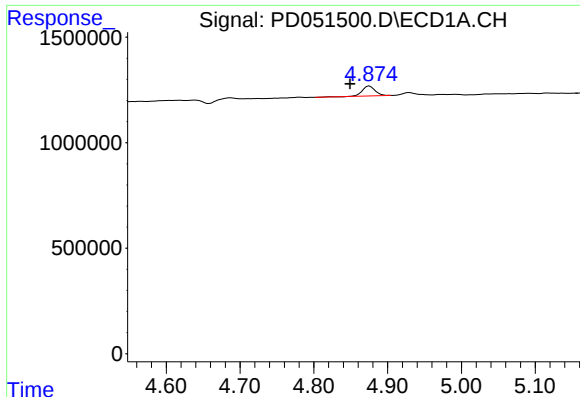

#8 Heptachlor epoxide


R.T.: 4.875 min
Delta R.T.: 0.026 min
Response: 557747
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

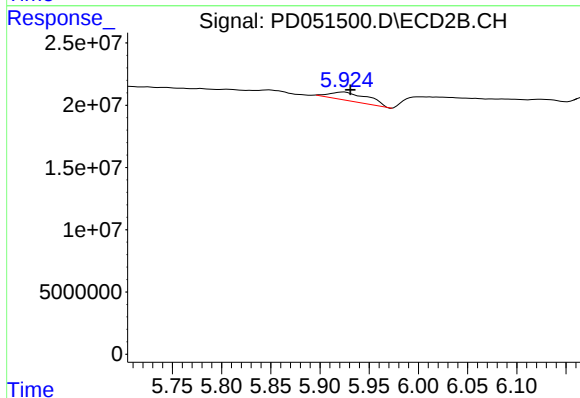


#8 Heptachlor epoxide

R.T.: 5.925 min
Delta R.T.: -0.006 min
Response: 18854903
Conc: 0.59 ng/ml

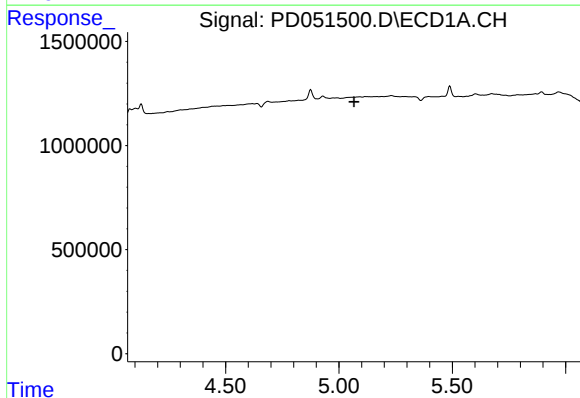


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.066 min
Response: 0
Conc: N.D.

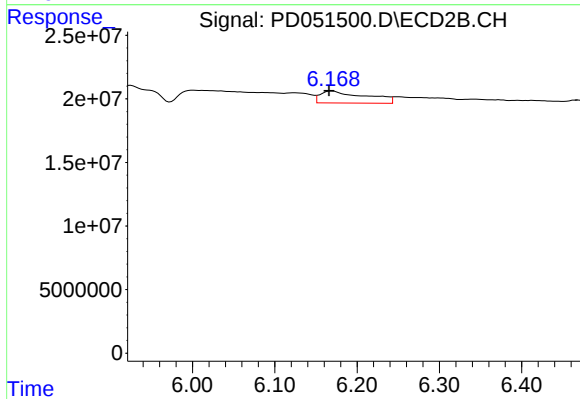

#10 gamma-Chlordane


R.T.: 6.169 min
Delta R.T.: 0.003 min
Response: 36233882
Conc: 1.13 ng/ml

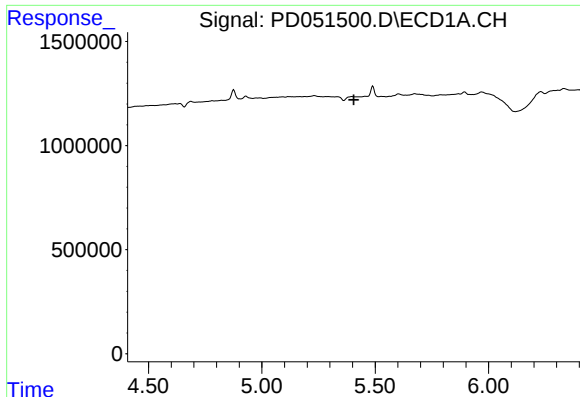

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

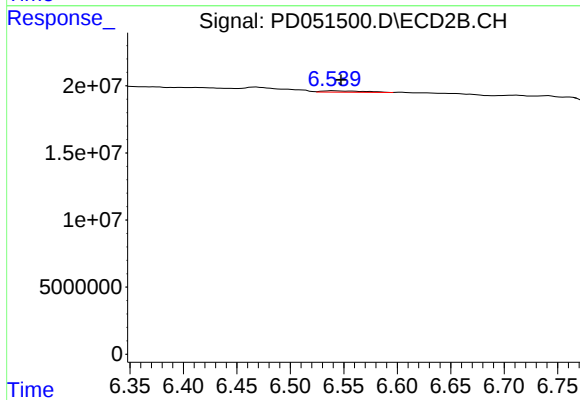


#13 Dieldrin

R.T.: 6.540 min
Delta R.T.: -0.008 min
Response: 2843153
Conc: 0.09 ng/ml

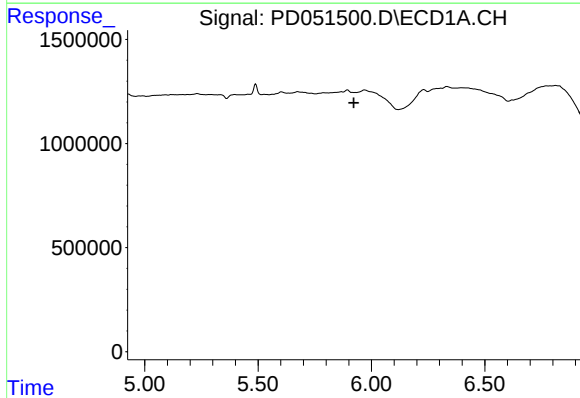


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.923 min
Response: 0
Conc: N.D.

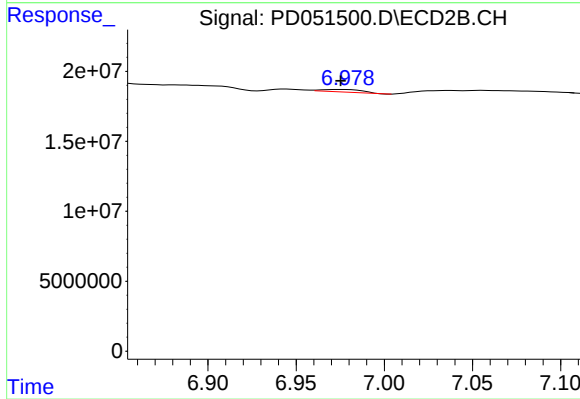

#15 Endosulfan II


R.T.: 6.977 min
Delta R.T.: 0.002 min
Response: 2914633
Conc: 0.11 ng/ml

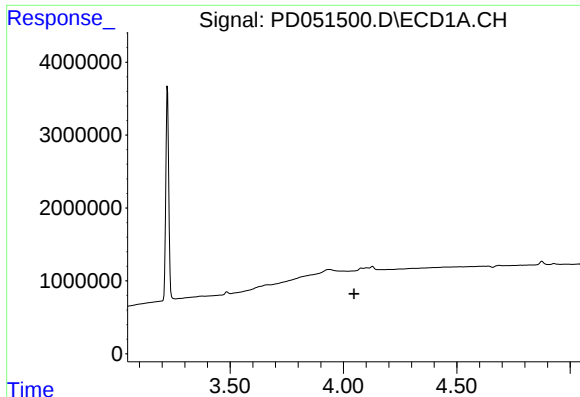

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

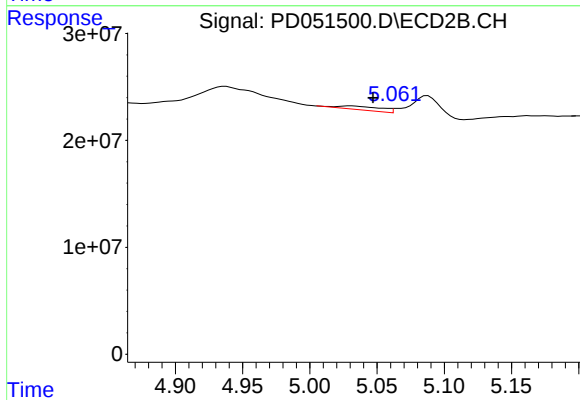


#23 Chlordane-1

R.T.: 5.031 min
Delta R.T.: -0.016 min
Response: 8136856
Conc: 5.31 ng/ml

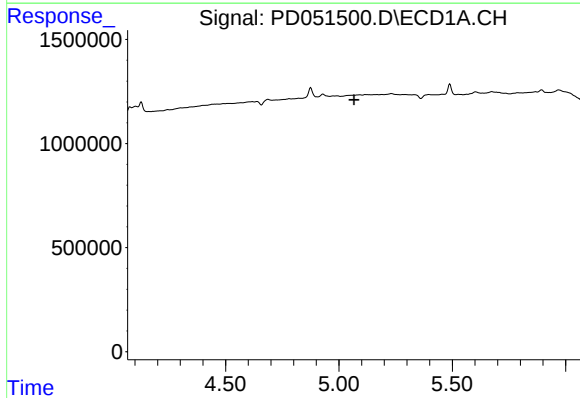


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

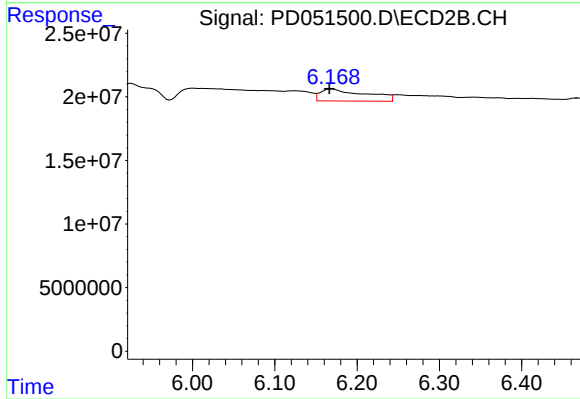

#25 Chlordane-3


R.T.: 6.169 min
Delta R.T.: 0.003 min
Response: 36233882
Conc: 8.14 ng/ml

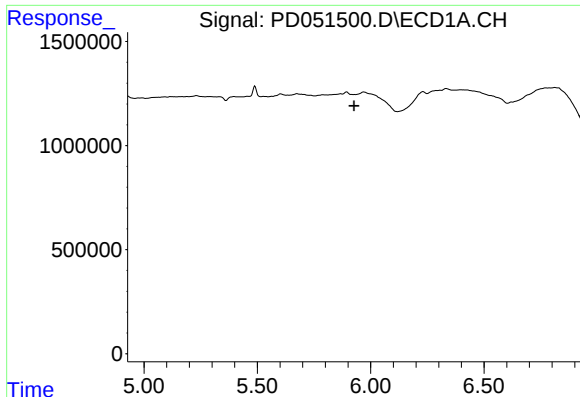

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 5.927 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

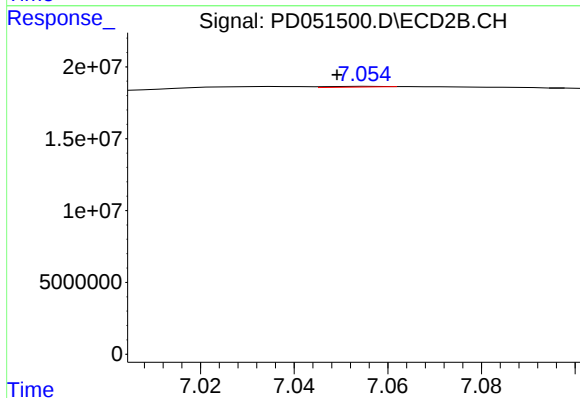


#27 Chlorodane-5

R.T.: 7.056 min
Delta R.T.: 0.007 min
Response: 165706
Conc: 0.16 ng/ml

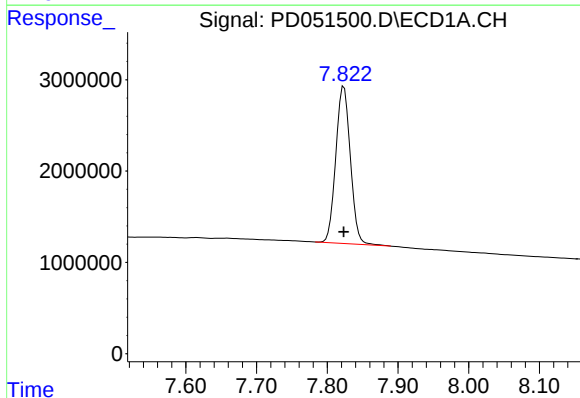

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 24614513
Conc: 21.65 ng/ml

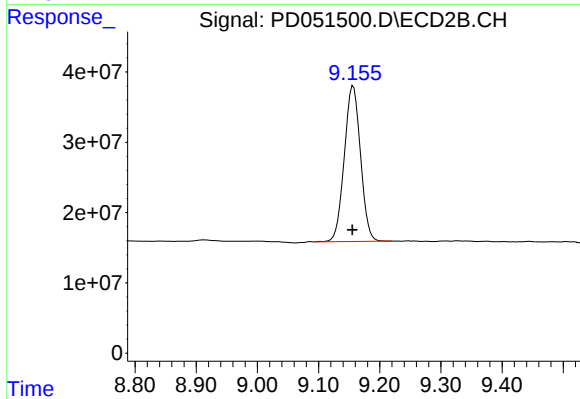

#28 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.002 min
Response: 407825490
Conc: 22.33 ng/ml