

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051512.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2019 1:16
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 03:03:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	26082912	613.7E6	19.671	21.399
28)	SA Decachlor...	7.824	9.157	26070196	409.9E6	22.935	22.437
Target Compounds							
3)	MA gamma-BHC...	3.933f	0.000	744265	0	0.356	N.D. #
4)	MA Heptachlor	0.000	5.209f	0	3345752	N.D.	0.087 #
7)	B delta-BHC	0.000	5.088f	0	24003246	N.D.	0.698 #
8)	B Heptachlo...	4.876f	5.926	545748	47273273	0.278	1.474 #
10)	B gamma-Chl...	0.000	6.170	0	144.9E6	N.D.	4.531 #
15)	B Endosulfa...	0.000	6.979	0	3569527	N.D.	0.139 #
25)	Chlordane-3	0.000	6.170	0	144.9E6	N.D.	32.537 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051512.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2019 1:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 03:03:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

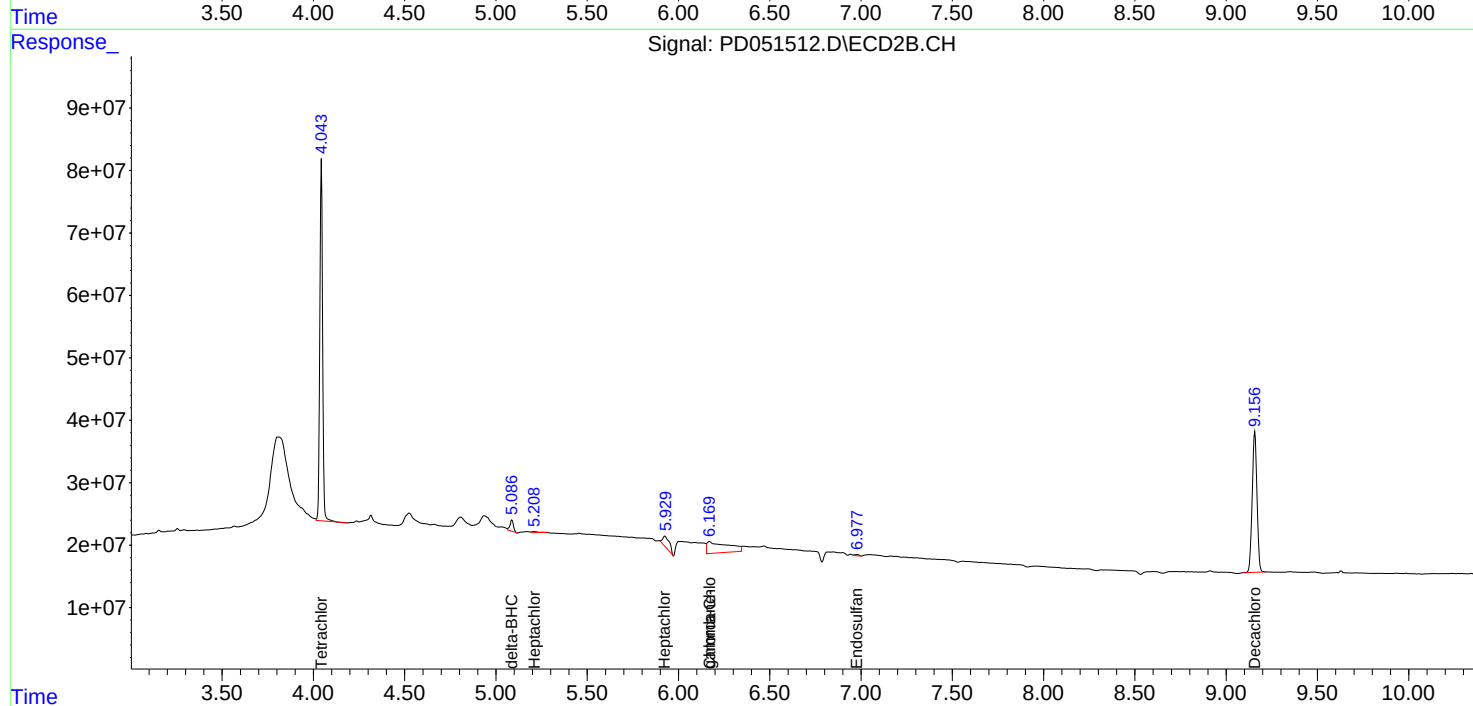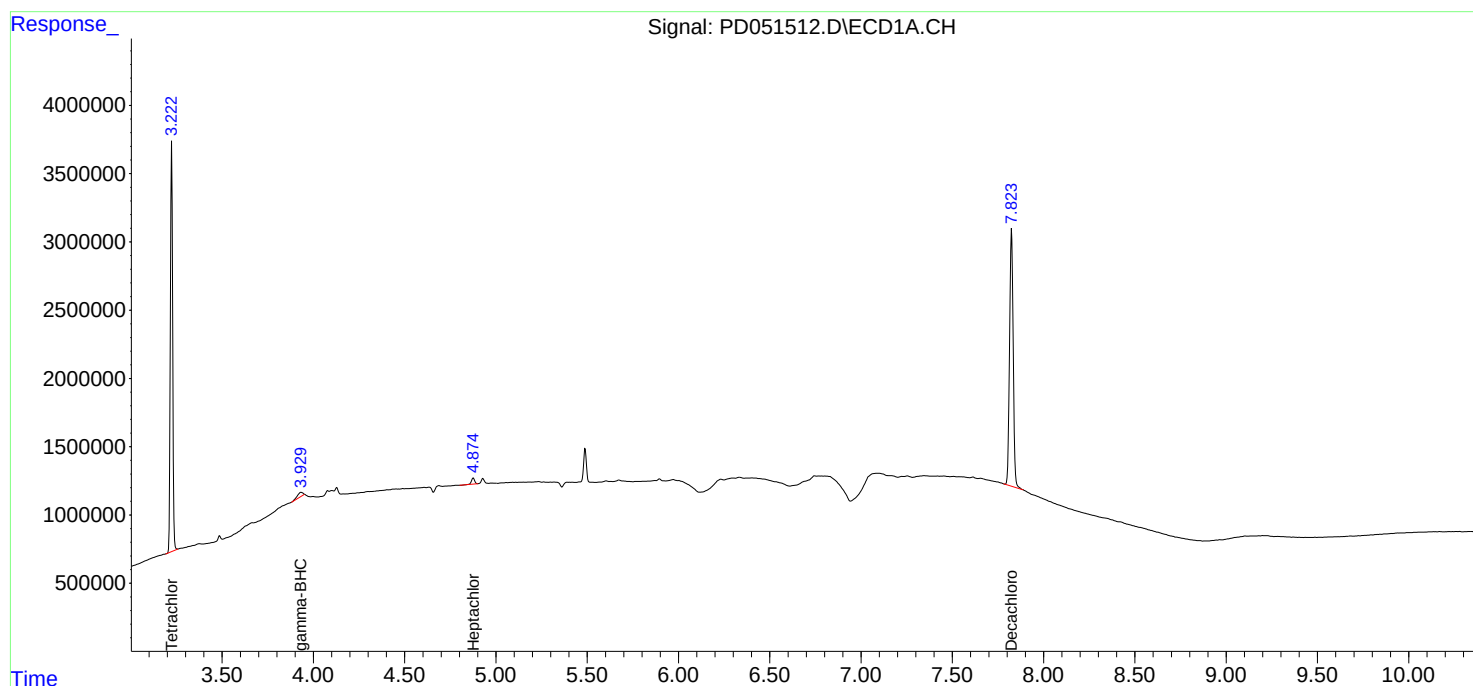


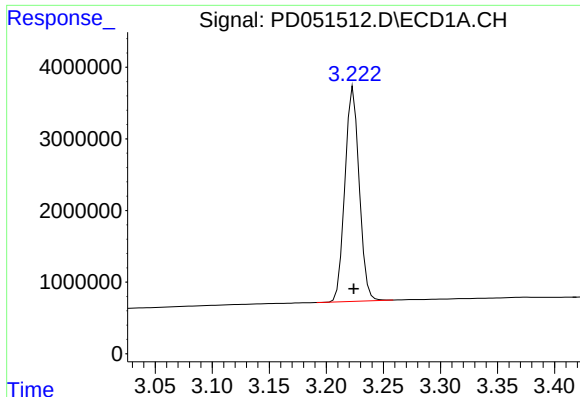

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 26082912
Conc: 19.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

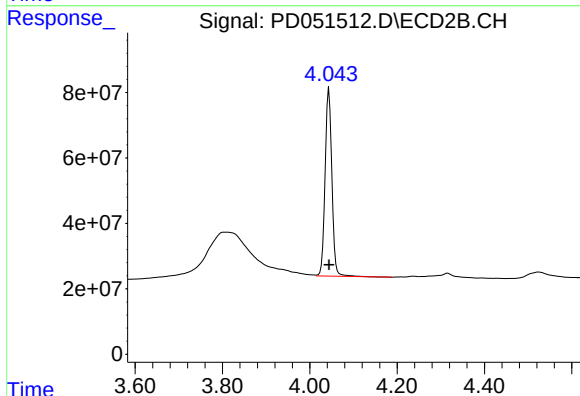


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 613666595
Conc: 21.40 ng/ml

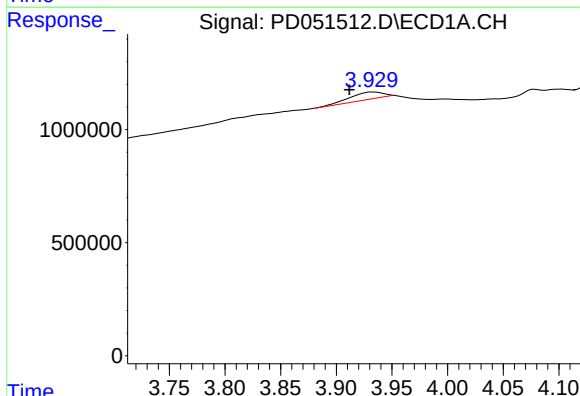


#3 gamma-BHC (Lindane)

R.T.: 3.933 min
Delta R.T.: 0.021 min
Response: 744265
Conc: 0.36 ng/ml

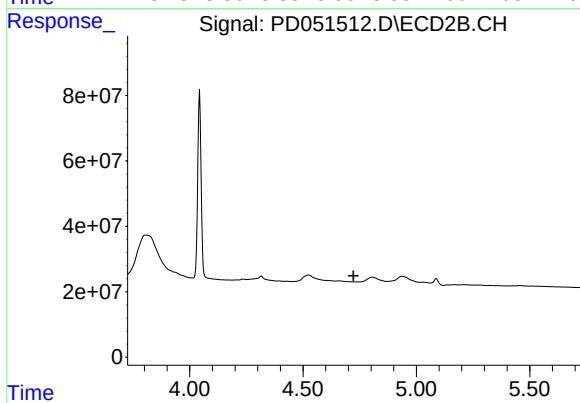

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

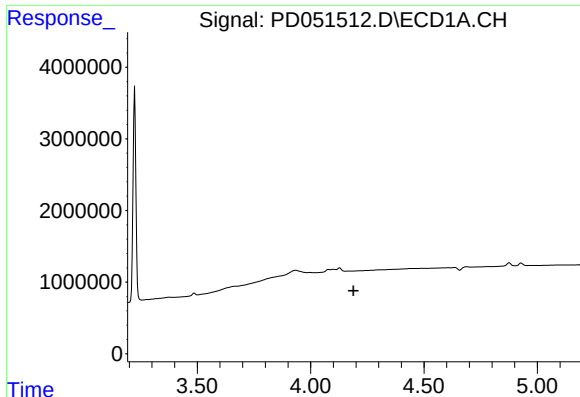

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

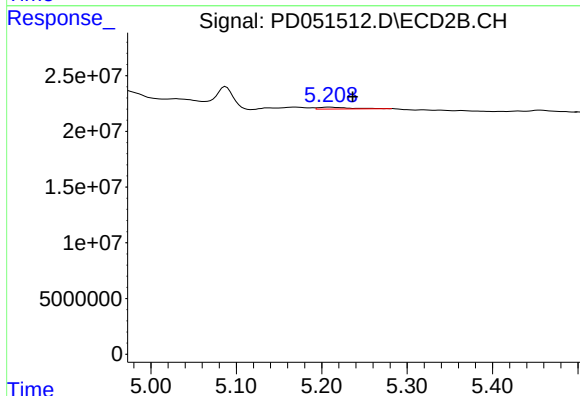


#4 Heptachlor

R.T.: 5.209 min
Delta R.T.: -0.028 min
Response: 3345752
Conc: 0.09 ng/ml

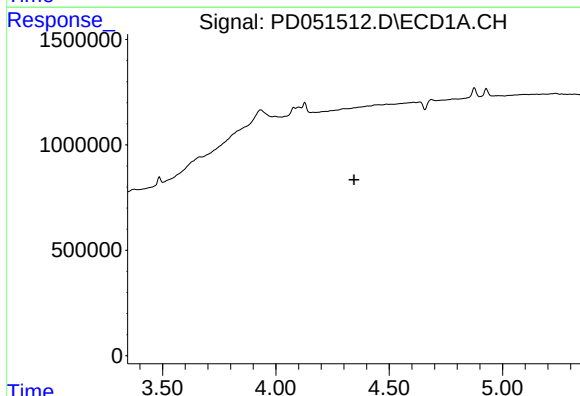


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.346 min
Response: 0
Conc: N.D.

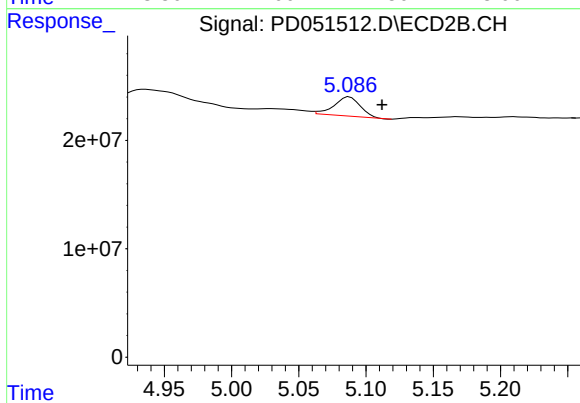

#7 delta-BHC


R.T.: 5.088 min
Delta R.T.: -0.024 min
Response: 24003246
Conc: 0.70 ng/ml

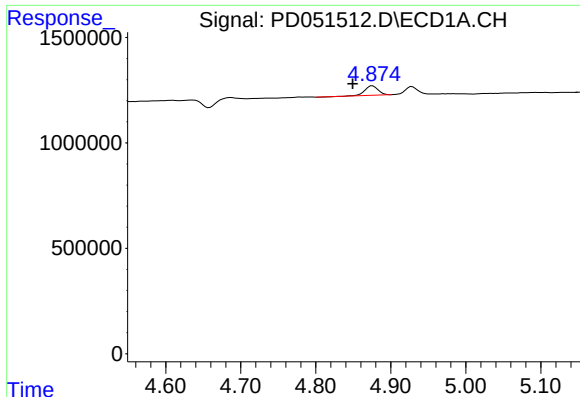

#8 Heptachlor epoxide


R.T.: 4.876 min
Delta R.T.: 0.027 min
Response: 545748
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

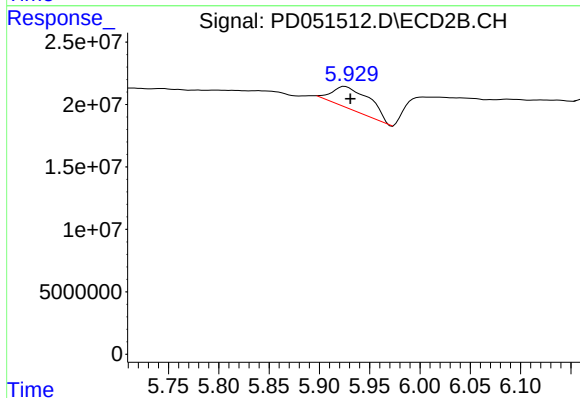


#8 Heptachlor epoxide

R.T.: 5.926 min
Delta R.T.: -0.005 min
Response: 47273273
Conc: 1.47 ng/ml

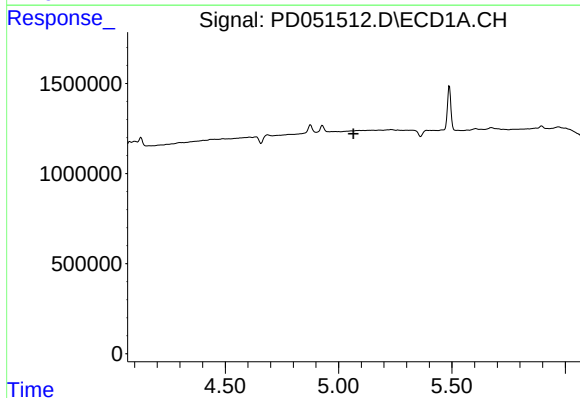


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

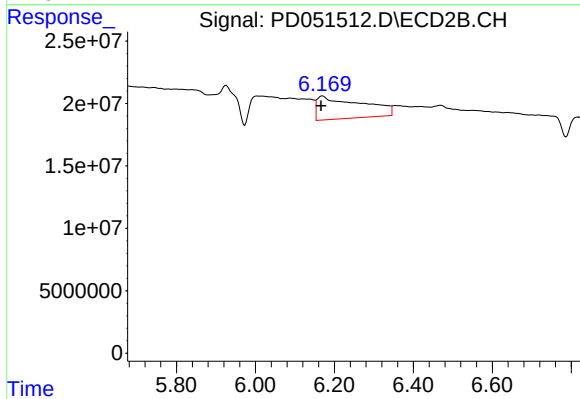

#10 gamma-Chlordane


R.T.: 6.170 min
Delta R.T.: 0.004 min
Response: 144888789
Conc: 4.53 ng/ml

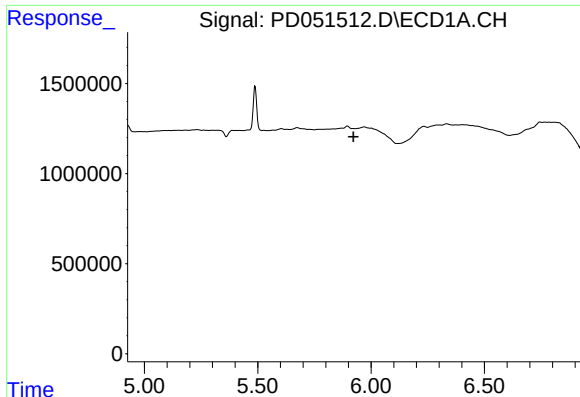

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.923 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

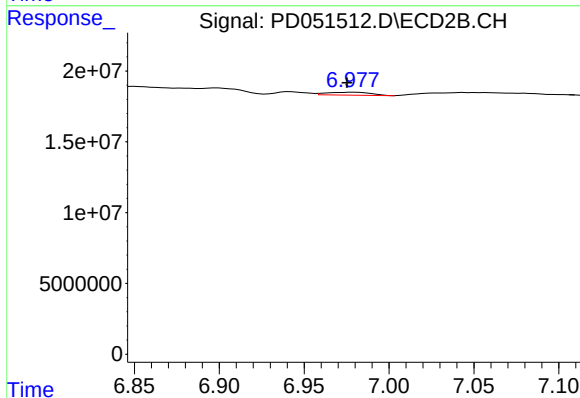


#15 Endosulfan II

R.T.: 6.979 min
Delta R.T.: 0.004 min
Response: 3569527
Conc: 0.14 ng/ml

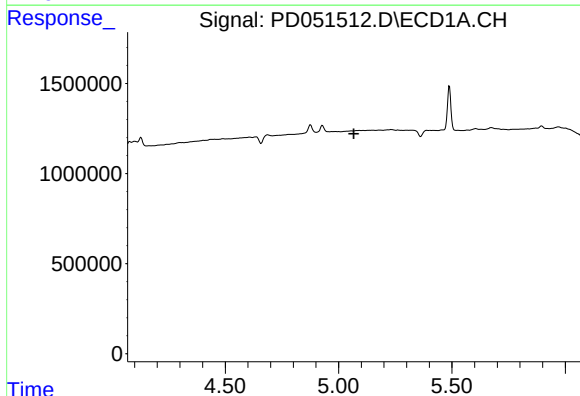


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

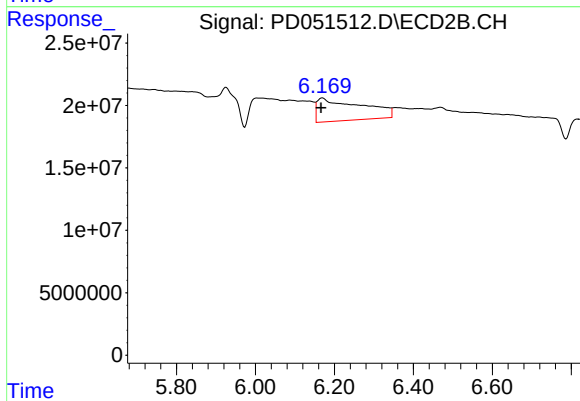

#25 Chlordane-3


R.T.: 6.170 min
Delta R.T.: 0.003 min
Response: 144888789
Conc: 32.54 ng/ml

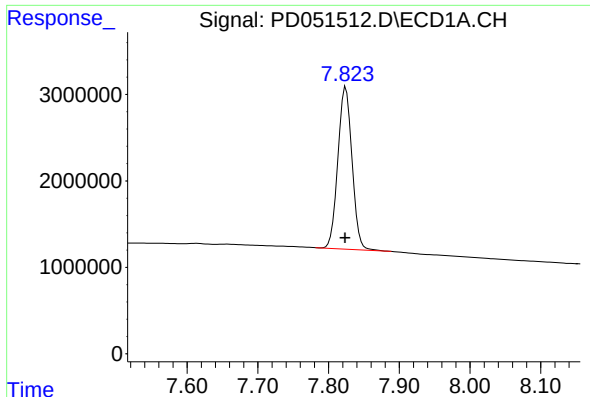

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.001 min
Response: 26070196
Conc: 22.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

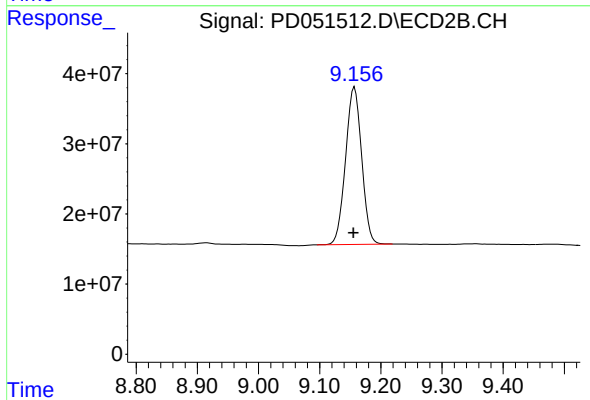

#28 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.002 min
Response: 409850551
Conc: 22.44 ng/ml