

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051530.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2019 7:07
 Operator : AJ\SJ
 Sample : PB117517BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB117517BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:17:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:43:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	25391064	603.4E6	19.150	21.040
28)	SA Decachlor...	7.824	9.158	25241352	400.9E6	22.206	21.948
Target Compounds							
2)	A alpha-BHC	0.000	4.423	0	957273	N.D.	0.022 #
3)	MA gamma-BHC...	3.923	0.000	1523911	0	0.729	N.D. #
4)	MA Heptachlor	0.000	5.240	0	2785307	N.D.	0.073 #
7)	B delta-BHC	0.000	5.087f	0	28100263	N.D.	0.818 #
8)	B Heptachlo...	0.000	5.919	0	3879555	N.D.	0.121 #
10)	B gamma-Chl...	0.000	6.191f	0	9375568	N.D.	0.293 #
17)	MA 4,4'-DDT	0.000	7.165f	0	1603766	N.D.	0.079 #
25)	Chlordane-3	0.000	6.191f	0	9375568	N.D.	2.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2019 7:07
Operator : AJ\SJ
Sample : PB117517BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB117517BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:17:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:43:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

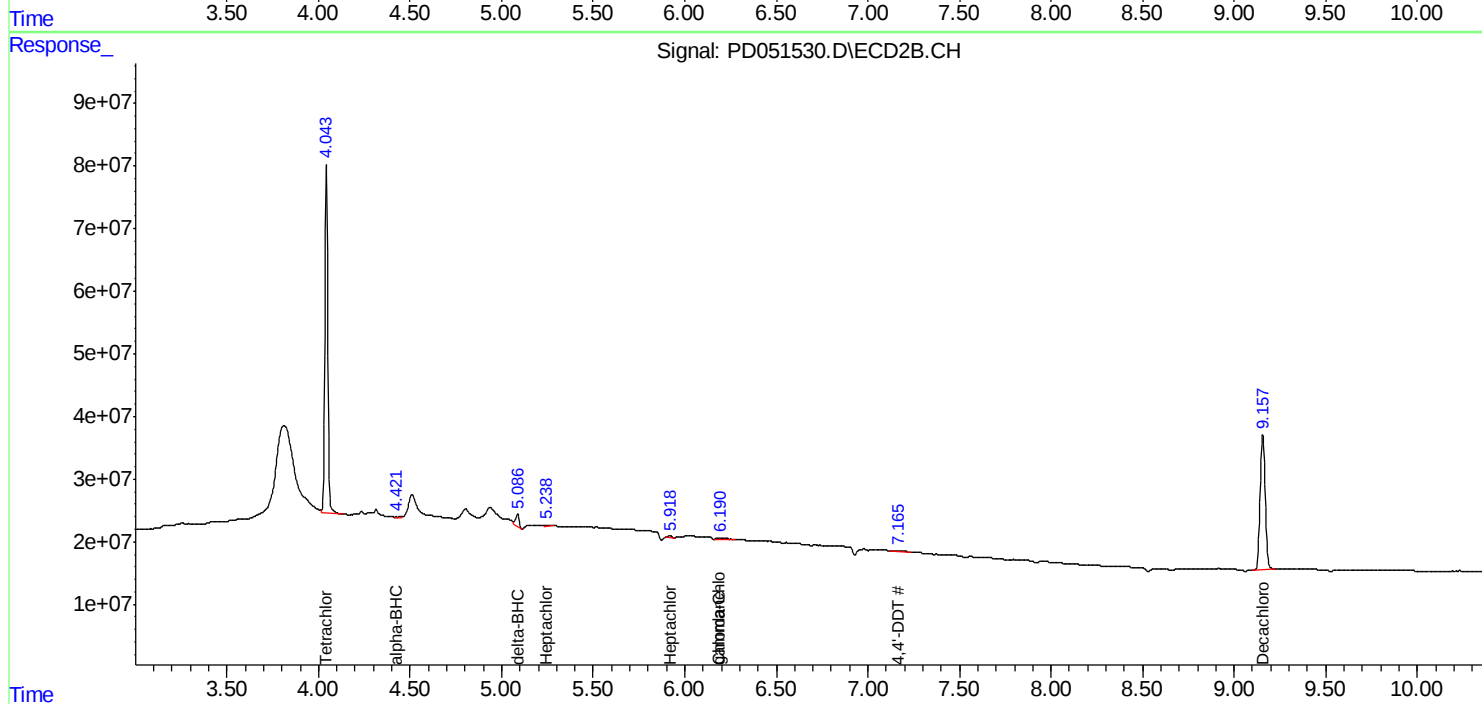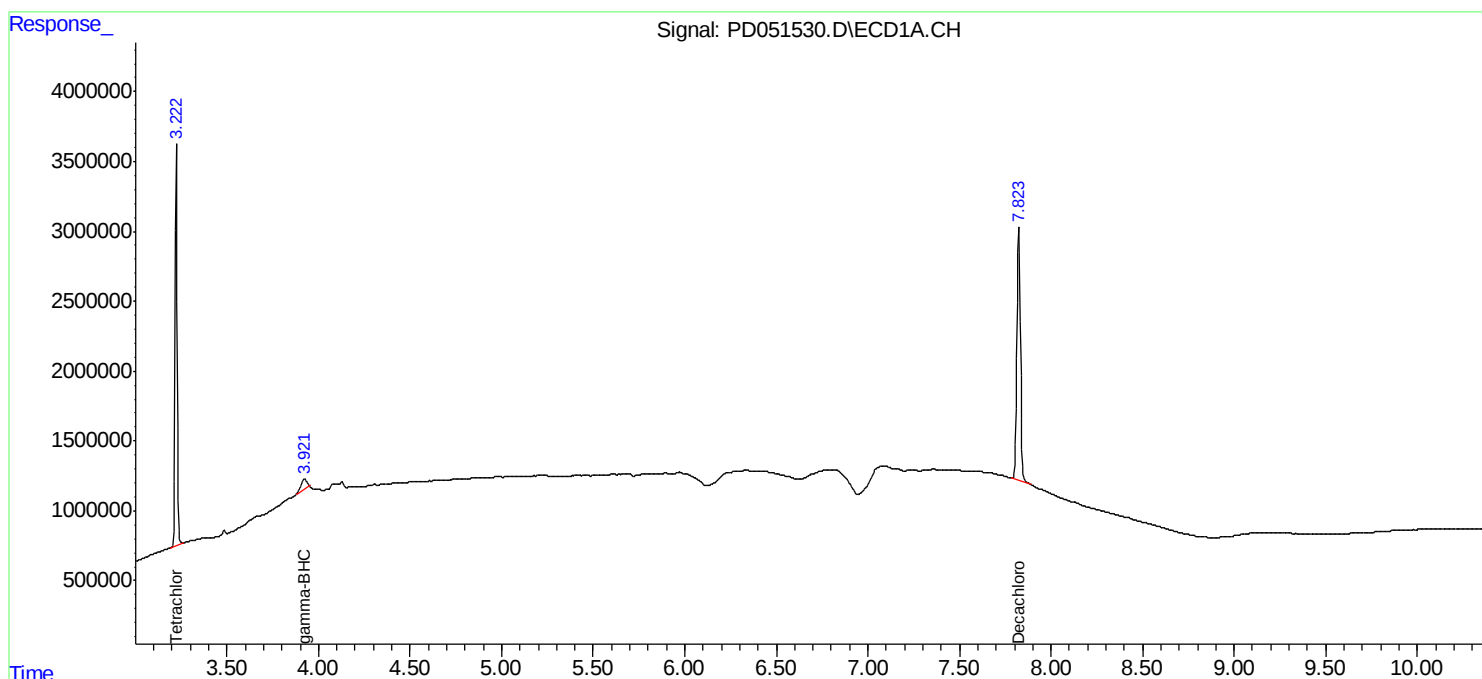


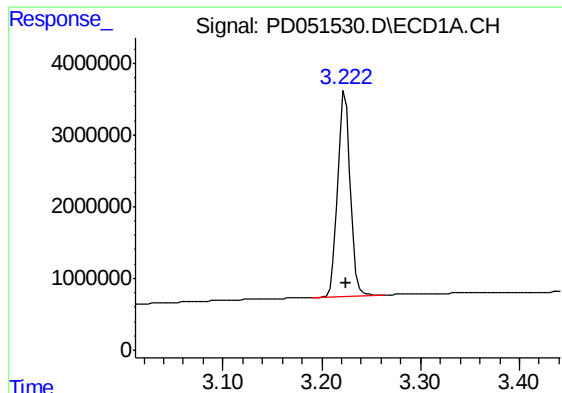

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 25391064
Conc: 19.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB117517BL

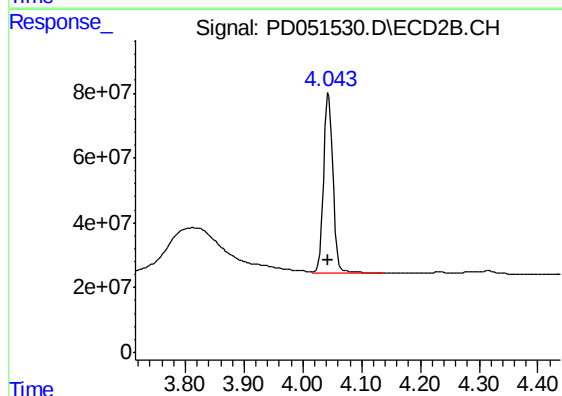


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 603368020
Conc: 21.04 ng/ml

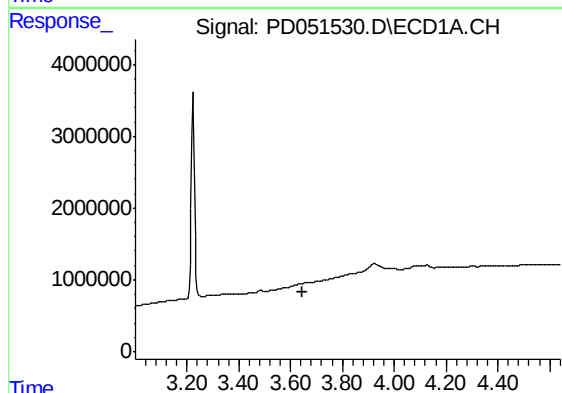


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.644 min
Response: 0
Conc: N.D.

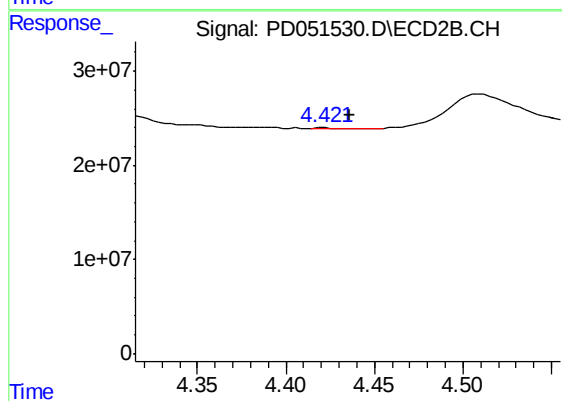

#2 alpha-BHC


R.T.: 4.423 min
Delta R.T.: -0.013 min
Response: 957273
Conc: 0.02 ng/ml

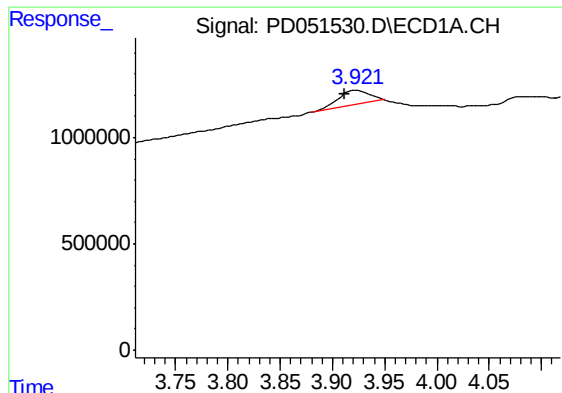

#3 gamma-BHC (Lindane)


R.T.: 3.923 min
Delta R.T.: 0.011 min
Response: 1523911
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB117517BL

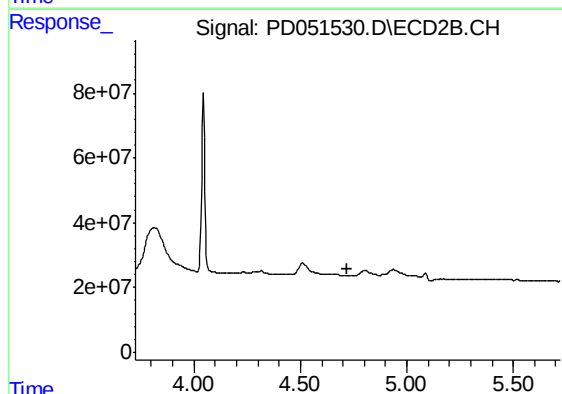


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

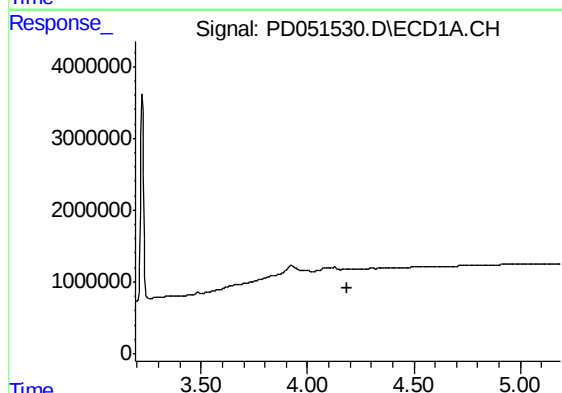


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.190 min
Response: 0
Conc: N.D.

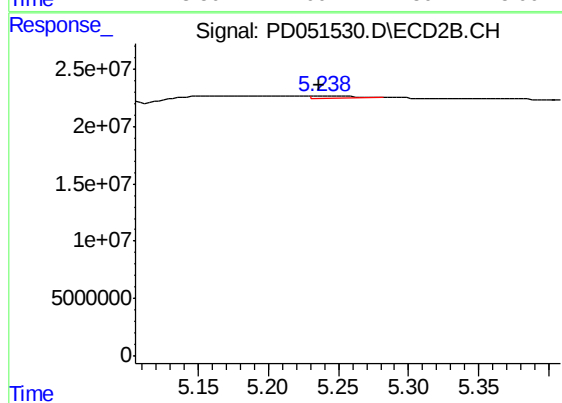

#4 Heptachlor


R.T.: 5.240 min
Delta R.T.: 0.003 min
Response: 2785307
Conc: 0.07 ng/ml

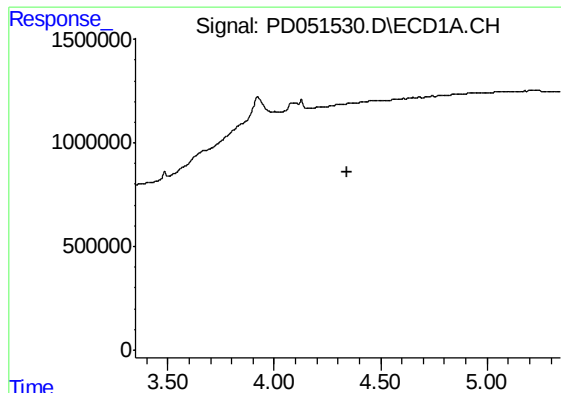

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB117517BL

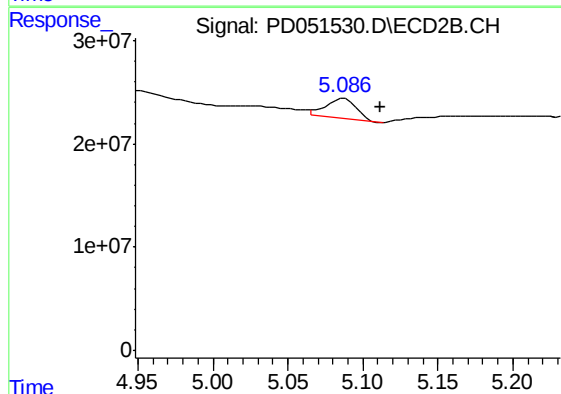


#7 delta-BHC

R.T.: 5.087 min
Delta R.T.: -0.025 min
Response: 28100263
Conc: 0.82 ng/ml

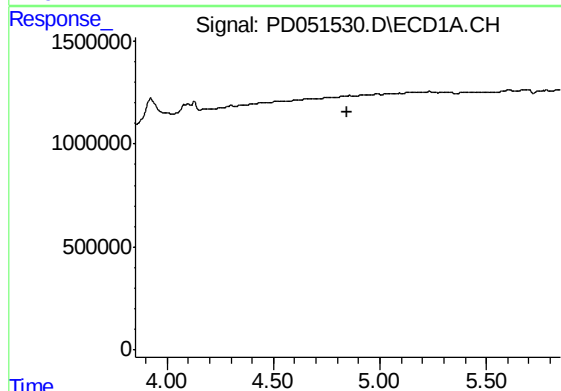


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.849 min
Response: 0
Conc: N.D.

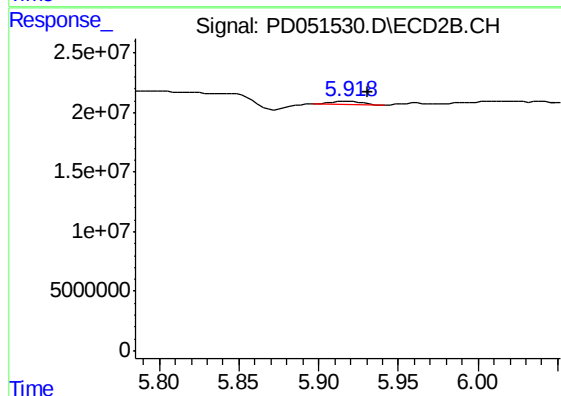

#8 Heptachlor epoxide


R.T.: 5.919 min
Delta R.T.: -0.012 min
Response: 3879555
Conc: 0.12 ng/ml

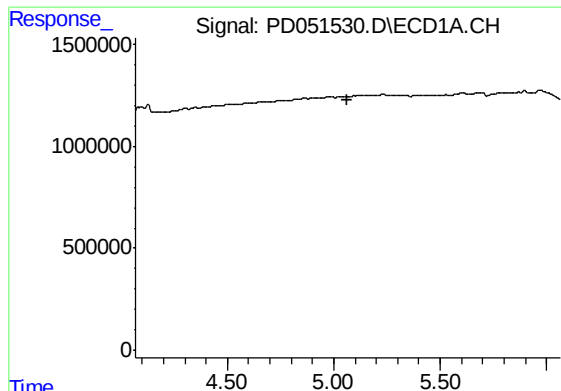

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB117517BL

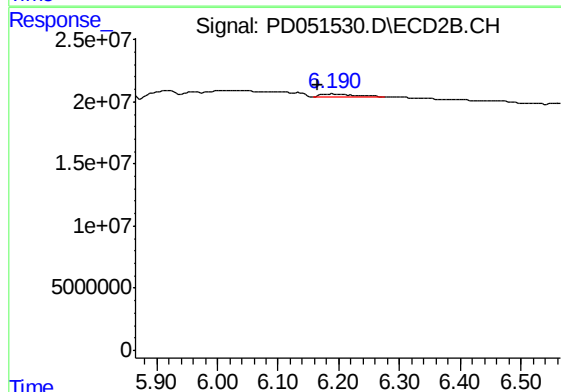


#10 gamma-Chlordane

R.T.: 6.191 min
Delta R.T.: 0.025 min
Response: 9375568
Conc: 0.29 ng/ml

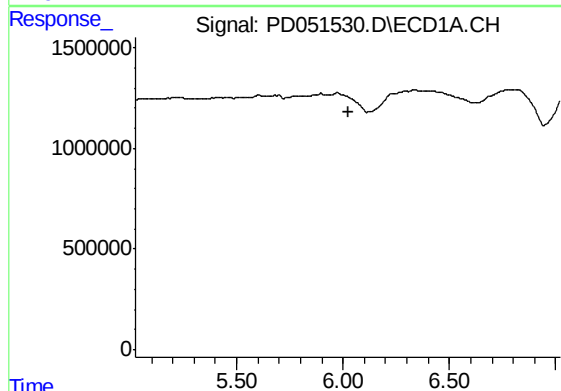


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

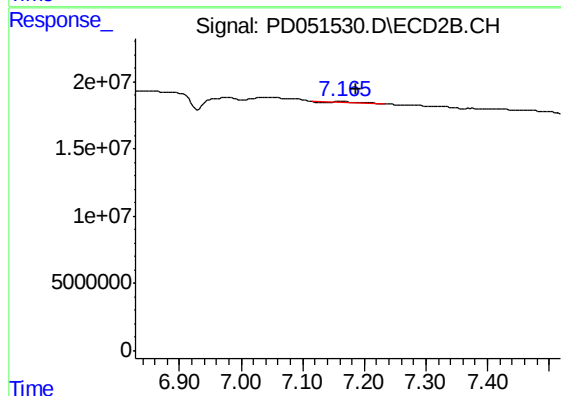

#17 4,4'-DDT


R.T.: 7.165 min
Delta R.T.: -0.022 min
Response: 1603766
Conc: 0.08 ng/ml

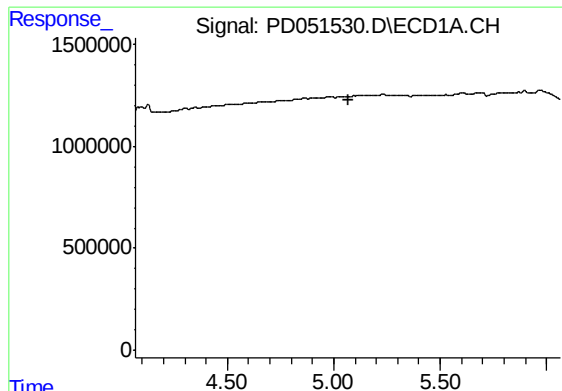

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB117517BL

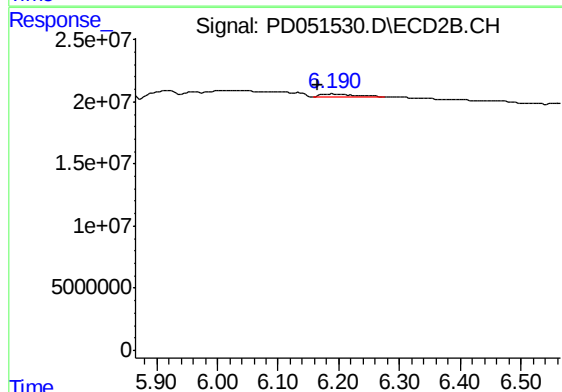


#25 Chlordane-3

R.T.: 6.191 min
Delta R.T.: 0.024 min
Response: 9375568
Conc: 2.11 ng/ml

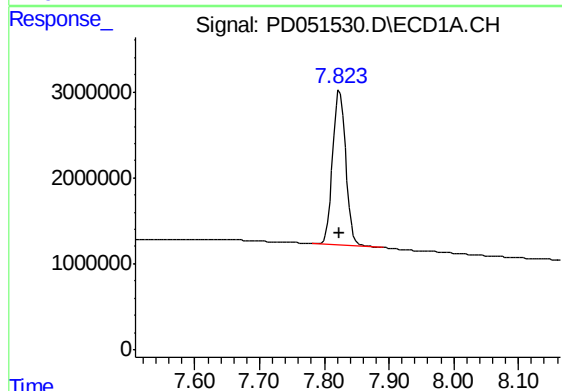

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.000 min
Response: 25241352
Conc: 22.21 ng/ml

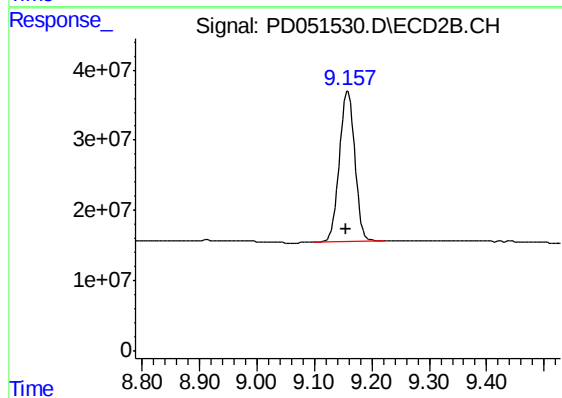

#28 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.003 min
Response: 400933059
Conc: 21.95 ng/ml