

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051488.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 18:59
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 23:29:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:29:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.223	4.044	101.4E6	1892.6E6	75.143	71.037
28)	SA Decachlor...	7.823	9.155	76166561	1164.6E6	71.446	69.634
Target Compounds							
23)	Chlordane-1	4.046	5.046	48846337	1064.7E6	743.254	707.526
24)	Chlordane-2	4.525	5.517	56873630	955.0E6	718.403	695.461
25)	Chlordane-3	5.066	6.166	182.5E6	3081.1E6	760.628	704.588
26)	Chlordane-4	5.121	6.241	173.0E6	3598.1E6	747.910	701.763
27)	Chlordane-5	5.926	7.049	54283665	720.8E6	725.715	725.651



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051488.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 18:59
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:29:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:29:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

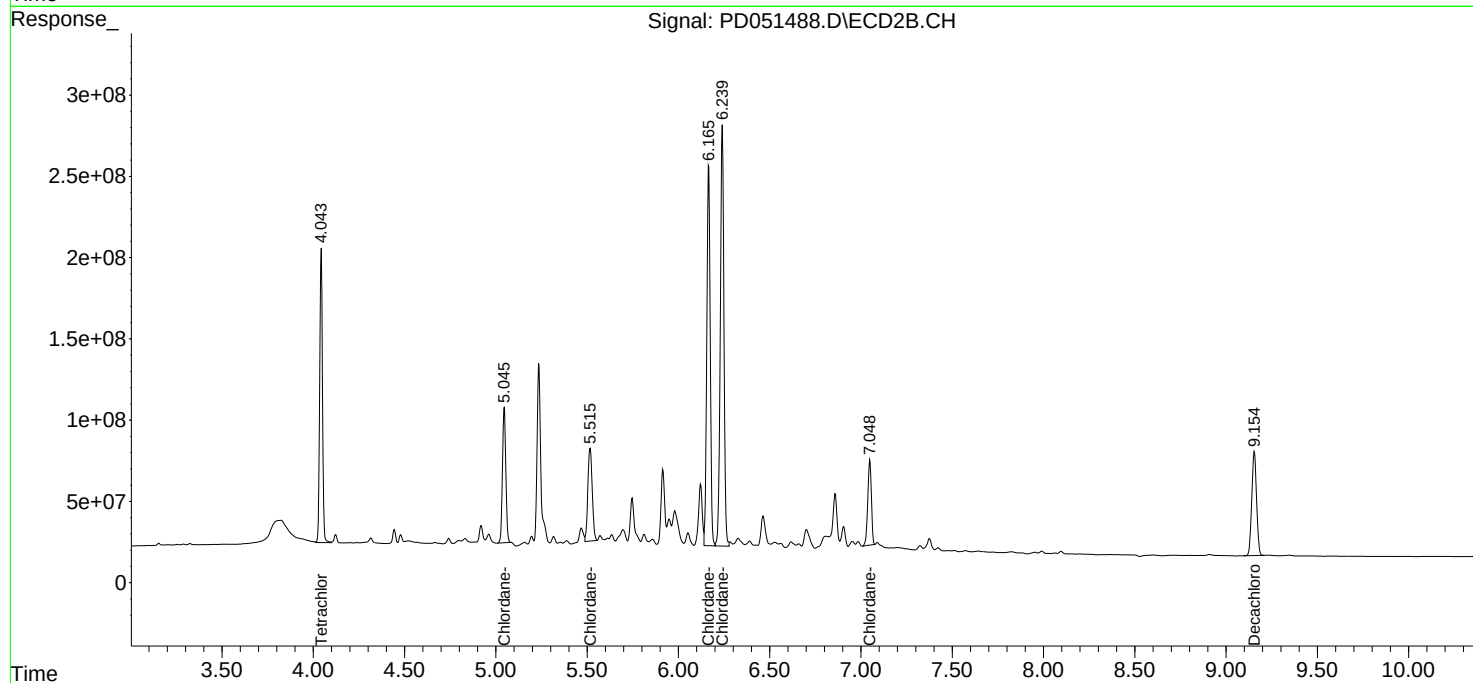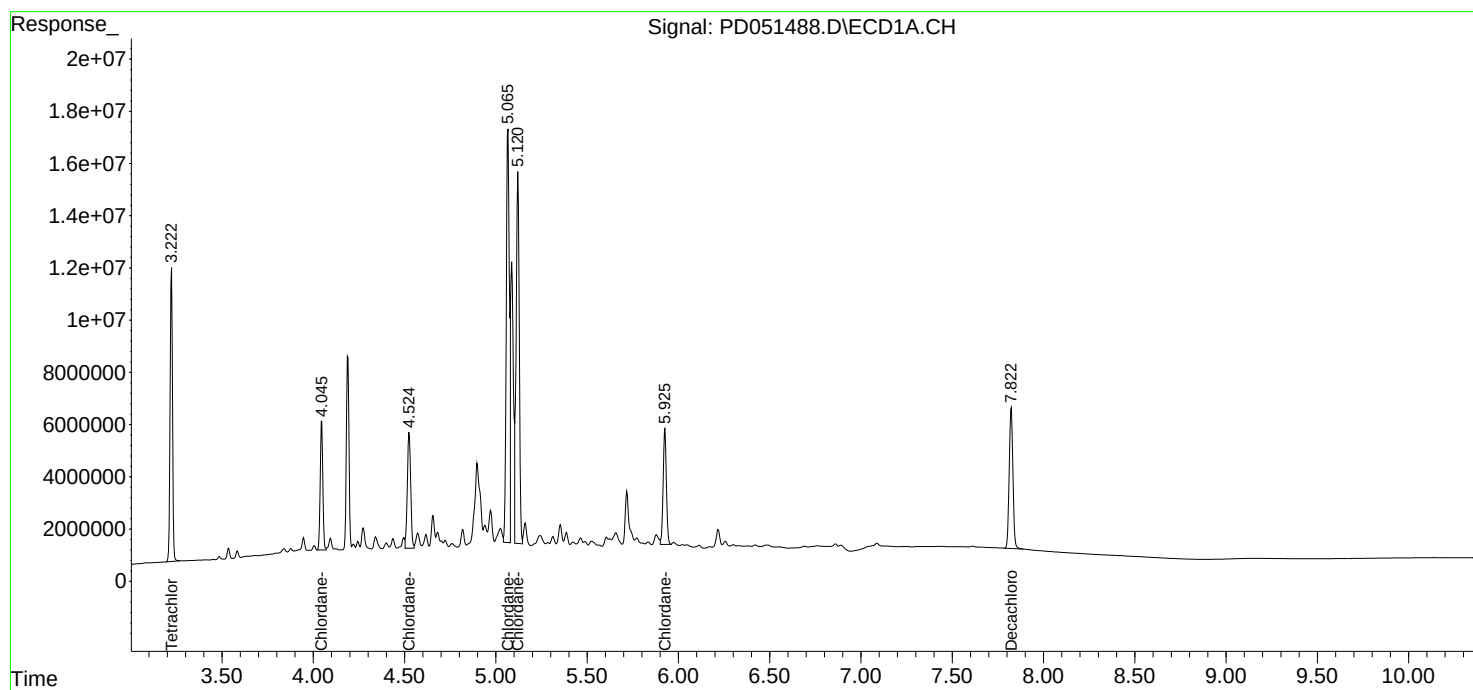


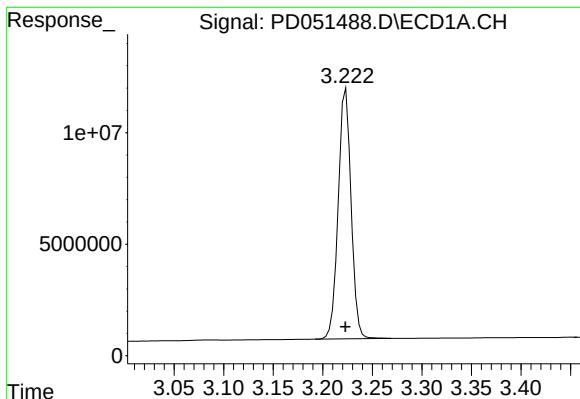

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.000 min
Response: 101409435
Conc: 75.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

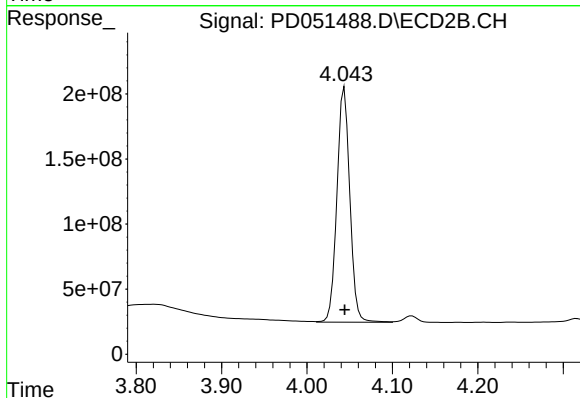


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 1892643553
Conc: 71.04 ng/ml

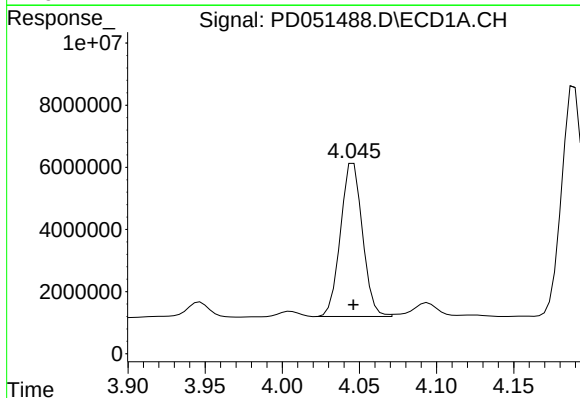


#23 Chlordane-1

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 48846337
Conc: 743.25 ng/ml

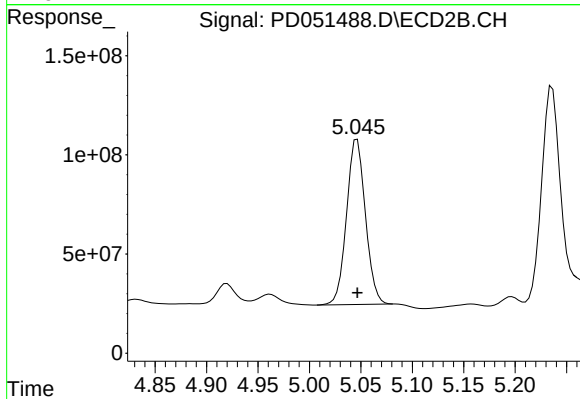

#23 Chlordane-1


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 1064672613
Conc: 707.53 ng/ml

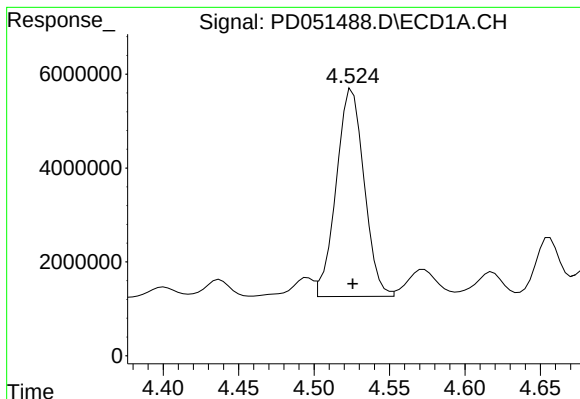

#24 Chlordane-2


R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 56873630
Conc: 718.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

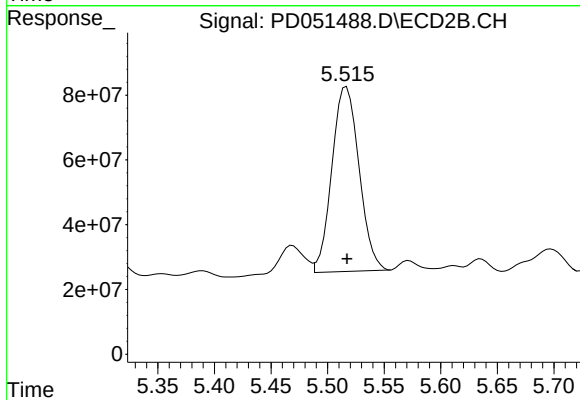


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 954955531
Conc: 695.46 ng/ml

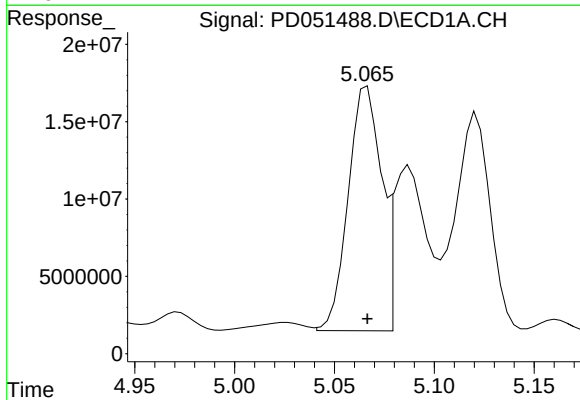


#25 Chlordane-3

R.T.: 5.066 min
Delta R.T.: 0.000 min
Response: 182492189
Conc: 760.63 ng/ml

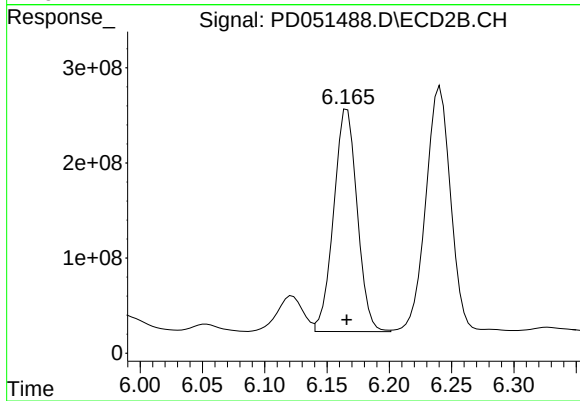

#25 Chlordane-3


R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 3081073978
Conc: 704.59 ng/ml

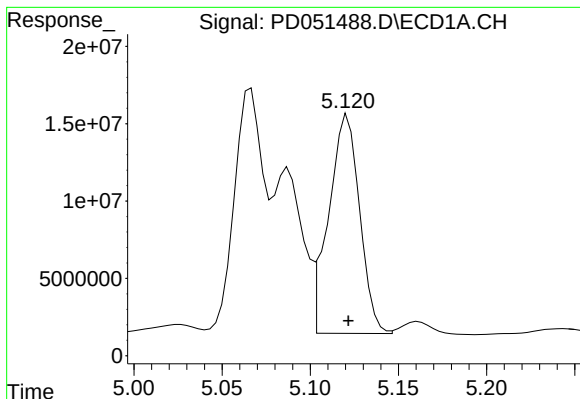

#26 Chlordane-4


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 172992423
Conc: 747.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

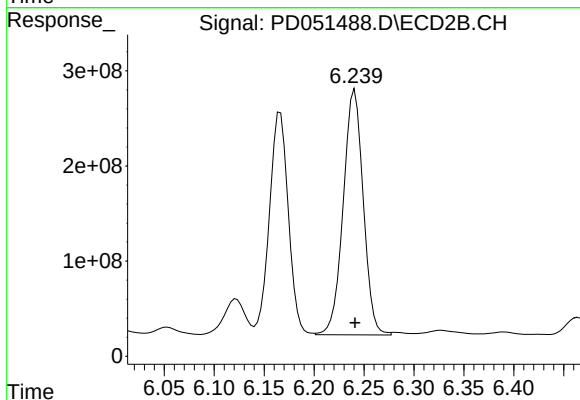


#26 Chlordane-4

R.T.: 6.241 min
Delta R.T.: 0.000 min
Response: 3598083943
Conc: 701.76 ng/ml

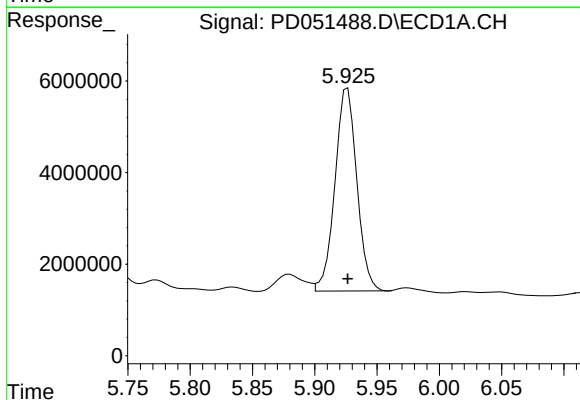


#27 Chlordane-5

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 54283665
Conc: 725.71 ng/ml

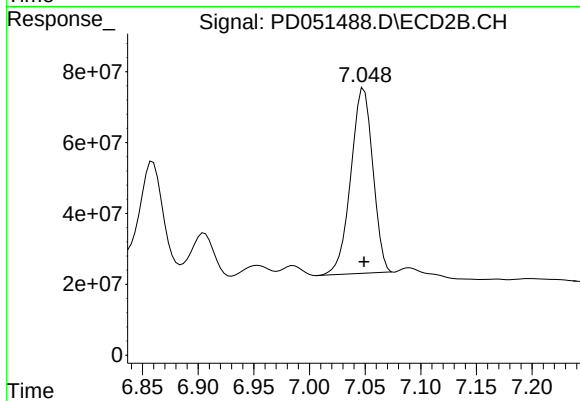

#27 Chlordane-5

R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 720814972
Conc: 725.65 ng/ml

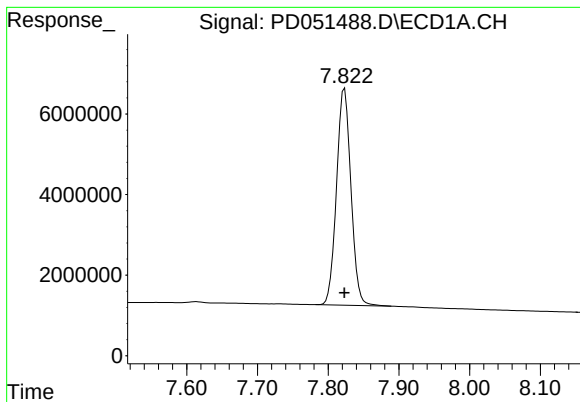

#28 Decachlorobiphenyl


R.T.: 7.823 min

Delta R.T.: 0.000 min

Response: 76166561

Conc: 71.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

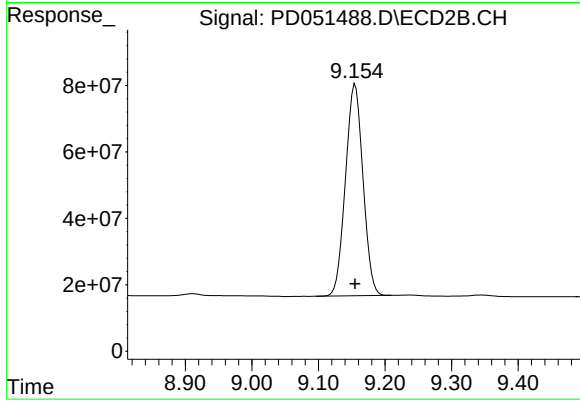

#28 Decachlorobiphenyl

R.T.: 9.155 min

Delta R.T.: 0.000 min

Response: 1164555365

Conc: 69.63 ng/ml