

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
 Data File : PD051498.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 21:18
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD030219CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 23:37:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 23:36:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	66438965	1336.6E6	50.500	49.035
28)	SA Decachlor...	7.823	9.156	53739621	840.5E6	49.159	48.233
Target Compounds							
23)	Chlordane-1	4.046	5.047	32865181	757.0E6	513.827	494.348
24)	Chlordane-2	4.526	5.517	39695759	691.6E6	507.185	487.750
25)	Chlordane-3	5.067	6.167	120.8E6	2208.3E6	519.191	495.911
26)	Chlordane-4	5.122	6.241	116.2E6	2575.7E6	519.450	491.820
27)	Chlordane-5	5.927	7.049	37851492	501.9E6	526.984	495.452



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030219\
Data File : PD051498.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 21:18
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD030219CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:37:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 23:36:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

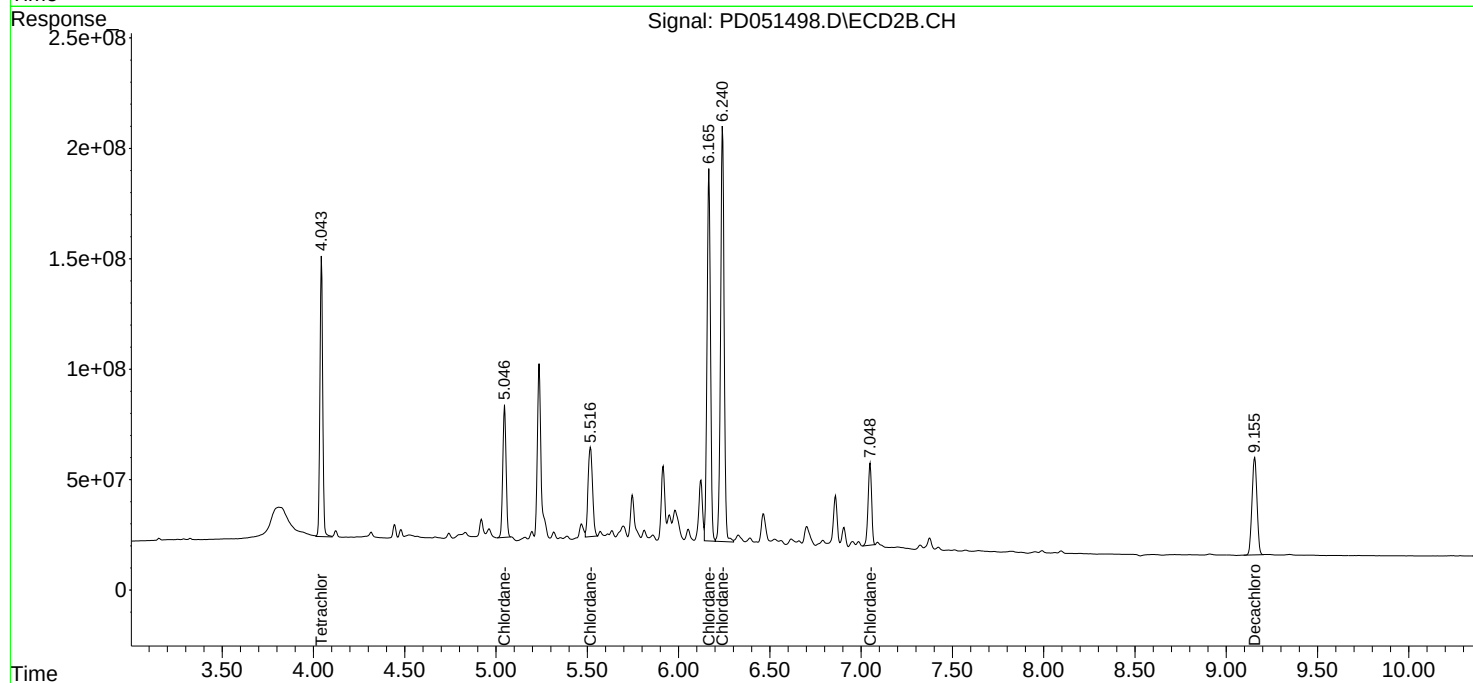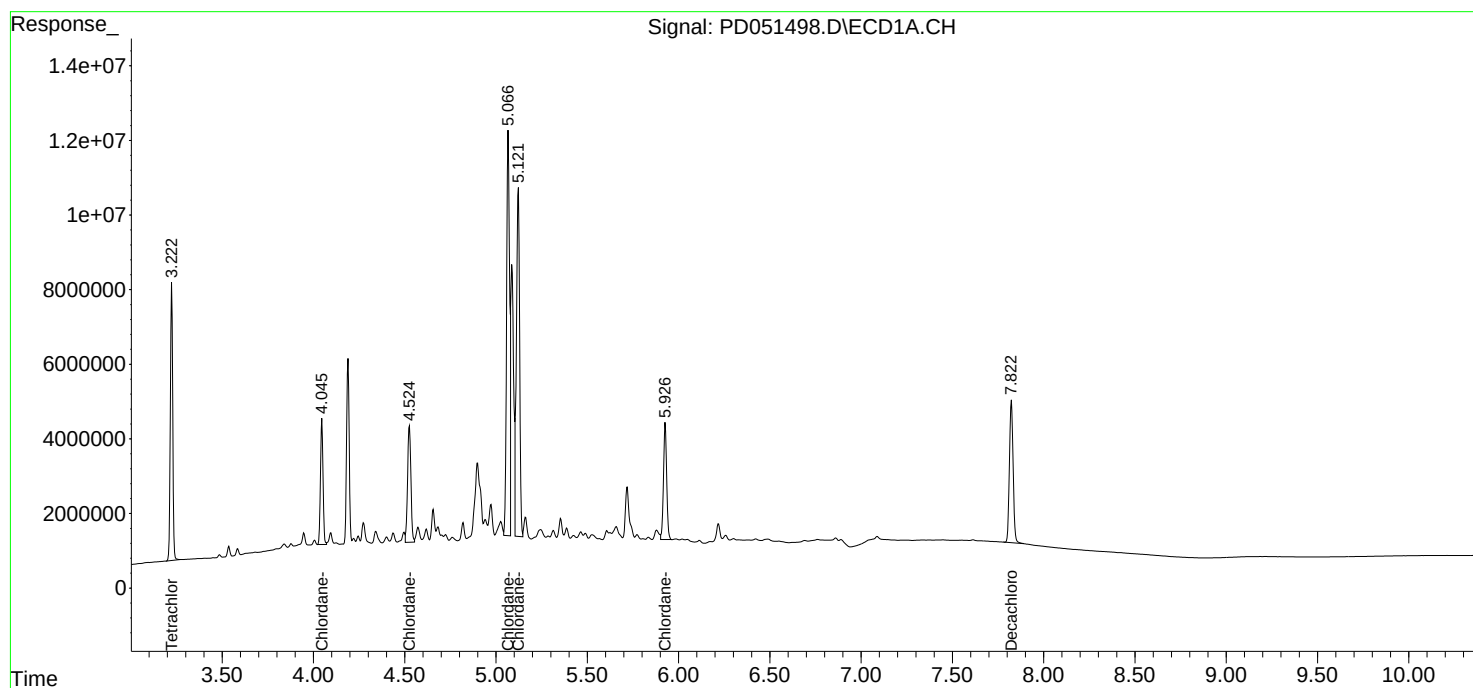


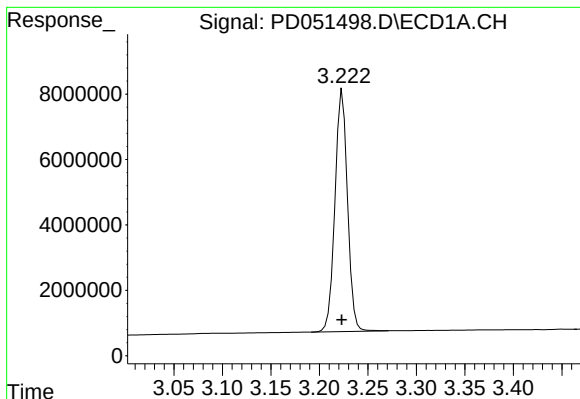

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 66438965
Conc: 50.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030219CHLOR

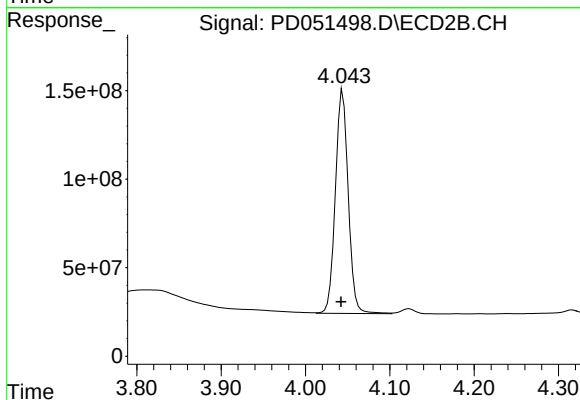


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.002 min
Response: 1336559826
Conc: 49.04 ng/ml

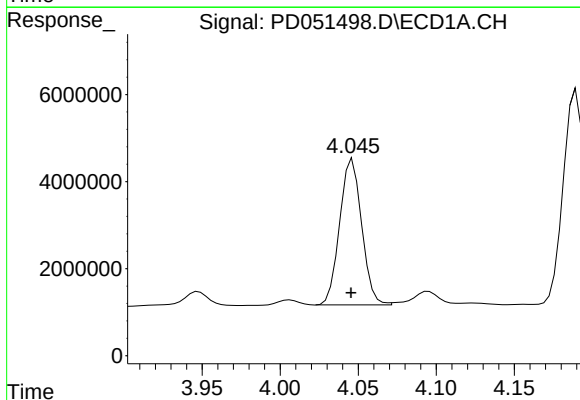


#23 Chlordane-1

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 32865181
Conc: 513.83 ng/ml

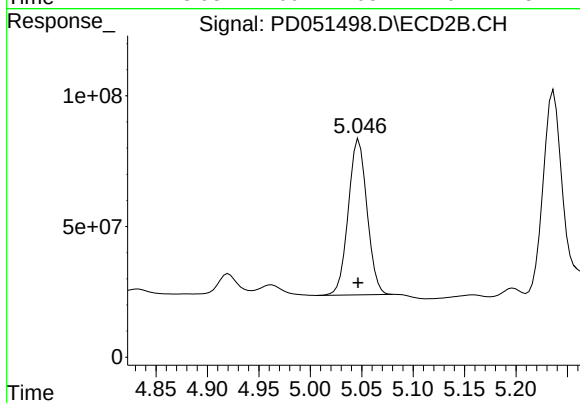

#23 Chlordane-1


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 756955379
Conc: 494.35 ng/ml

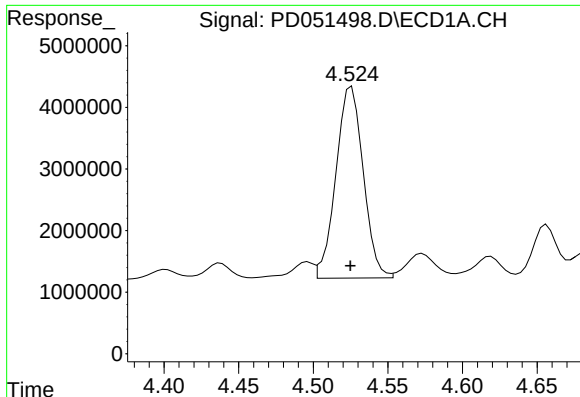

#24 Chlordane-2


R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 39695759
Conc: 507.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030219CHLOR

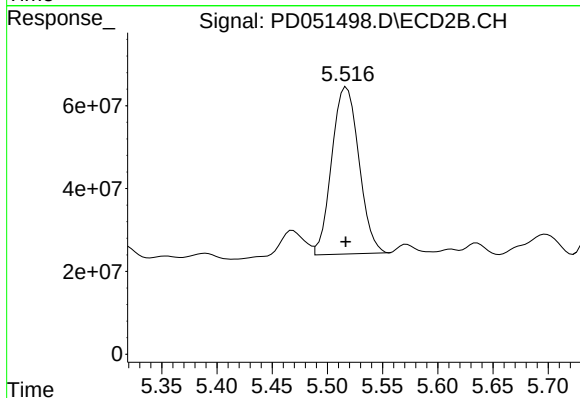


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 691624602
Conc: 487.75 ng/ml

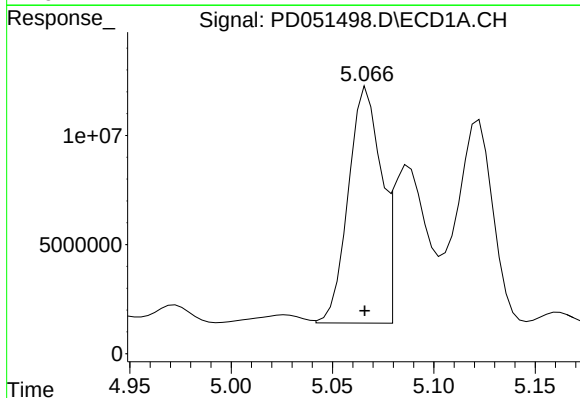


#25 Chlordane-3

R.T.: 5.067 min
Delta R.T.: 0.001 min
Response: 120836311
Conc: 519.19 ng/ml

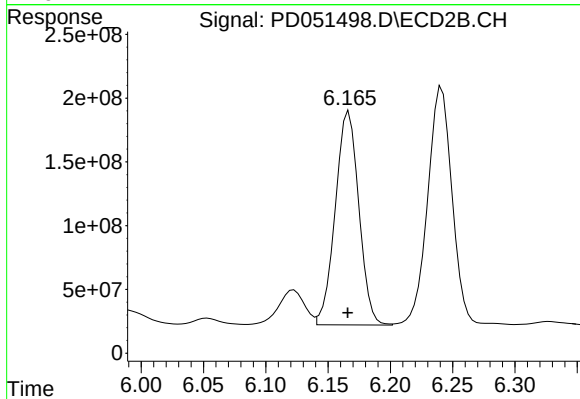

#25 Chlordane-3


R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 2208345274
Conc: 495.91 ng/ml

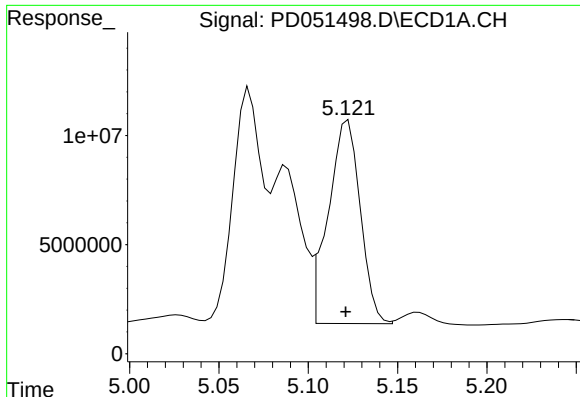

#26 Chlordane-4


R.T.: 5.122 min
Delta R.T.: 0.001 min
Response: 116152559
Conc: 519.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030219CHLOR

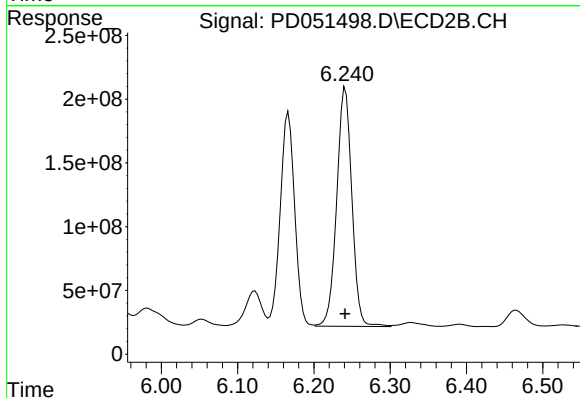


#26 Chlordane-4

R.T.: 6.241 min
Delta R.T.: 0.000 min
Response: 2575693328
Conc: 491.82 ng/ml

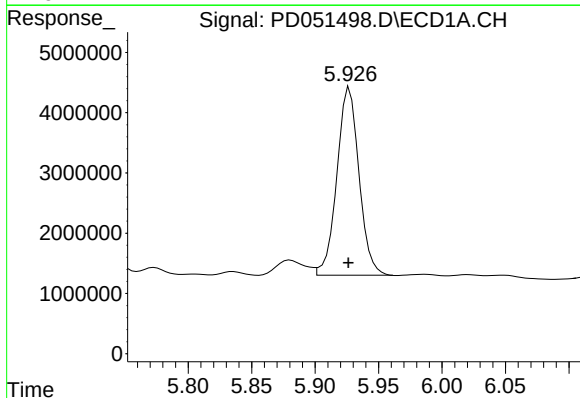


#27 Chlordane-5

R.T.: 5.927 min
Delta R.T.: 0.001 min
Response: 37851492
Conc: 526.98 ng/ml

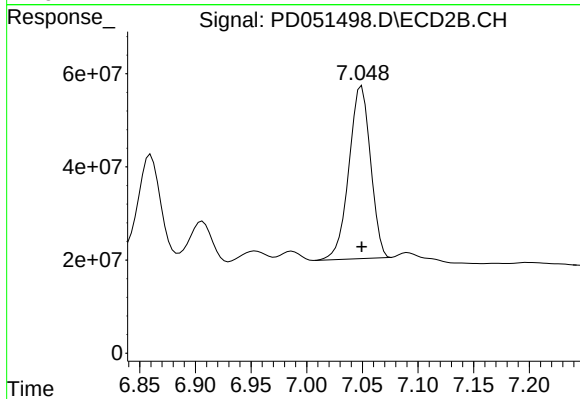

#27 Chlordane-5


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 501883624
Conc: 495.45 ng/ml

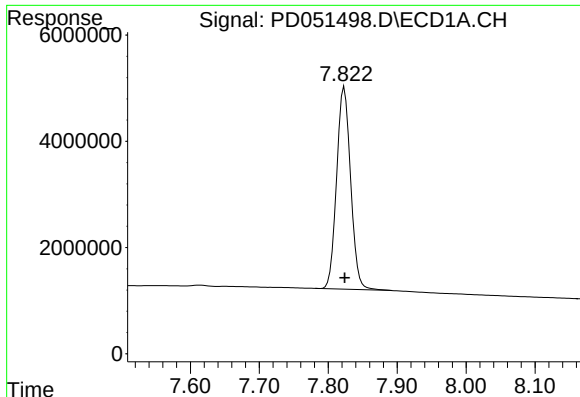

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 53739621
Conc: 49.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD030219CHLOR

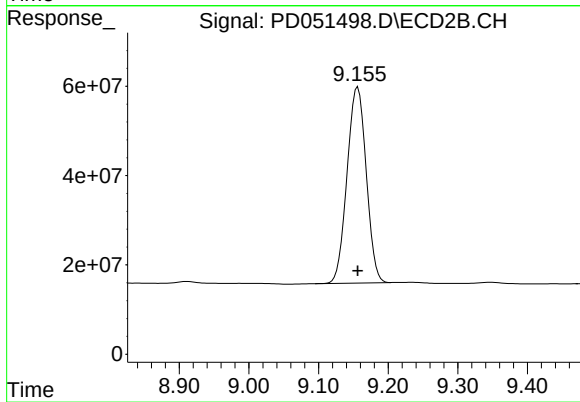

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 840477048
Conc: 48.23 ng/ml