

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030223\
 Data File : PD074092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2023 15:38
 Operator : AR\AJ
 Sample : PB151133BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 20:36:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.775	45486482	22768110	19.854	19.223
28)	SA Decachlor...	9.098	7.929	56397803	25252627	21.158	20.625
Target Compounds							
7)	B delta-BHC	4.780	0.000	5280571	0	1.884	N.D. #
8)	B Heptachlo...	5.698	0.000	1272175	0	0.447	N.D. #
9)	A Endosulfan I	6.103	0.000	92452	0	0.032	N.D. #
11)	B alpha-Chl...	6.064f	0.000	176872	0	0.057	N.D. #
15)	B Endosulfa...	6.843f	0.000	145417	0	0.050	N.D. #
17)	MA 4,4'-DDT	7.023f	0.000	143367	0	0.053	N.D. #
21)	B Endrin ke...	7.699f	0.000	263585	0	0.090	N.D. #
26)	Chlordane-4	6.064f	0.000	176872	0	0.282	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030223\
Data File : PD074092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2023 15:38
Operator : AR\AJ
Sample : PB151133BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 20:36:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

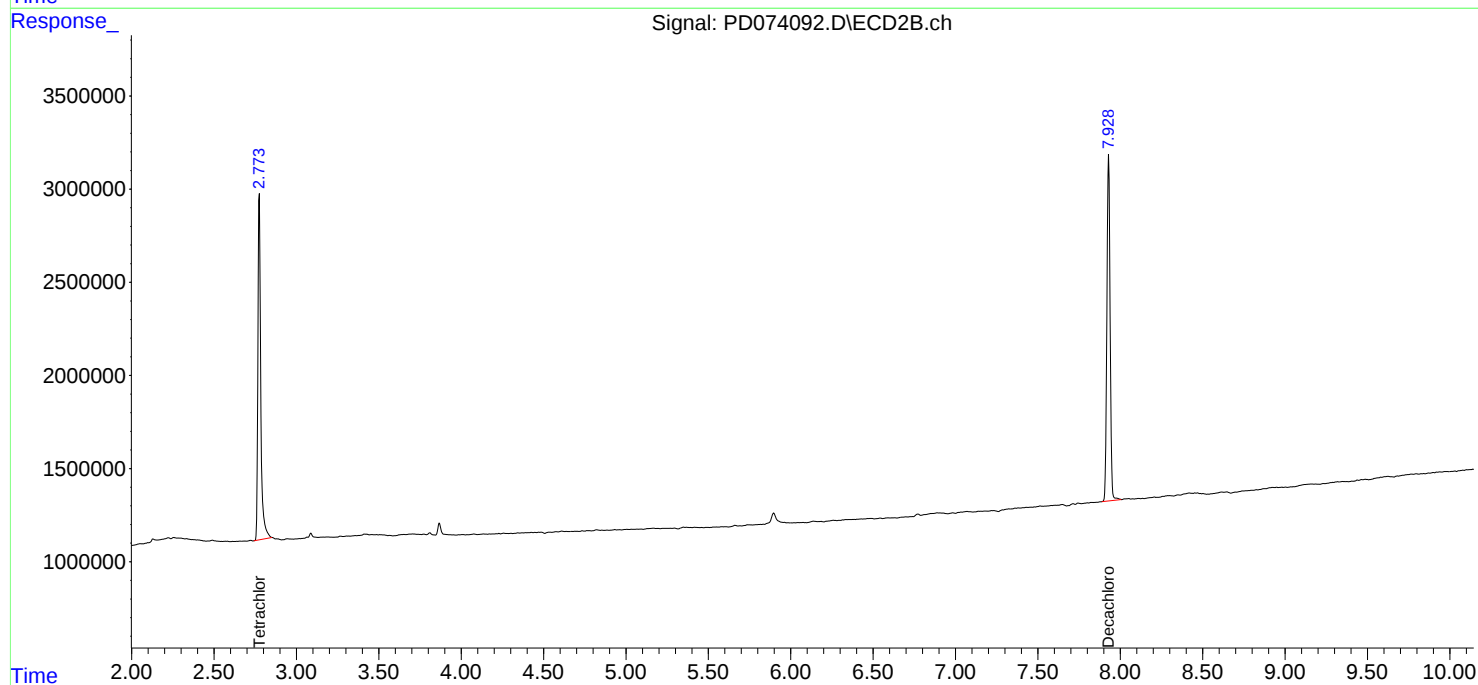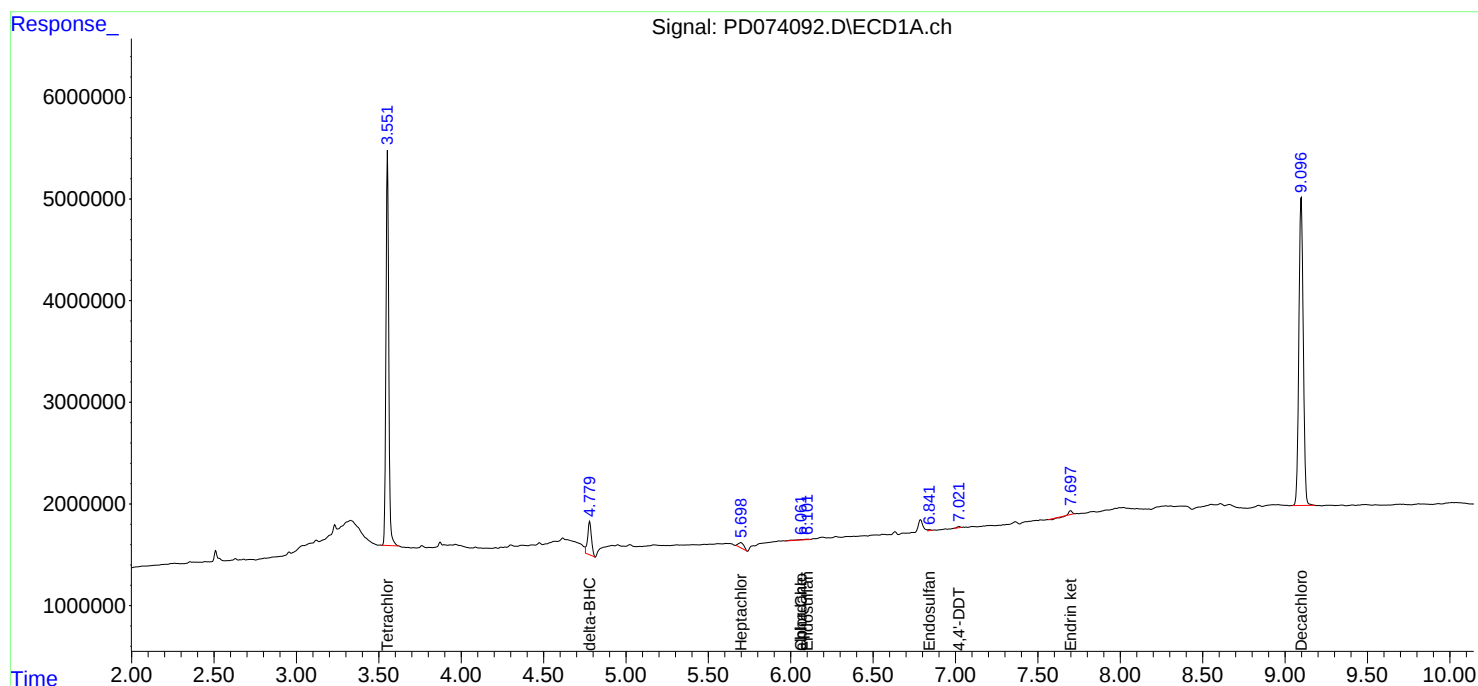


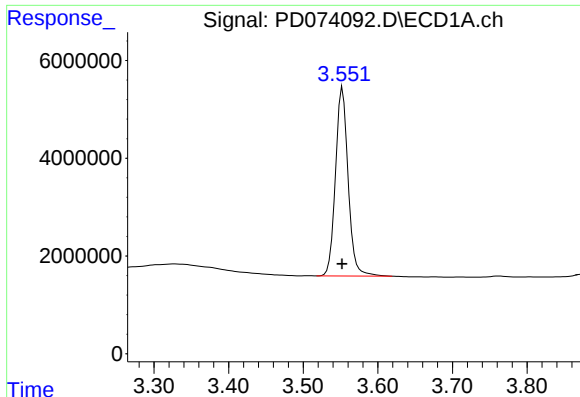

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.000 min
Response: 45486482
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

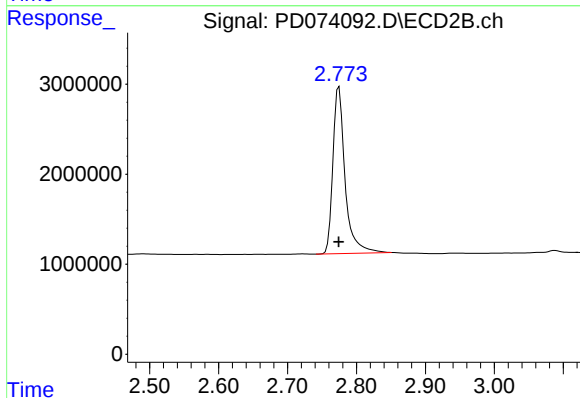


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 22768110
Conc: 19.22 ng/ml

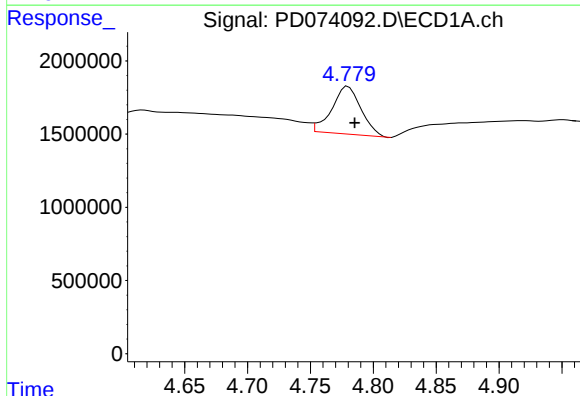


#7 delta-BHC

R.T.: 4.780 min
Delta R.T.: -0.005 min
Response: 5280571
Conc: 1.88 ng/ml

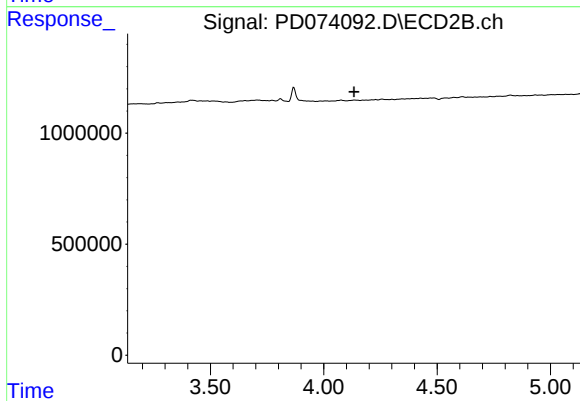

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.135 min
Response: 0
Conc: N.D.

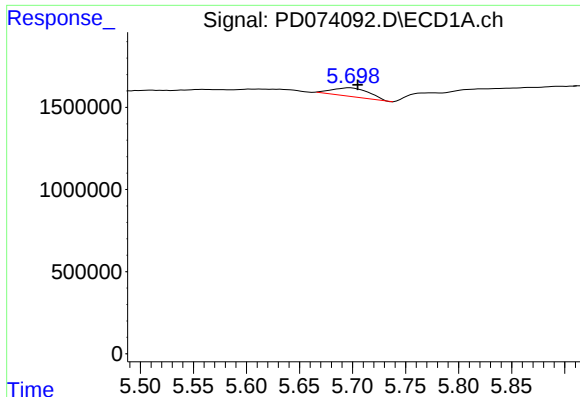

#8 Heptachlor epoxide


R.T.: 5.698 min
Delta R.T.: -0.007 min
Response: 1272175
Conc: 0.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

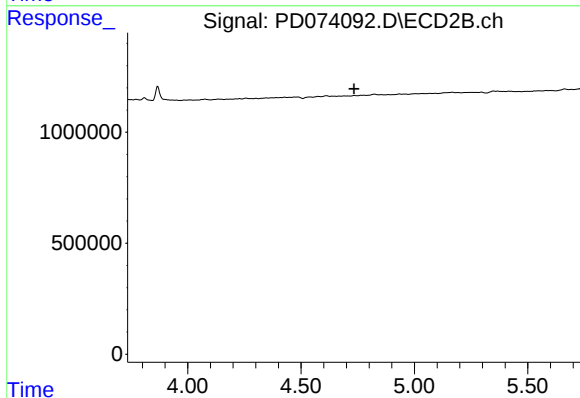


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

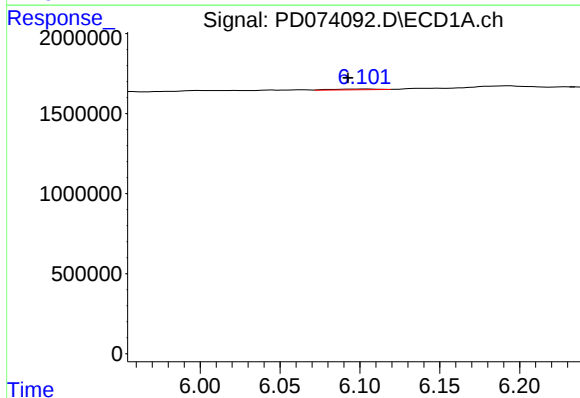


#9 Endosulfan I

R.T.: 6.103 min
Delta R.T.: 0.010 min
Response: 92452
Conc: 0.03 ng/ml

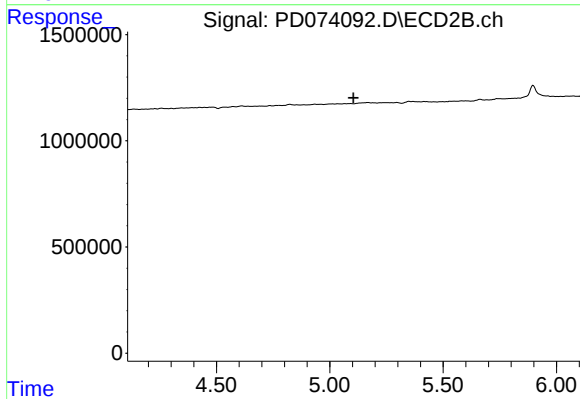

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.105 min
Response: 0
Conc: N.D.

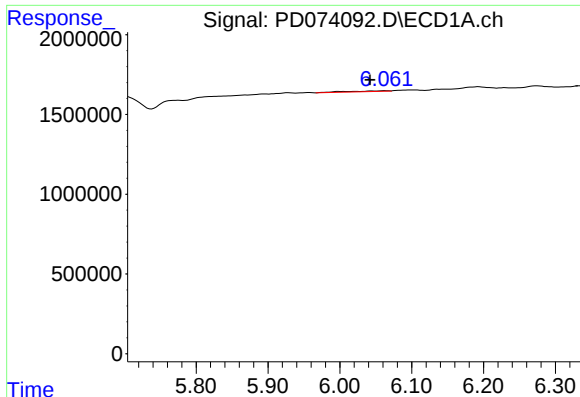

#11 alpha-Chlordane


R.T.: 6.064 min
Delta R.T.: 0.022 min
Response: 176872
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

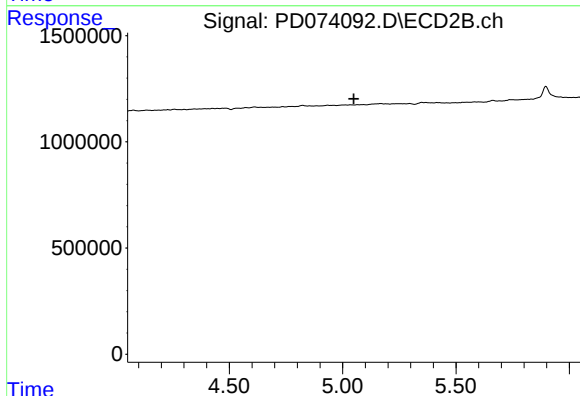


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

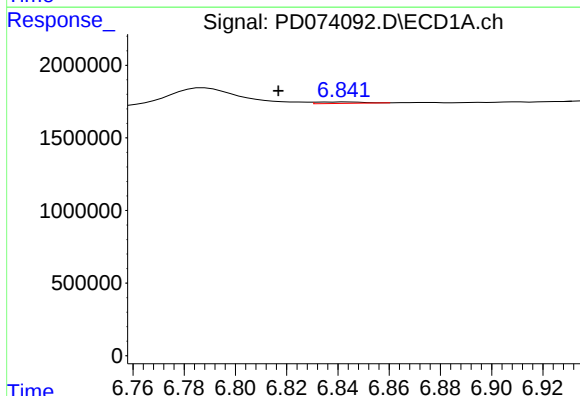


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.026 min
Response: 145417
Conc: 0.05 ng/ml

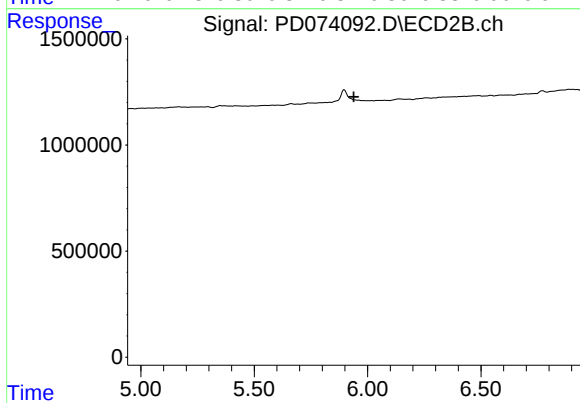

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

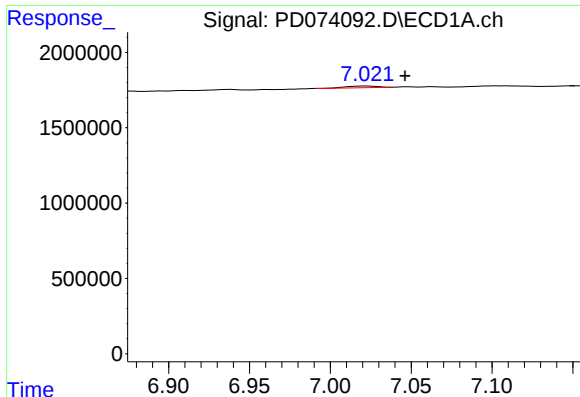

#17 4,4'-DDT


R.T.: 7.023 min
Delta R.T.: -0.023 min
Response: 143367
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

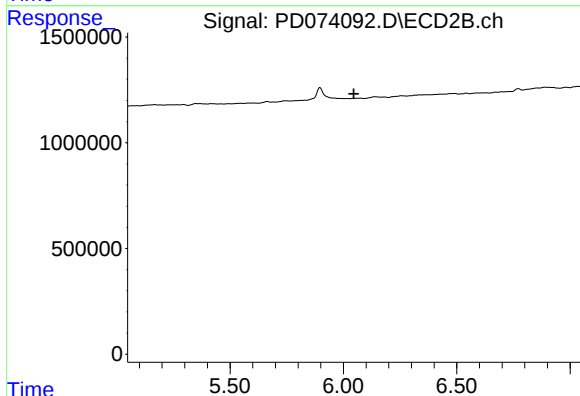


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

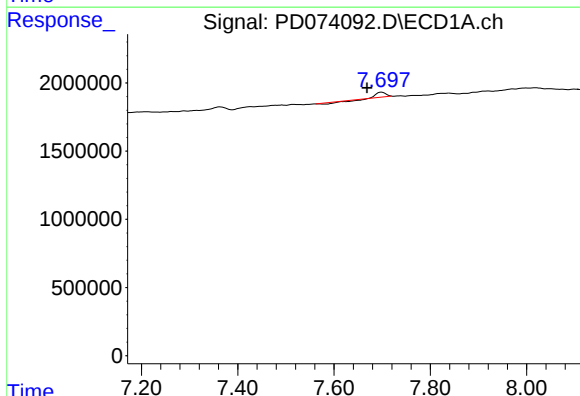


#21 Endrin ketone

R.T.: 7.699 min
Delta R.T.: 0.030 min
Response: 263585
Conc: 0.09 ng/ml

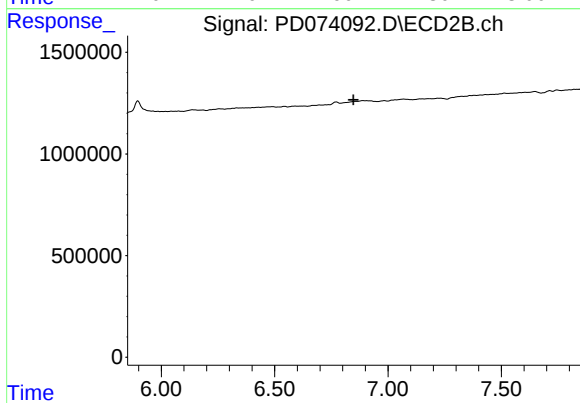

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

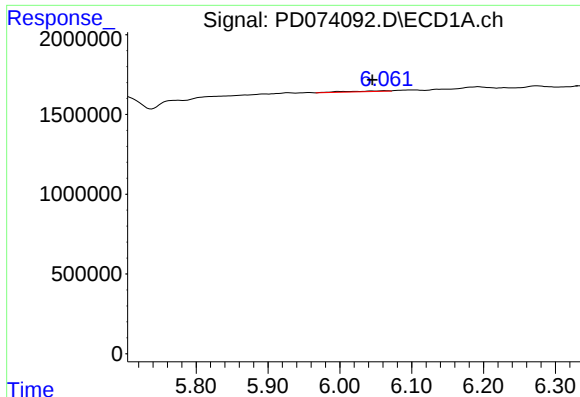

#26 Chlordane-4


R.T.: 6.064 min
Delta R.T.: 0.018 min
Response: 176872
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

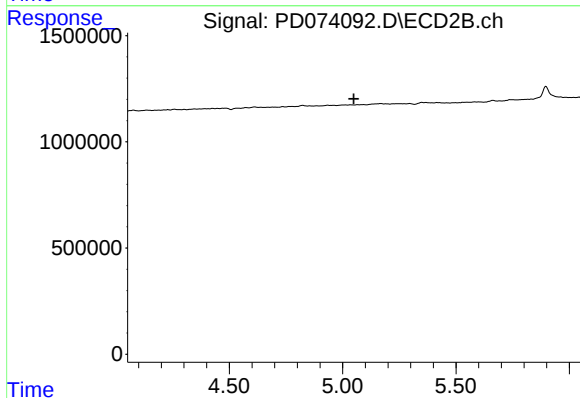


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

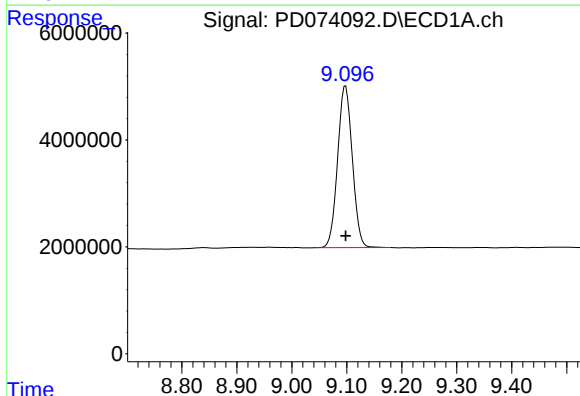

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 56397803
Conc: 21.16 ng/ml

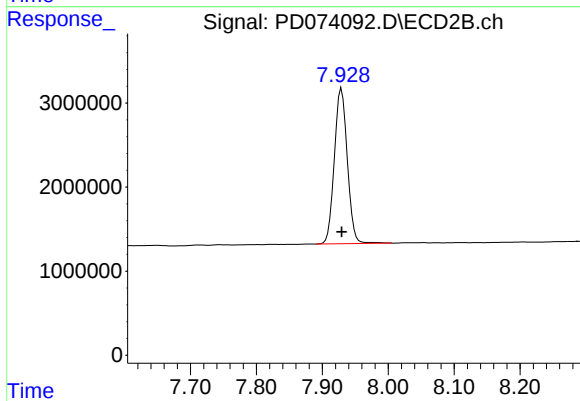

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 25252627
Conc: 20.62 ng/ml