

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030223\
 Data File : PD074101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2023 19:17
 Operator : AR\AJ
 Sample : PB151055BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 20:46:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.775	41785904	20972988	18.238	17.707
28)	SA Decachlor...	9.098	7.929	46121356	19429576	17.303	15.869
Target Compounds							
7)	B delta-BHC	4.779	0.000	3860848	0	1.377	N.D. #
8)	B Heptachlo...	5.697	0.000	1078926	0	0.379	N.D. #
9)	A Endosulfan I	6.064f	0.000	117457	0	0.041	N.D. #
11)	B alpha-Chl...	6.064f	0.000	117457	0	0.038	N.D. #
12)	B 4,4'-DDE	6.190f	0.000	146257	0	0.051	N.D. #
15)	B Endosulfa...	6.837f	0.000	528290	0	0.182	N.D. #
17)	MA 4,4'-DDT	7.017f	0.000	210534	0	0.077	N.D. #
21)	B Endrin ke...	7.660	0.000	47222	0	0.016	N.D. #
24)	Chlordane-2	5.244	0.000	144984	0	1.074	N.D. #
26)	Chlordane-4	6.064f	0.000	117457	0	0.187	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030223\
Data File : PD074101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2023 19:17
Operator : AR\AJ
Sample : PB151055BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 20:46:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

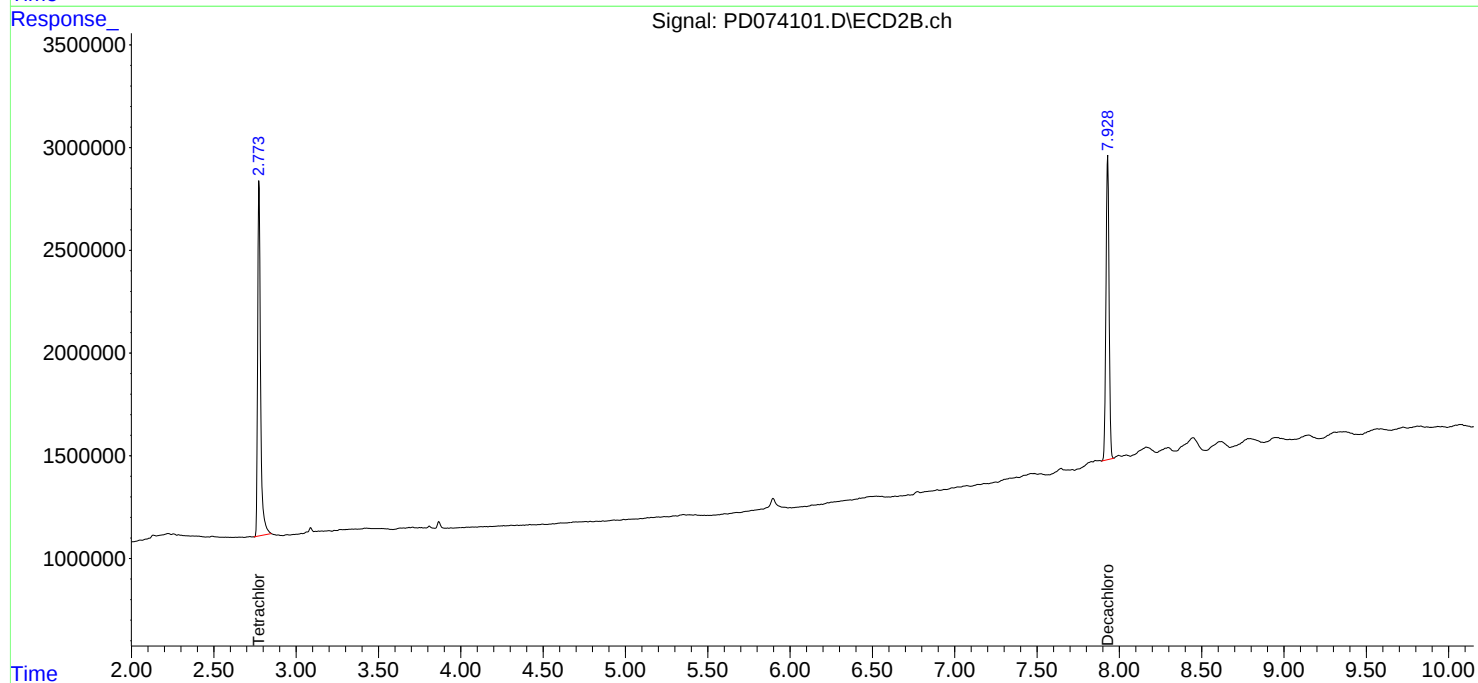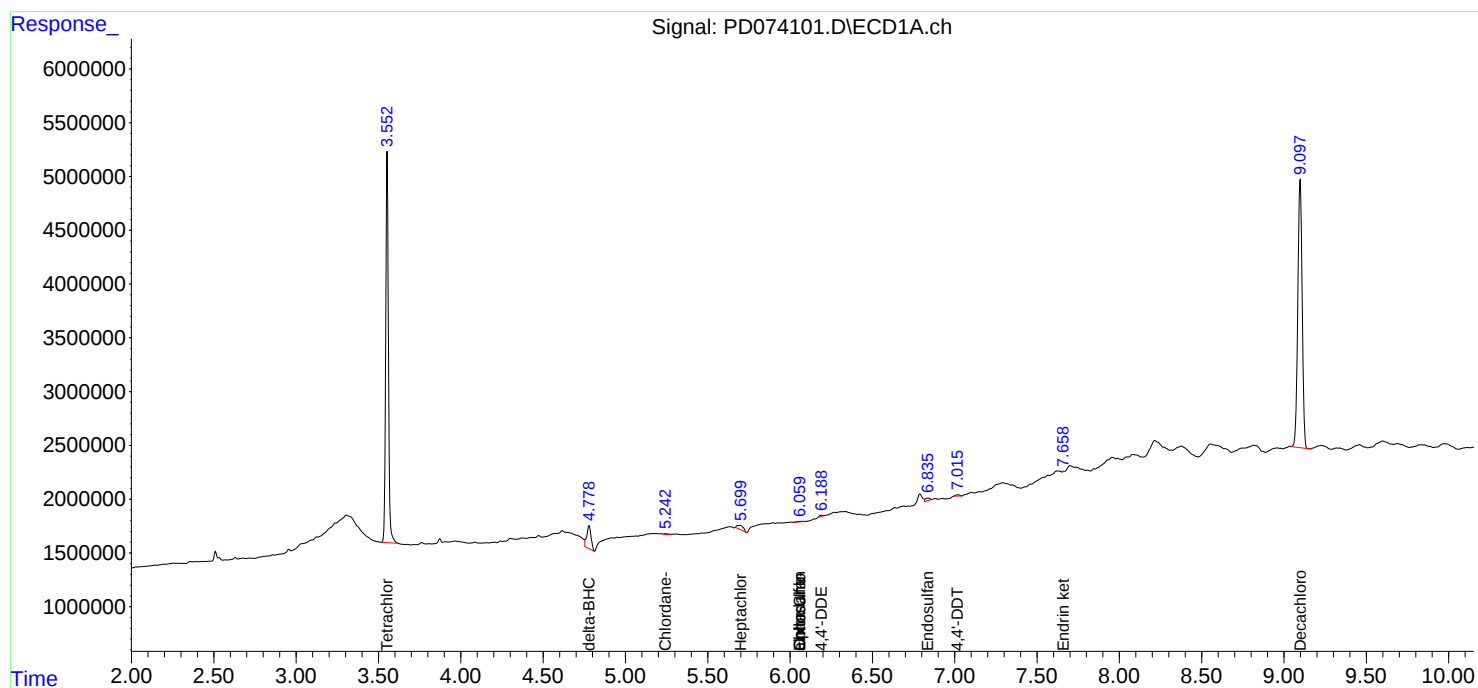


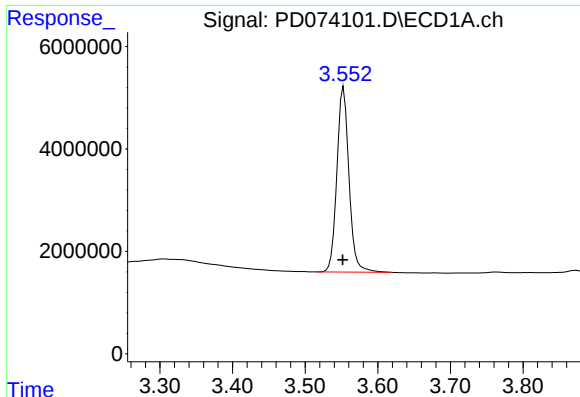

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.001 min
Response: 41785904
Conc: 18.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

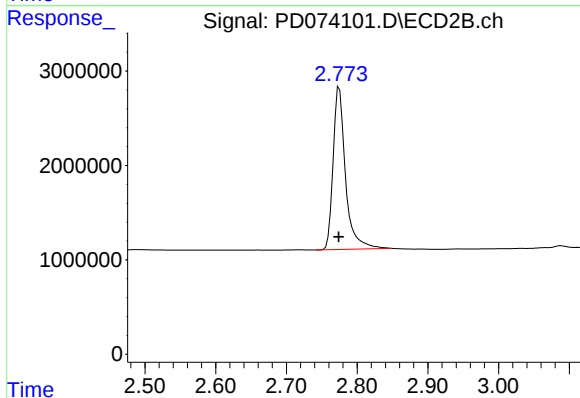


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 20972988
Conc: 17.71 ng/ml

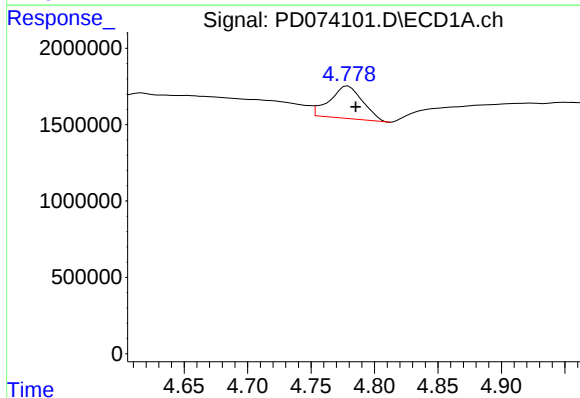


#7 delta-BHC

R.T.: 4.779 min
Delta R.T.: -0.006 min
Response: 3860848
Conc: 1.38 ng/ml

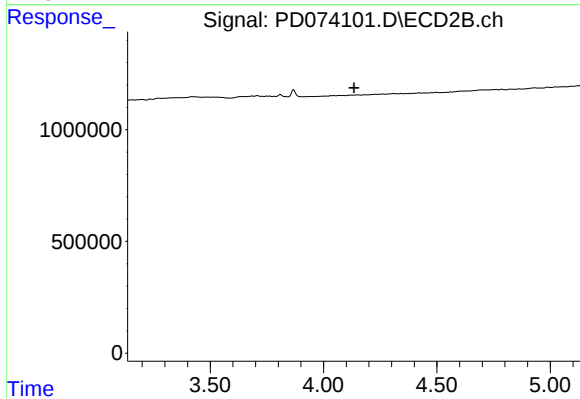

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.135 min
Response: 0
Conc: N.D.

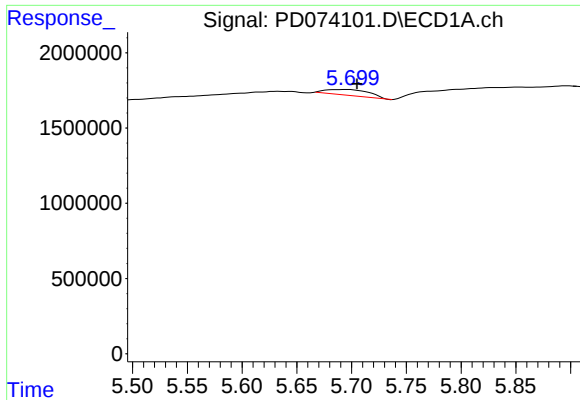

#8 Heptachlor epoxide


R.T.: 5.697 min
Delta R.T.: -0.008 min
Response: 1078926
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

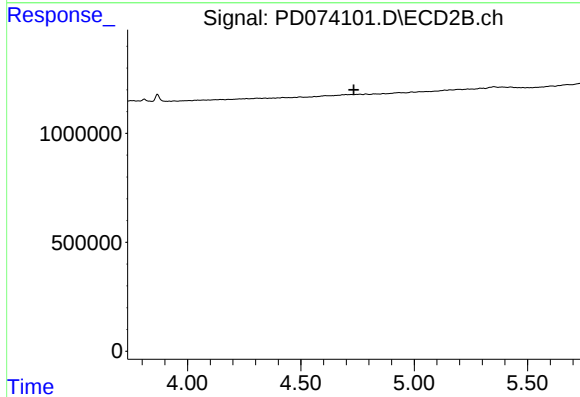


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

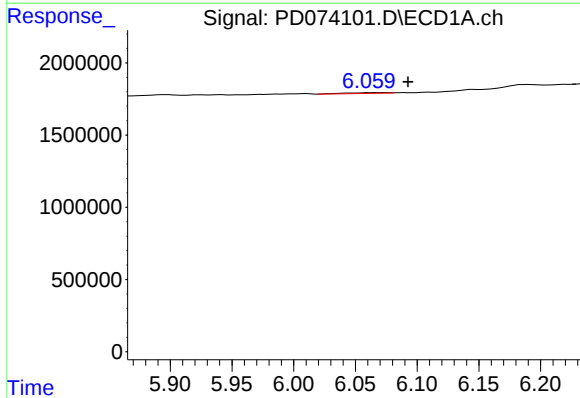


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: -0.028 min
Response: 117457
Conc: 0.04 ng/ml

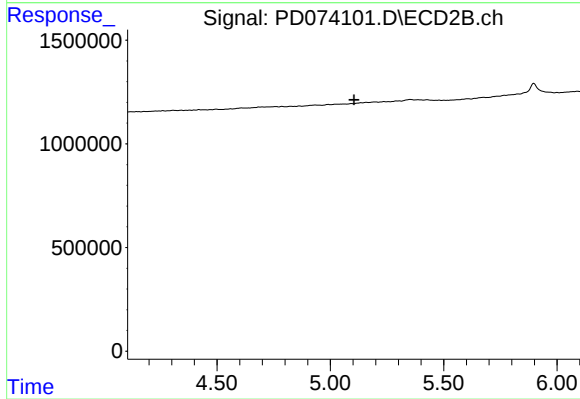

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.105 min
Response: 0
Conc: N.D.

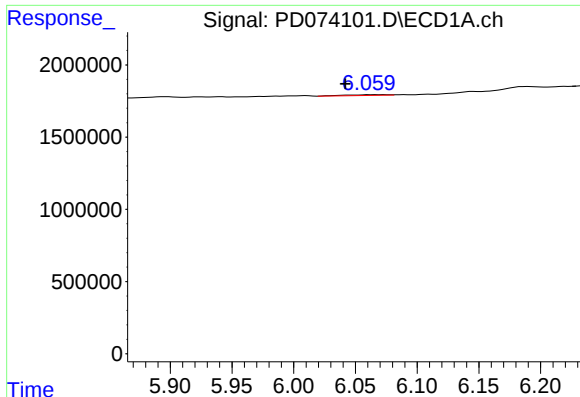

#11 alpha-Chlordane


R.T.: 6.064 min
Delta R.T.: 0.022 min
Response: 117457
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

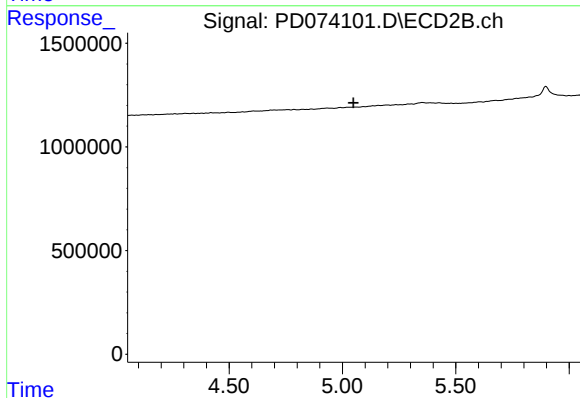


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

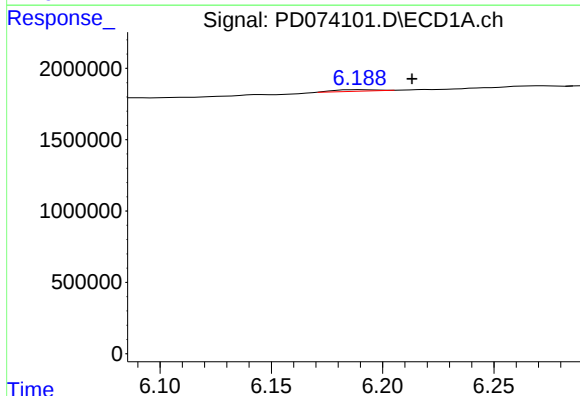


#12 4,4'-DDE

R.T.: 6.190 min
Delta R.T.: -0.023 min
Response: 146257
Conc: 0.05 ng/ml

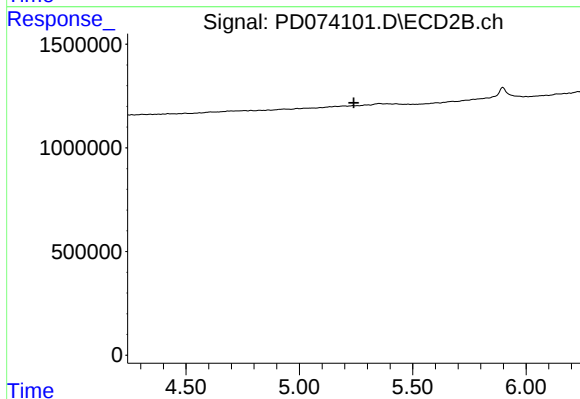

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

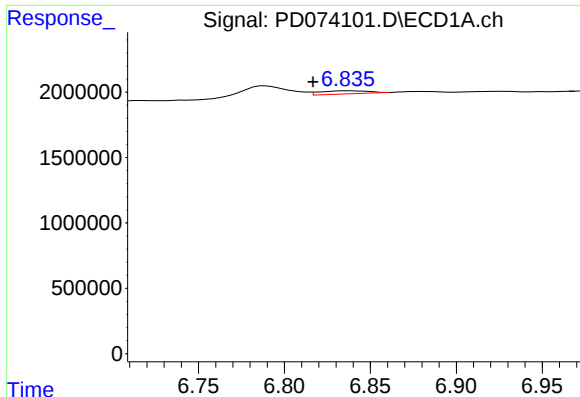

#15 Endosulfan II


R.T.: 6.837 min
Delta R.T.: 0.021 min
Response: 528290
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

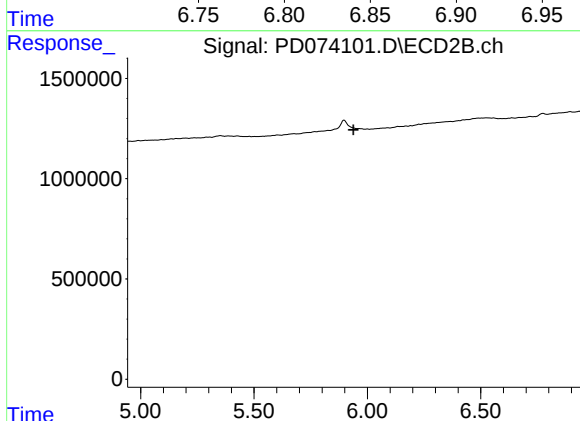


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.939 min
Response: 0
Conc: N.D.

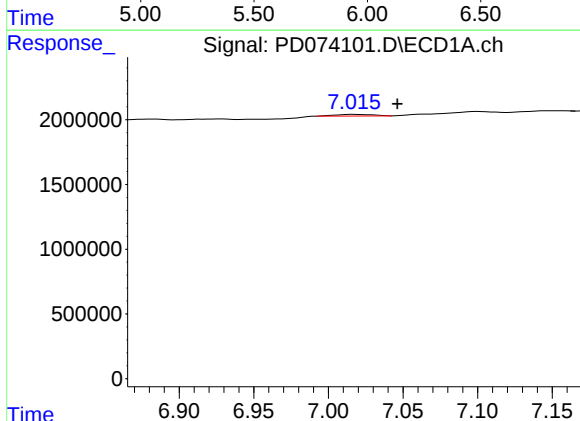


#17 4,4'-DDT

R.T.: 7.017 min
Delta R.T.: -0.029 min
Response: 210534
Conc: 0.08 ng/ml

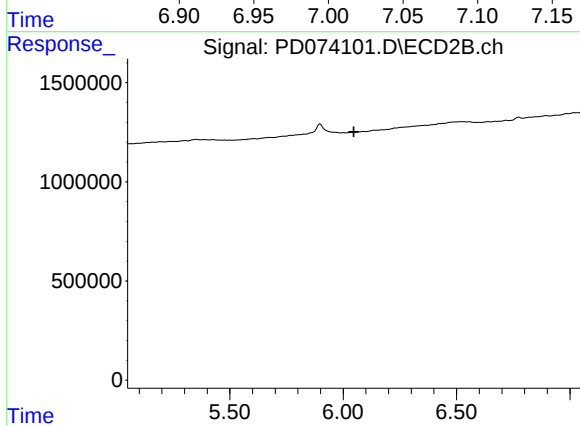

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

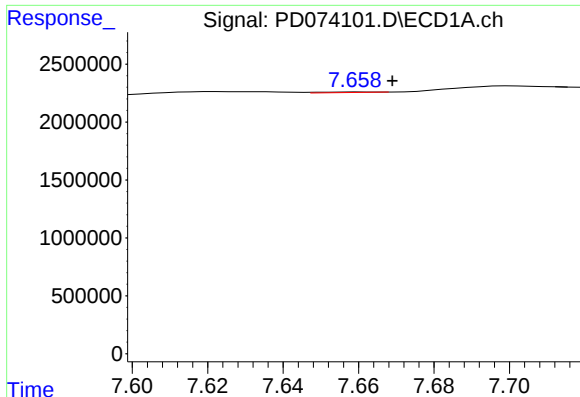

#21 Endrin ketone


R.T.: 7.660 min
Delta R.T.: -0.009 min
Response: 47222
Conc: 0.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

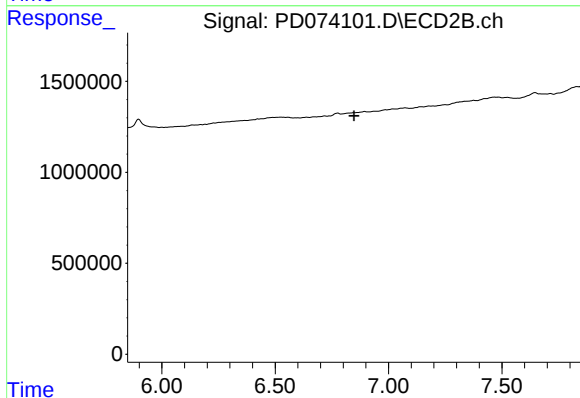


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

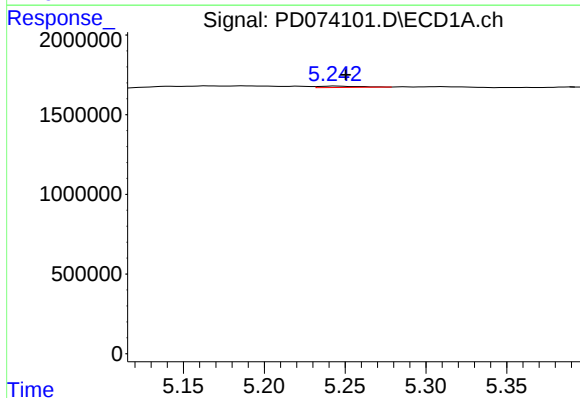


#24 Chlordane-2

R.T.: 5.244 min
Delta R.T.: -0.006 min
Response: 144984
Conc: 1.07 ng/ml

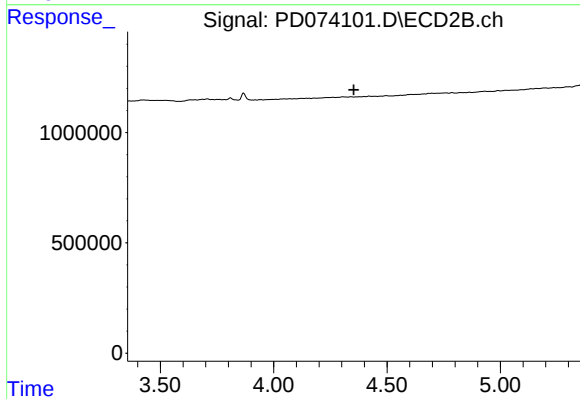

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.353 min
Response: 0
Conc: N.D.

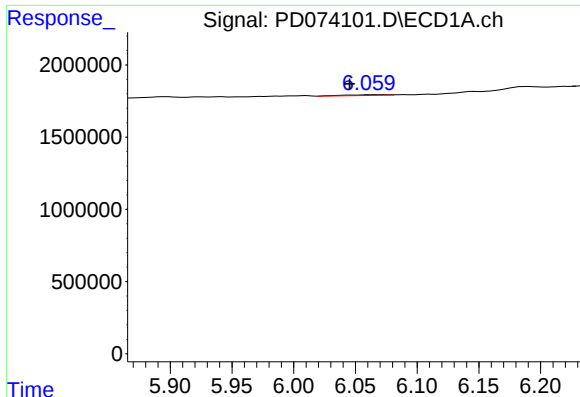

#26 Chlordane-4


R.T.: 6.064 min
Delta R.T.: 0.019 min
Response: 117457
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

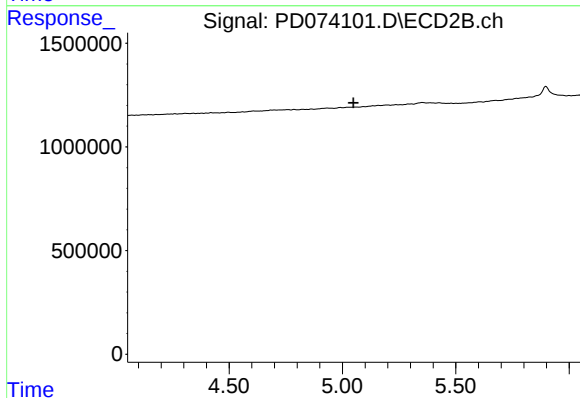


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

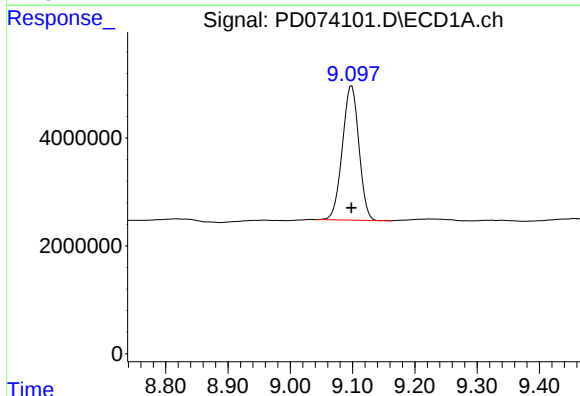

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 46121356
Conc: 17.30 ng/ml

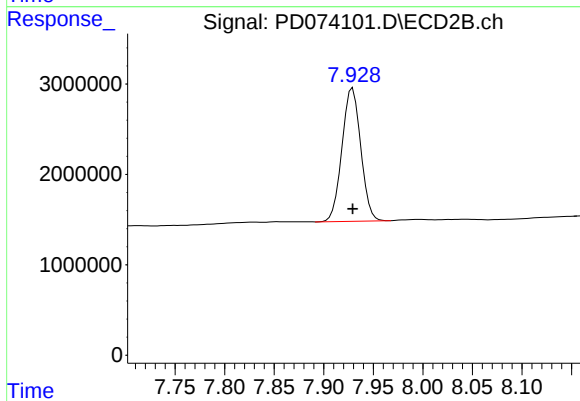

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: 0.000 min
Response: 19429576
Conc: 15.87 ng/ml