

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030223\
 Data File : PD074084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2023 13:50
 Operator : AR\AJ
 Sample : 01736-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 20:26:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 01:35:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.553	2.775	30473567	15419470	13.301	13.019
28) SA Decachlor...	9.099	7.928	33476422	13155252	12.559	10.744
Target Compounds						
10) B gamma-Chl...	5.961	4.985	3859817	827450	1.261m	0.543m#
11) B alpha-Chl...	6.045	5.048	7995263	1938121	2.594	1.287m#
12) B 4,4'-DDE	6.211	5.239	1682332	1071125	0.592	0.772 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030223\
Data File : PD074084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2023 13:50
Operator : AR\AJ
Sample : 01736-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 20:26:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 01:35:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

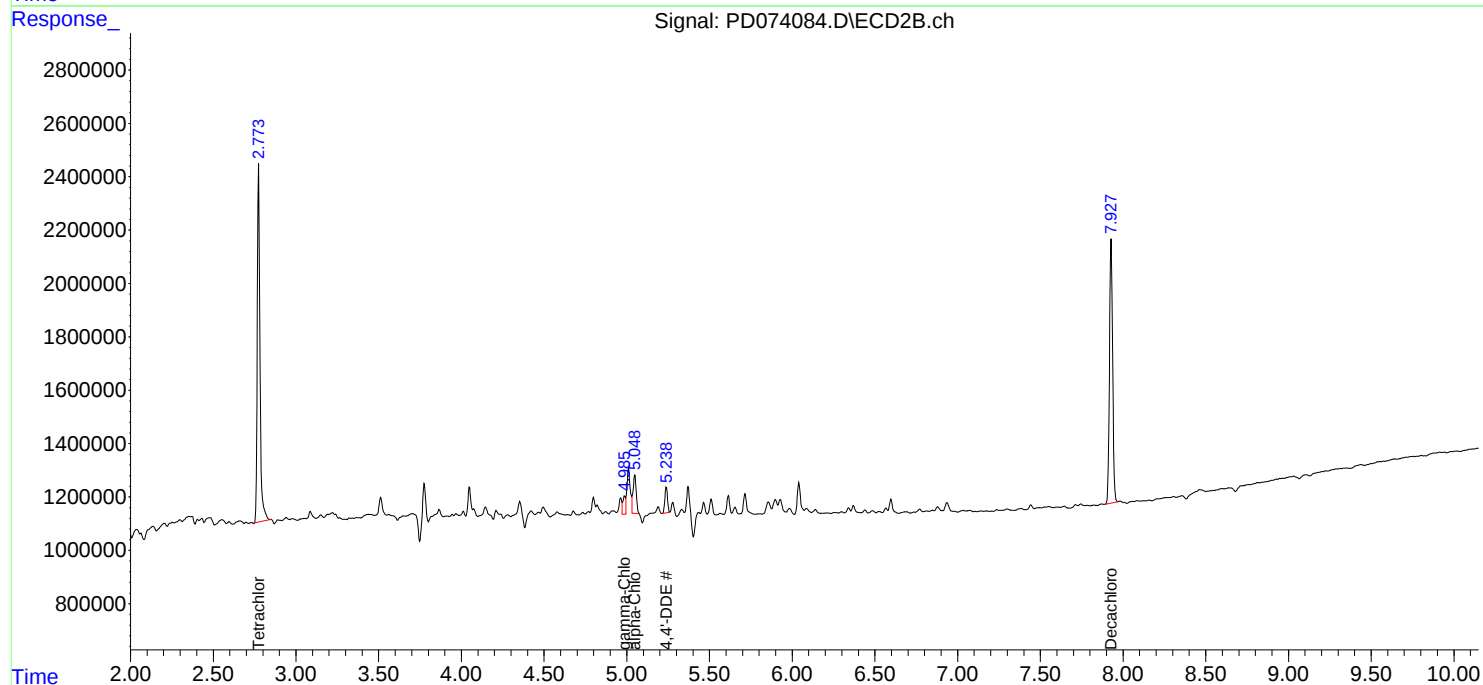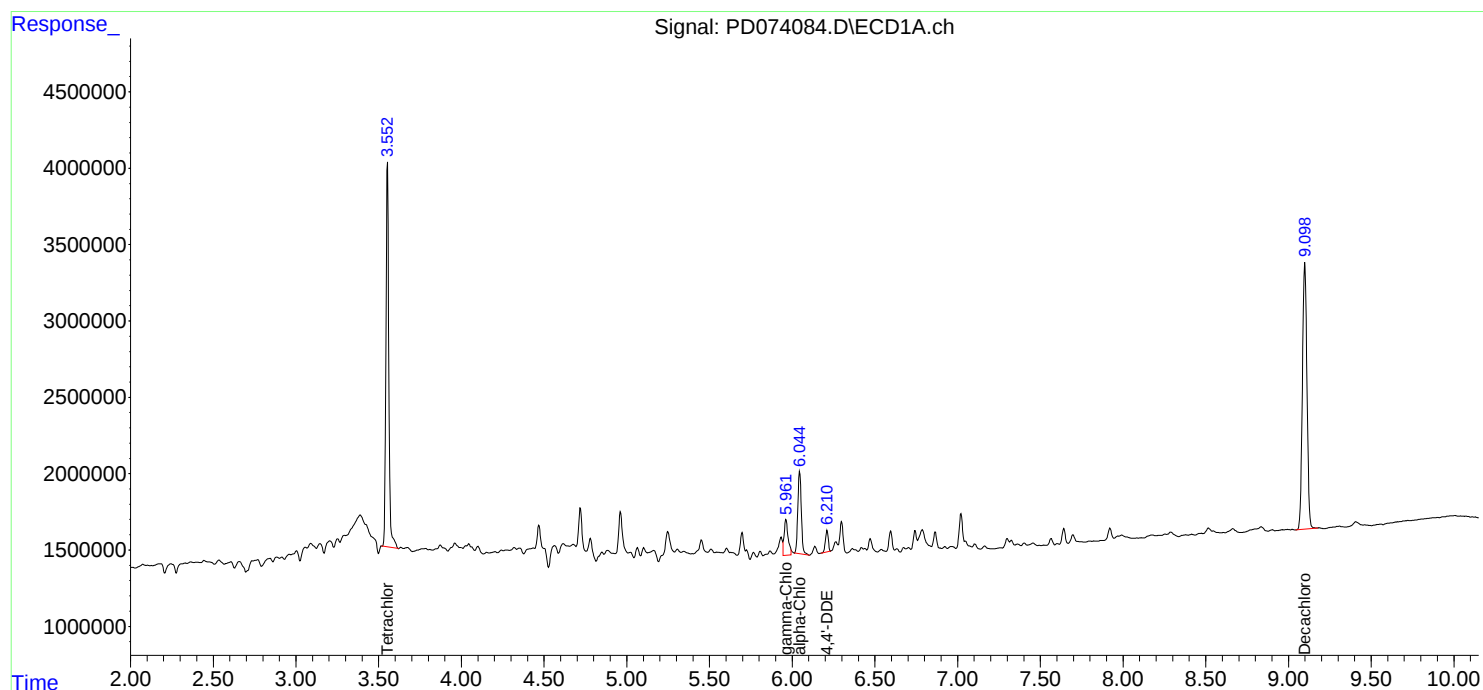


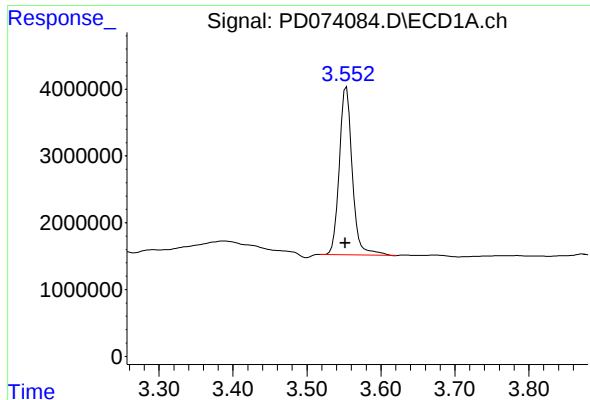

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.001 min
Response: 30473567
Conc: 13.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

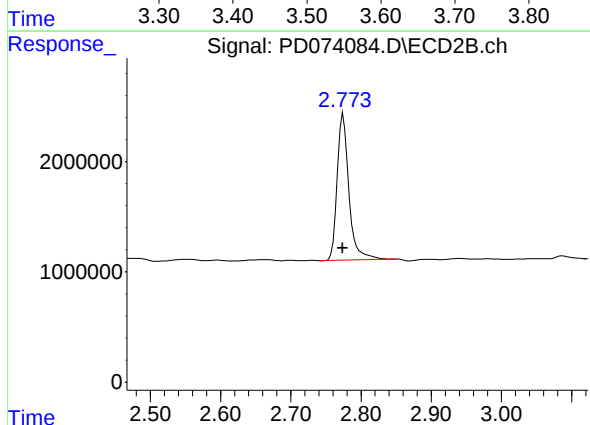


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 15419470
Conc: 13.02 ng/ml

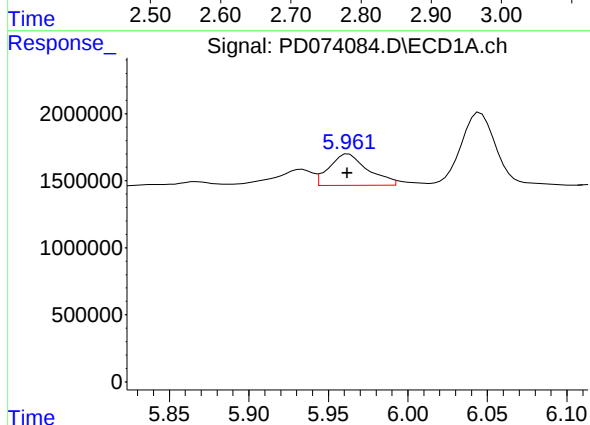


#10 gamma-Chlordane

R.T.: 5.961 min
Delta R.T.: 0.000 min
Response: 3859817
Conc: 1.26 ng/ml m

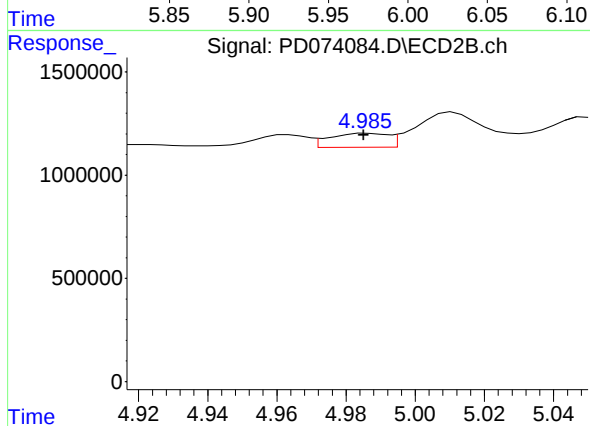

#10 gamma-Chlordane


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 827450
Conc: 0.54 ng/ml m

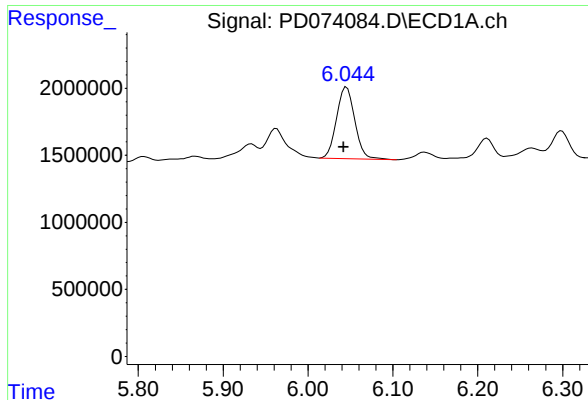

#11 alpha-Chlordane


R.T.: 6.045 min
Delta R.T.: 0.003 min
Response: 7995263
Conc: 2.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

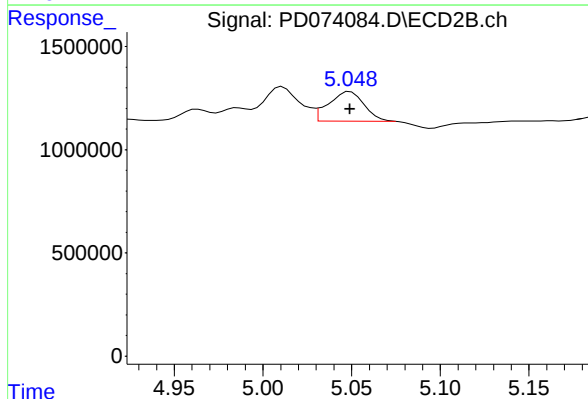


#11 alpha-Chlordane

R.T.: 5.048 min
Delta R.T.: -0.001 min
Response: 1938121
Conc: 1.29 ng/ml

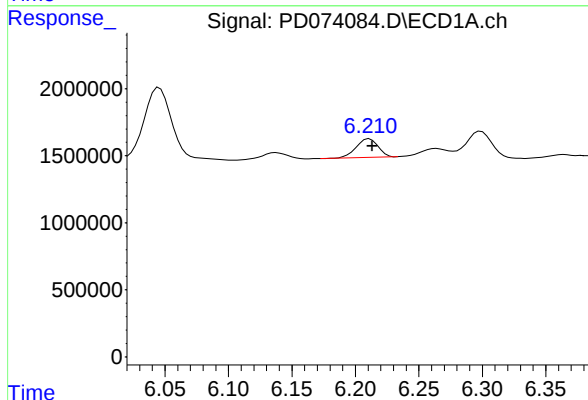


#12 4,4'-DDE

R.T.: 6.211 min
Delta R.T.: -0.002 min
Response: 1682332
Conc: 0.59 ng/ml

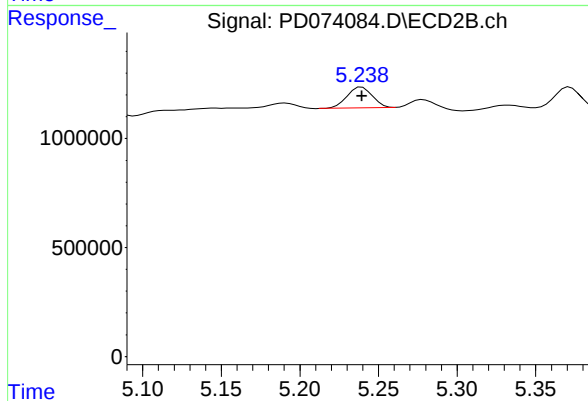

#12 4,4'-DDE


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 1071125
Conc: 0.77 ng/ml

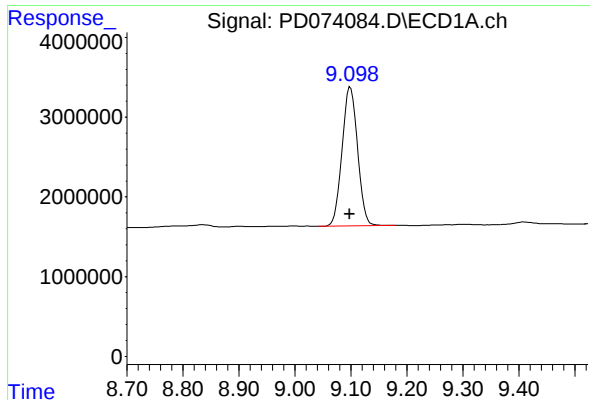

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.001 min
Response: 33476422
Conc: 12.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

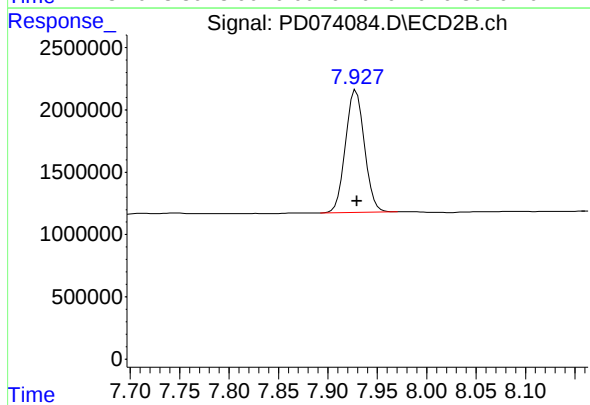

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: 0.000 min
Response: 13155252
Conc: 10.74 ng/ml