

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030322\
 Data File : PD068281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2022 11:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/03/2022
 Supervised By : Ankita Jodhani 03/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 00:27:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.457	4.177	25110110	213.1E6	21.420m	22.201
28) SA Decachlor...	8.227	9.378	26421403	133.2E6	22.704	22.473

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030322\
Data File : PD068281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2022 11:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/03/2022
Supervised By :Ankita Jodhani 03/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 00:27:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

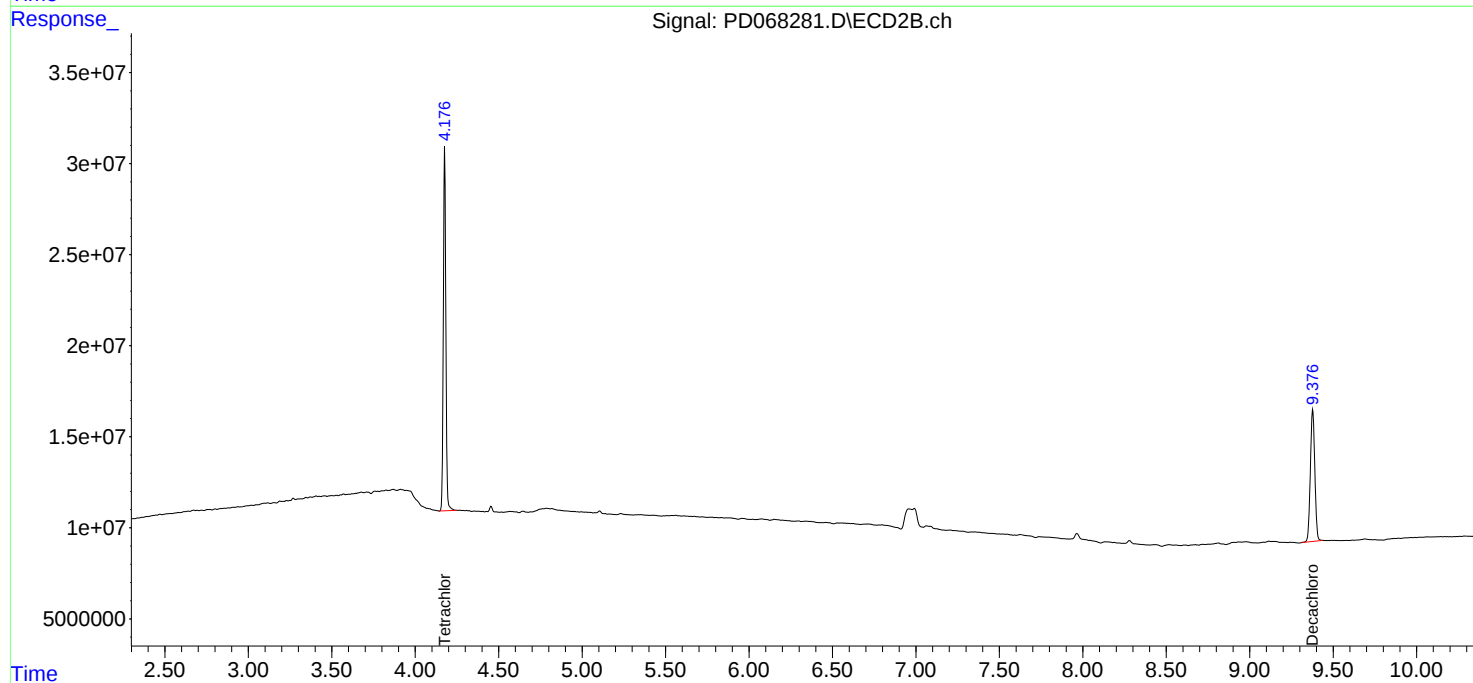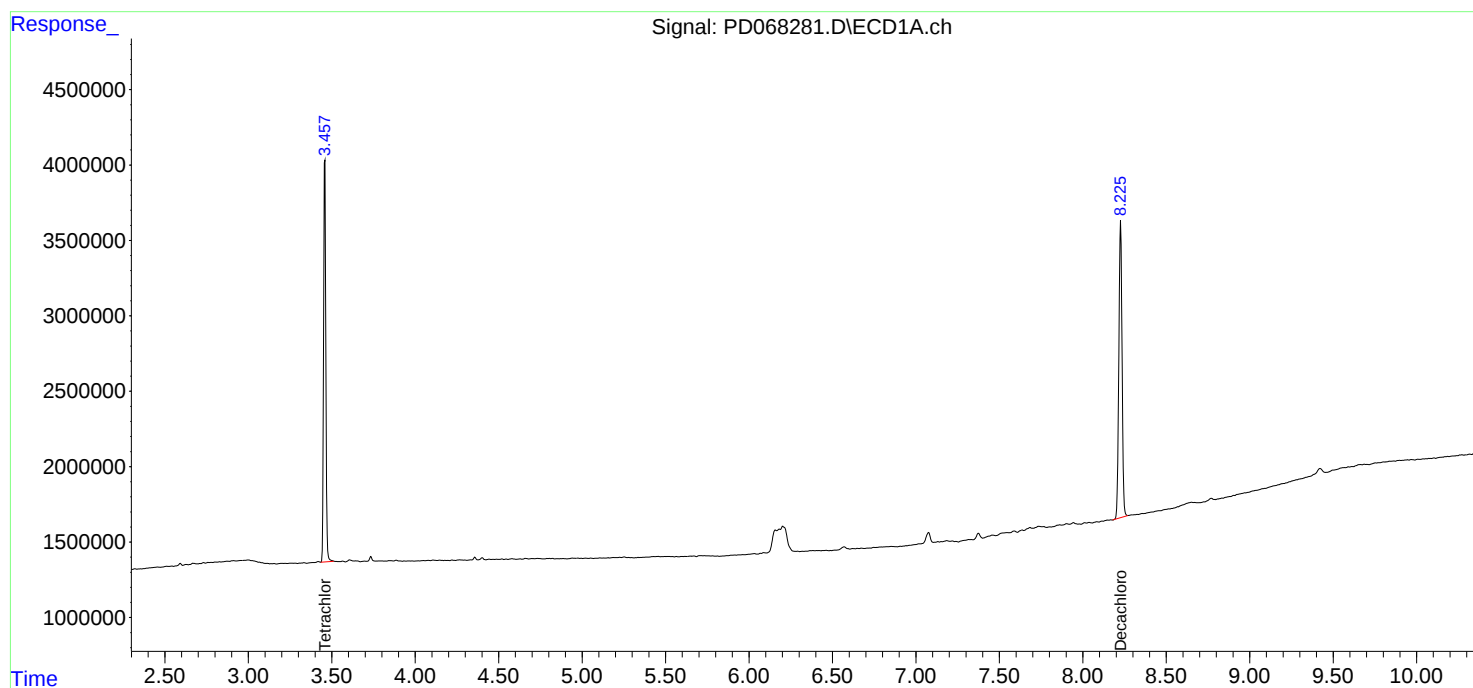

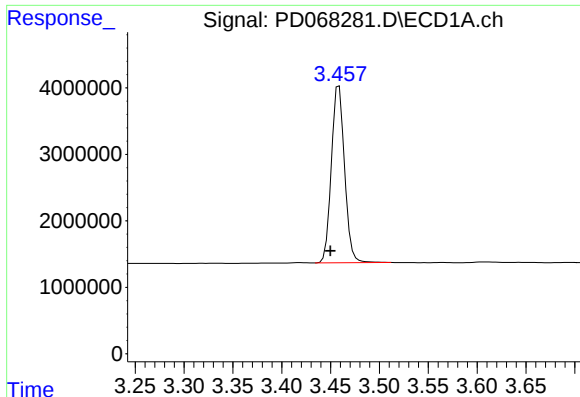

#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: 0.007 min
Response: 25110110
Conc: 21.42 ng/ml

Instrument :


ECD_D

ClientSampleId :

I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/03/2022
Supervised By :Ankita Jodhani 03/03/2022

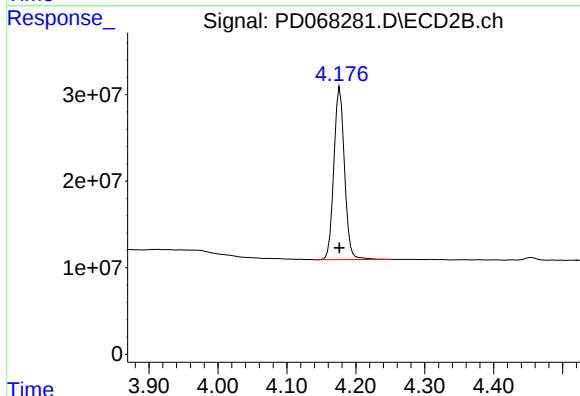


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 213085906
Conc: 22.20 ng/ml

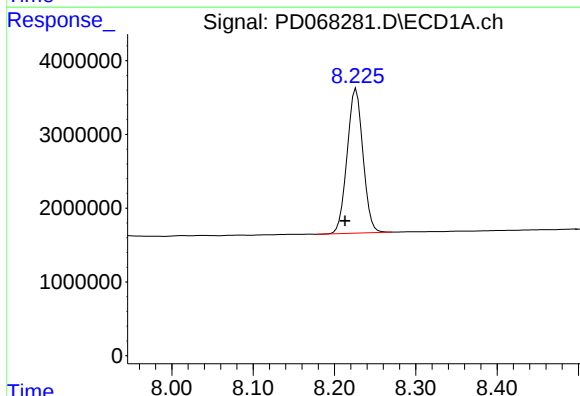

#28 Decachlorobiphenyl

R.T.: 8.227 min
Delta R.T.: 0.014 min
Response: 26421403
Conc: 22.70 ng/ml

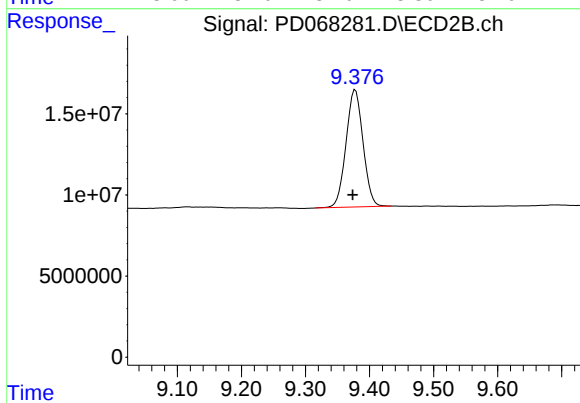

#28 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: 0.004 min
Response: 133239437
Conc: 22.47 ng/ml