

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051556.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 10:11
 Operator : AJ\SJ
 Sample : K1606-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5C6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:33:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	24380875	540.9E6	16.966	17.508
27)	SA Decachlor...	7.826	9.159	40877256	598.3E6	33.990	31.558
Target Compounds							
8)	B Heptachlo...	0.000	5.919	0 19922824	N.D.	0.556	
9)	A Endosulfan I	0.000	6.242f	0 17934947	N.D.	0.541	
11)	B cis-Chlor...	0.000	6.242	0 17934947	N.D.	0.518	
15)	B Endosulfa...	0.000	6.983	0 17966882	N.D.	0.655	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051556.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 10:11
Operator : AJ\SJ
Sample : K1606-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:33:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

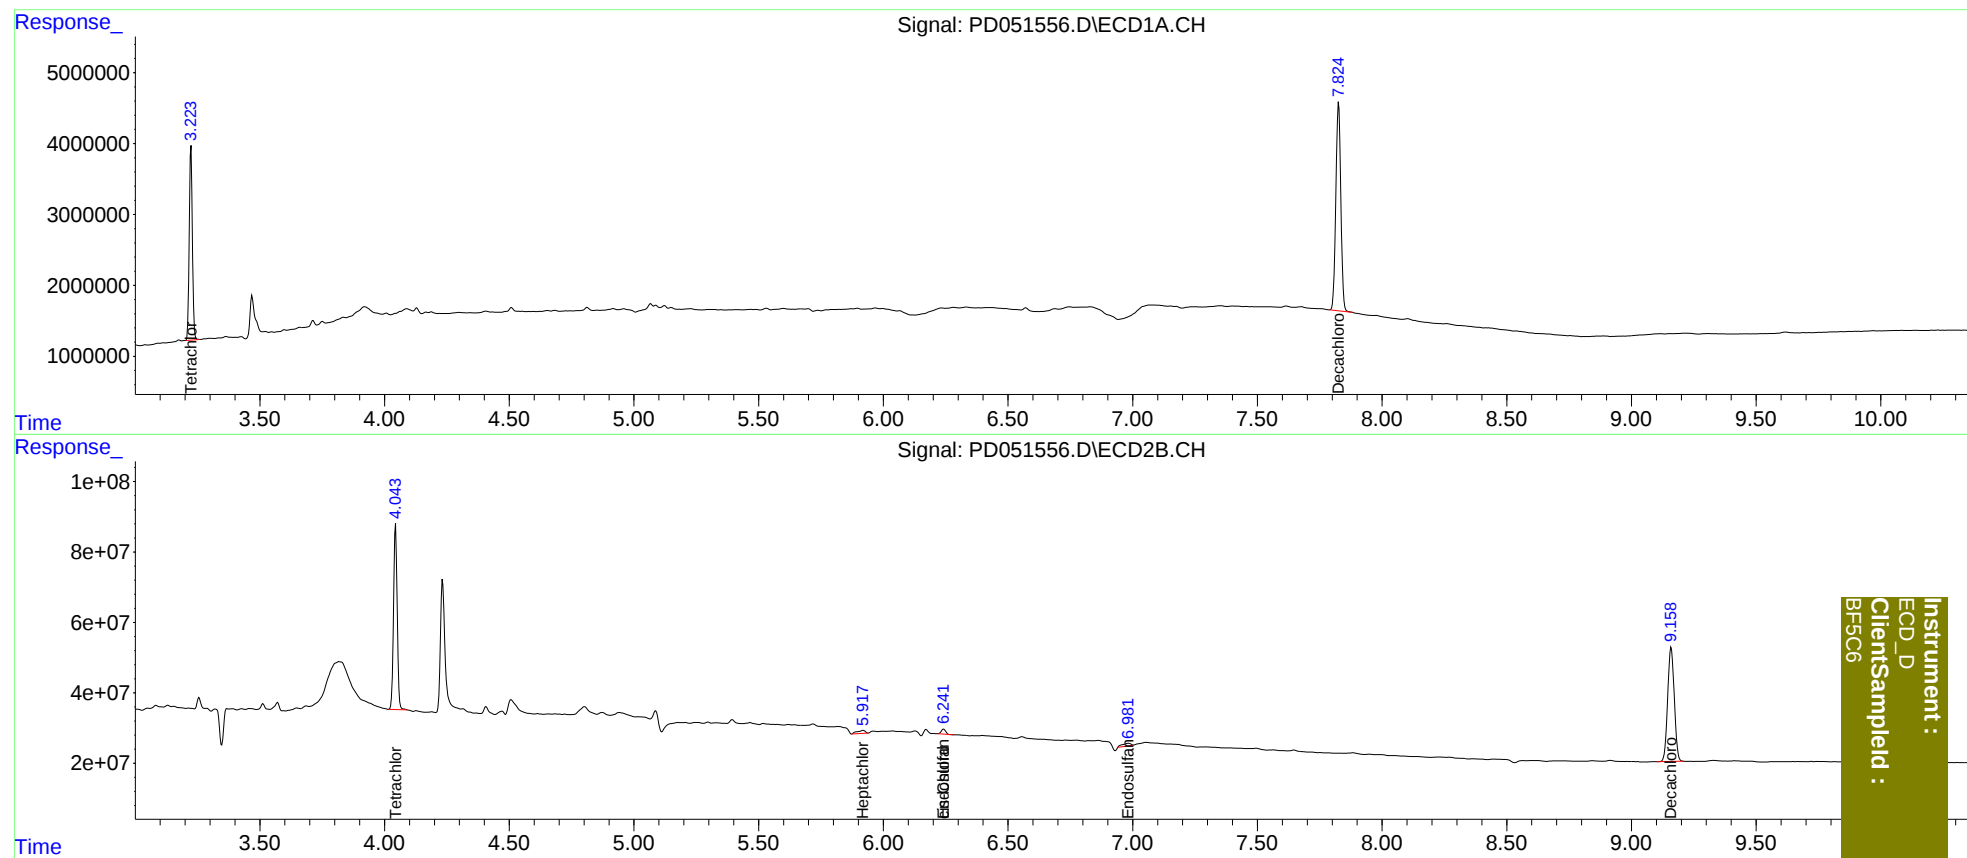


Instrument :
ECD_D
ClientSampleId :
BF5C6

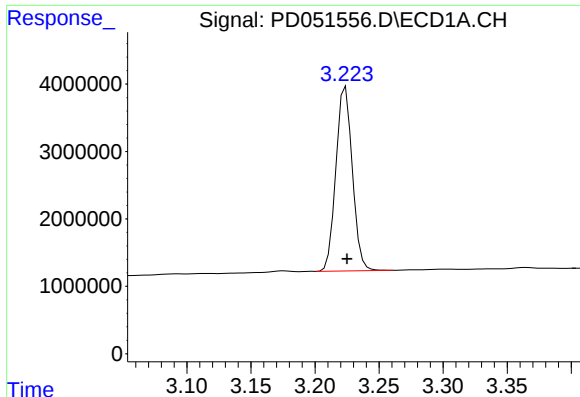

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 24380875
Conc: 16.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5C6

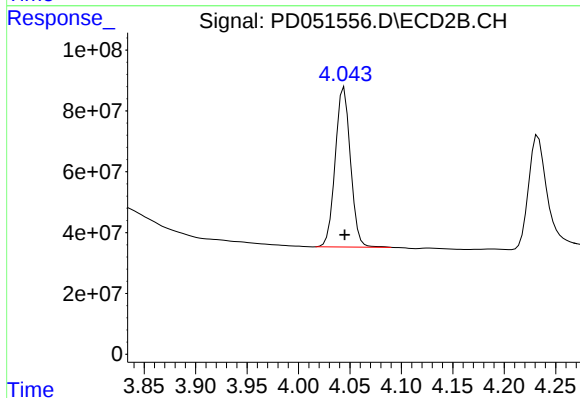


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 540938334
Conc: 17.51 ng/ml

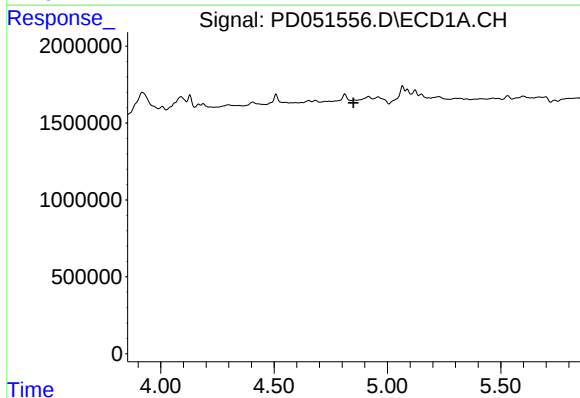


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

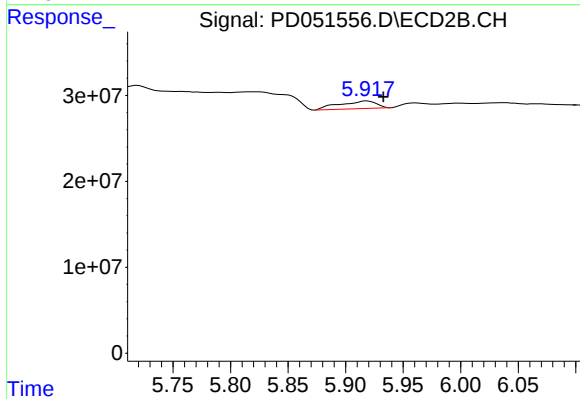

#8 Heptachlor epoxide


R.T.: 5.919 min
Delta R.T.: -0.014 min
Response: 19922824
Conc: 0.56 ng/ml

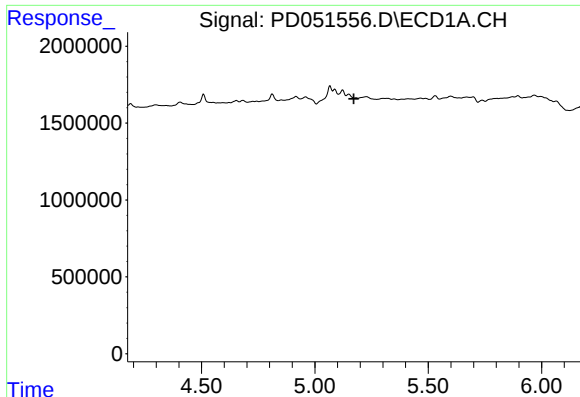

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5C6

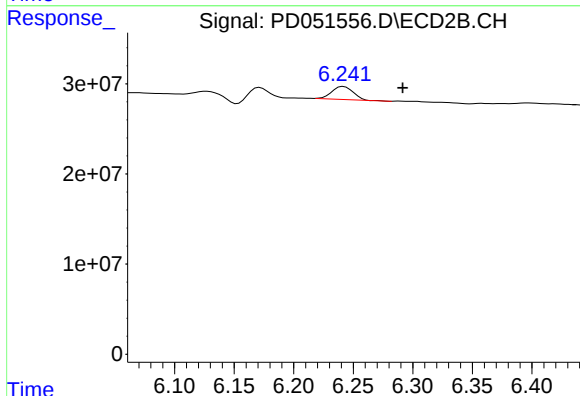


#9 Endosulfan I

R.T.: 6.242 min
Delta R.T.: -0.050 min
Response: 17934947
Conc: 0.54 ng/ml

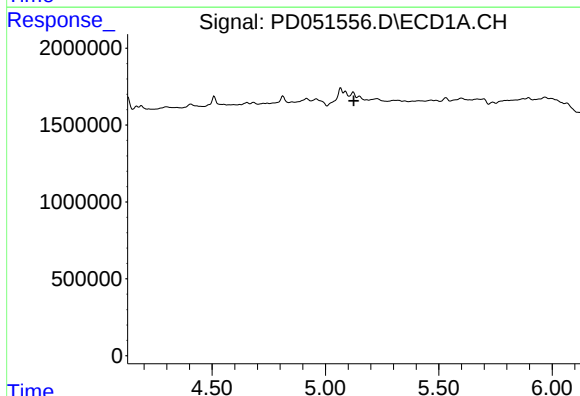


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.125 min
Response: 0
Conc: N.D.

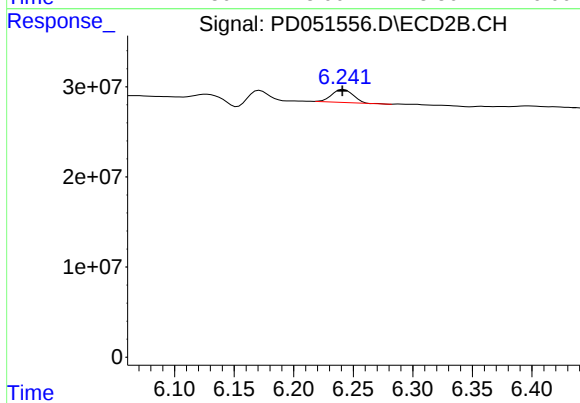

#11 cis-Chlordane


R.T.: 6.242 min
Delta R.T.: 0.001 min
Response: 17934947
Conc: 0.52 ng/ml

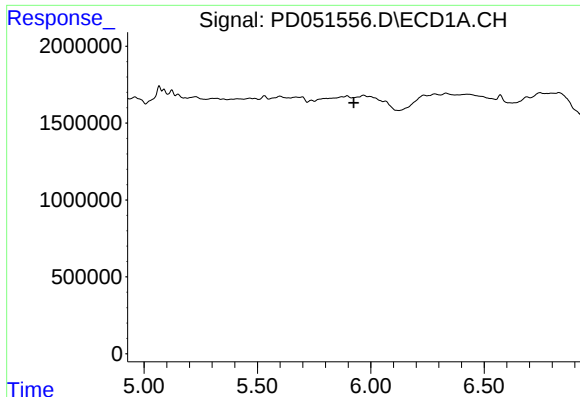

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5C6

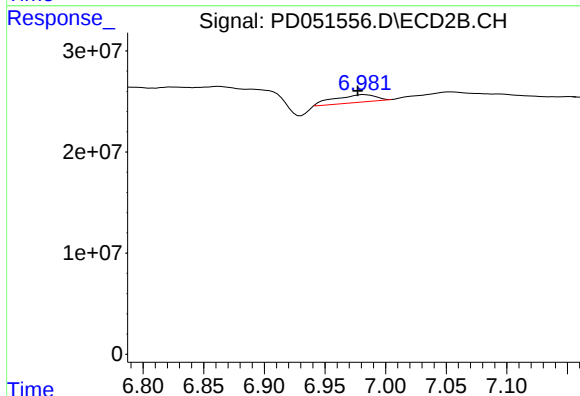


#15 Endosulfan II

R.T.: 6.983 min
Delta R.T.: 0.006 min
Response: 17966882
Conc: 0.65 ng/ml

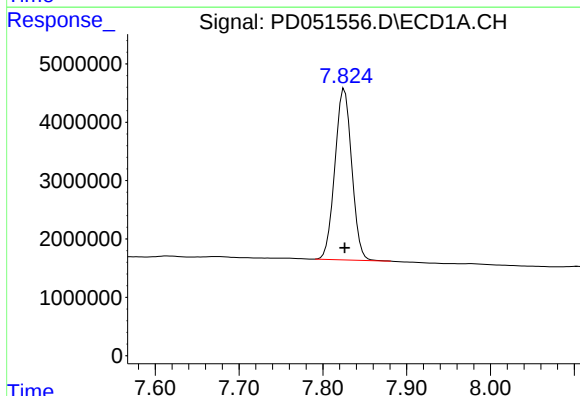

#27 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 40877256
Conc: 33.99 ng/ml

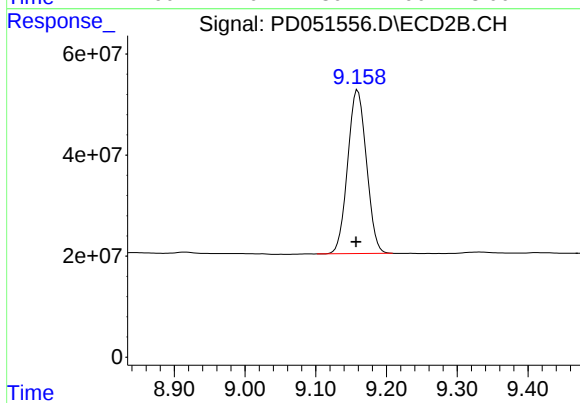

#27 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 598257200
Conc: 31.56 ng/ml