

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051560.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 11:07
 Operator : AJ\SJ
 Sample : K1606-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5C9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:34:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	16895934	374.2E6	11.758	12.112
27)	SA Decachlor...	7.826	9.159	28380261	418.4E6	23.598	22.071
Target Compounds							
6)	B beta-BHC	0.000	4.940f	0	22959797	N.D.	1.157
8)	B Heptachlo...	0.000	5.918	0	27475886	N.D.	0.767
10)	B trans-Chl...	0.000	6.176	0	21820663	N.D.	0.604
11)	B cis-Chlor...	0.000	6.176f	0	21820663	N.D.	0.630
15)	B Endosulfa...	0.000	6.989	0	17365648	N.D.	0.633


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 11:07
Operator : AJ\SJ
Sample : K1606-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:34:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

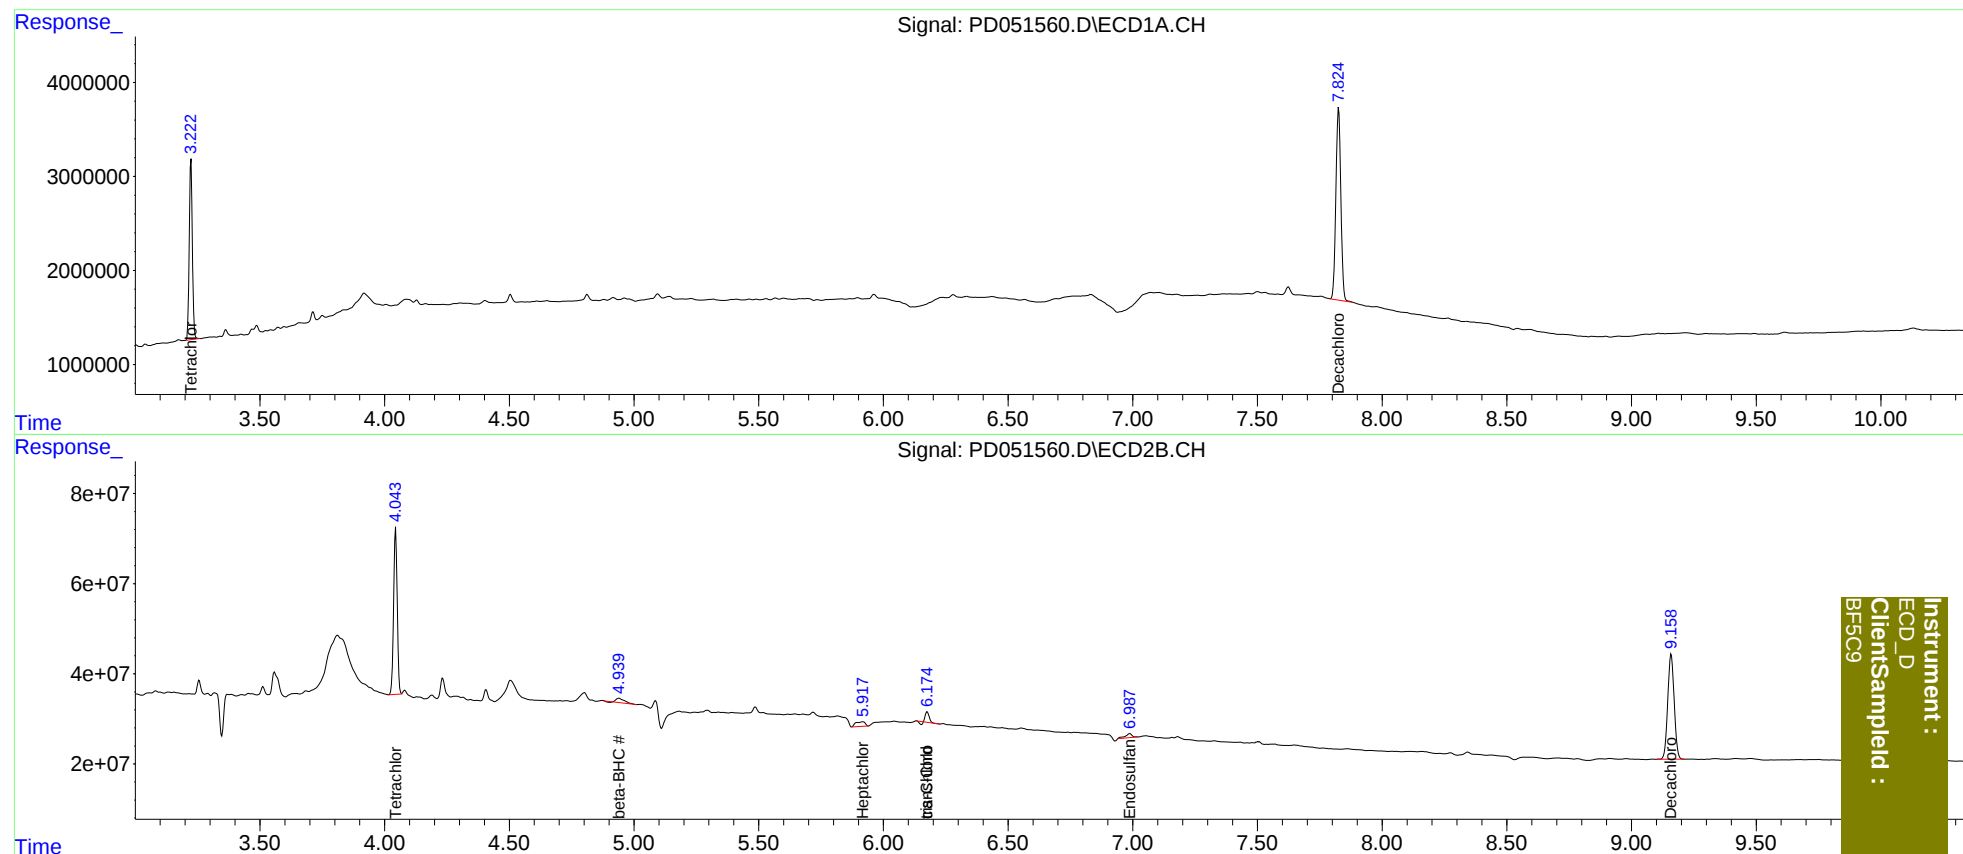


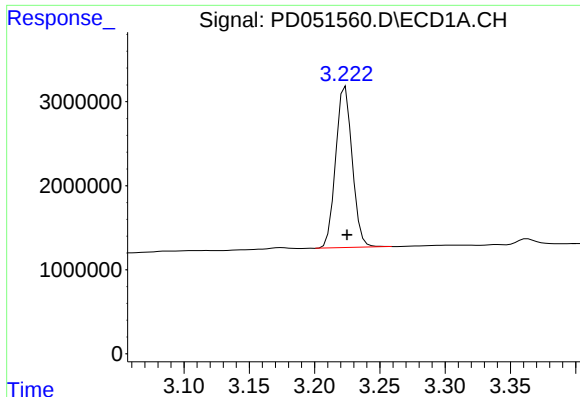

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 16895934
Conc: 11.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5C9

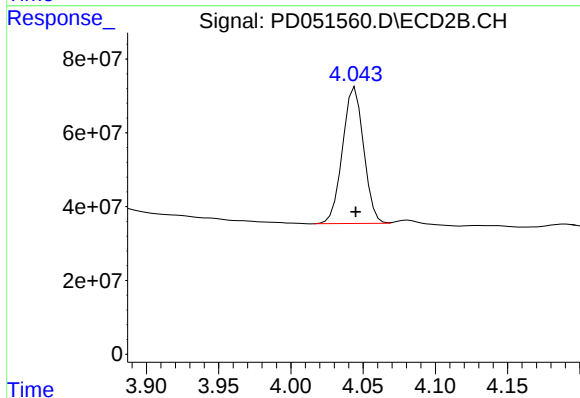


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 374216968
Conc: 12.11 ng/ml

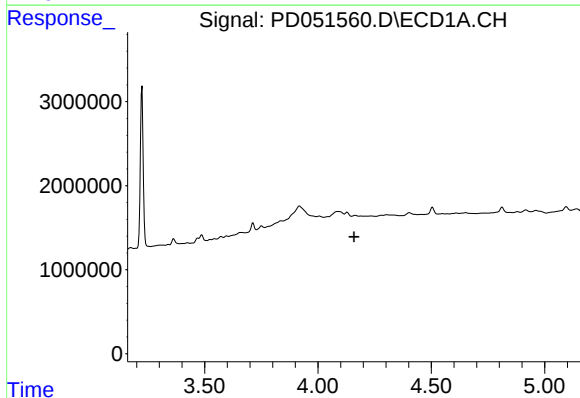


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

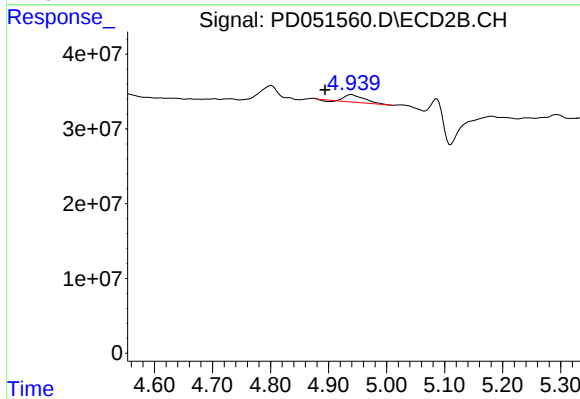

#6 beta-BHC


R.T.: 4.940 min
Delta R.T.: 0.046 min
Response: 22959797
Conc: 1.16 ng/ml

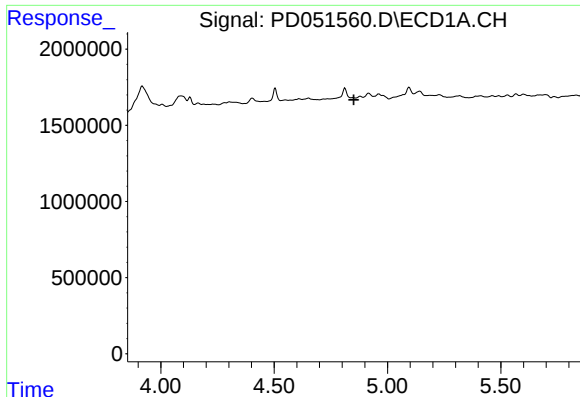

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5C9

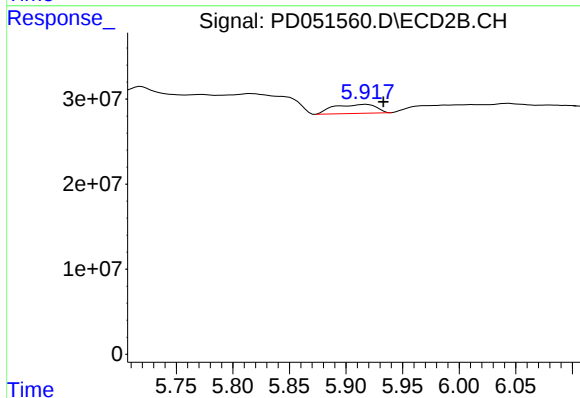


#8 Heptachlor epoxide

R.T.: 5.918 min
Delta R.T.: -0.015 min
Response: 27475886
Conc: 0.77 ng/ml

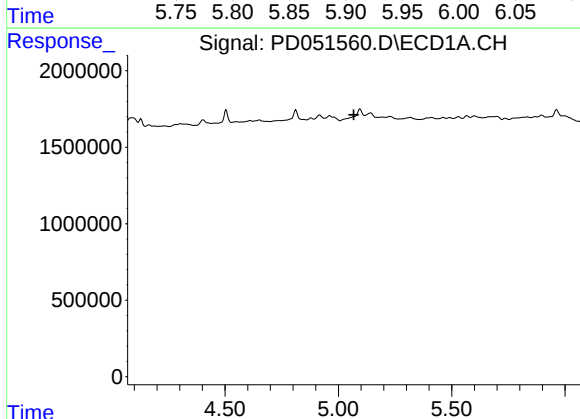


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

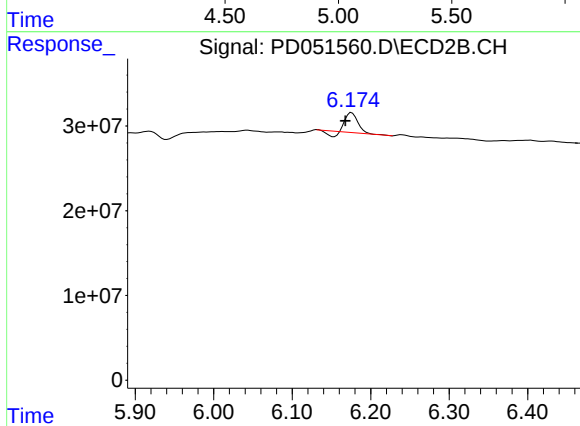

#10 trans-Chlordane


R.T.: 6.176 min
Delta R.T.: 0.008 min
Response: 21820663
Conc: 0.60 ng/ml

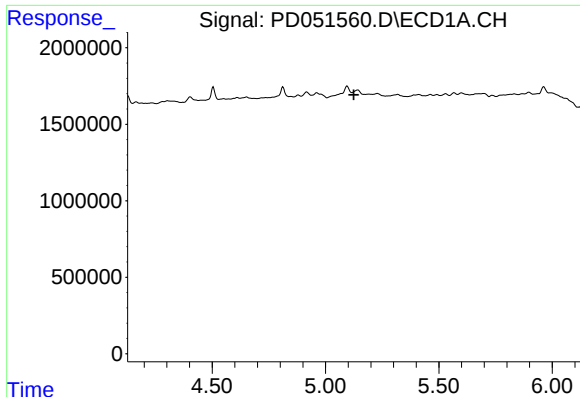

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5C9

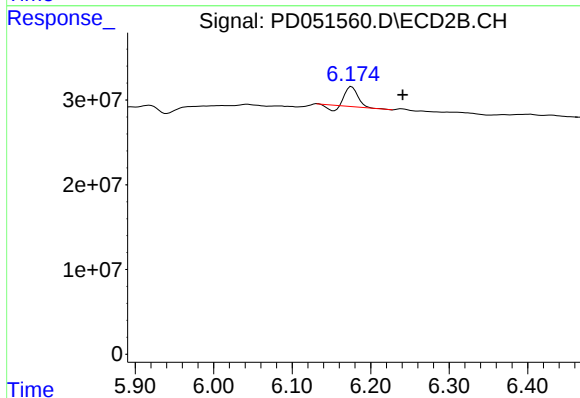


#11 cis-Chlordane

R.T.: 6.176 min
Delta R.T.: -0.065 min
Response: 21820663
Conc: 0.63 ng/ml

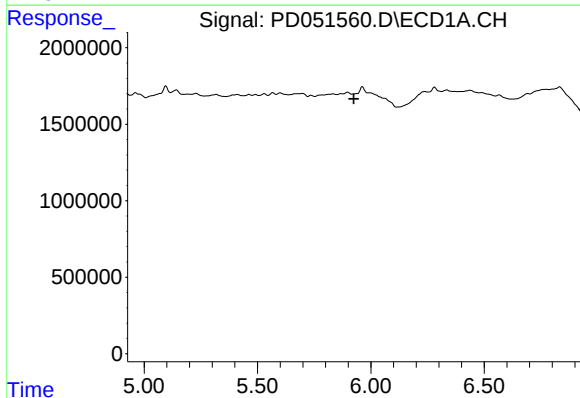


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

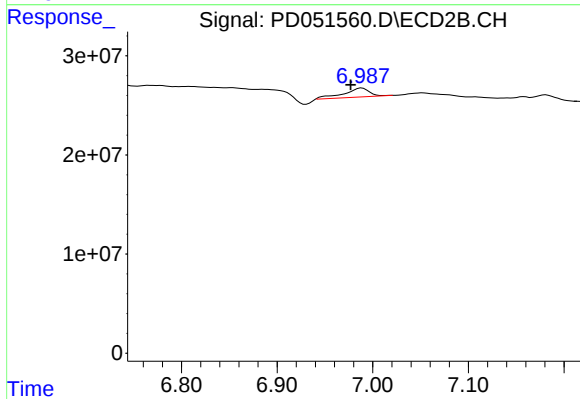

#15 Endosulfan II


R.T.: 6.989 min
Delta R.T.: 0.012 min
Response: 17365648
Conc: 0.63 ng/ml

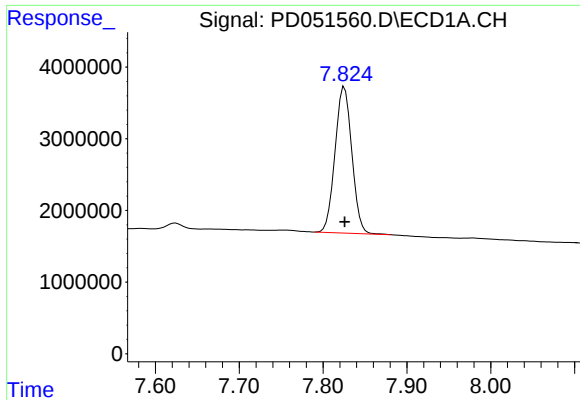

#27 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 28380261
Conc: 23.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5C9

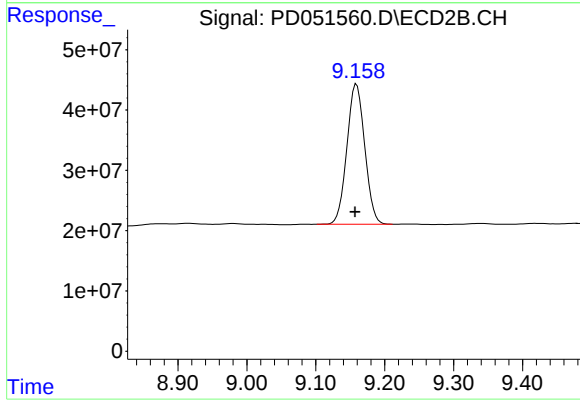

#27 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 418411170
Conc: 22.07 ng/ml