

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051562.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 11:35
 Operator : AJ\SJ
 Sample : PB117543BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK43

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:34:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.224	4.045	27309797	600.4E6	19.004	19.433
2) SA Decachlor...	7.826	9.160	47784381	694.2E6	39.733	36.620
Target Compounds						
6) B beta-BHC	0.000	4.936f	0 50515879	N.D.	2.546	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 11:35
Operator : AJ\SJ
Sample : PB117543BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:34:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

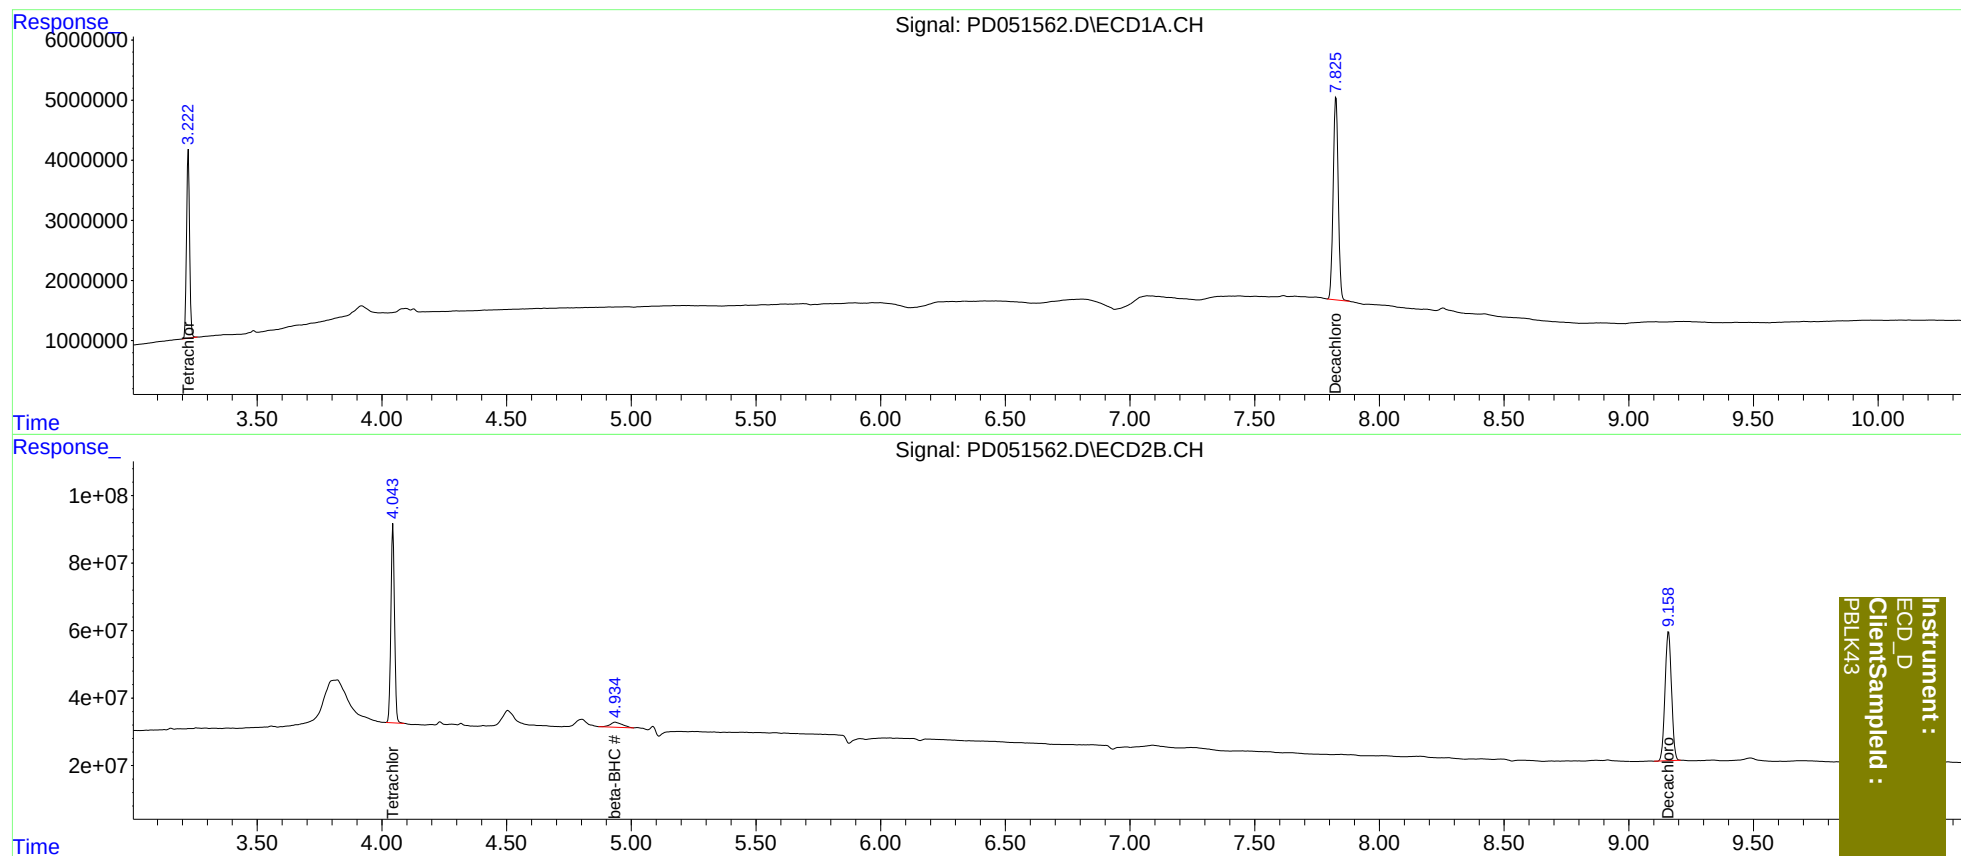


Instrument :
ECD_D
ClientSampleId :
PBLK43

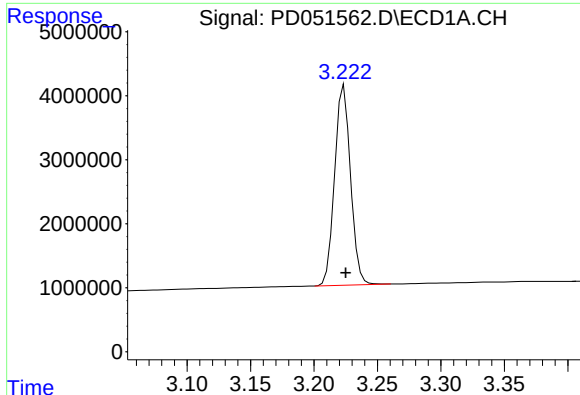

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 27309797
Conc: 19.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK43

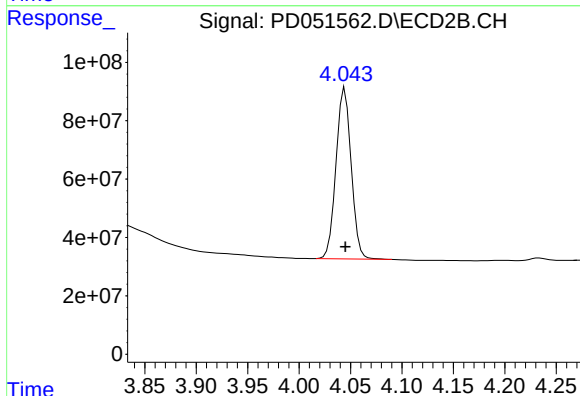


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 600407726
Conc: 19.43 ng/ml

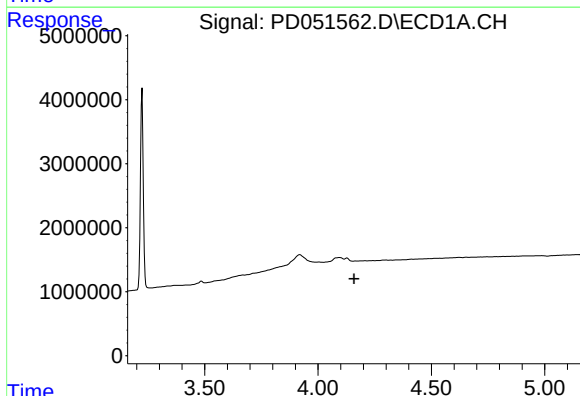


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

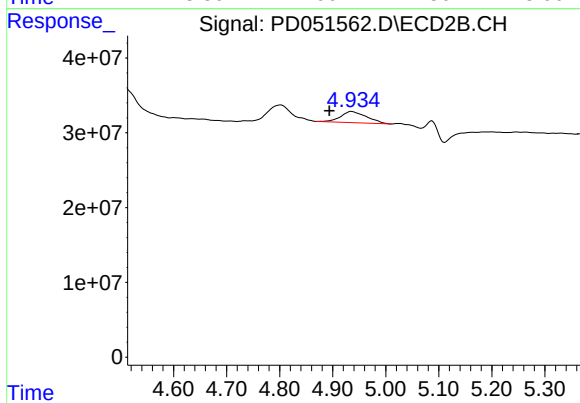

#6 beta-BHC


R.T.: 4.936 min
Delta R.T.: 0.042 min
Response: 50515879
Conc: 2.55 ng/ml

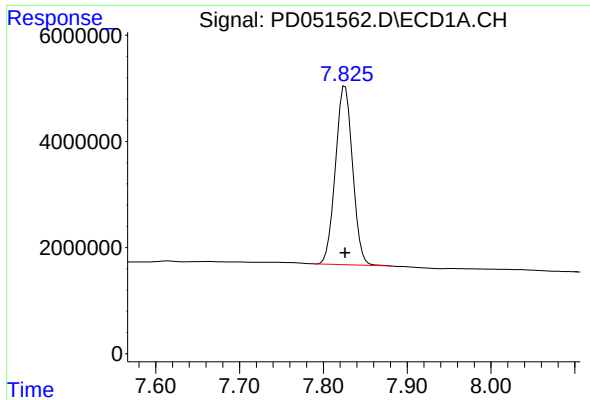

#27 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 47784381
Conc: 39.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK43

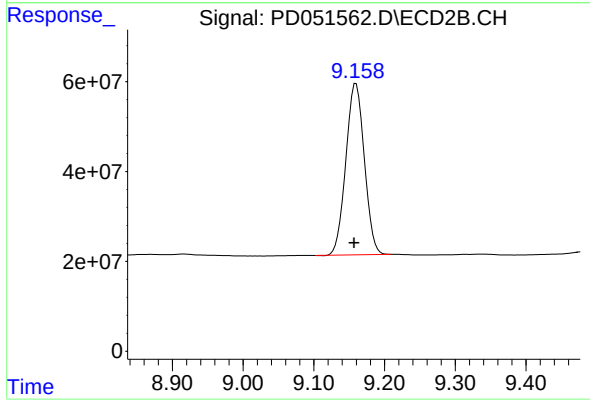

#27 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: 0.002 min
Response: 694214482
Conc: 36.62 ng/ml