

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051570.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 13:27
 Operator : AJ\SJ
 Sample : K1622-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF5J0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:35:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	22470985	486.8E6	15.637	15.755
27)	SA Decachlor...	7.825	9.159	27475250	415.5E6	22.846	21.919
Target Compounds							
6)	B beta-BHC	0.000	4.942f	0 25907975	N.D.	1.306	
8)	B Heptachlo...	0.000	5.919	0 46499467	N.D.	1.299	
15)	B Endosulfa...	0.000	6.986	0 15434393	N.D.	0.562	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 13:27
Operator : AJ\SJ
Sample : K1622-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:35:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

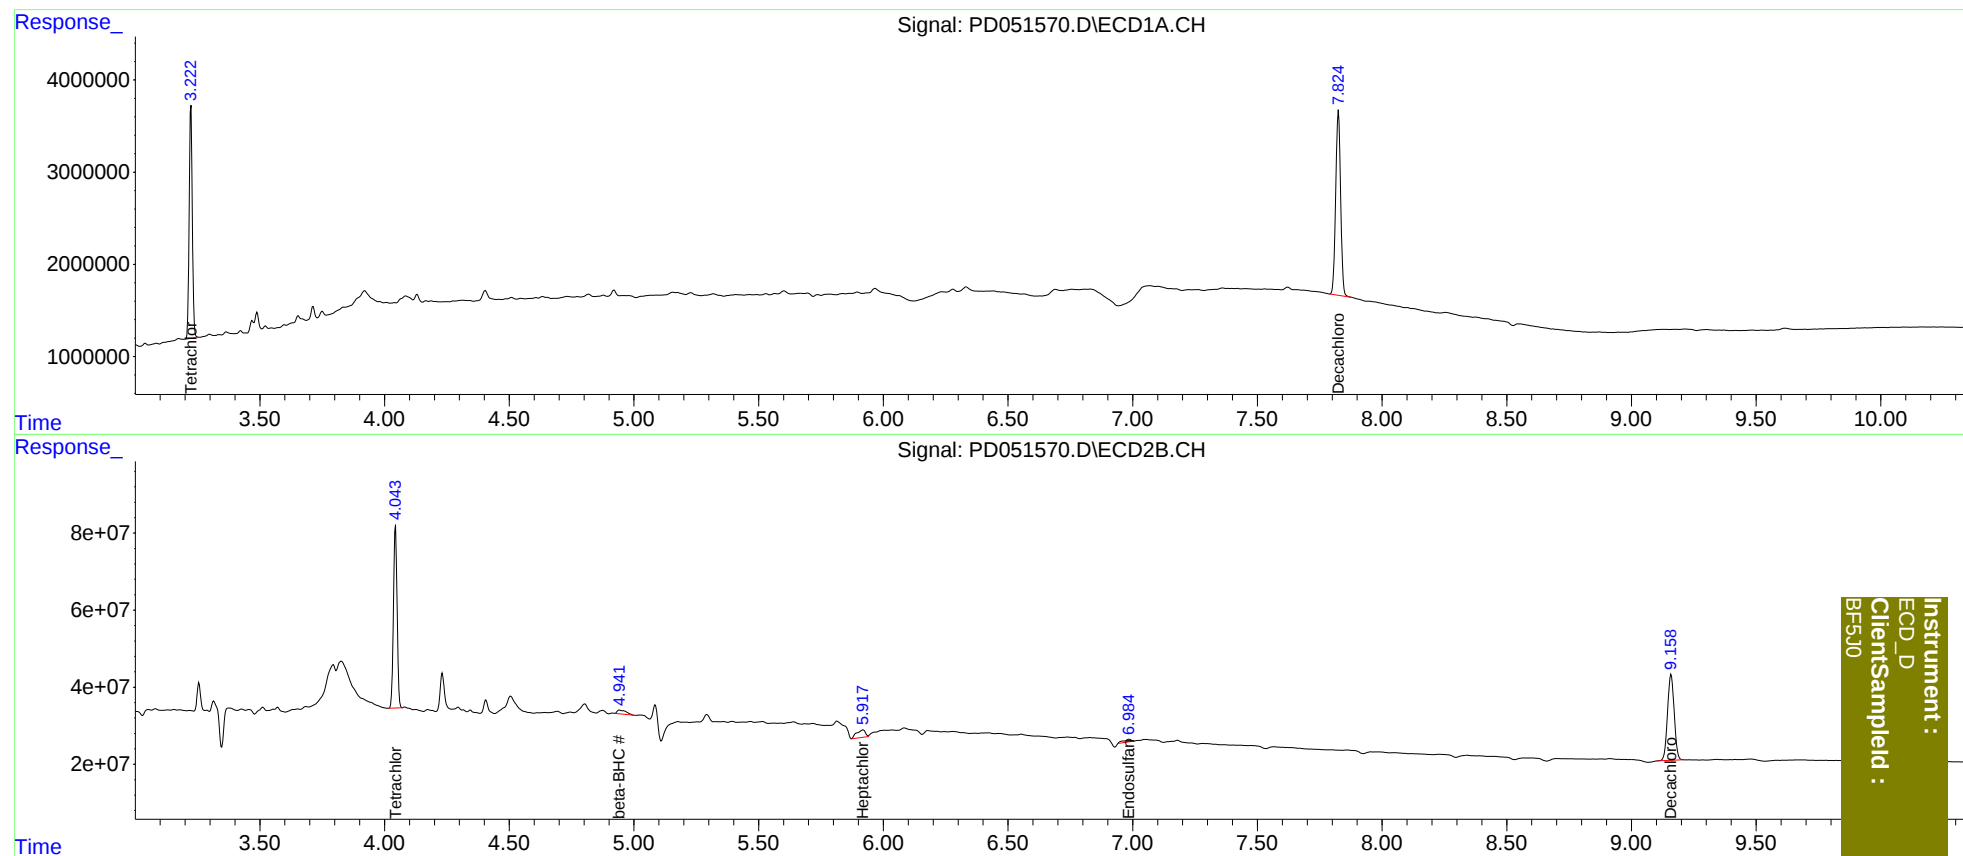


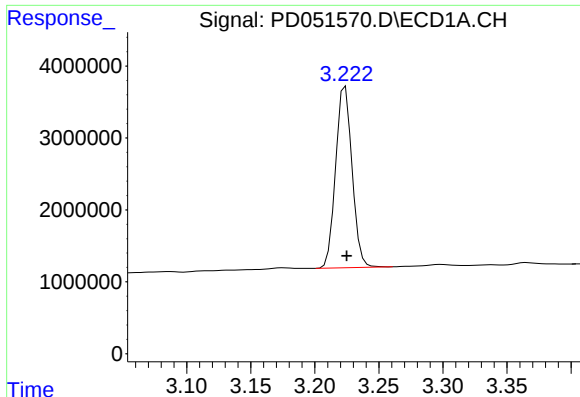

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 22470985
Conc: 15.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5J0

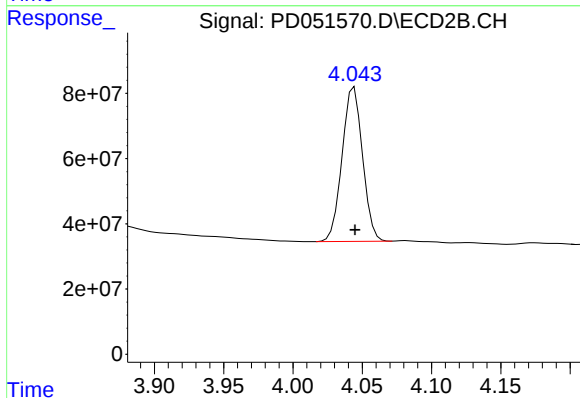


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 486759735
Conc: 15.75 ng/ml

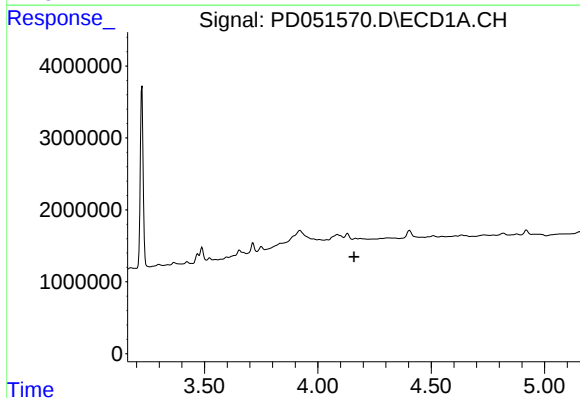


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

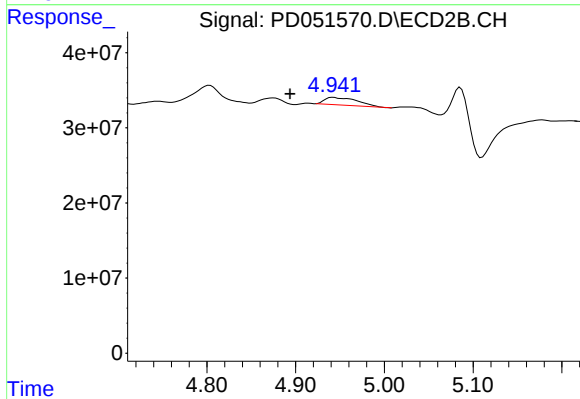

#6 beta-BHC


R.T.: 4.942 min
Delta R.T.: 0.048 min
Response: 25907975
Conc: 1.31 ng/ml

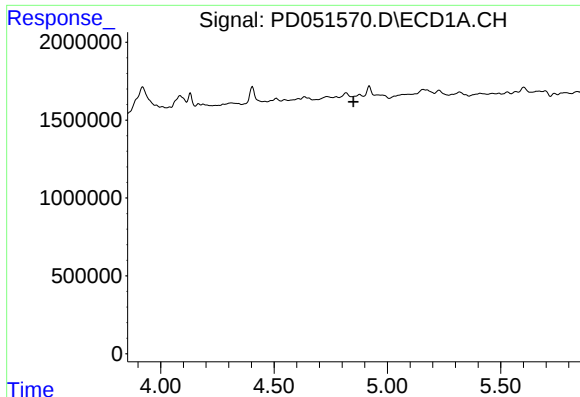

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF5J0

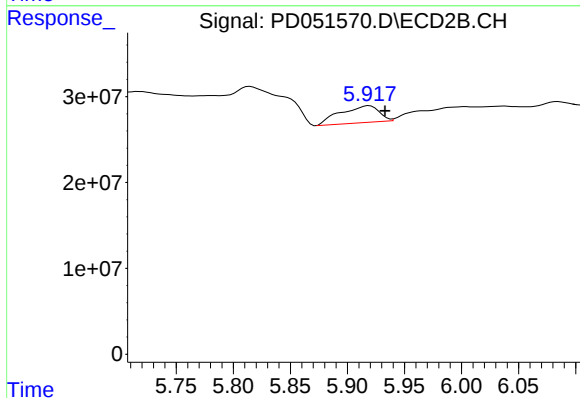


#8 Heptachlor epoxide

R.T.: 5.919 min
Delta R.T.: -0.014 min
Response: 46499467
Conc: 1.30 ng/ml

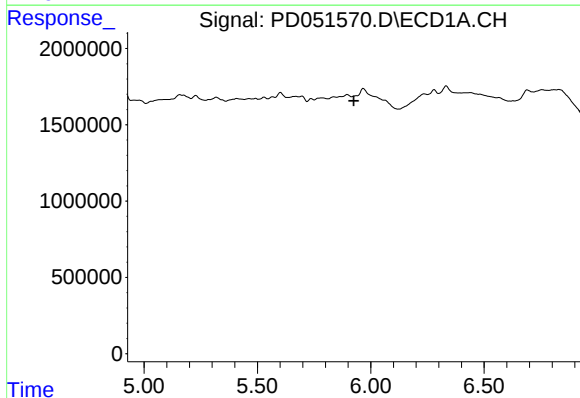


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

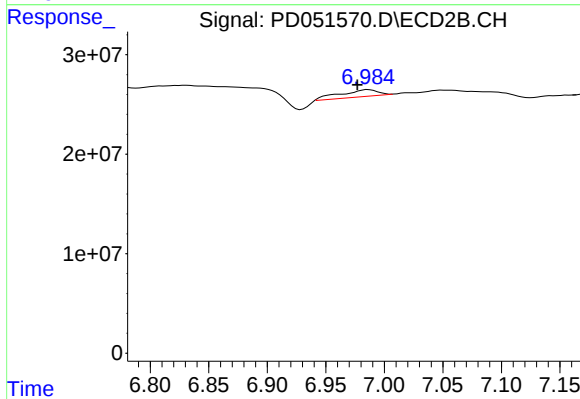

#15 Endosulfan II


R.T.: 6.986 min
Delta R.T.: 0.009 min
Response: 15434393
Conc: 0.56 ng/ml

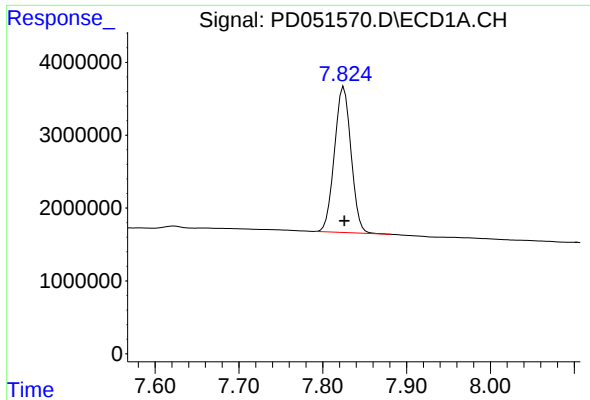

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 27475250
Conc: 22.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF5J0

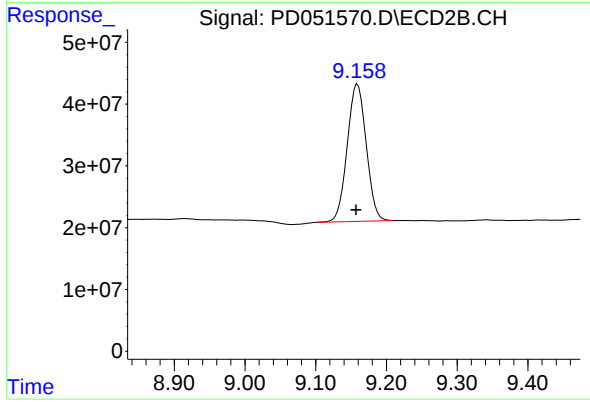

#27 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 415528970
Conc: 21.92 ng/ml