

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051575.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 15:19
 Operator : AJ\SJ
 Sample : K1661-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFC74

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:36:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.224	4.044	28305908	597.3E6	19.698	19.332
27) SA Decachlor...	7.825	9.159	45925071	633.0E6	38.187	33.391
Target Compounds						
6) B beta-BHC	0.000	4.935f	0	40454609	N.D.	2.039
8) B Heptachlo...	0.000	5.919	0	24566810	N.D.	0.686
15) B Endosulfa...	0.000	6.985	0	15003048	N.D.	0.547


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051575.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 15:19
Operator : AJ\SJ
Sample : K1661-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:36:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

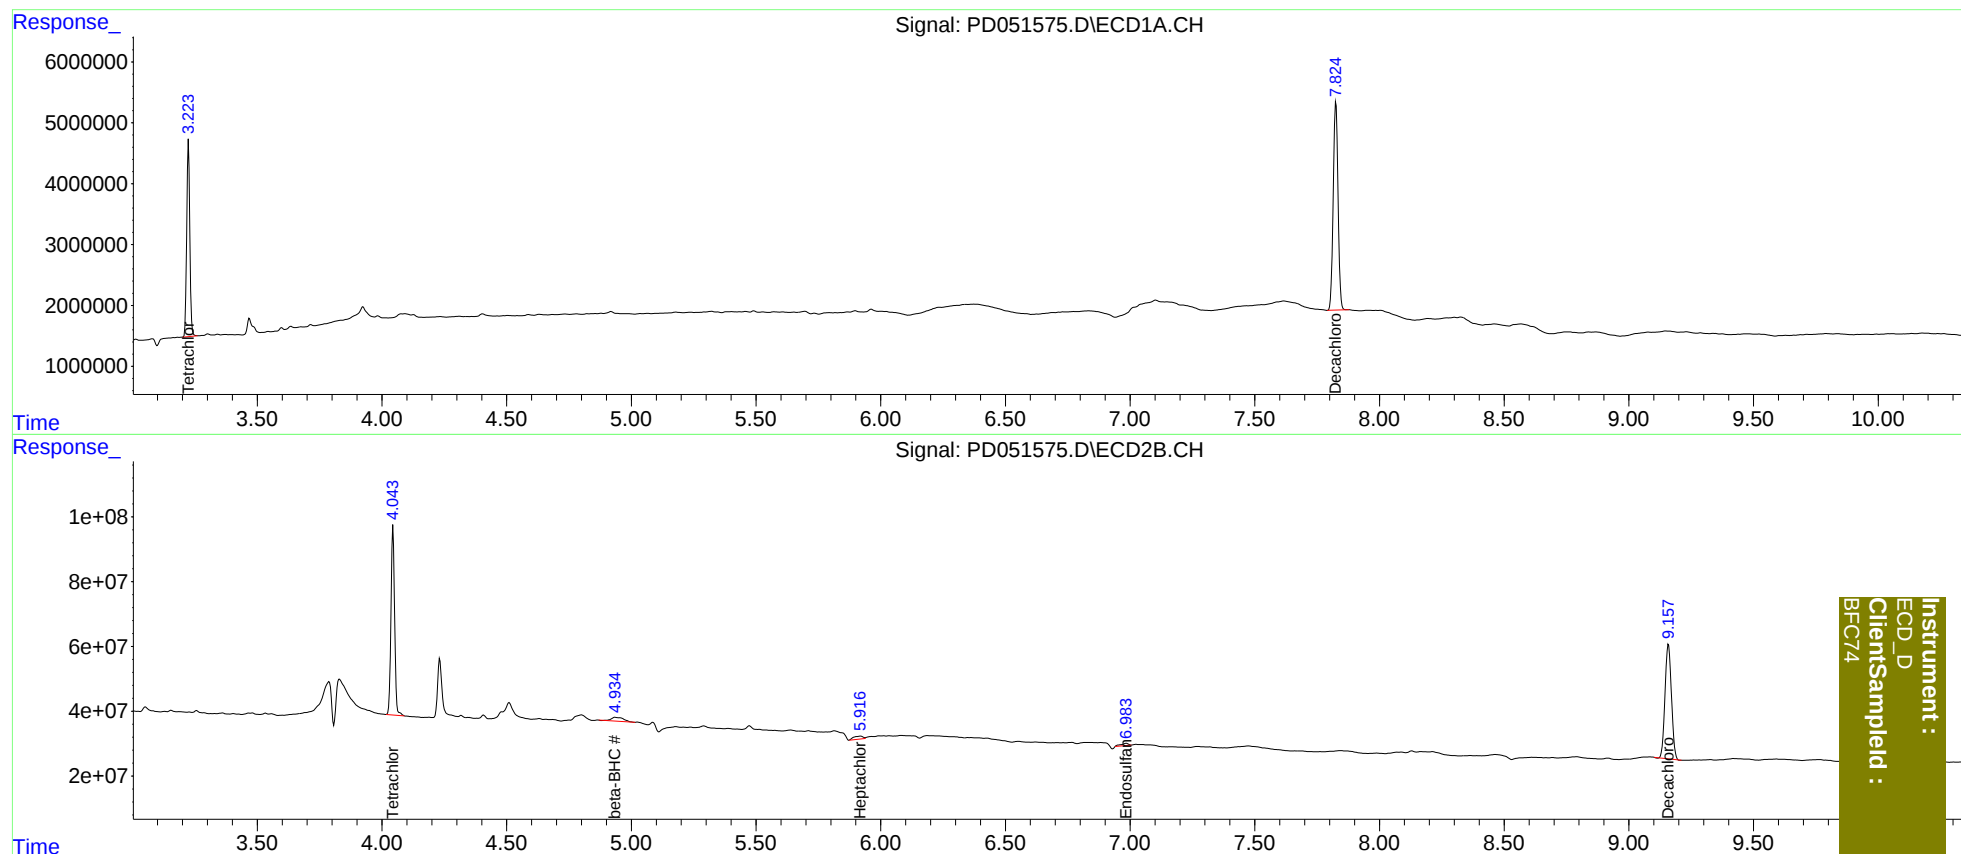


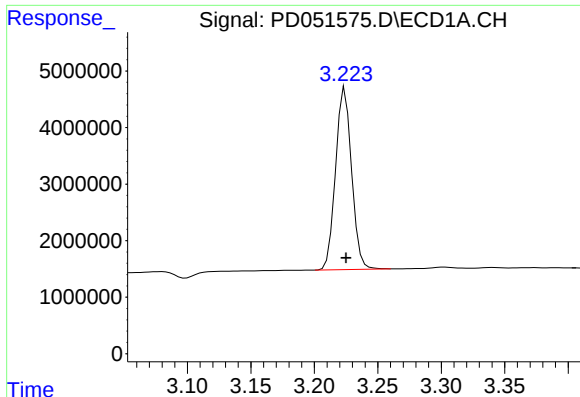

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 28305908
Conc: 19.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC74

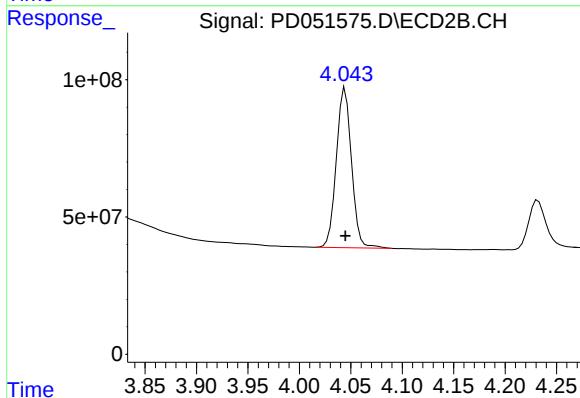


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 597272305
Conc: 19.33 ng/ml

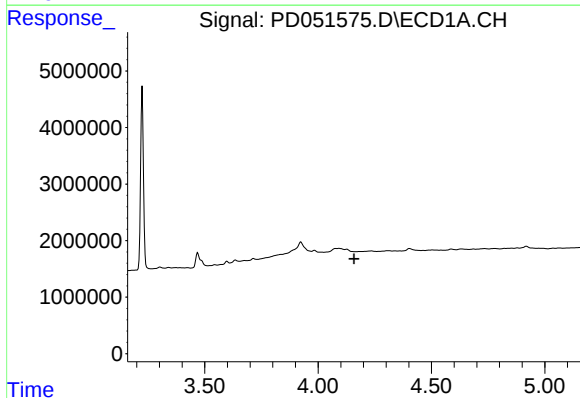


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

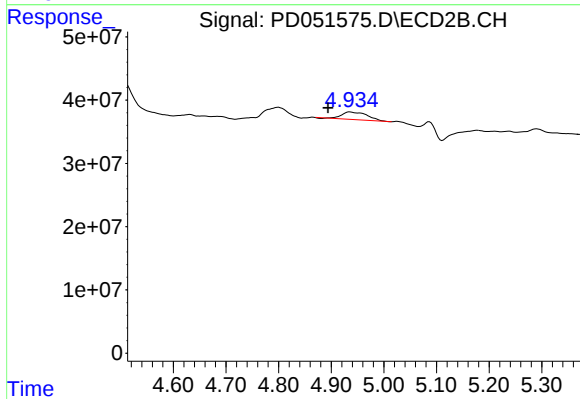

#6 beta-BHC


R.T.: 4.935 min
Delta R.T.: 0.041 min
Response: 40454609
Conc: 2.04 ng/ml

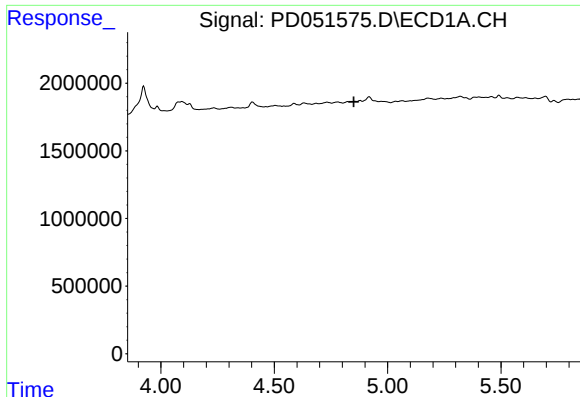

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC74

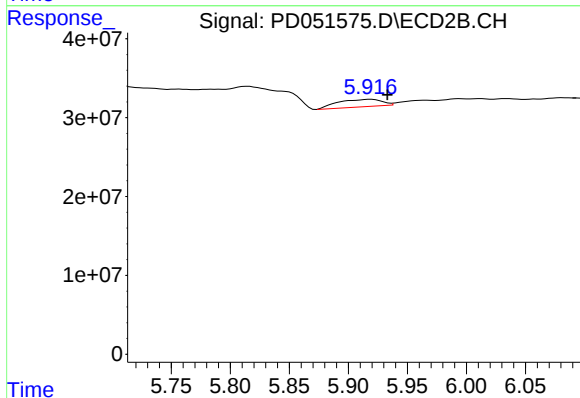


#8 Heptachlor epoxide

R.T.: 5.919 min
Delta R.T.: -0.014 min
Response: 24566810
Conc: 0.69 ng/ml

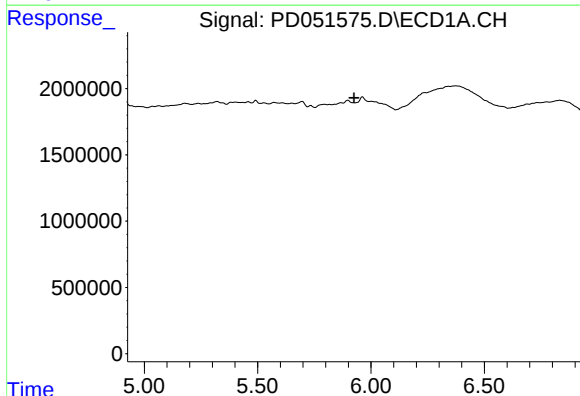


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.925 min
Response: 0
Conc: N.D.

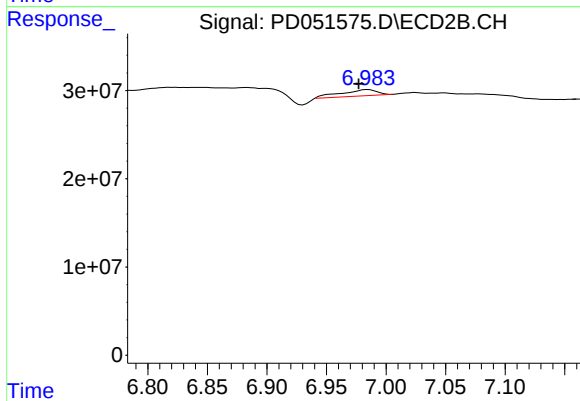

#15 Endosulfan II


R.T.: 6.985 min
Delta R.T.: 0.008 min
Response: 15003048
Conc: 0.55 ng/ml

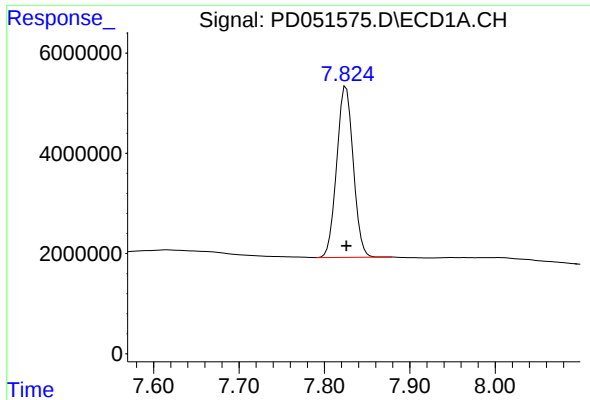

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 45925071
Conc: 38.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC74

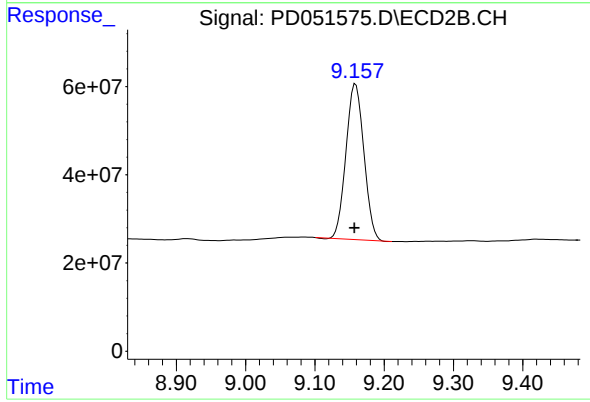

#27 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 633005556
Conc: 33.39 ng/ml