

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 17:38
 Operator : AJ\SJ
 Sample : K1661-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFC76

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:38:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.045	29860420	650.6E6	20.779	21.059
2)	SA Decachlor...	7.825	9.158	47370612	678.1E6	39.389	35.771
Target Compounds							
3)	MA gamma-BHC...	3.925	0.000	4704224	0	2.235	N.D. #
6)	B beta-BHC	0.000	4.941f	0	39854018	N.D.	2.009
8)	B Heptachlo...	0.000	5.918	0	16959462	N.D.	0.474

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 17:38
Operator : AJ\SJ
Sample : K1661-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:38:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

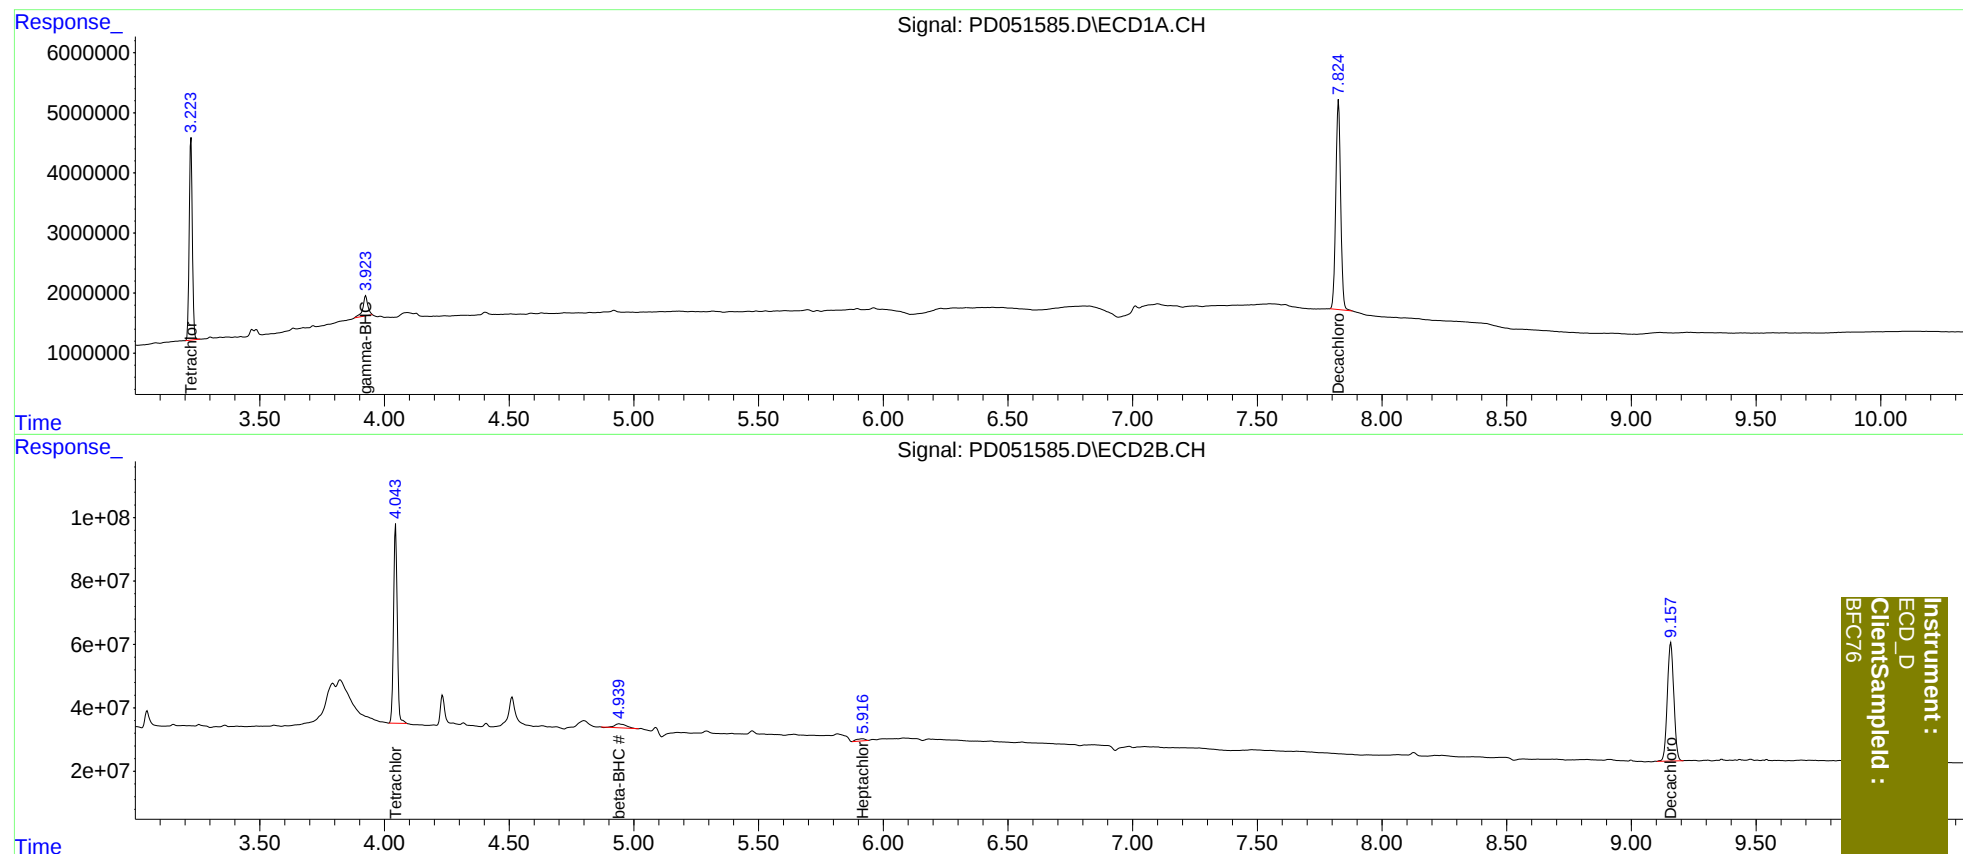


Instrument :
ECD_D
ClientSampleId :
BFC76

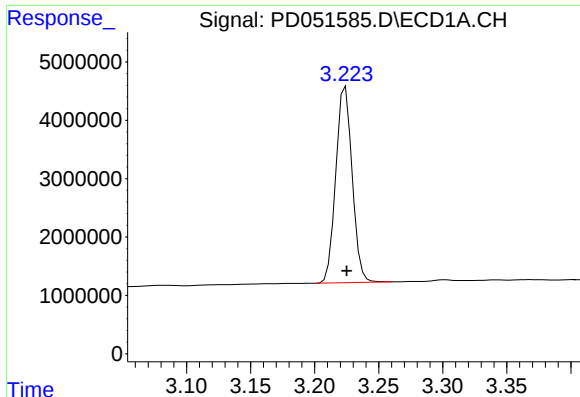

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 29860420
Conc: 20.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC76

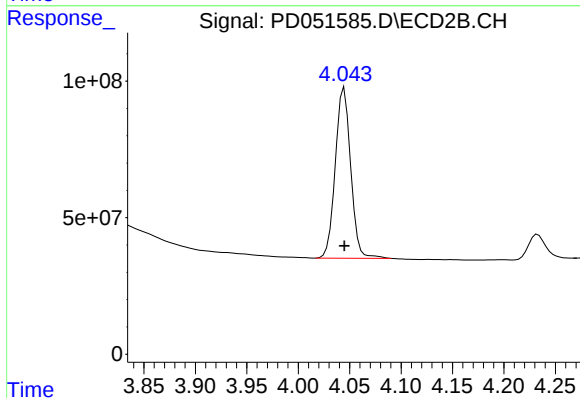


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 650641931
Conc: 21.06 ng/ml

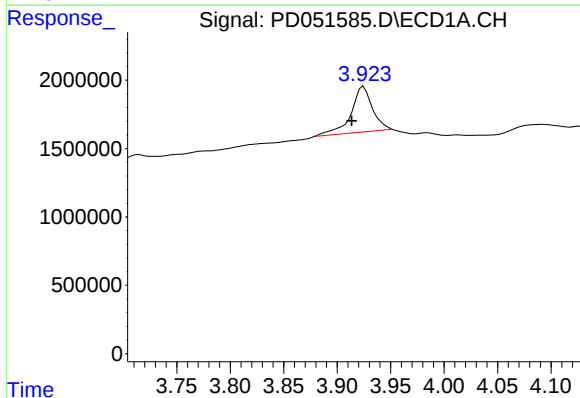


#3 gamma-BHC (Lindane)

R.T.: 3.925 min
Delta R.T.: 0.011 min
Response: 4704224
Conc: 2.23 ng/ml

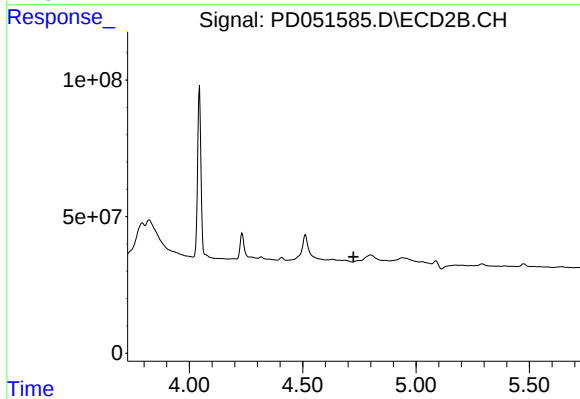

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.724 min
Response: 0
Conc: N.D.

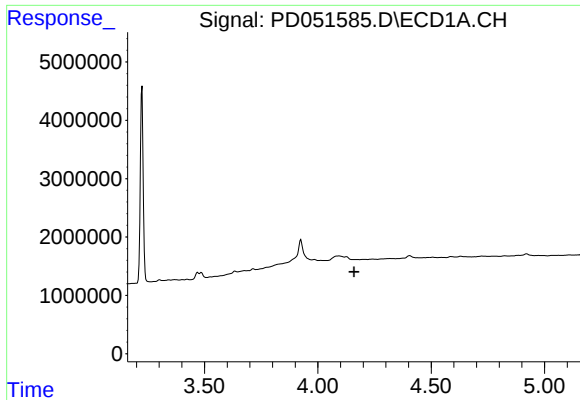

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.159 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC76

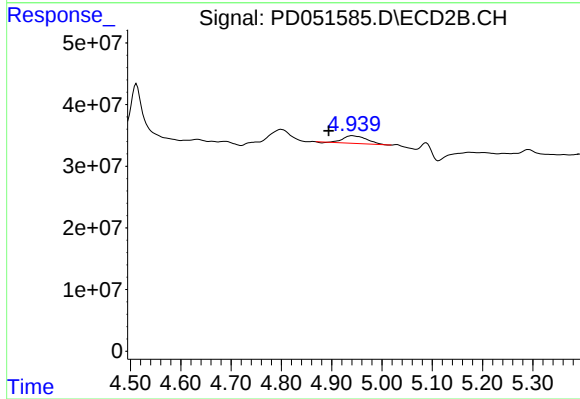


#6 beta-BHC

R.T.: 4.941 min
Delta R.T.: 0.047 min
Response: 39854018
Conc: 2.01 ng/ml

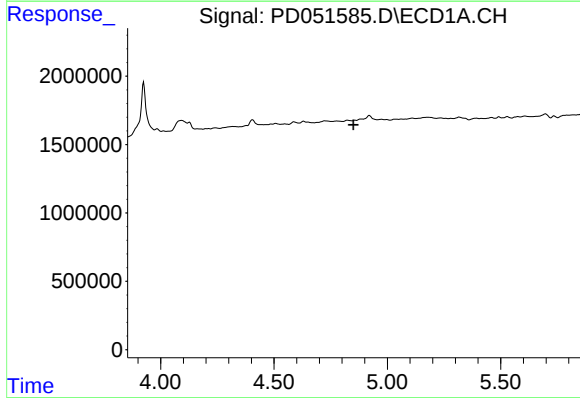


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

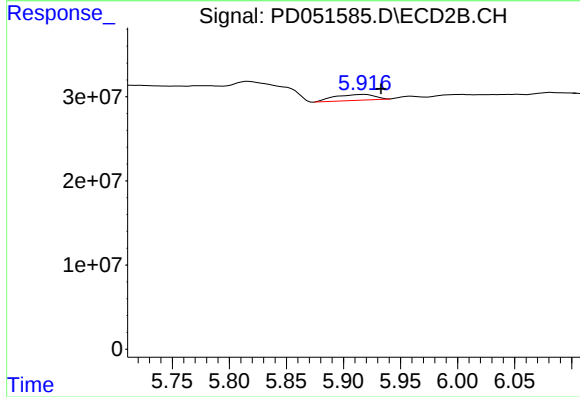

#8 Heptachlor epoxide


R.T.: 5.918 min
Delta R.T.: -0.015 min
Response: 16959462
Conc: 0.47 ng/ml

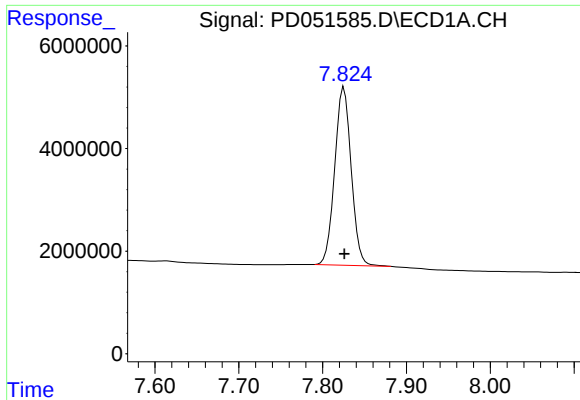

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 47370612
Conc: 39.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC76

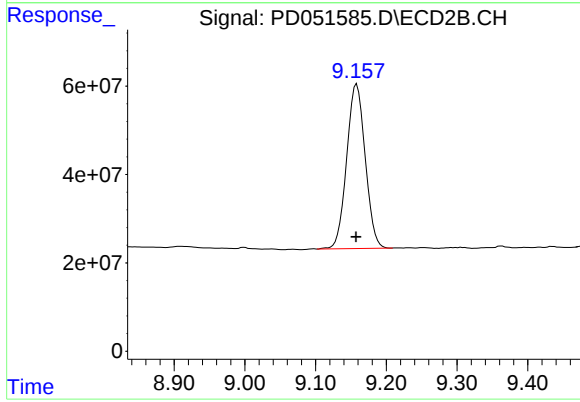

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: 0.001 min
Response: 678126873
Conc: 35.77 ng/ml